

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 13:49
 Operator : AJ\MA
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PEM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 15:22:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.015	221.7E6	63120373	21.165	21.586
28)	SA Decachlor...	8.252	9.092	201.9E6	48390067	19.176	21.393
Target Compounds							
2)	A alpha-BHC	3.936	4.404	175.6E6	43192499	9.852	9.868
3)	MA gamma-BHC...	4.220	4.689	154.9E6	40121913	9.461	9.784
6)	B beta-BHC	4.470	4.860	67507222	17742786	10.249	10.822
14)	MA Endrin	6.054	6.722	652.1E6	126.7E6	46.410	48.330
16)	A 4,4'-DDD	6.178	0.000	24382124	0	2.268	N.D. #
17)	MA 4,4'-DDT	6.418	7.145	1077.9E6	221.5E6	98.627	96.504
20)	A Methoxychlor	6.963	7.605	1253.9E6	276.7E6	236.041	225.681
21)	B Endrin ke...	7.198	0.000	20463256	0	1.564	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056177.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 13:49
Operator : AJ\MA
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PEM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 15:22:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

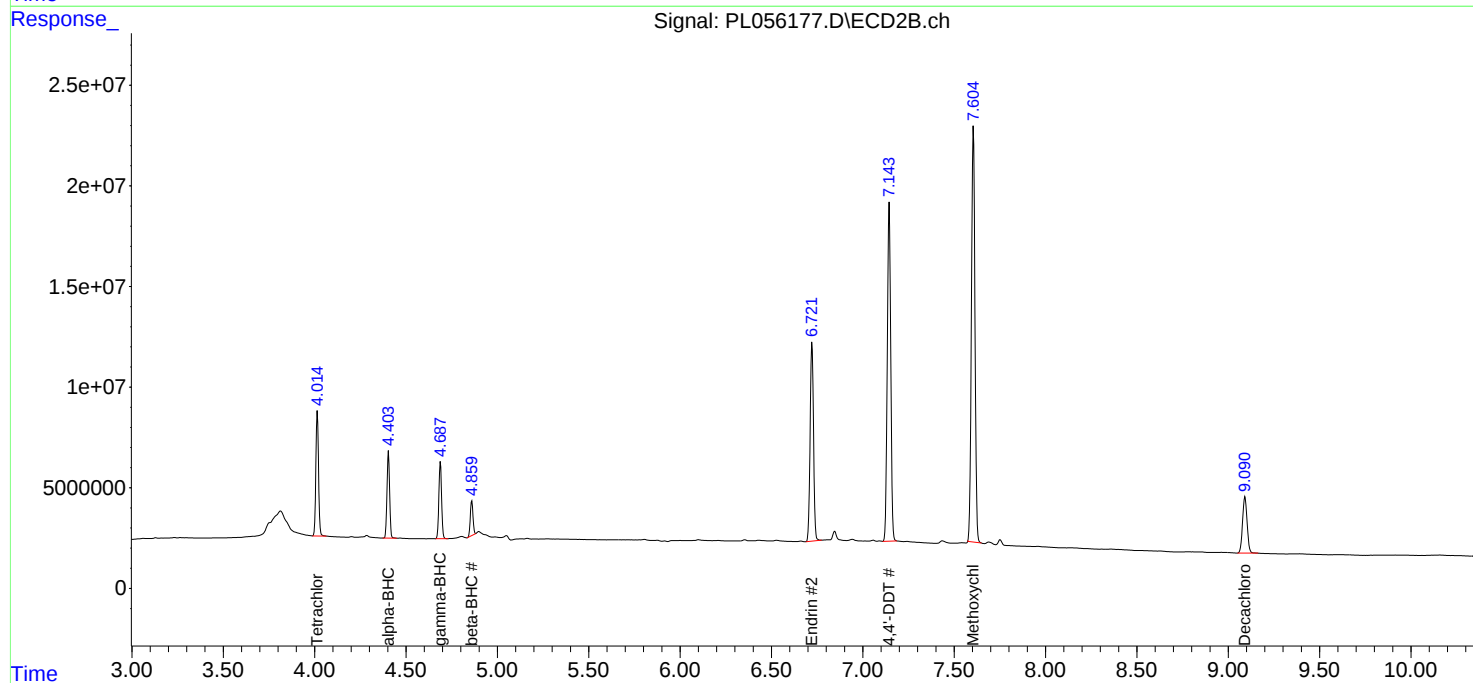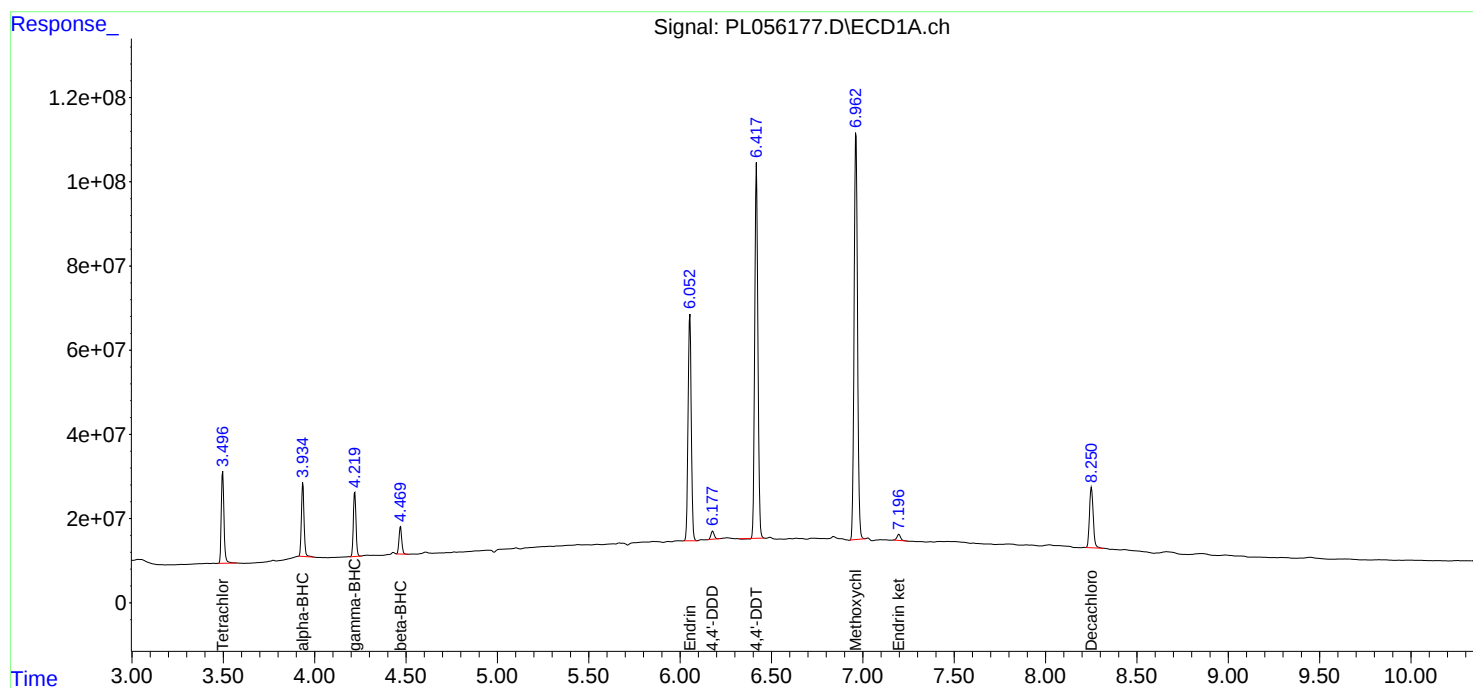


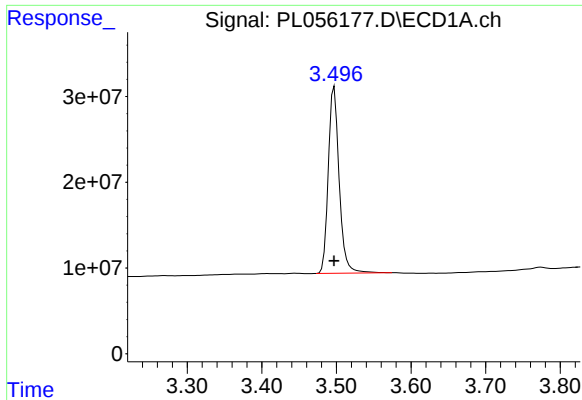

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 221664517
Conc: 21.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

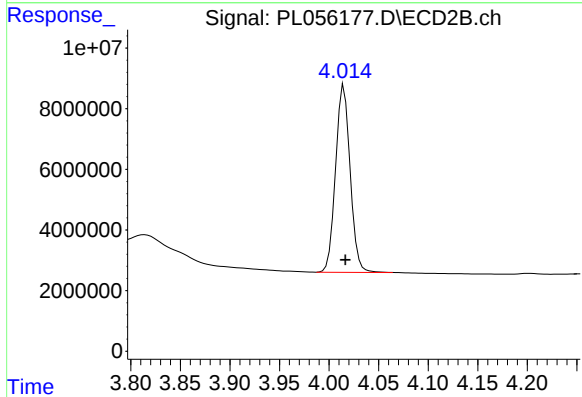


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.001 min
Response: 63120373
Conc: 21.59 ng/ml

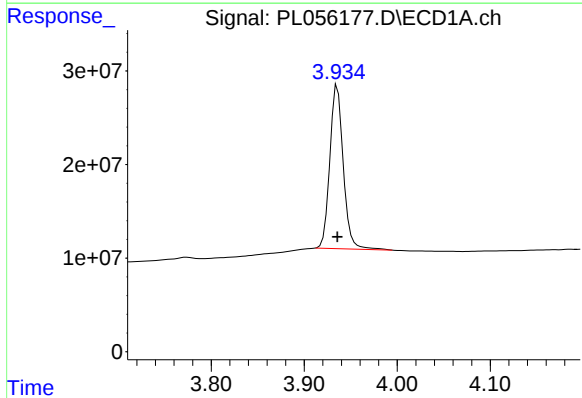


#2 alpha-BHC

R.T.: 3.936 min
Delta R.T.: 0.000 min
Response: 175561026
Conc: 9.85 ng/ml

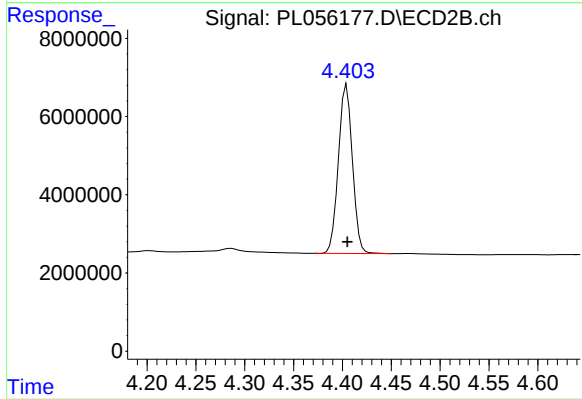

#2 alpha-BHC


R.T.: 4.404 min
Delta R.T.: 0.000 min
Response: 43192499
Conc: 9.87 ng/ml

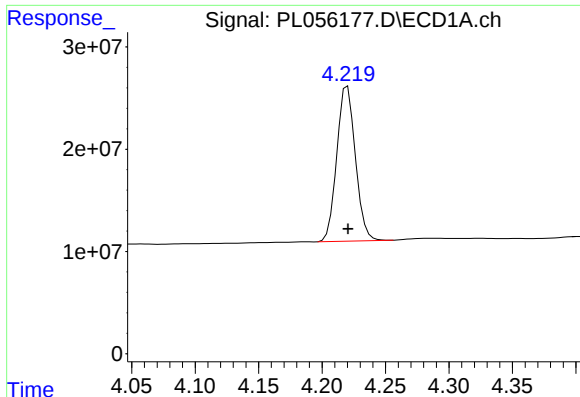

#3 gamma-BHC (Lindane)


R.T.: 4.220 min
Delta R.T.: 0.000 min
Response: 154919464
Conc: 9.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

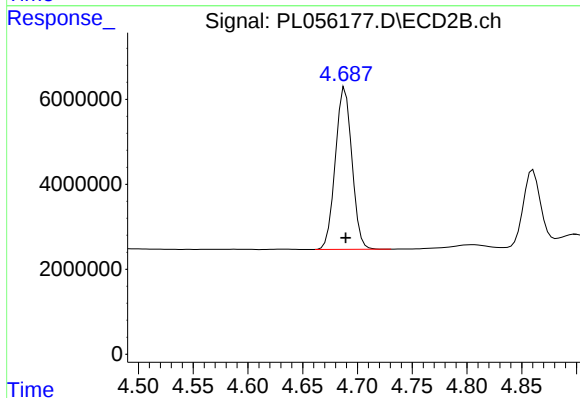


#3 gamma-BHC (Lindane)

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 40121913
Conc: 9.78 ng/ml

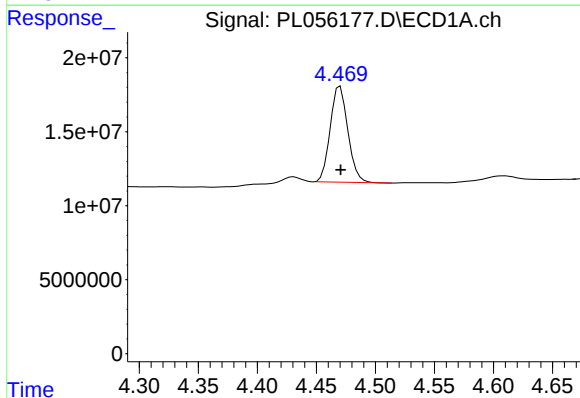


#6 beta-BHC

R.T.: 4.470 min
Delta R.T.: 0.000 min
Response: 67507222
Conc: 10.25 ng/ml

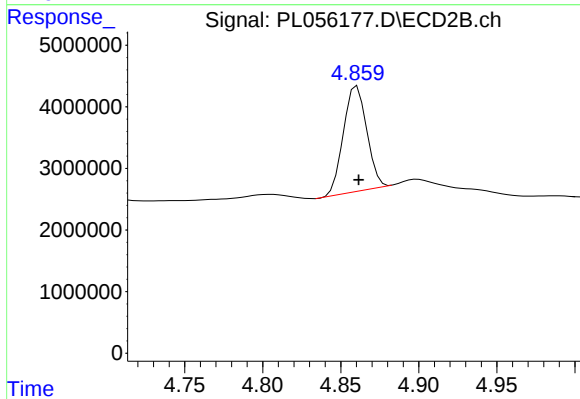

#6 beta-BHC


R.T.: 4.860 min
Delta R.T.: -0.001 min
Response: 17742786
Conc: 10.82 ng/ml

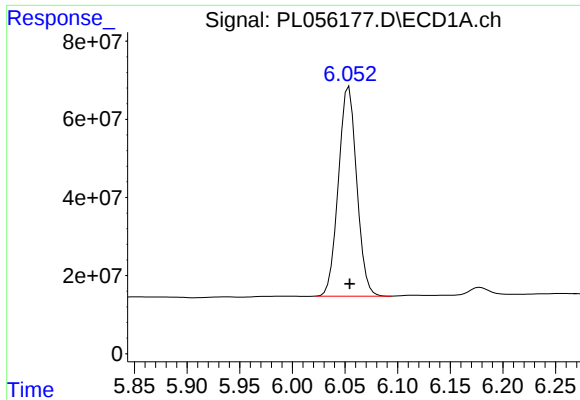

#14 Endrin


R.T.: 6.054 min
Delta R.T.: 0.000 min
Response: 652141384
Conc: 46.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

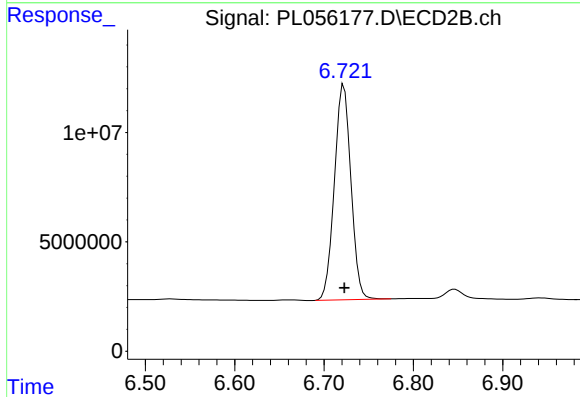


#14 Endrin

R.T.: 6.722 min
Delta R.T.: 0.000 min
Response: 126658503
Conc: 48.33 ng/ml

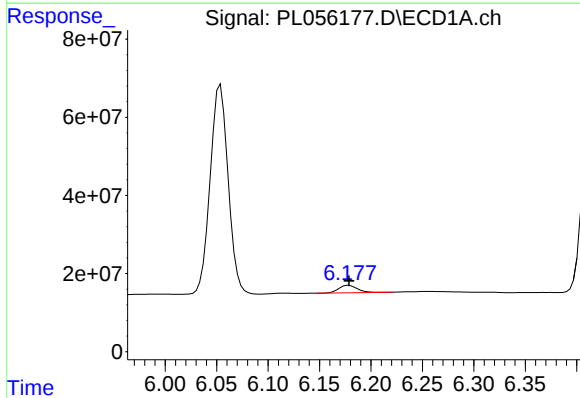


#16 4,4'-DDD

R.T.: 6.178 min
Delta R.T.: 0.000 min
Response: 24382124
Conc: 2.27 ng/ml

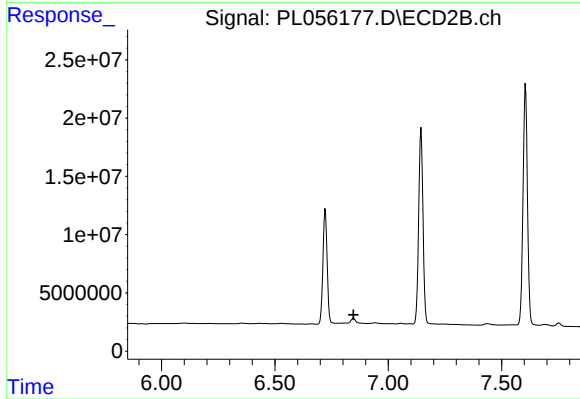

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.847 min
Response: 0
Conc: N.D.

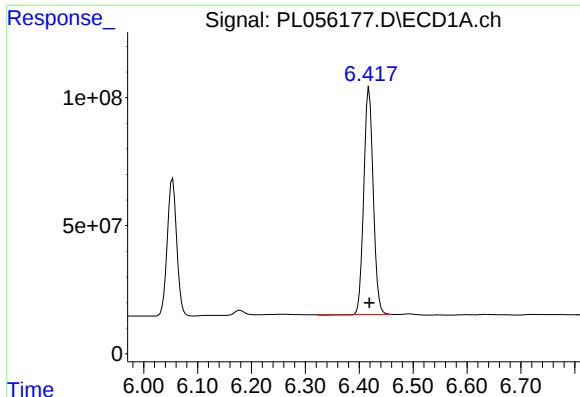

#17 4,4'-DDT


R.T.: 6.418 min
Delta R.T.: 0.000 min
Response: 1077875422
Conc: 98.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

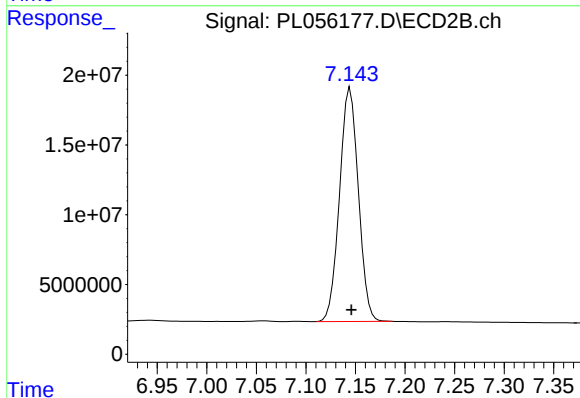


#17 4,4'-DDT

R.T.: 7.145 min
Delta R.T.: -0.001 min
Response: 221549473
Conc: 96.50 ng/ml

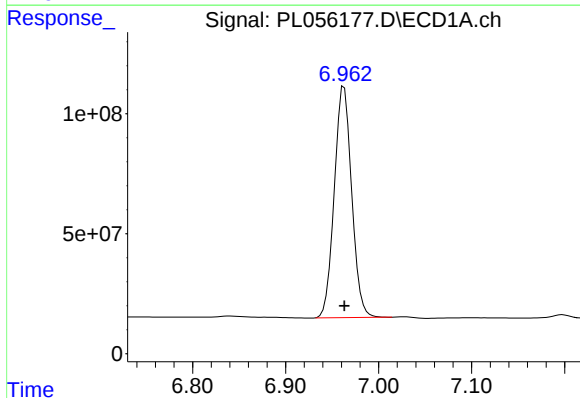


#20 Methoxychlor

R.T.: 6.963 min
Delta R.T.: 0.000 min
Response: 1253902766
Conc: 236.04 ng/ml

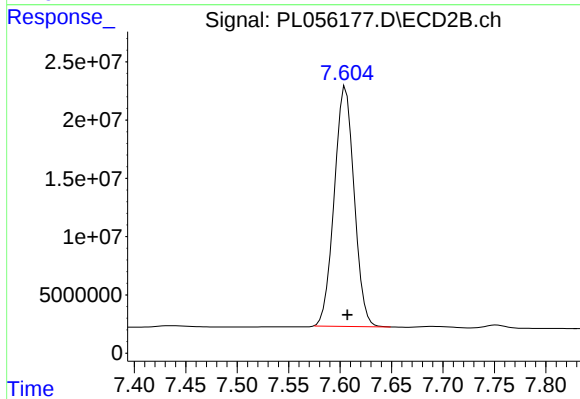

#20 Methoxychlor


R.T.: 7.605 min
Delta R.T.: -0.002 min
Response: 276705960
Conc: 225.68 ng/ml

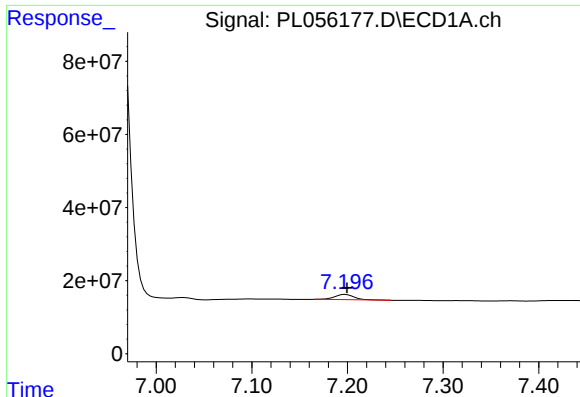

#21 Endrin ketone


R.T.: 7.198 min
Delta R.T.: -0.002 min
Response: 20463256
Conc: 1.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
PEM

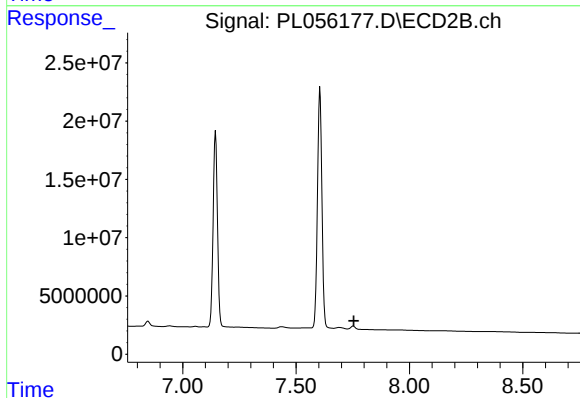


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.755 min
Response: 0
Conc: N.D.

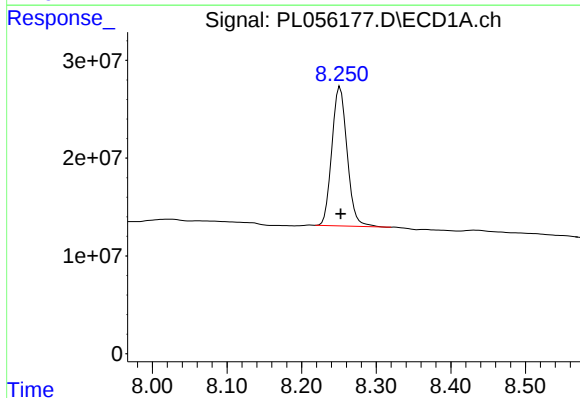

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 201885826
Conc: 19.18 ng/ml

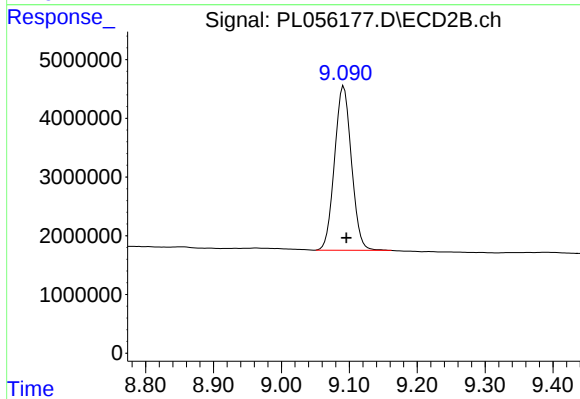

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.004 min
Response: 48390067
Conc: 21.39 ng/ml