

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056184.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 15:27
 Operator : AJ\MA
 Sample : L1287-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 AOC-3-EXC-PIT-(0-5)-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 16:17:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	183.8E6	56121064	17.553	19.193
28)	SA Decachlor...	8.252	9.092	145.6E6	35974620	13.833	15.904
Target Compounds							
2)	A alpha-BHC	3.941	0.000	28217229	0	1.583	N.D. #
23)	Chlordane-1	4.373	0.000	21670683	0	57.248	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056184.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 15:27
Operator : AJ\MA
Sample : L1287-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 16:17:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

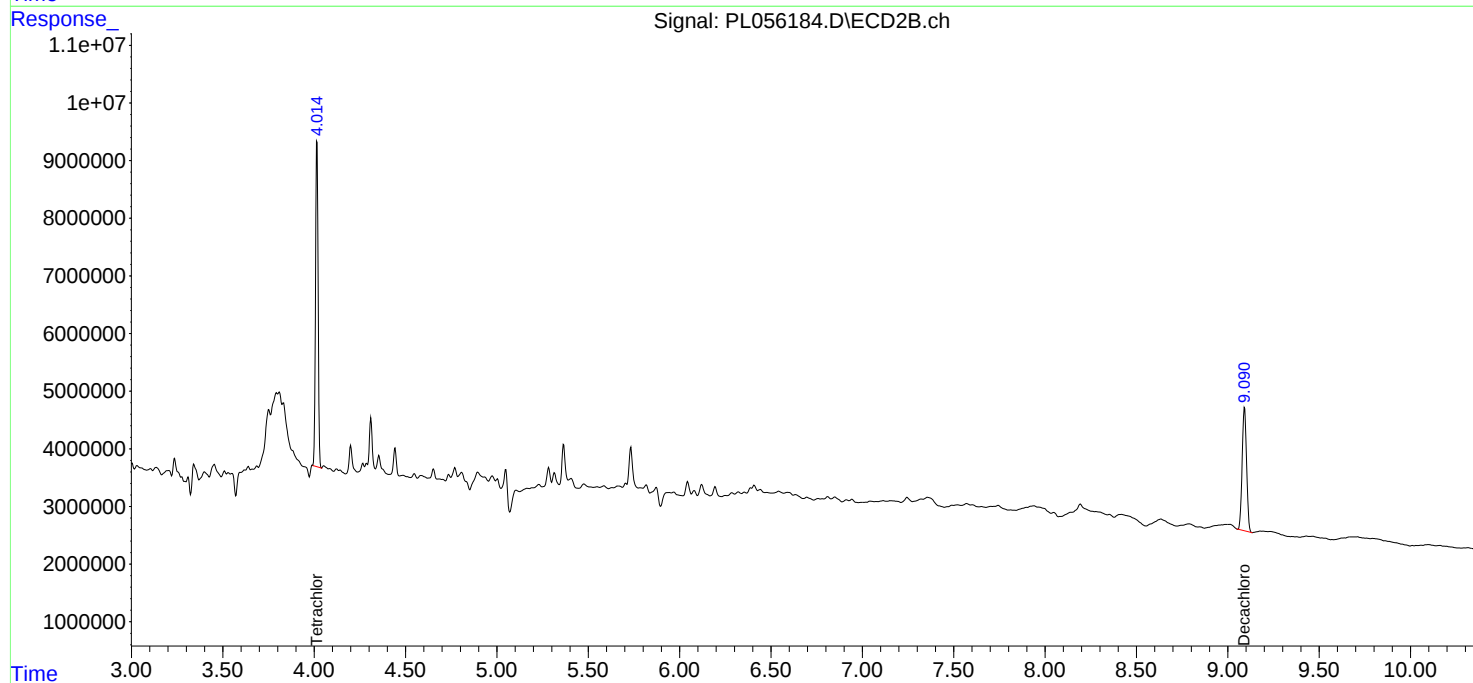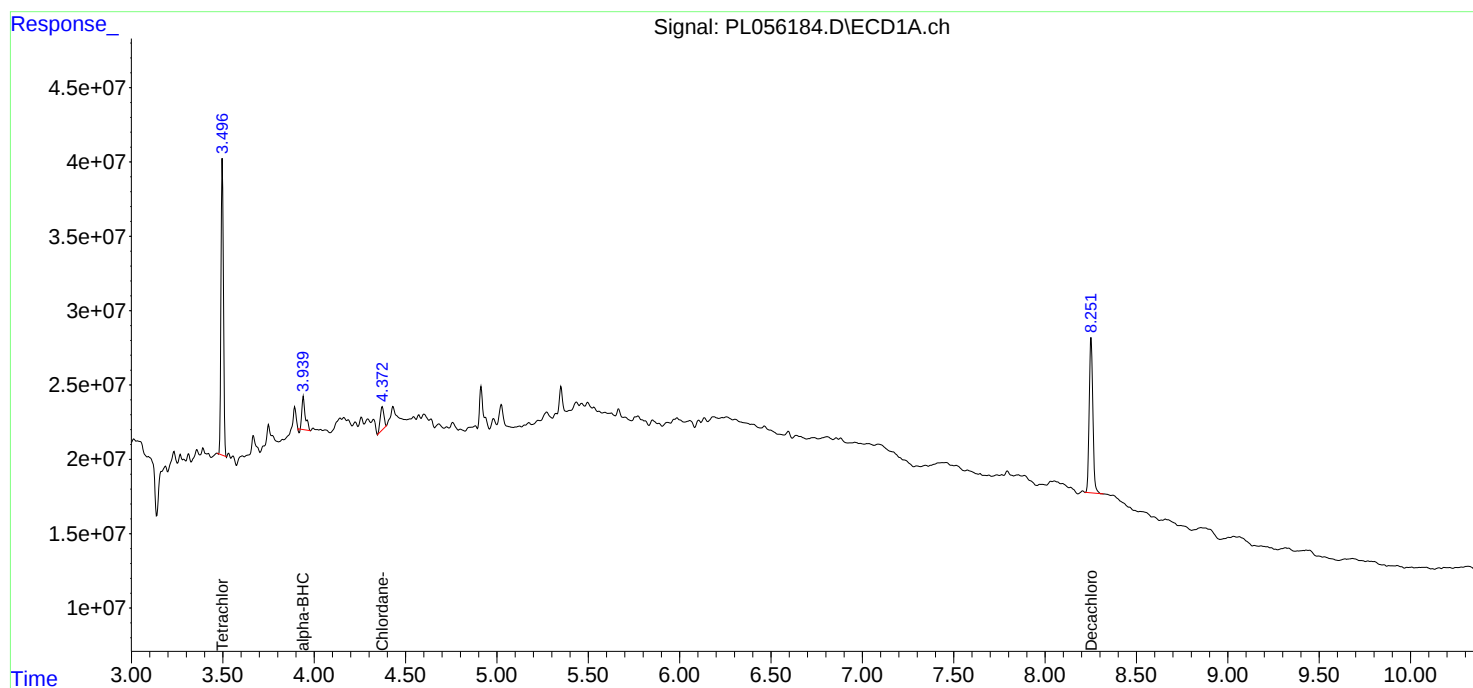


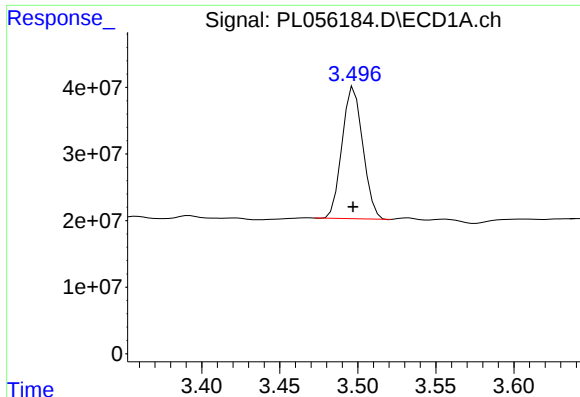

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 183837140
Conc: 17.55 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-B

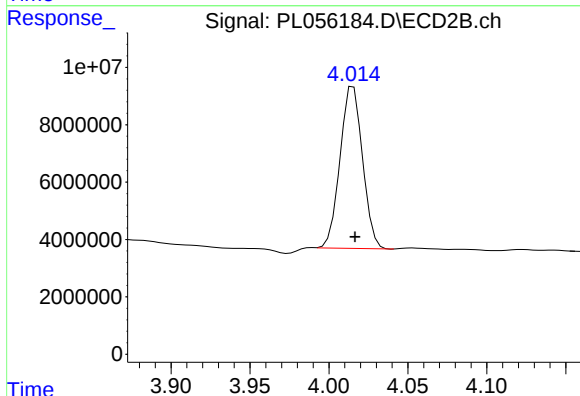


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 56121064
Conc: 19.19 ng/ml

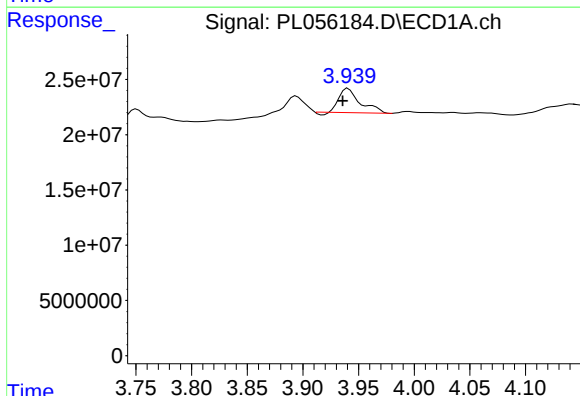


#2 alpha-BHC

R.T.: 3.941 min
Delta R.T.: 0.005 min
Response: 28217229
Conc: 1.58 ng/ml

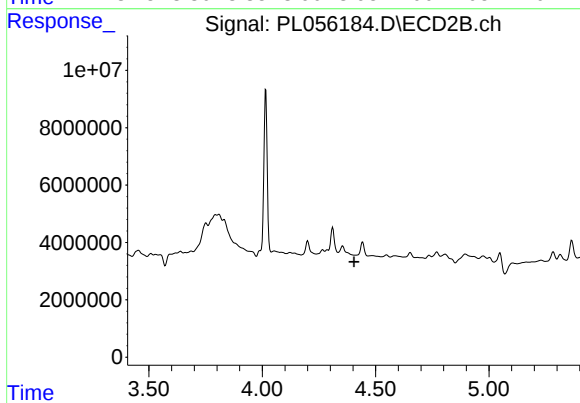

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.405 min
Response: 0
Conc: N.D.

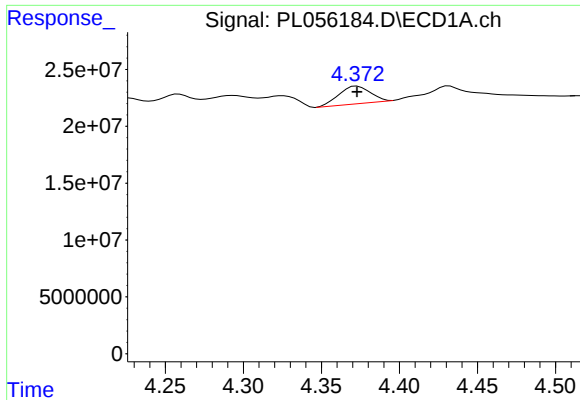

#23 Chlordane-1


R.T.: 4.373 min
Delta R.T.: 0.000 min
Response: 21670683
Conc: 57.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
AOC-3-EXC-PIT-(0-5)-B

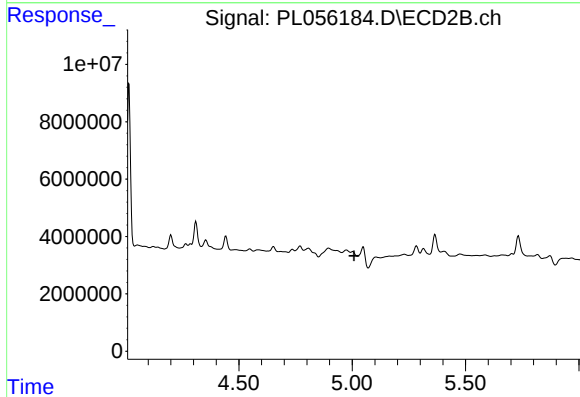


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

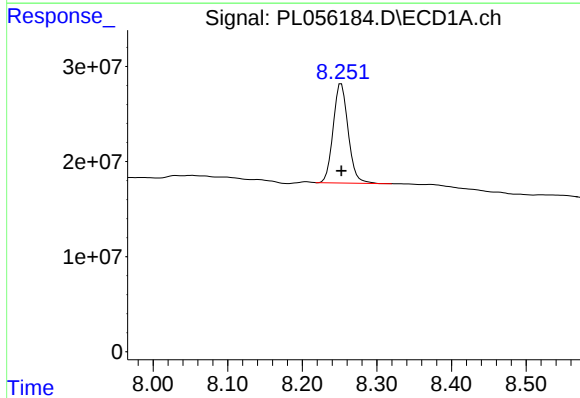

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 145632103
Conc: 13.83 ng/ml

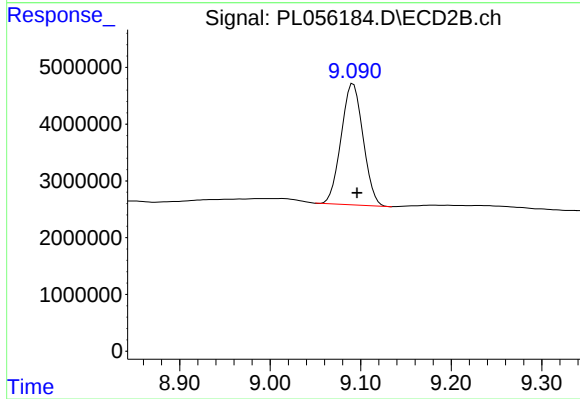

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.004 min
Response: 35974620
Conc: 15.90 ng/ml