

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 19:27
 Operator : AJ\MA
 Sample : L1289-22
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TP-32-33-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 04:12:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	195.3E6	58598653	18.645	20.040
28)	SA Decachlor...	8.252	9.091	180.6E6	46903575	17.150	20.736
Target Compounds							
19)	B Endosulfa...	6.724f	0.000	2427878	0	0.200	N.D. #
23)	Chlordane-1	4.392f	0.000	210237	0	0.555	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056199.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 19:27
Operator : AJ\MA
Sample : L1289-22
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TP-32-33-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 04:12:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

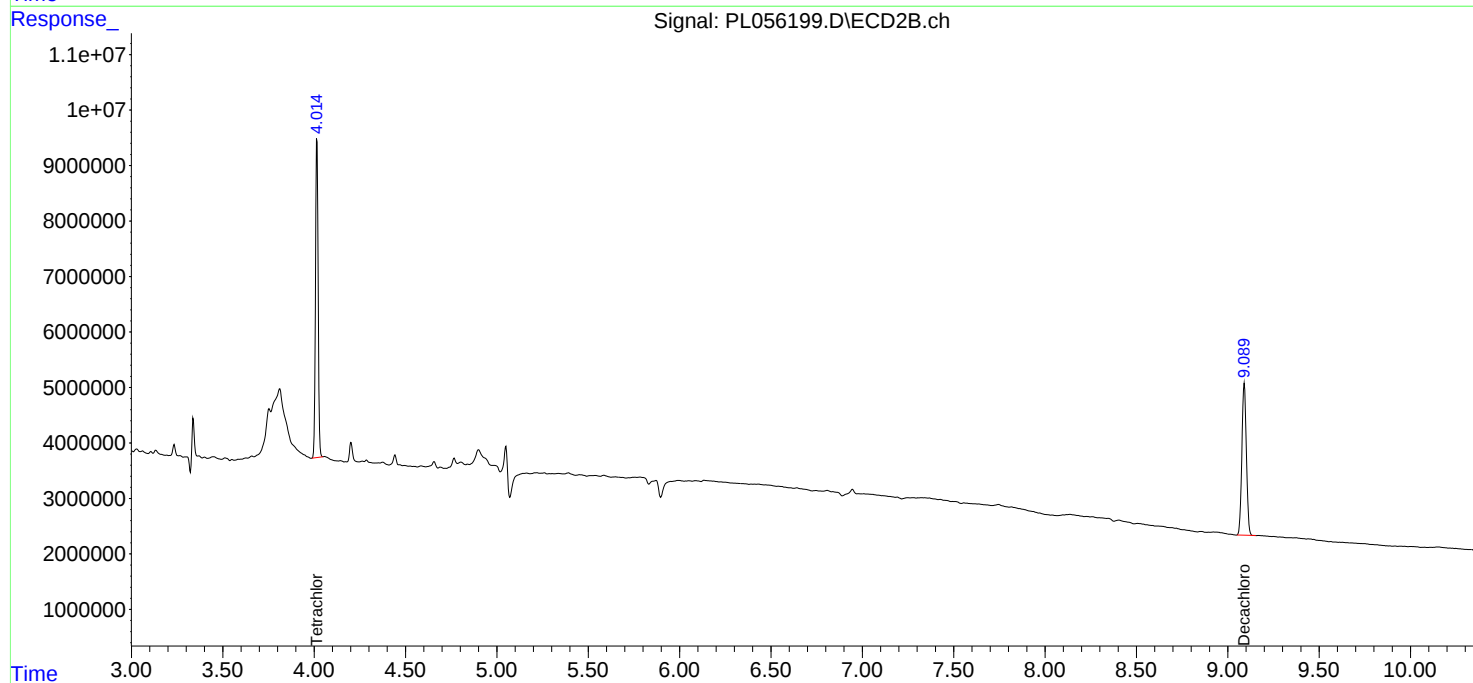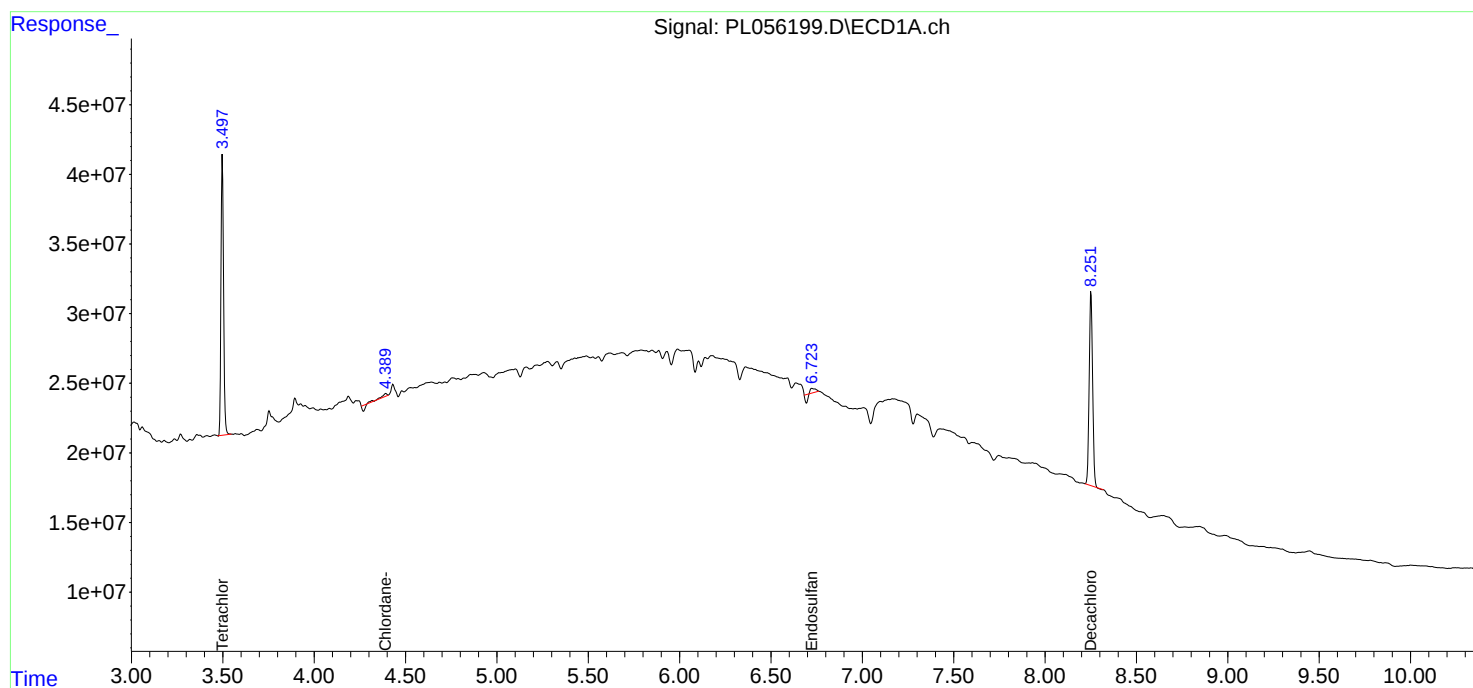


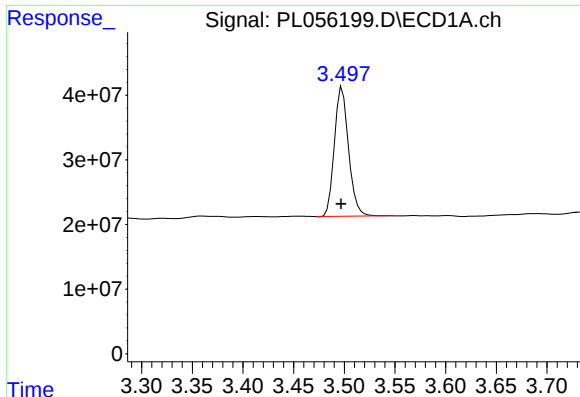

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.001 min
Response: 195267268
Conc: 18.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32-33-COMP

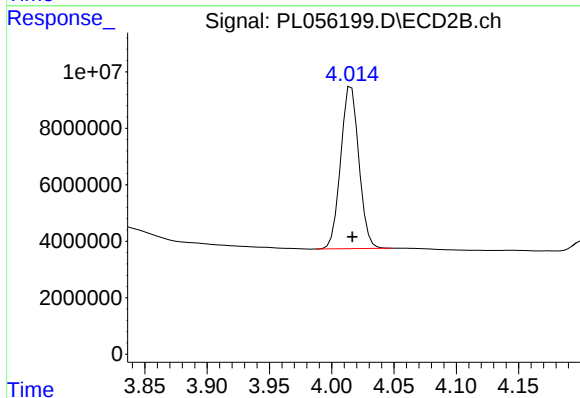


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 58598653
Conc: 20.04 ng/ml

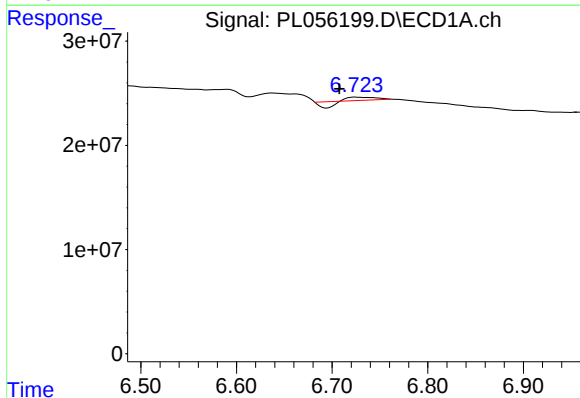


#19 Endosulfan Sulfate

R.T.: 6.724 min
Delta R.T.: 0.016 min
Response: 2427878
Conc: 0.20 ng/ml

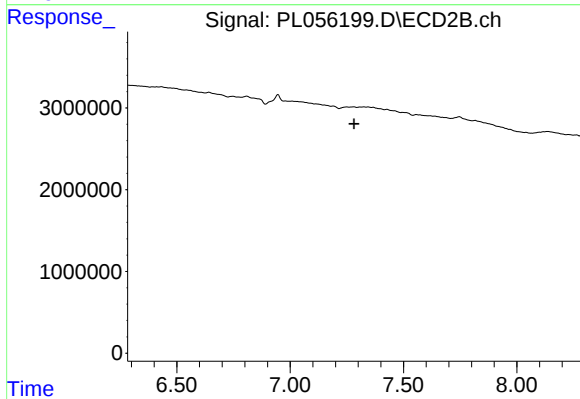

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.282 min
Response: 0
Conc: N.D.

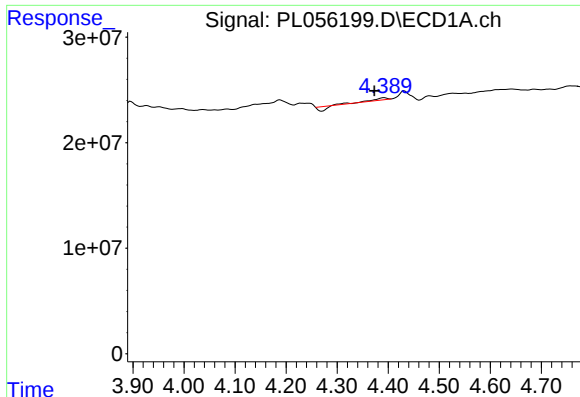

#23 Chlordane-1


R.T.: 4.392 min
Delta R.T.: 0.019 min
Response: 210237
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
TP-32-33-COMP

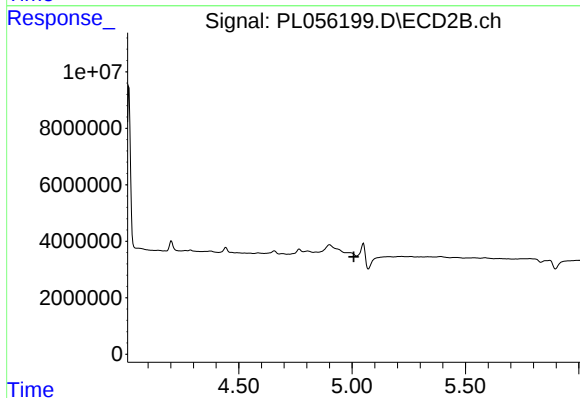


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

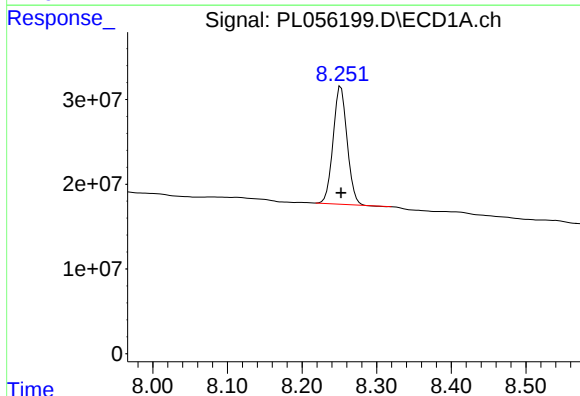

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 180553406
Conc: 17.15 ng/ml

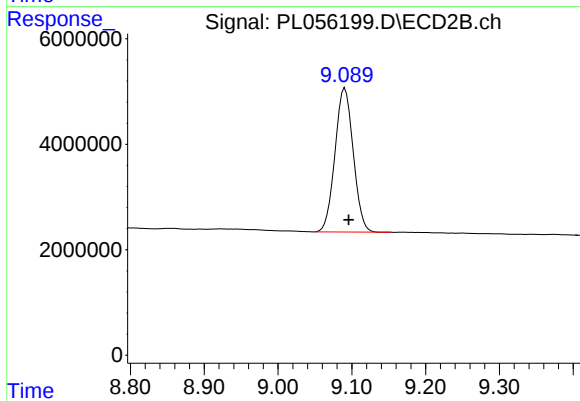

#28 Decachlorobiphenyl

R.T.: 9.091 min
Delta R.T.: -0.005 min
Response: 46903575
Conc: 20.74 ng/ml