

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
 Data File : PL056179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2020 14:17
 Operator : AJ\MA
 Sample : L1274-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BORING-B2-SAMPLE-S1

Manual Integrations
 APPROVED

mohammad
 1/30/2020 11:32:19 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 16:16:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.500	4.013	239.3E6	35707217	22.851m	12.211m#
28)	SA Decachlor...	8.255	9.092	160.5E6	25996785	15.242	11.493

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012920\
Data File : PL056179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2020 14:17
Operator : AJ\MA
Sample : L1274-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BORING-B2-SAMPLE-S1


Manual Integrations
APPROVED

mohammad
1/30/2020 11:32:19 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 16:16:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

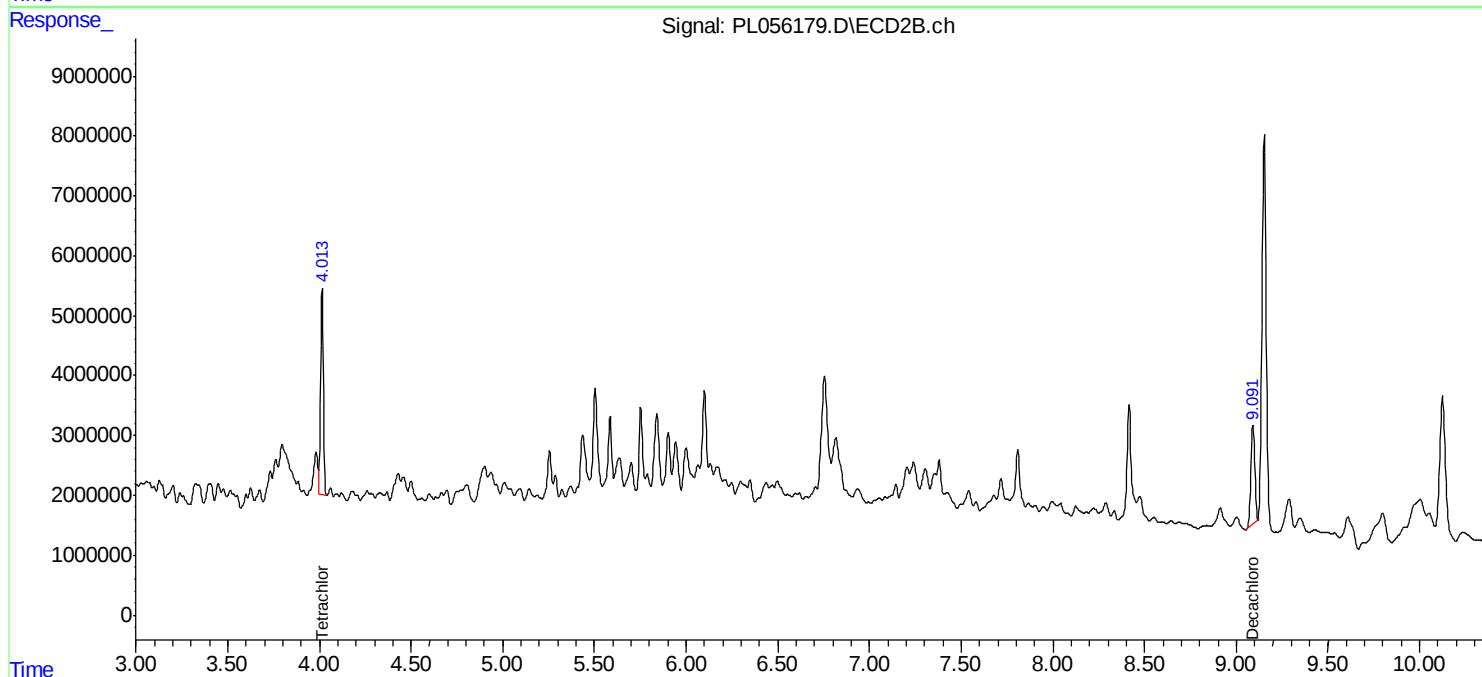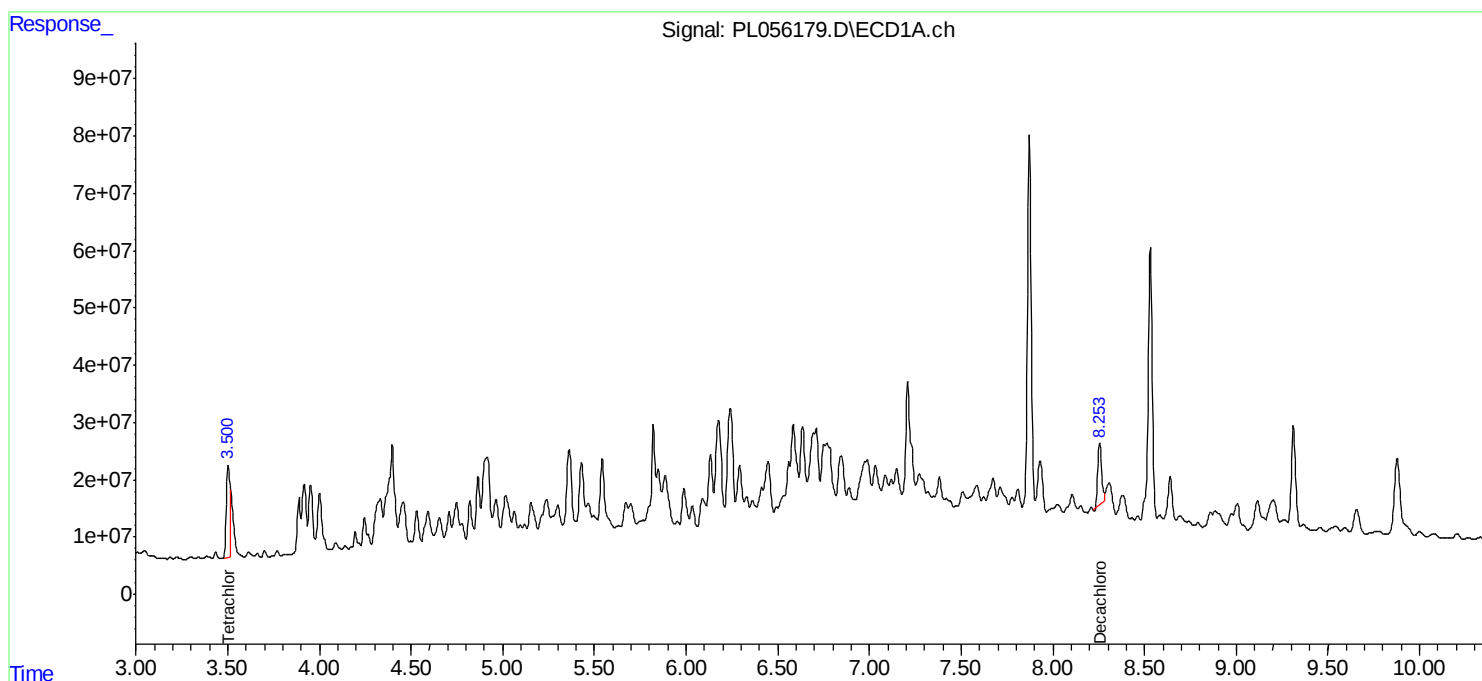

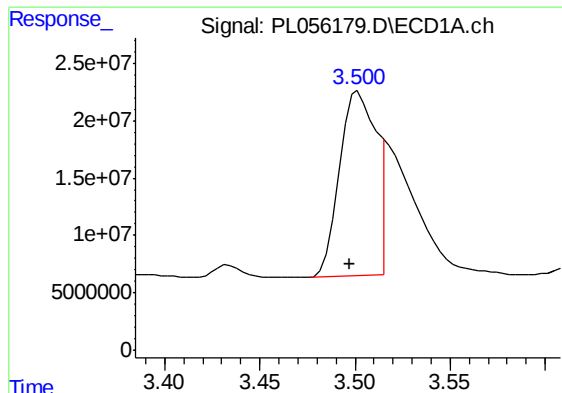


#1 Tetrachloro-m-xylene

R.T.: 3.500 min
Delta R.T.: 0.003 min
Response: 239320054
Conc: 22.85 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BORING-B2-SAMPLE-S1


Manual Integrations
APPROVED

mohammad
1/30/2020 11:32:19 AM

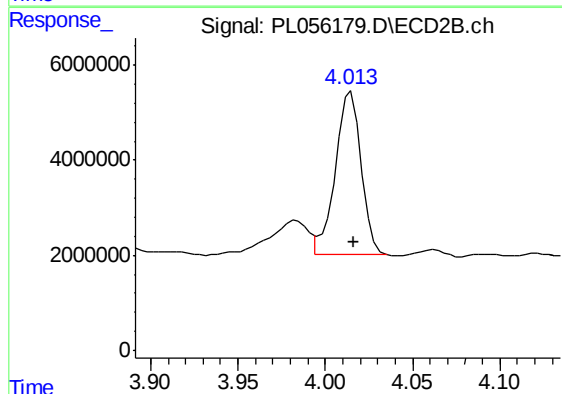


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.003 min
Response: 35707217
Conc: 12.21 ng/ml m

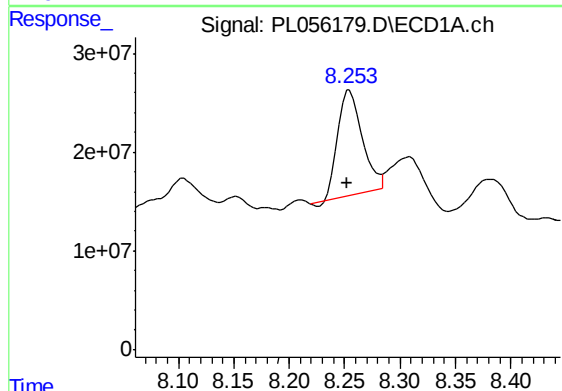

#28 Decachlorobiphenyl

R.T.: 8.255 min
Delta R.T.: 0.002 min
Response: 160468720
Conc: 15.24 ng/ml

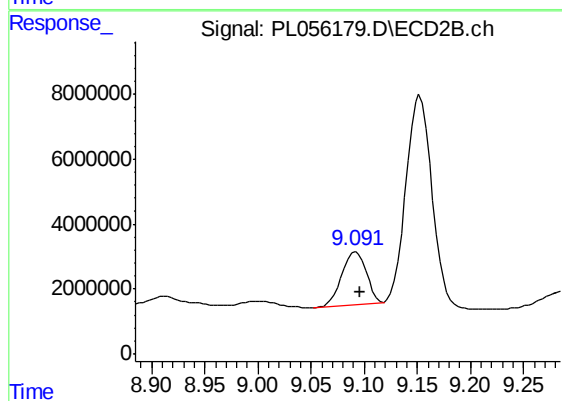

#28 Decachlorobiphenyl

R.T.: 9.092 min
Delta R.T.: -0.003 min
Response: 25996785
Conc: 11.49 ng/ml