

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064483.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 20:57
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:52:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	61503154	47711774	20.204	20.030
28)	SA Decachlor...	8.162	9.268	64374926	41340074	20.428	20.192
Target Compounds							
6)	B beta-BHC	0.000	4.986	0	2120079	N.D.	1.253 #
7)	B delta-BHC	0.000	5.222f	0	3973954	N.D.	1.290 #
23)	Chlordane-1	4.321f	0.000	236574	0	2.152	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064483.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 20:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:52:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

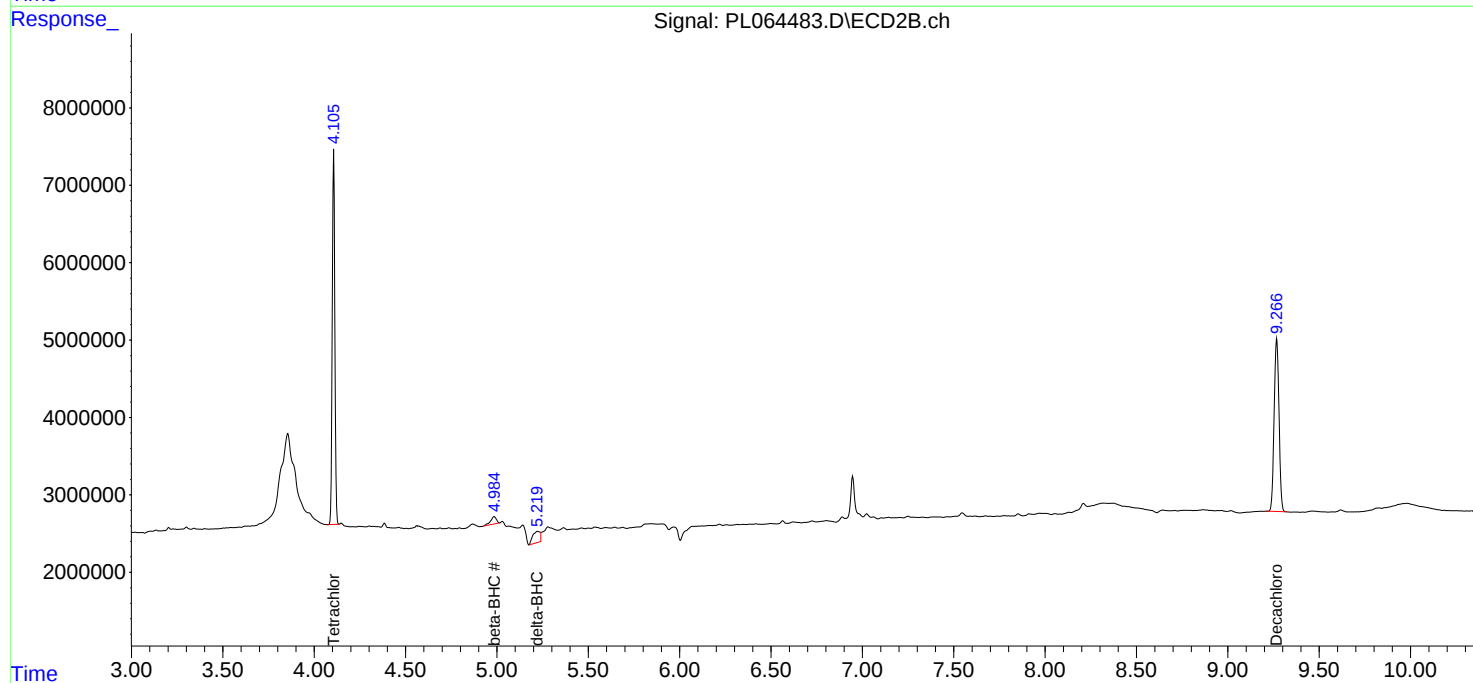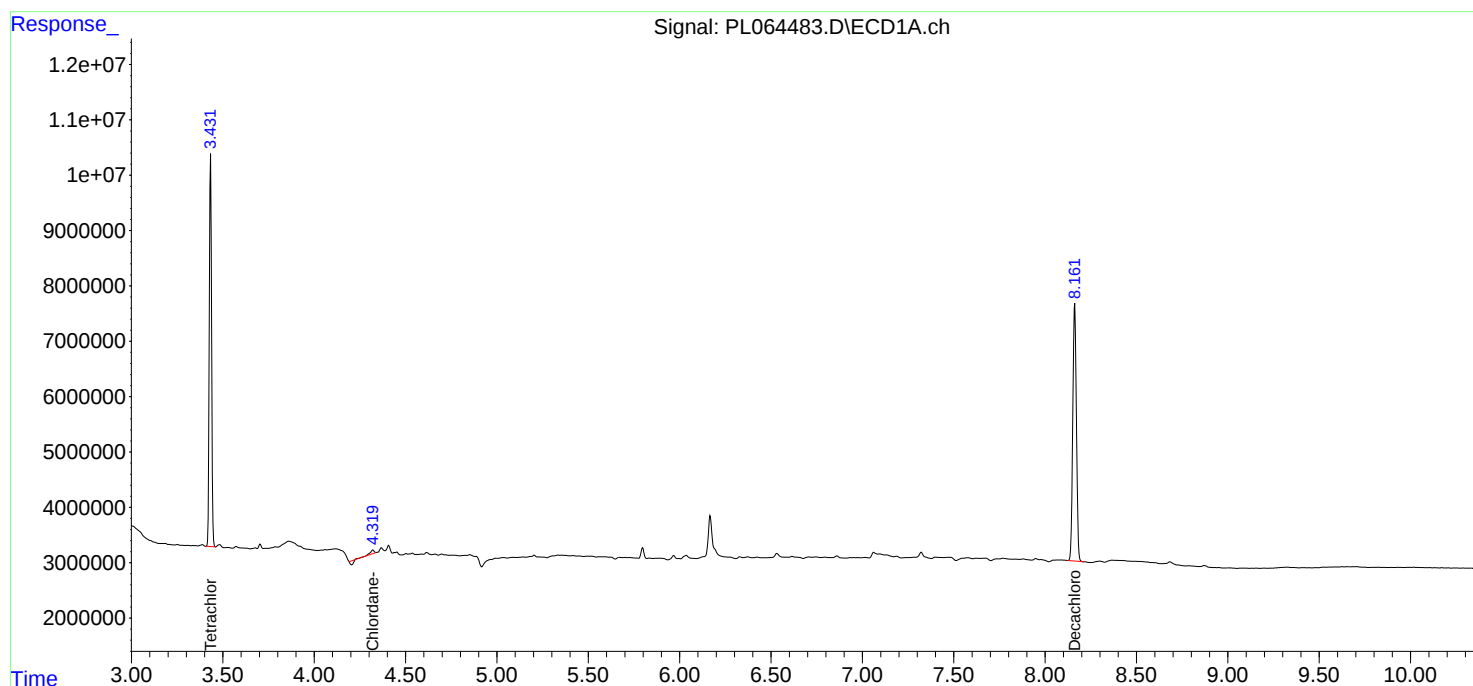


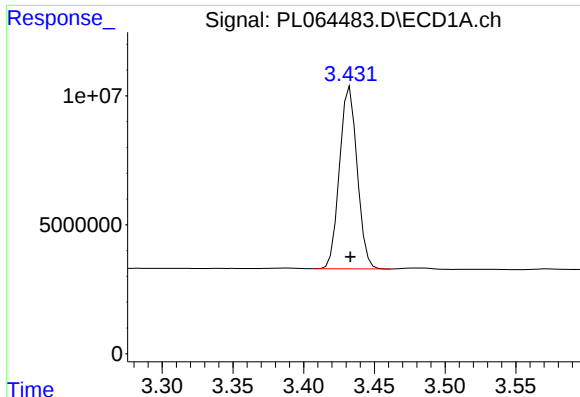

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 61503154
Conc: 20.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

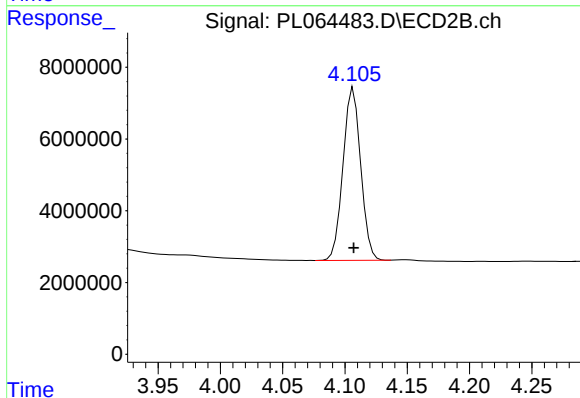


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 47711774
Conc: 20.03 ng/ml

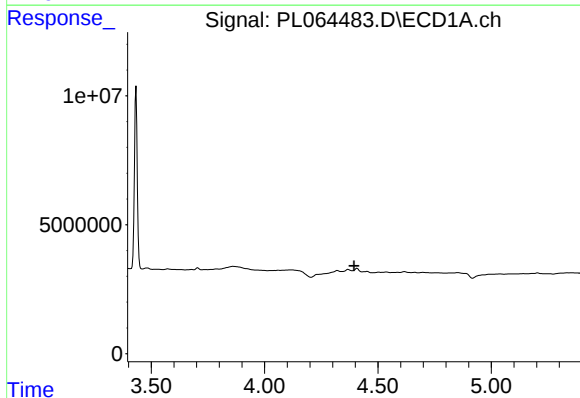


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.395 min
Response: 0
Conc: N.D.

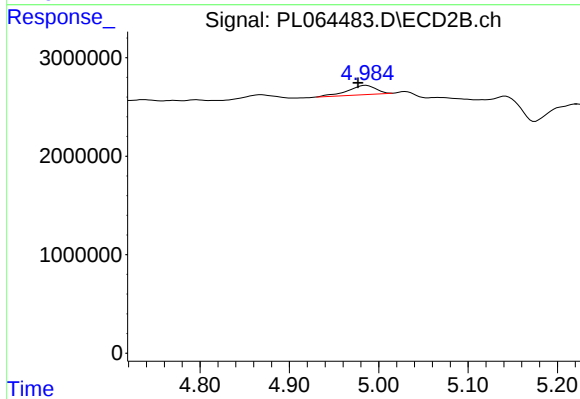

#6 beta-BHC


R.T.: 4.986 min
Delta R.T.: 0.009 min
Response: 2120079
Conc: 1.25 ng/ml

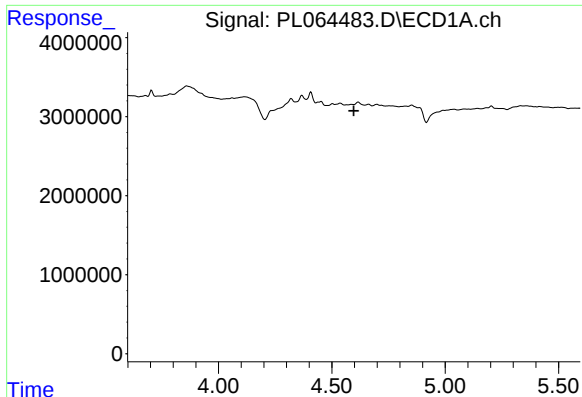

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

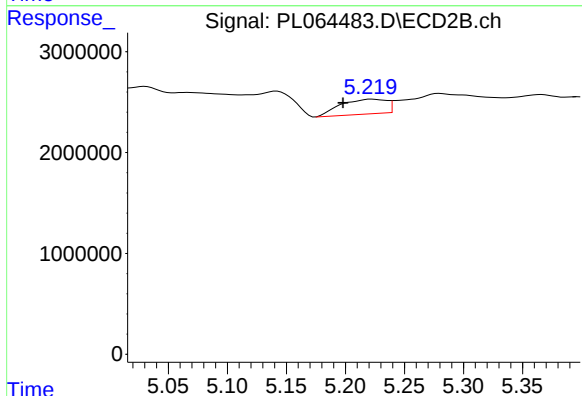


#7 delta-BHC

R.T.: 5.222 min
Delta R.T.: 0.024 min
Response: 3973954
Conc: 1.29 ng/ml

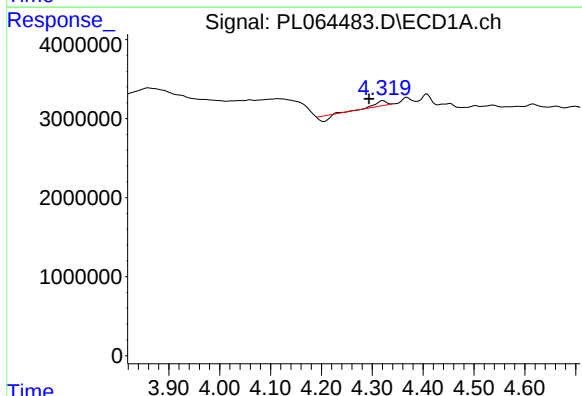


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.028 min
Response: 236574
Conc: 2.15 ng/ml

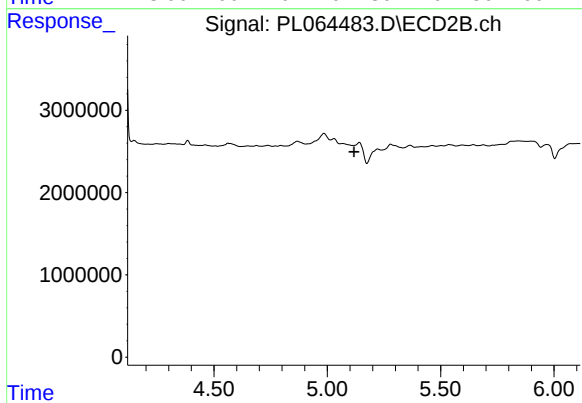

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

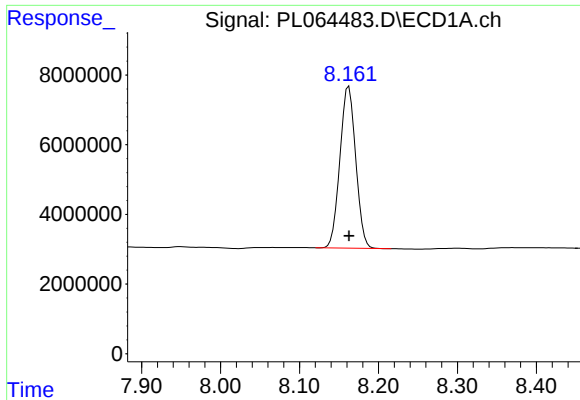

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 64374926
Conc: 20.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

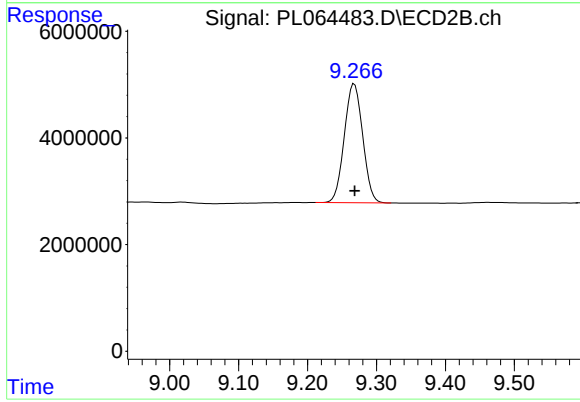

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 41340074
Conc: 20.19 ng/ml