

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064491.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 22:51
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:38:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:37:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	351.1E6	242.0E6	100.879	101.087
28)	SA Decachlor...	8.164	9.268	282.3E6	185.6E6	94.090	94.641
Target Compounds							
23)	Chlordane-1	4.295	5.121	106.7E6	93551210	969.810	955.602
24)	Chlordane-2	4.793	5.597	120.4E6	101.9E6	938.834	931.831
25)	Chlordane-3	5.358	6.253	363.4E6	372.5E6	1005.086	1024.621
26)	Chlordane-4	5.415	6.327	296.1E6	447.4E6	993.349	1007.168
27)	Chlordane-5	6.244	7.146	120.7E6	69266719	997.574	1004.512



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064491.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 22:51
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:38:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:37:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

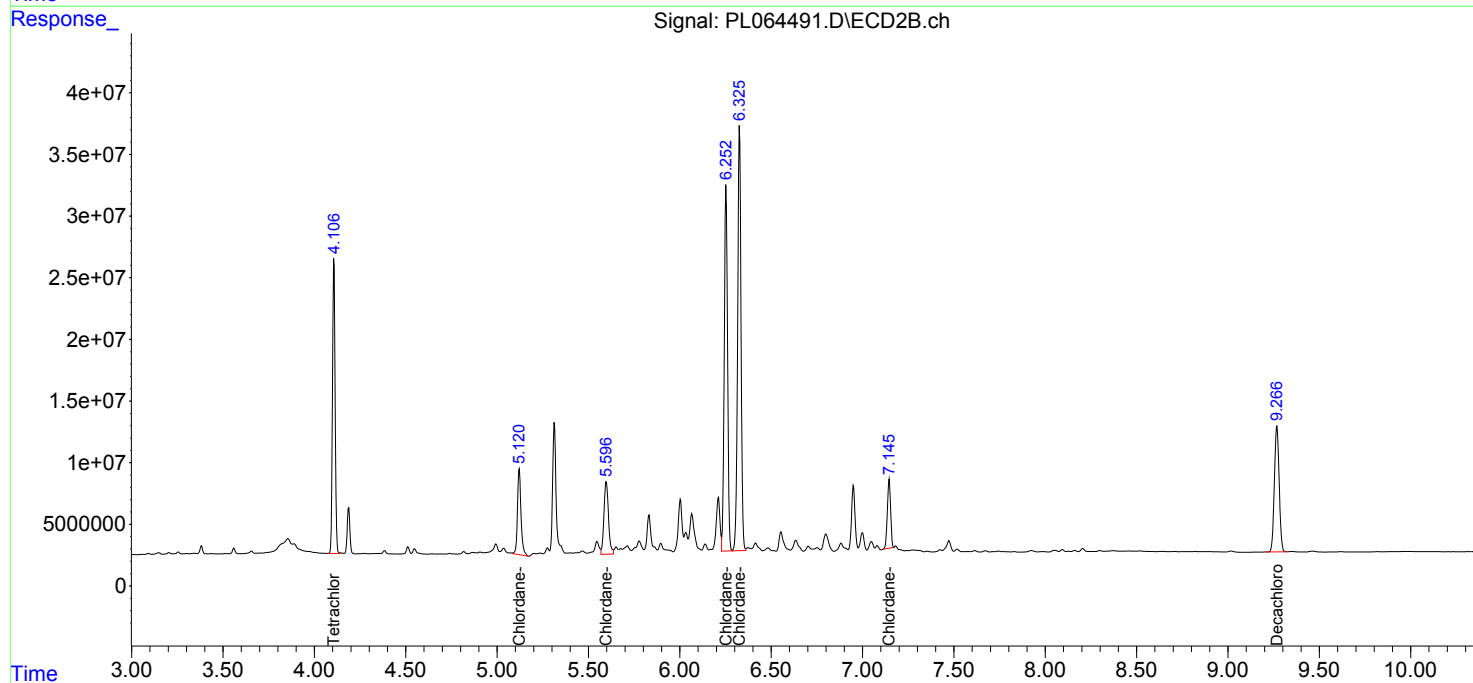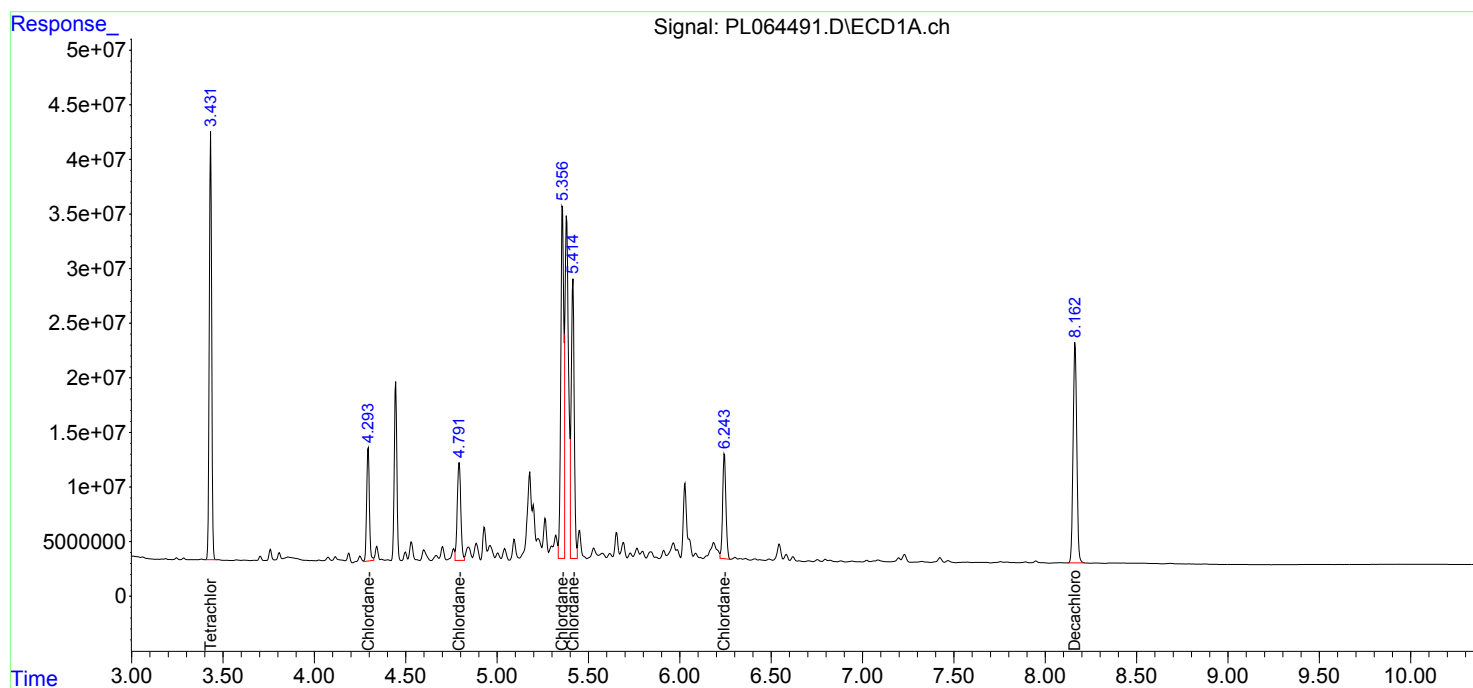


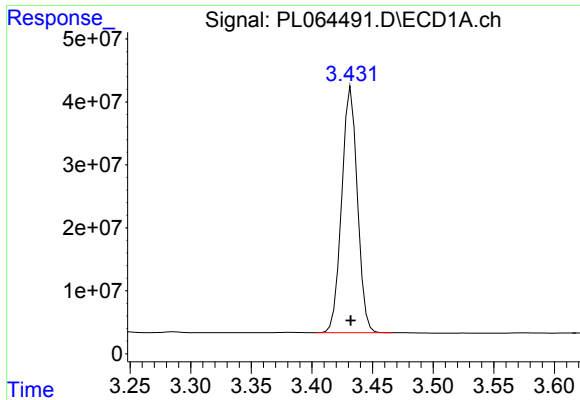

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 351074861
Conc: 100.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

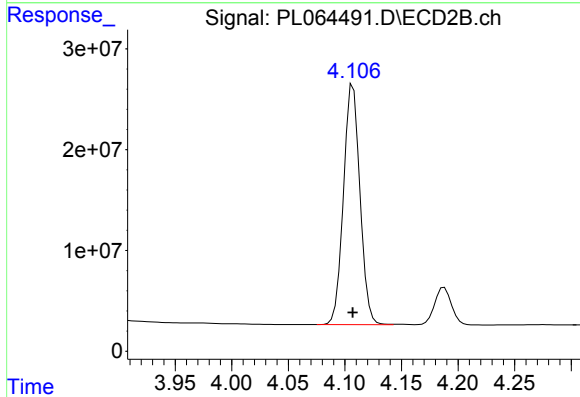


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 242012834
Conc: 101.09 ng/ml

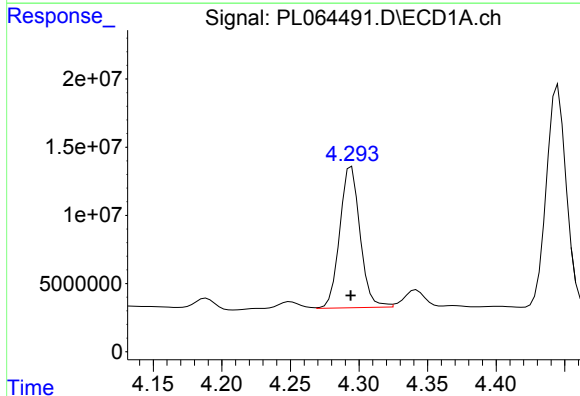


#23 Chlordane-1

R.T.: 4.295 min
Delta R.T.: 0.000 min
Response: 106728317
Conc: 969.81 ng/ml

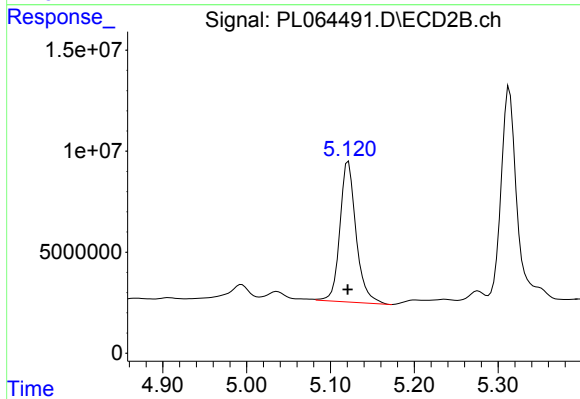

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 93551210
Conc: 955.60 ng/ml

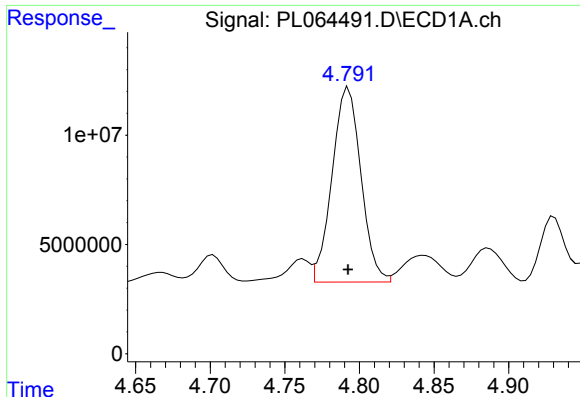

#24 Chlordane-2


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 120377128
Conc: 938.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

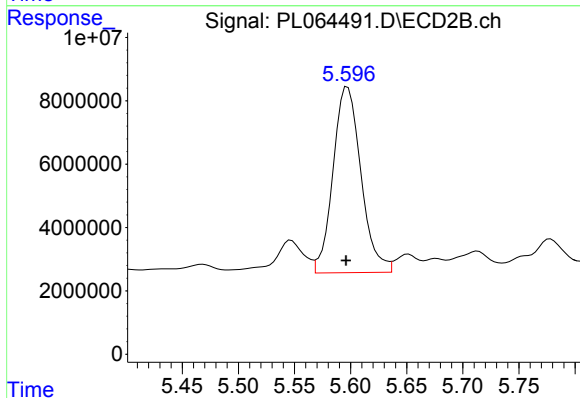


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.001 min
Response: 101851537
Conc: 931.83 ng/ml

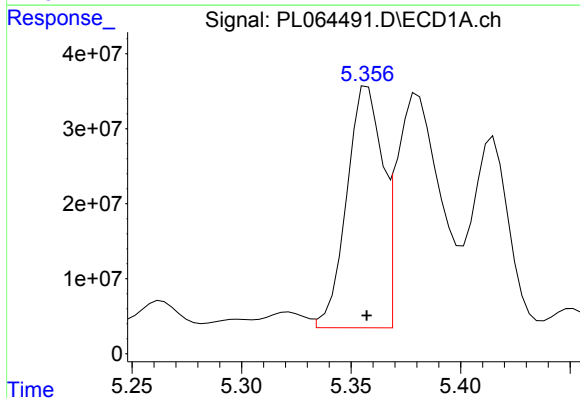


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.000 min
Response: 363384929
Conc: 1005.09 ng/ml

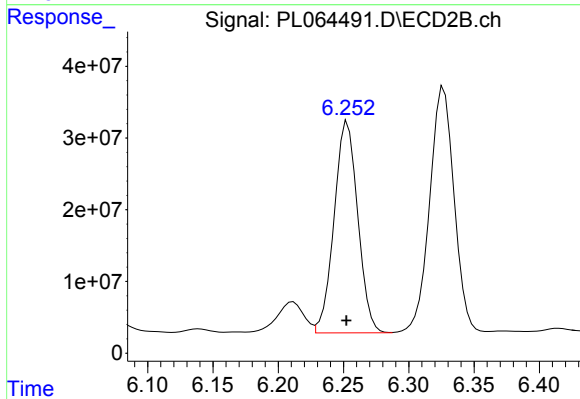

#25 Chlordane-3


R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 372530930
Conc: 1024.62 ng/ml

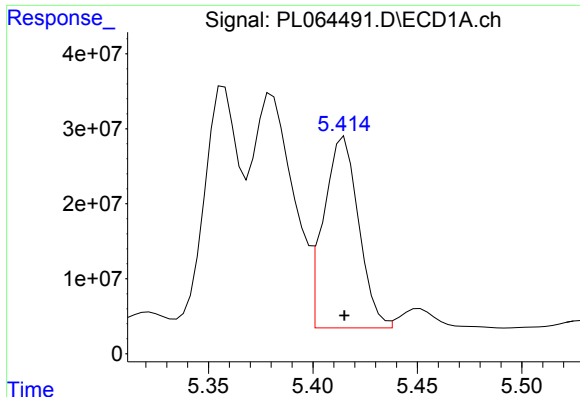

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 296107973
Conc: 993.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

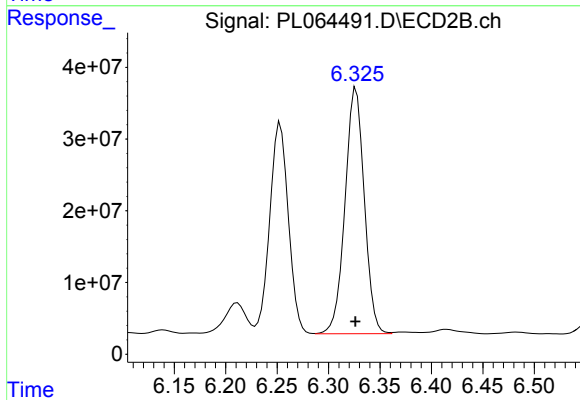


#26 Chlordane-4

R.T.: 6.327 min
Delta R.T.: 0.000 min
Response: 447375417
Conc: 1007.17 ng/ml

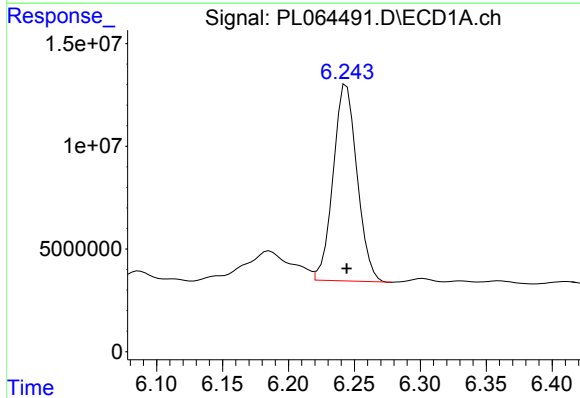


#27 Chlordane-5

R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 120674196
Conc: 997.57 ng/ml

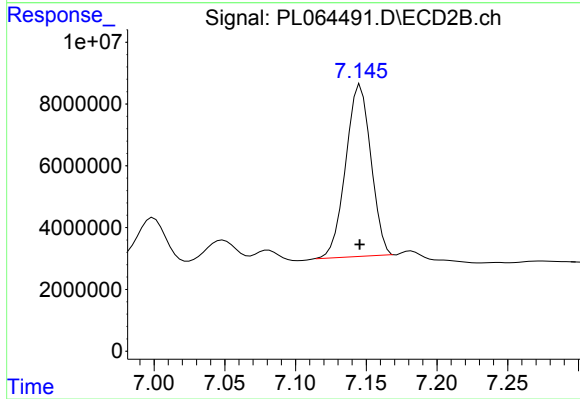

#27 Chlordane-5


R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 69266719
Conc: 1004.51 ng/ml

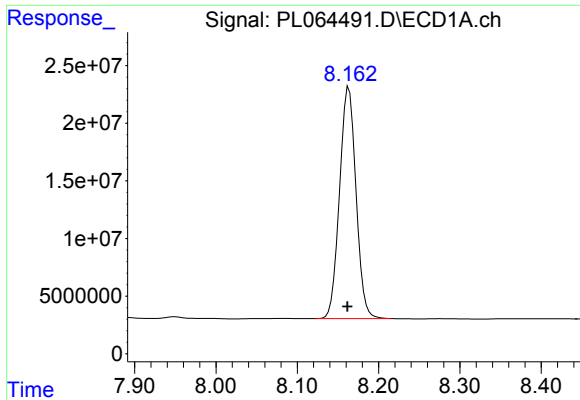

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 282260782
Conc: 94.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC1000

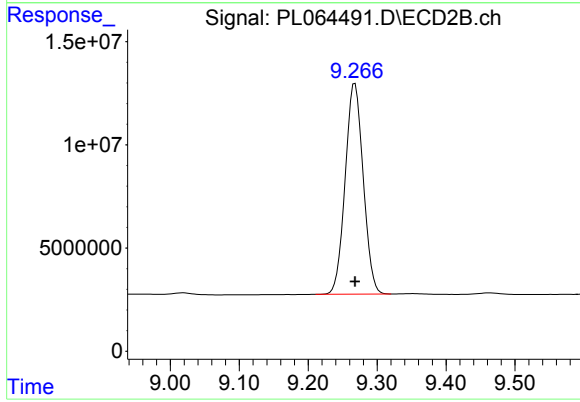

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 185634404
Conc: 94.64 ng/ml