

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 23:06
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:39:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:37:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	267.4E6	182.1E6	76.844	76.055
28)	SA Decachlor...	8.162	9.268	221.5E6	144.7E6	73.839	73.797
Target Compounds							
23)	Chlordane-1	4.294	5.121	82503060	72022114	749.682	735.687
24)	Chlordane-2	4.792	5.597	93922714	79263577	732.513	725.175
25)	Chlordane-3	5.357	6.253	275.3E6	279.4E6	761.479	768.537
26)	Chlordane-4	5.415	6.326	226.9E6	338.4E6	761.263	761.873
27)	Chlordane-5	6.245	7.146	91770554	52400785	758.637	759.920



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 23:06
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:39:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:37:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

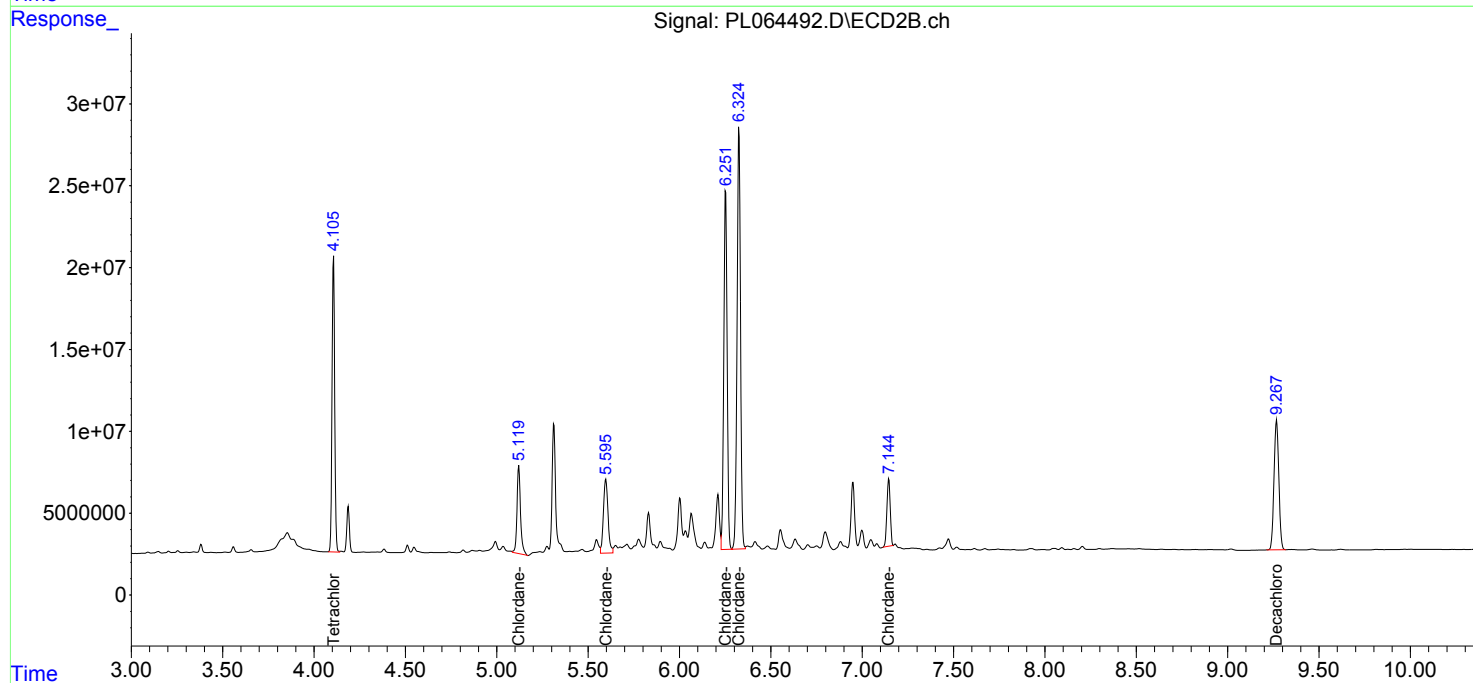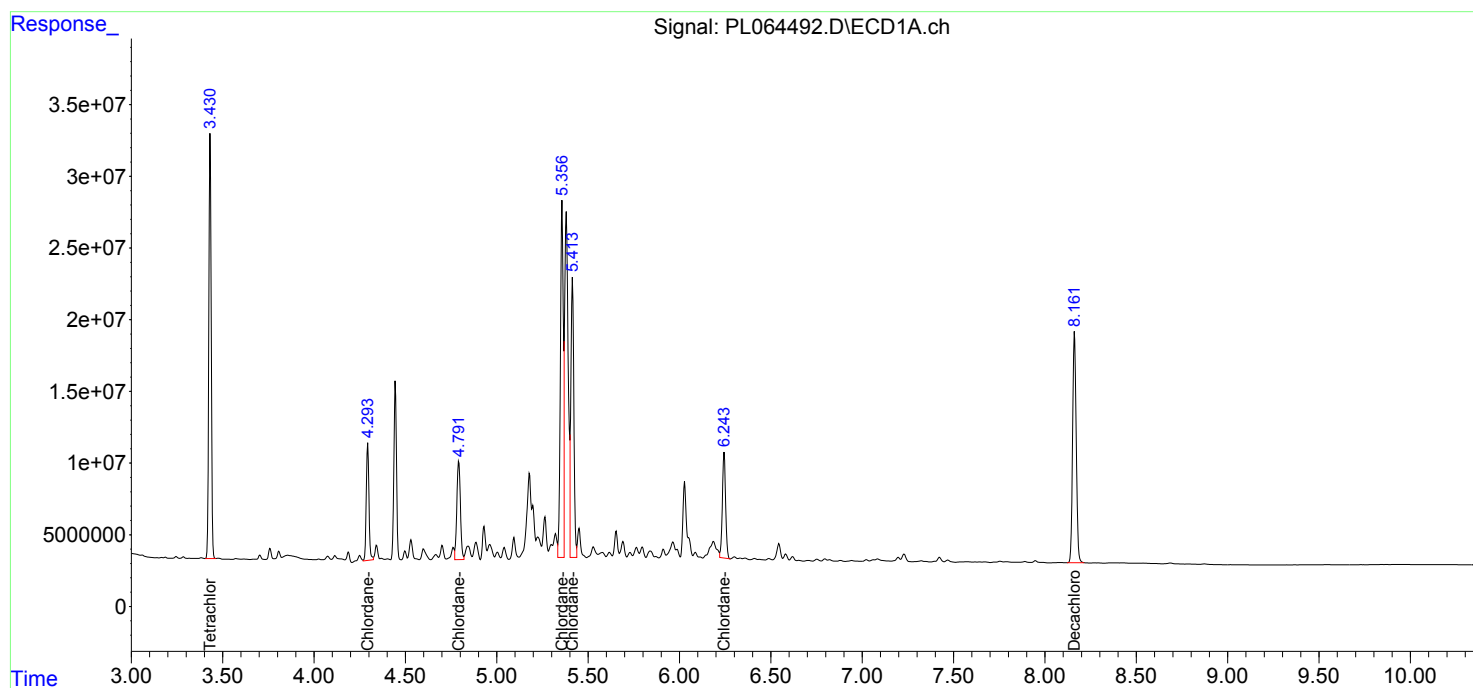


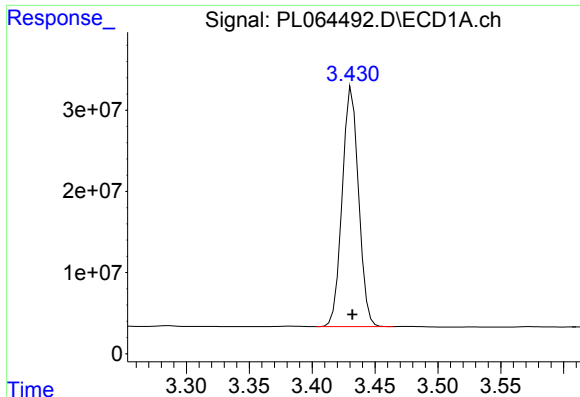

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 267429958
Conc: 76.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

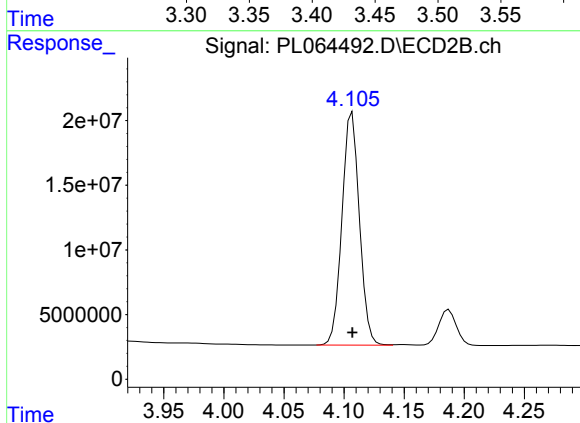


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 182084571
Conc: 76.06 ng/ml

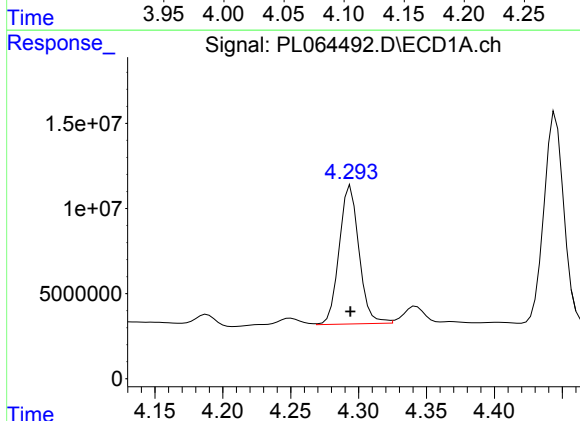


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 82503060
Conc: 749.68 ng/ml

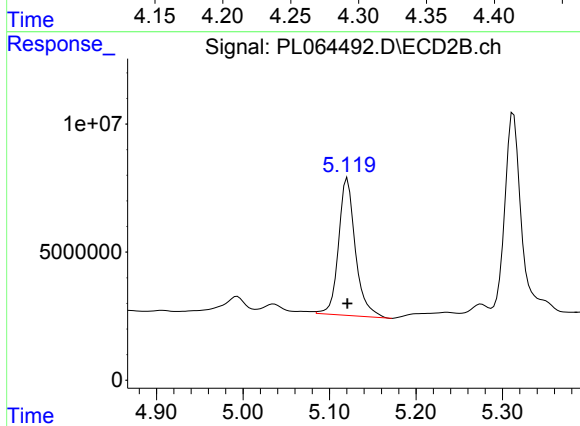

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 72022114
Conc: 735.69 ng/ml

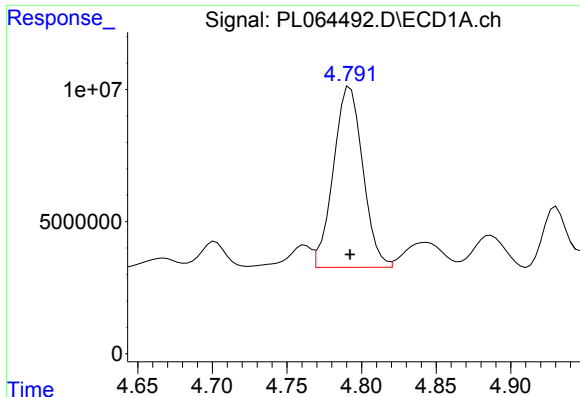

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 93922714
Conc: 732.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

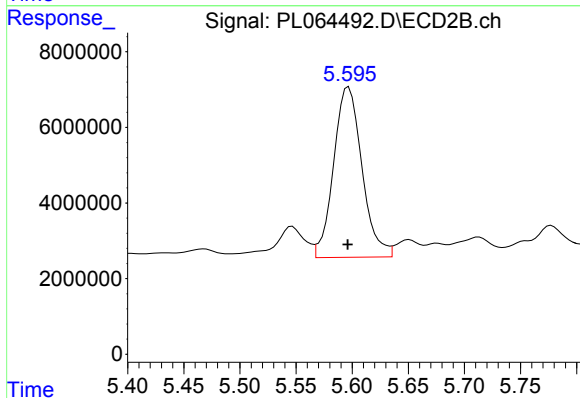


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.000 min
Response: 79263577
Conc: 725.18 ng/ml

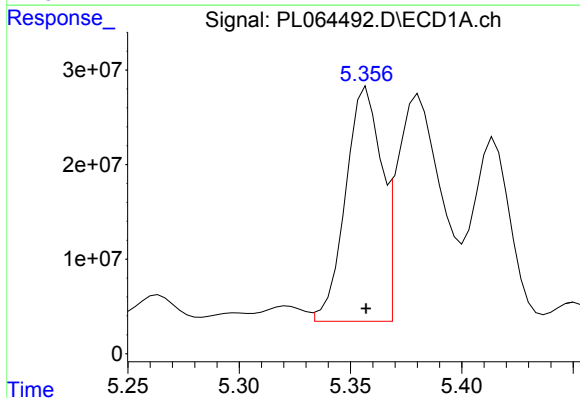


#25 Chlordane-3

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 275309787
Conc: 761.48 ng/ml

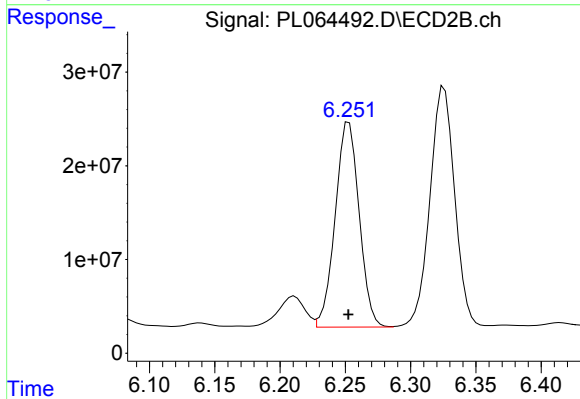

#25 Chlordane-3


R.T.: 6.253 min
Delta R.T.: 0.000 min
Response: 279424010
Conc: 768.54 ng/ml

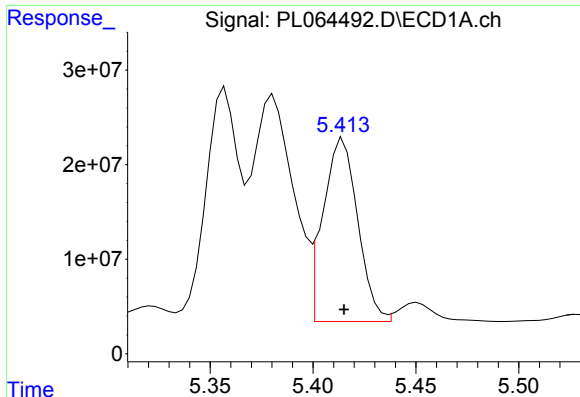

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 226925179
Conc: 761.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

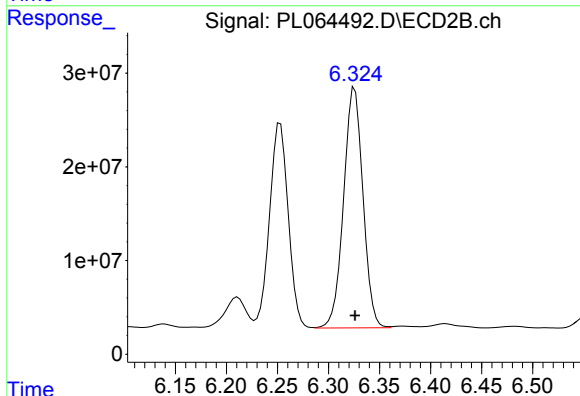


#26 Chlordane-4

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 338417290
Conc: 761.87 ng/ml

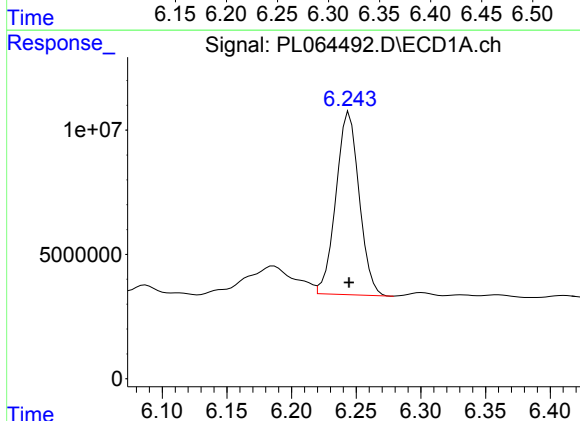


#27 Chlordane-5

R.T.: 6.245 min
Delta R.T.: 0.000 min
Response: 91770554
Conc: 758.64 ng/ml

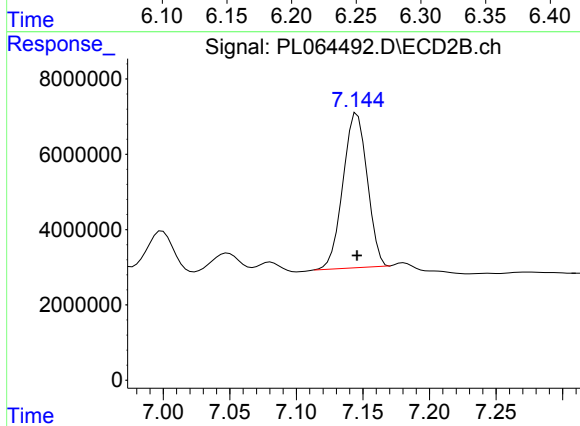

#27 Chlordane-5


R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 52400785
Conc: 759.92 ng/ml

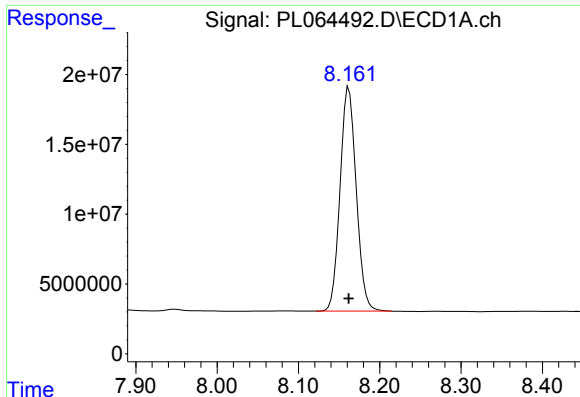

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 221511106
Conc: 73.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC750

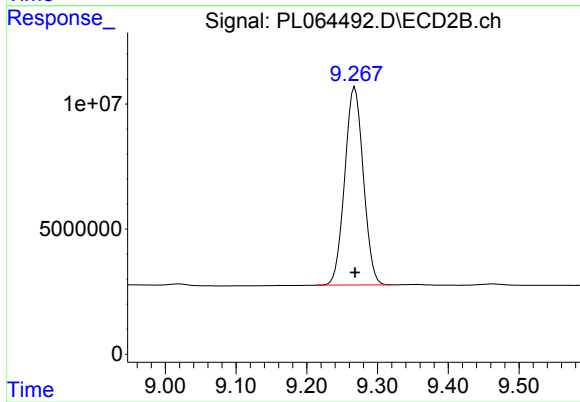

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 144749386
Conc: 73.80 ng/ml