

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064493.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 23:20
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:39:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:37:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	174.0E6	119.7E6	50.000	50.000
28)	SA Decachlor...	8.162	9.268	150.0E6	98072562	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.294	5.121	55025362	48948853	500.000	500.000
24)	Chlordane-2	4.792	5.596	64109918	54651315	500.000	500.000
25)	Chlordane-3	5.357	6.252	180.8E6	181.8E6	500.000	500.000
26)	Chlordane-4	5.415	6.326	149.0E6	222.1E6	500.000	500.000
27)	Chlordane-5	6.244	7.146	60483840	34477812	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064493.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 23:20
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:39:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:37:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

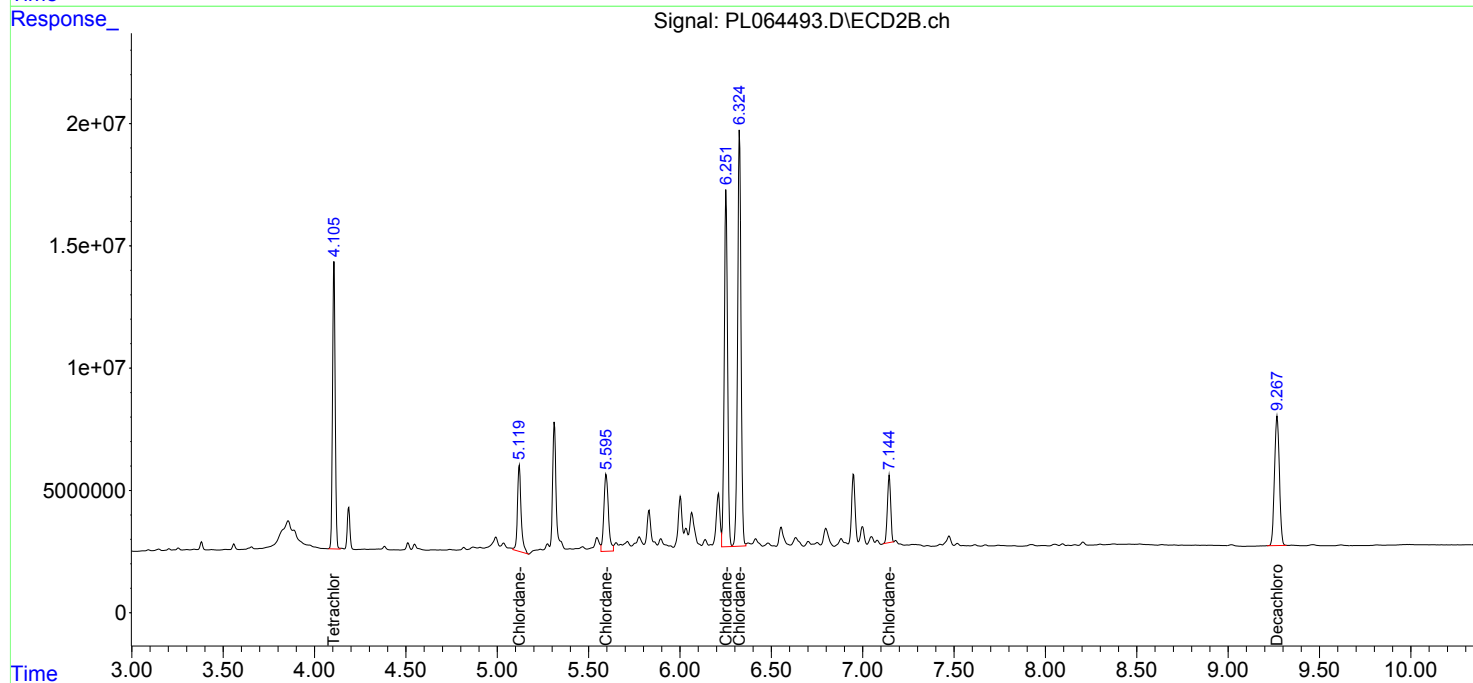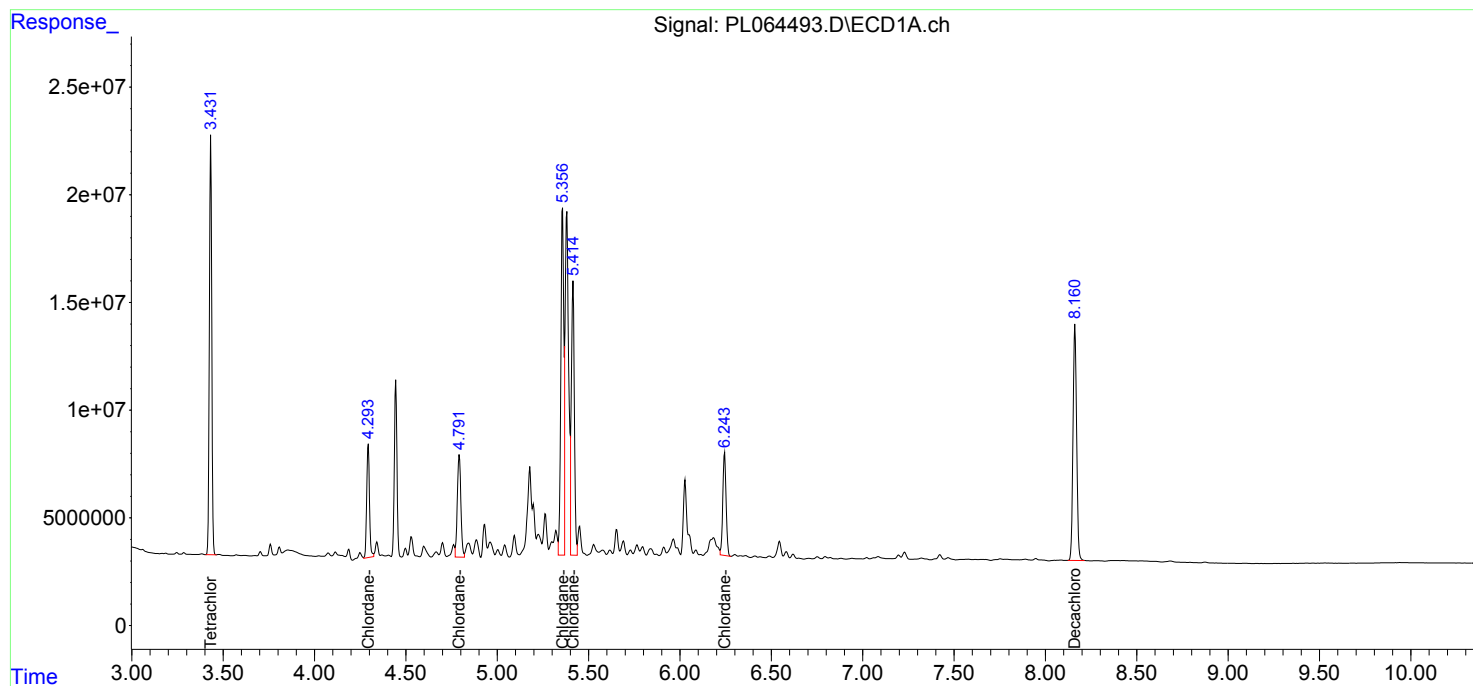


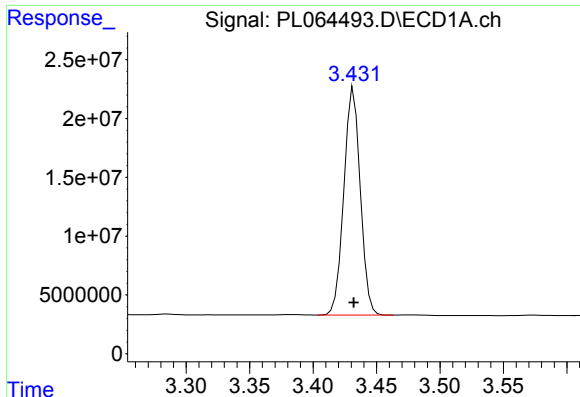

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 174007464
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

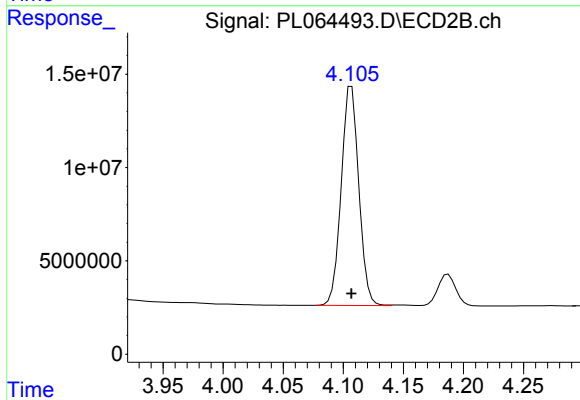


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 119705598
Conc: 50.00 ng/ml

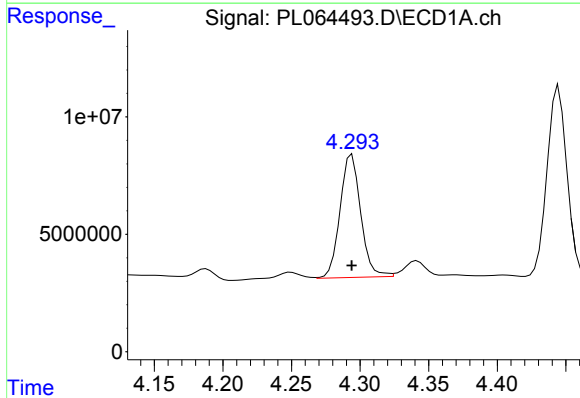


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 55025362
Conc: 500.00 ng/ml

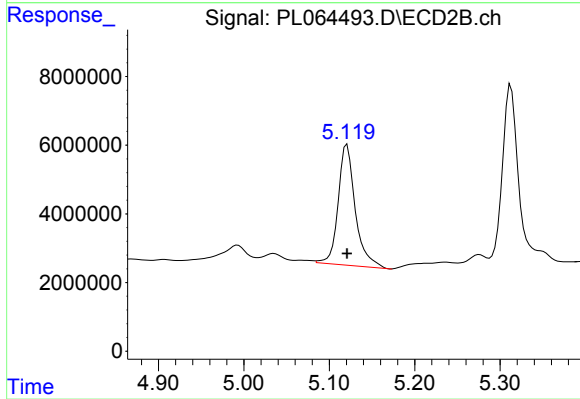

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 48948853
Conc: 500.00 ng/ml

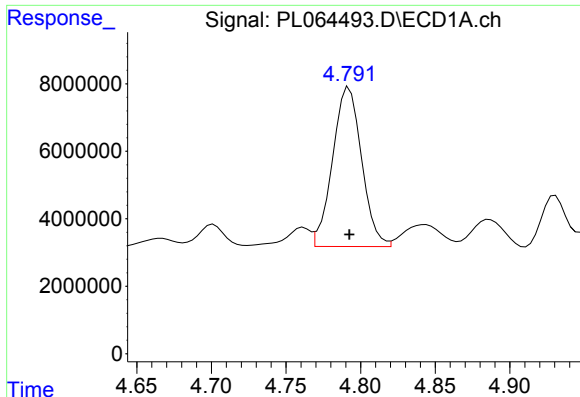

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 64109918
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

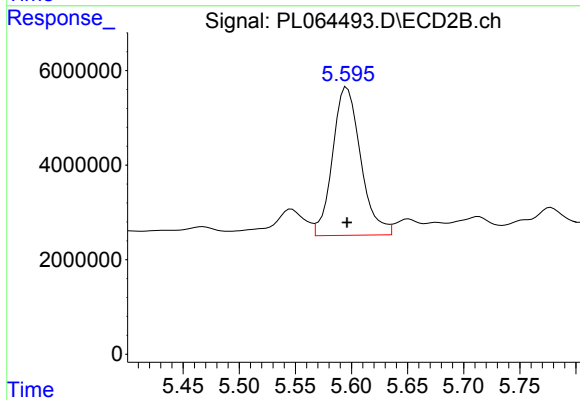


#24 Chlordane-2

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 54651315
Conc: 500.00 ng/ml

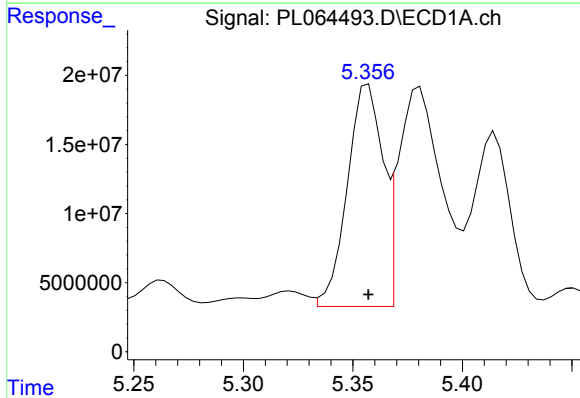


#25 Chlordane-3

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 180773082
Conc: 500.00 ng/ml

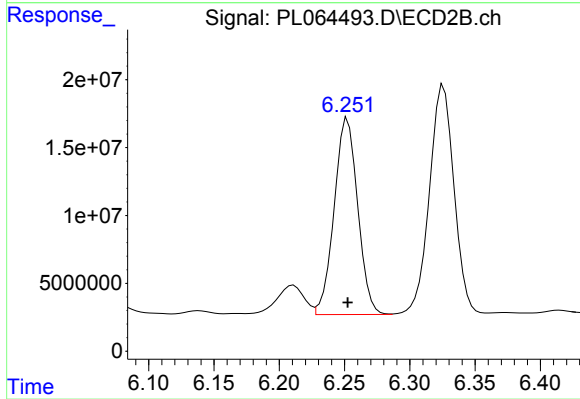

#25 Chlordane-3


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 181789539
Conc: 500.00 ng/ml

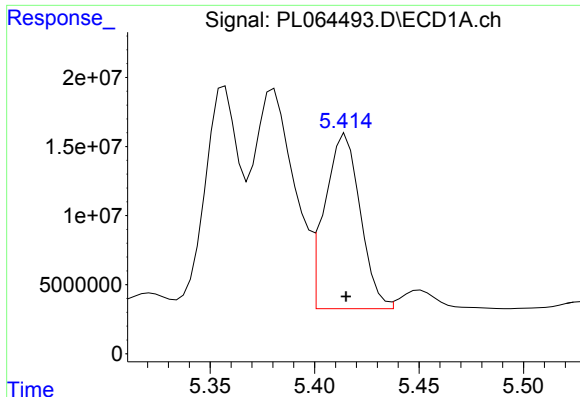

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 149045231
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

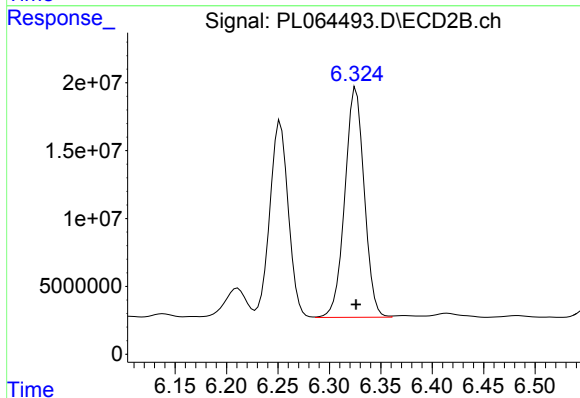


#26 Chlordane-4

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 222095748
Conc: 500.00 ng/ml

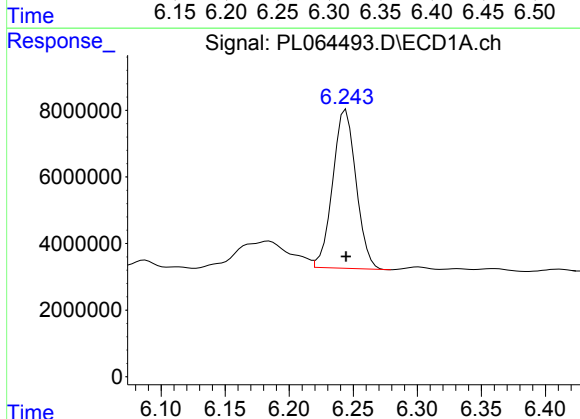


#27 Chlordane-5

R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 60483840
Conc: 500.00 ng/ml

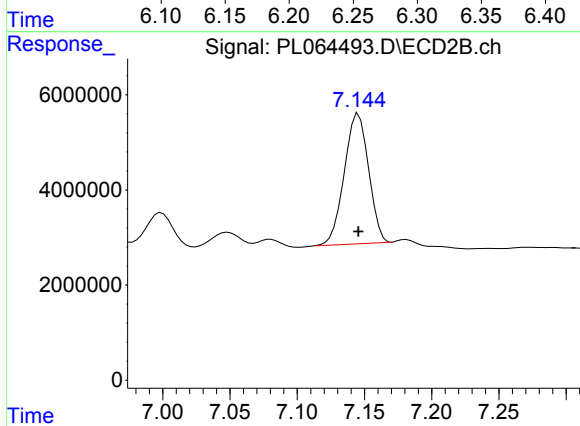

#27 Chlordane-5


R.T.: 7.146 min
Delta R.T.: 0.000 min
Response: 34477812
Conc: 500.00 ng/ml

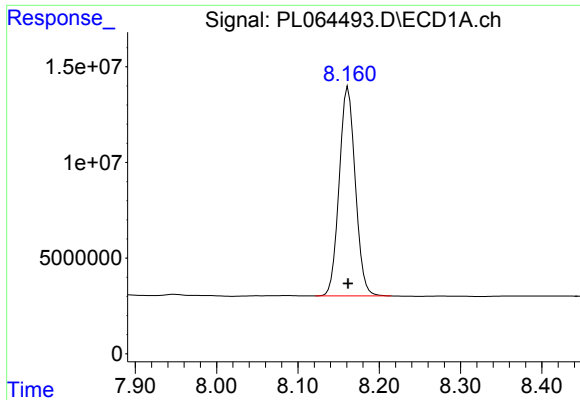

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 149995666
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

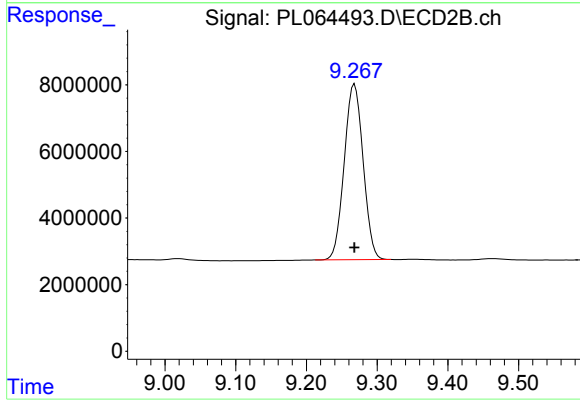

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 98072562
Conc: 50.00 ng/ml