

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064494.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jan 2021 23:34
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:39:37 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:37:55 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	85055871	58924123	24.440	24.612
28)	SA Decachlor...	8.162	9.267	79496402	51095398	26.500	26.050
Target Compounds							
23)	Chlordane-1	4.294	5.120	28769279	27202082	261.418	277.862
24)	Chlordane-2	4.792	5.596	35233149	25916982	274.787	237.112
25)	Chlordane-3	5.357	6.252	89551172	87542854	247.689	240.781
26)	Chlordane-4	5.414	6.326	74770154	108.8E6	250.830	245.046
27)	Chlordane-5	6.244	7.145	30199597	16844734	249.650	244.284



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064494.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jan 2021 23:34
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:39:37 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:37:55 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

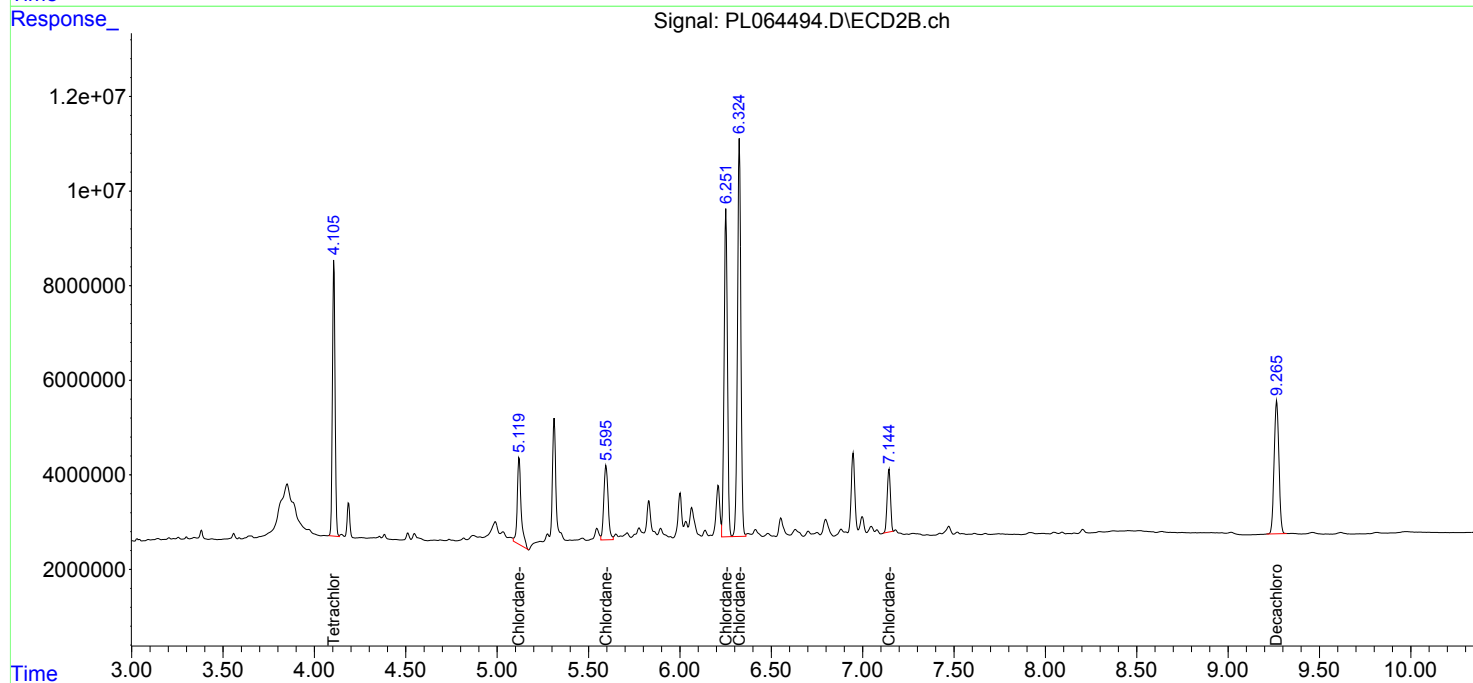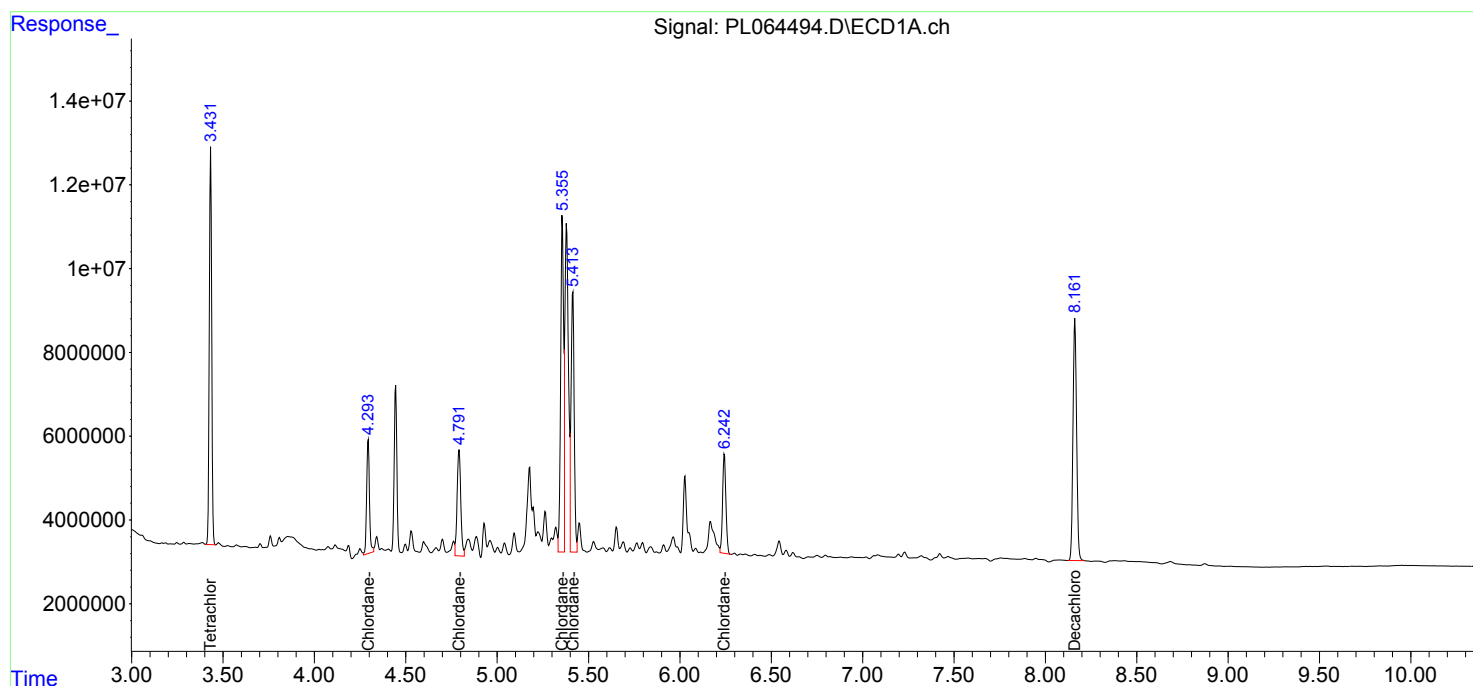


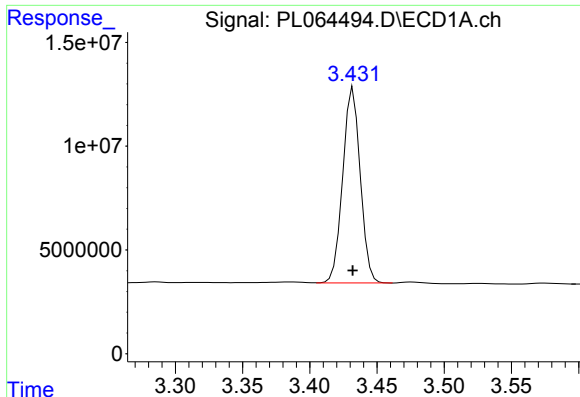

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 85055871
Conc: 24.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

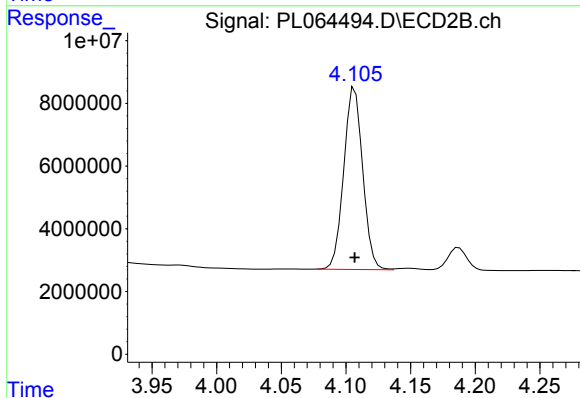


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 58924123
Conc: 24.61 ng/ml

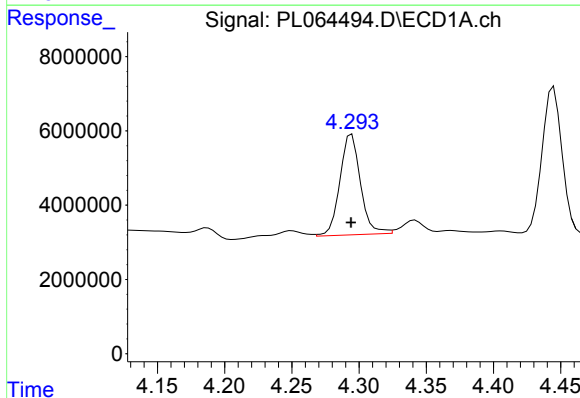


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 28769279
Conc: 261.42 ng/ml

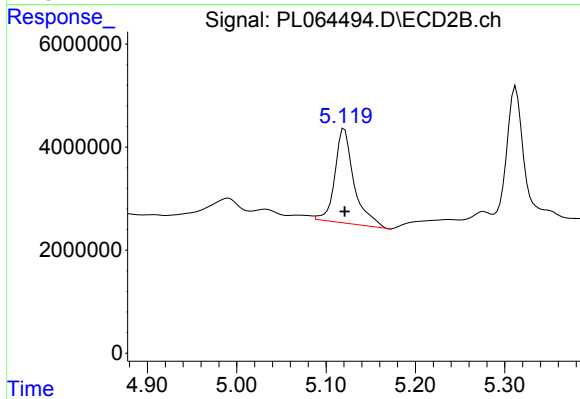

#23 Chlordane-1


R.T.: 5.120 min
Delta R.T.: 0.000 min
Response: 27202082
Conc: 277.86 ng/ml

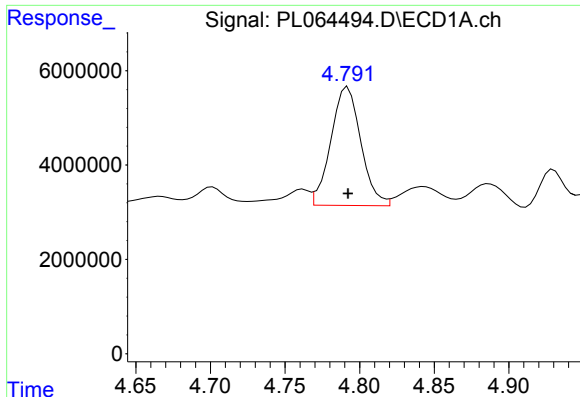

#24 Chlordane-2


R.T.: 4.792 min
Delta R.T.: 0.000 min
Response: 35233149
Conc: 274.79 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

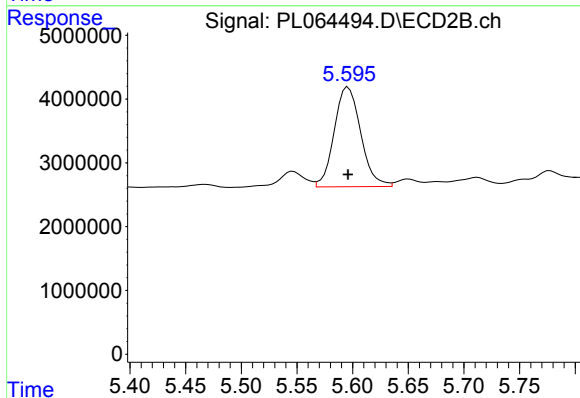


#24 Chlordane-2

R.T.: 5.596 min
Delta R.T.: 0.000 min
Response: 25916982
Conc: 237.11 ng/ml

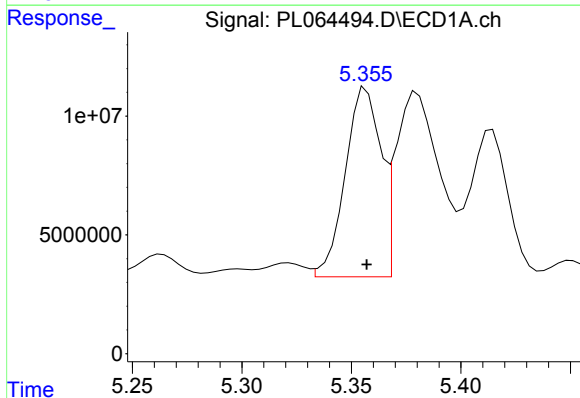


#25 Chlordane-3

R.T.: 5.357 min
Delta R.T.: 0.000 min
Response: 89551172
Conc: 247.69 ng/ml

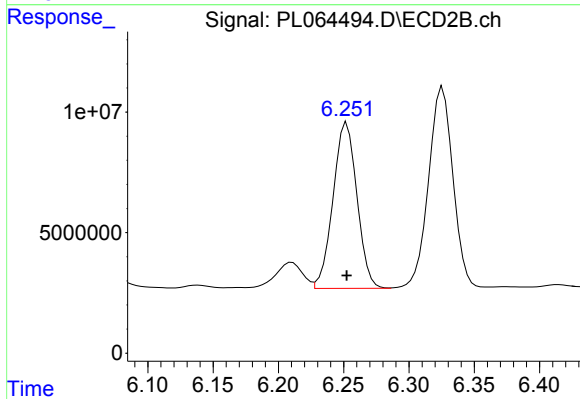

#25 Chlordane-3


R.T.: 6.252 min
Delta R.T.: 0.000 min
Response: 87542854
Conc: 240.78 ng/ml

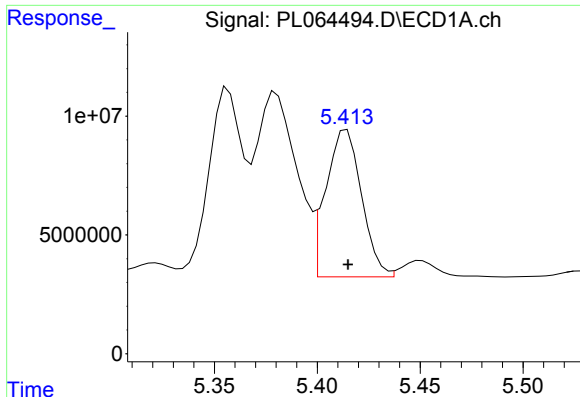

#26 Chlordane-4


R.T.: 5.414 min
Delta R.T.: 0.000 min
Response: 74770154
Conc: 250.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

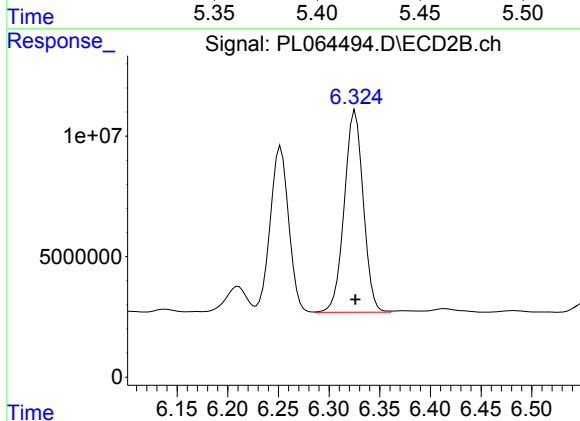


#26 Chlordane-4

R.T.: 6.326 min
Delta R.T.: 0.000 min
Response: 108847420
Conc: 245.05 ng/ml

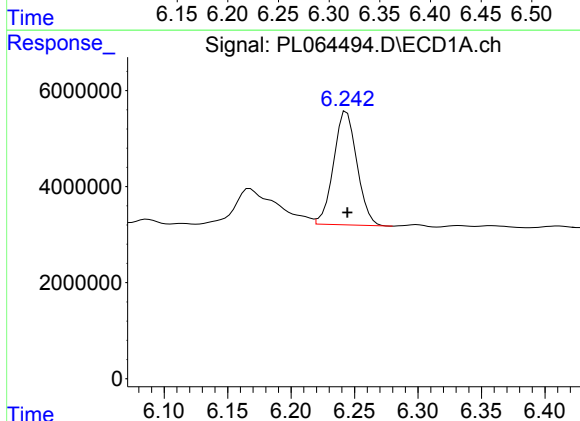


#27 Chlordane-5

R.T.: 6.244 min
Delta R.T.: 0.000 min
Response: 30199597
Conc: 249.65 ng/ml

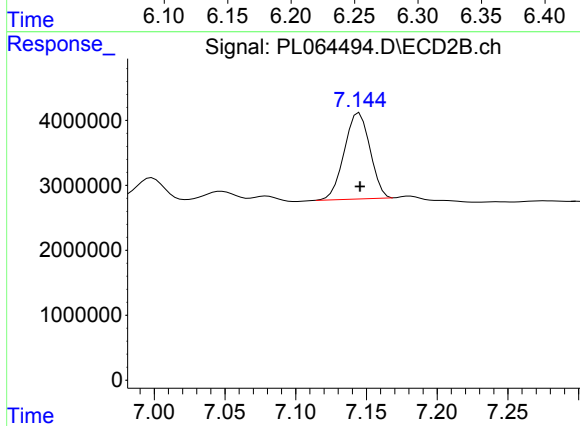

#27 Chlordane-5


R.T.: 7.145 min
Delta R.T.: 0.000 min
Response: 16844734
Conc: 244.28 ng/ml

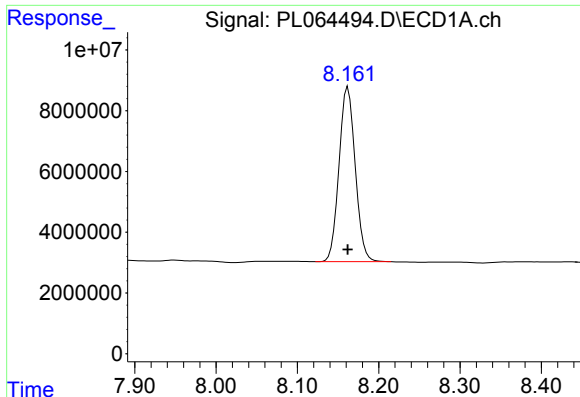

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 79496402
Conc: 26.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC250

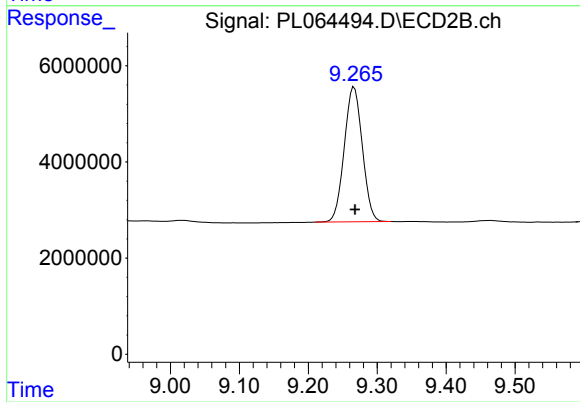

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.002 min
Response: 51095398
Conc: 26.05 ng/ml