

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
 Data File : PL064502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 01:28
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ICVPL012921CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 29 04:46:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:45:42 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	169.7E6	117.6E6	49.048	49.512
28)	SA Decachlor...	8.163	9.269	146.5E6	97015747	46.956	48.740
Target Compounds							
23)	Chlordane-1	4.294	5.121	53982769	47649717	491.096	506.699
24)	Chlordane-2	4.793	5.597	63199186	52873990	474.005	509.775
25)	Chlordane-3	5.358	6.253	176.3E6	176.4E6	488.805	492.156
26)	Chlordane-4	5.415	6.327	145.3E6	215.0E6	488.444	488.943
27)	Chlordane-5	6.244	7.146	58396857	33193136	490.529	496.360



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012921\
Data File : PL064502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 01:28
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ICVPL012921CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 29 04:46:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:45:42 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

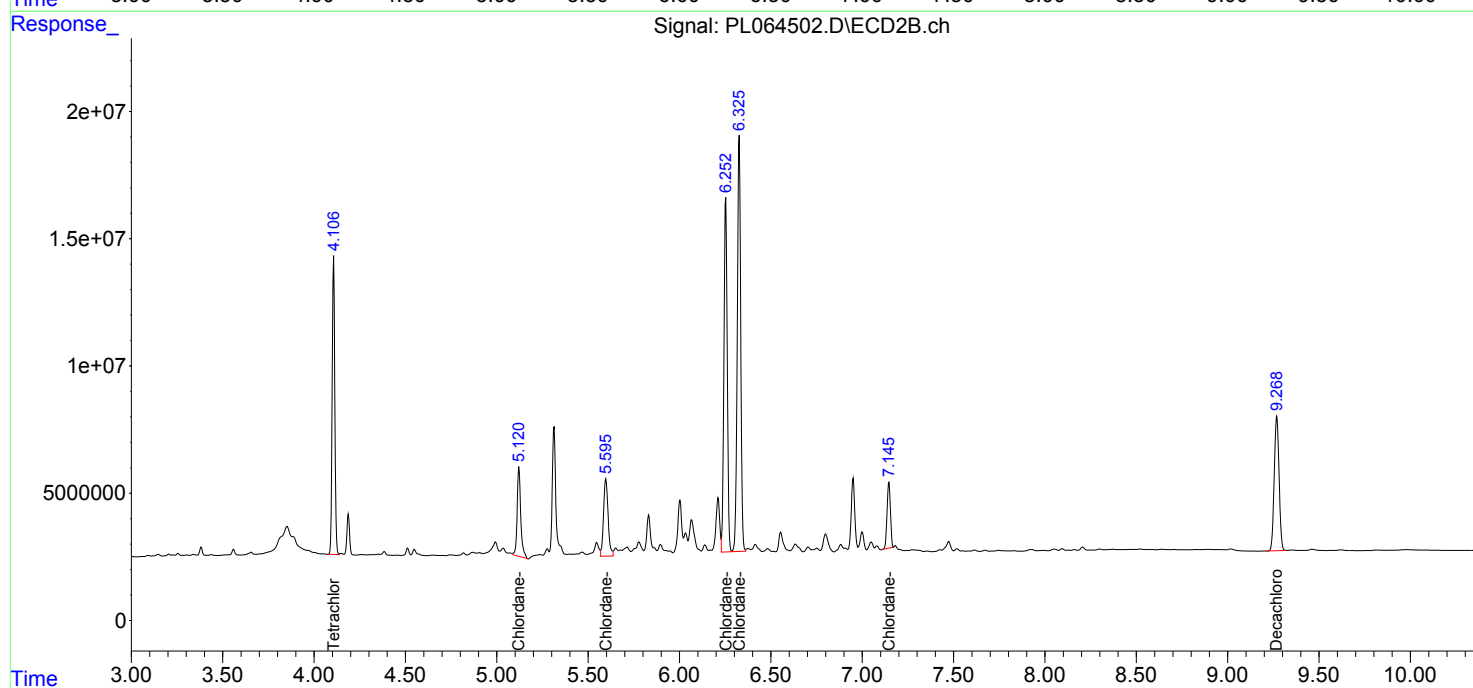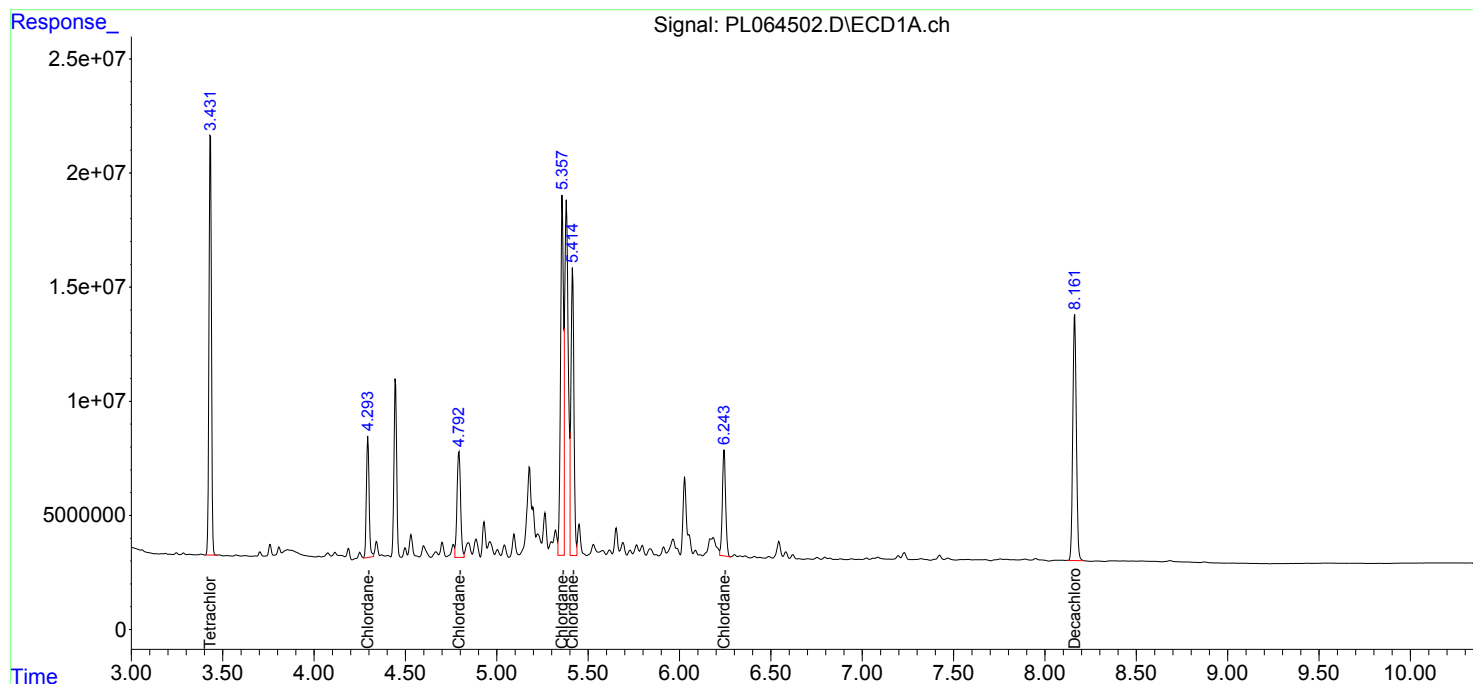


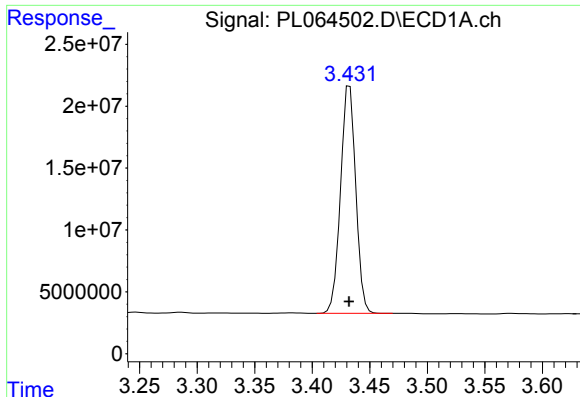

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 169650908
Conc: 49.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012921CHLOR

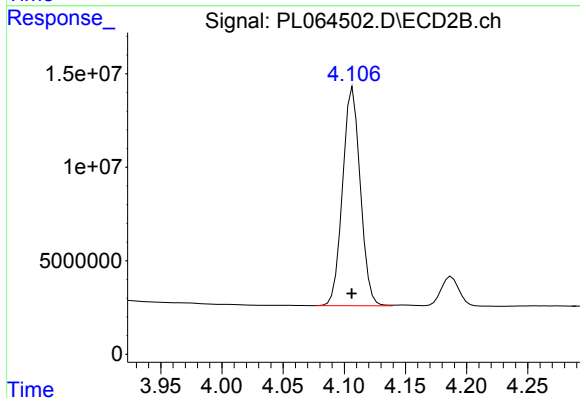


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.001 min
Response: 117567835
Conc: 49.51 ng/ml

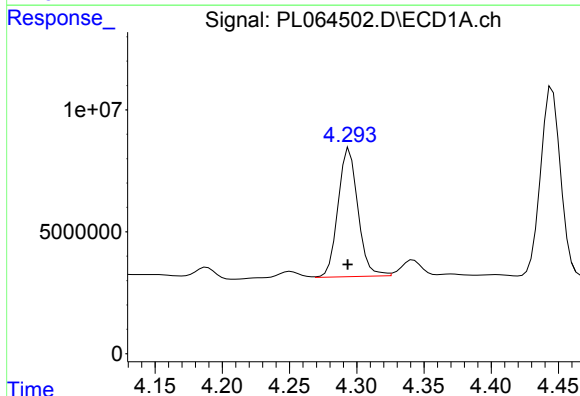


#23 Chlordane-1

R.T.: 4.294 min
Delta R.T.: 0.001 min
Response: 53982769
Conc: 491.10 ng/ml

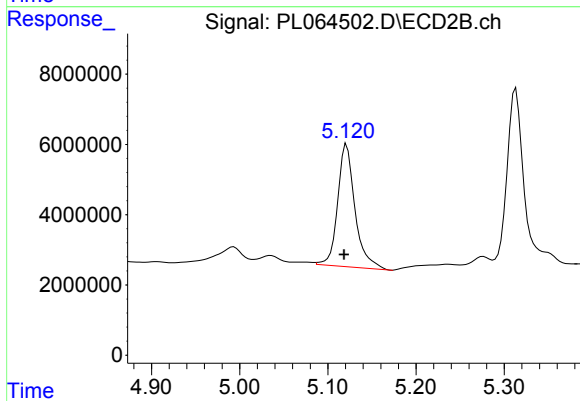

#23 Chlordane-1


R.T.: 5.121 min
Delta R.T.: 0.003 min
Response: 47649717
Conc: 506.70 ng/ml

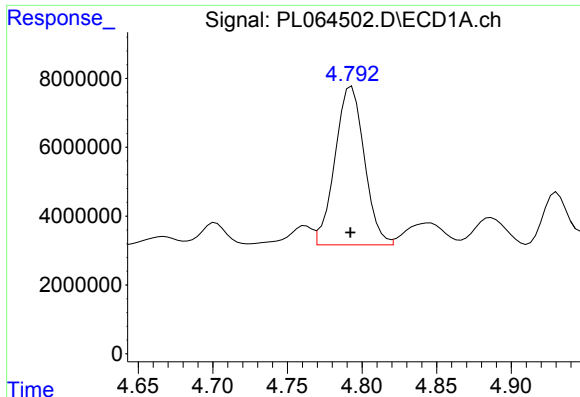

#24 Chlordane-2


R.T.: 4.793 min
Delta R.T.: 0.000 min
Response: 63199186
Conc: 474.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012921CHLOR

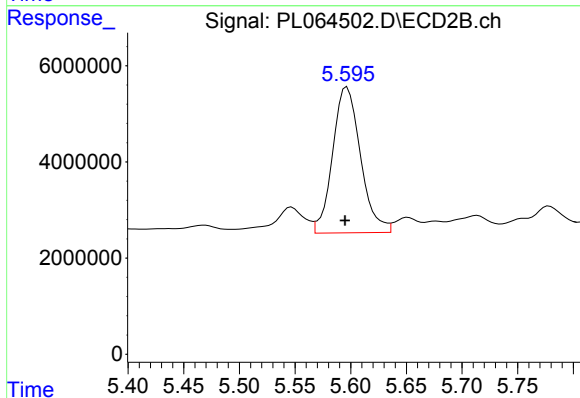


#24 Chlordane-2

R.T.: 5.597 min
Delta R.T.: 0.002 min
Response: 52873990
Conc: 509.78 ng/ml

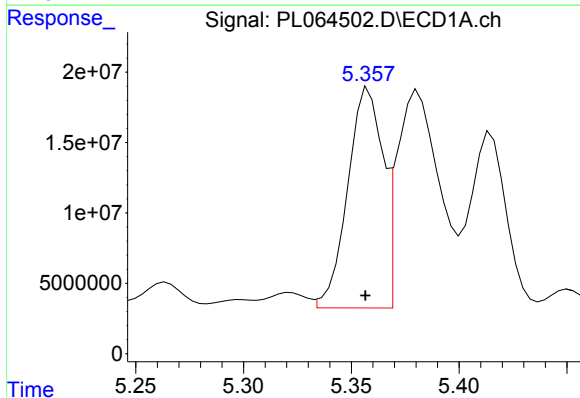


#25 Chlordane-3

R.T.: 5.358 min
Delta R.T.: 0.001 min
Response: 176325808
Conc: 488.81 ng/ml

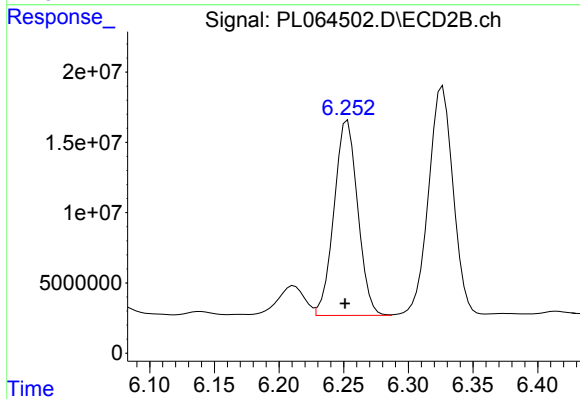

#25 Chlordane-3


R.T.: 6.253 min
Delta R.T.: 0.002 min
Response: 176432018
Conc: 492.16 ng/ml

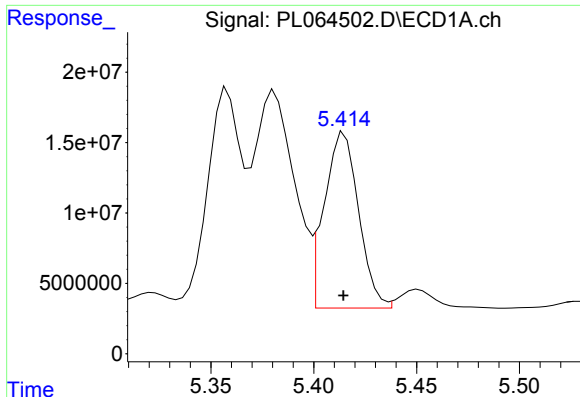

#26 Chlordane-4


R.T.: 5.415 min
Delta R.T.: 0.000 min
Response: 145285873
Conc: 488.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012921CHLOR

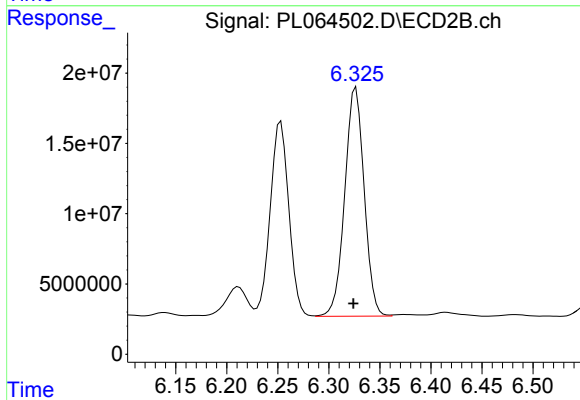


#26 Chlordane-4

R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 215016476
Conc: 488.94 ng/ml

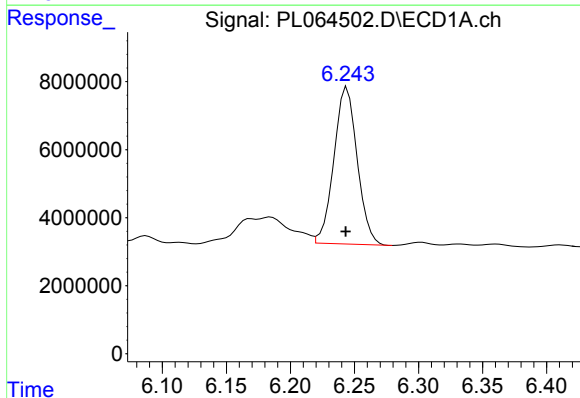


#27 Chlordane-5

R.T.: 6.244 min
Delta R.T.: 0.001 min
Response: 58396857
Conc: 490.53 ng/ml

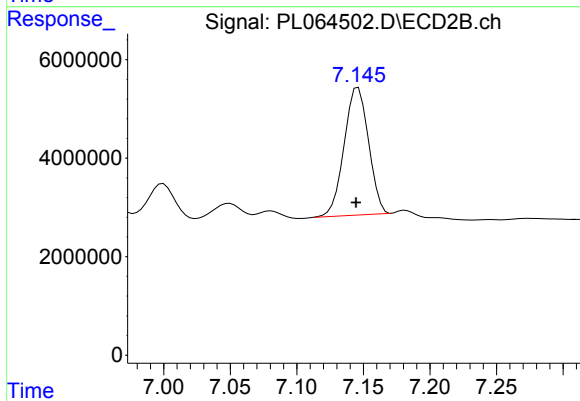

#27 Chlordane-5


R.T.: 7.146 min
Delta R.T.: 0.002 min
Response: 33193136
Conc: 496.36 ng/ml

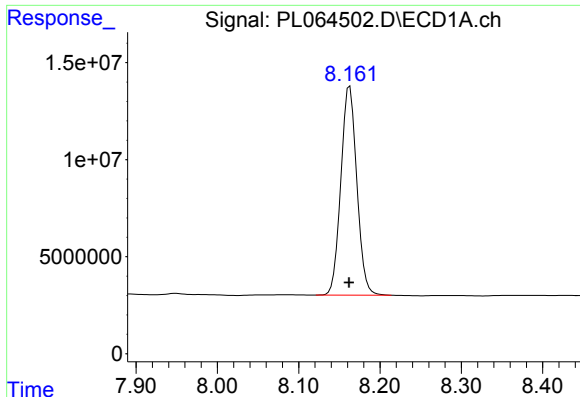

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 146506078
Conc: 46.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
ICVPL012921CHLOR

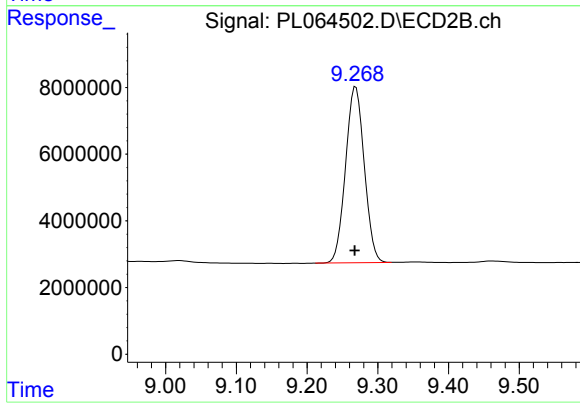

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.001 min
Response: 97015747
Conc: 48.74 ng/ml