

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012925\
 Data File : PL093860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2025 18:18
 Operator : AR\AJ
 Sample : Q1206-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JPP-20.1-012725

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 00:29:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.775	57894896	66771965	21.500	20.456
28)	SA Decachlor...	9.060	7.913	58124889	95383275	27.786	27.221
Target Compounds							
2)	A alpha-BHC	0.000	3.271	0	372306	N.D.	0.076 #
4)	MA Heptachlor	0.000	3.968f	0	76322	N.D.	0.016 #
5)	MB Aldrin	0.000	4.231	0	707454	N.D.	0.155 #
7)	B delta-BHC	4.764	4.130	9877223	370722	2.818	0.078 #
8)	B Heptachlo...	0.000	4.725	0	97472	N.D.	0.023 #
9)	A Endosulfan I	0.000	5.087	0	313239	N.D.	0.081 #
10)	B gamma-Chl...	0.000	4.973	0	3840835	N.D.	0.906 #
11)	B alpha-Chl...	0.000	5.014f	0	2787063	N.D.	0.666 #
12)	B 4,4'-DDE	0.000	5.253f	0	337624	N.D.	0.084 #
13)	MA Dieldrin	0.000	5.354	0	376366	N.D.	0.088 #
14)	MA Endrin	0.000	5.656f	0	1506631	N.D.	0.408 #
16)	A 4,4'-DDD	0.000	5.788	0	350710	N.D.	0.111 #
17)	MA 4,4'-DDT	0.000	6.033	0	859429	N.D.	0.264 #
20)	A Methoxychlor	0.000	6.614	0	609215	N.D.	0.341 #
23)	Chlordane-1	0.000	3.765	0	321214	N.D.	2.574 #
24)	Chlordane-2	0.000	4.317f	0	454744	N.D.	3.099 #
25)	Chlordane-3	0.000	4.973	0	3840835	N.D.	8.833 #
26)	Chlordane-4	0.000	5.014f	0	2787063	N.D.	6.578 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012925\
Data File : PL093860.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2025 18:18
Operator : AR\AJ
Sample : Q1206-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 00:29:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

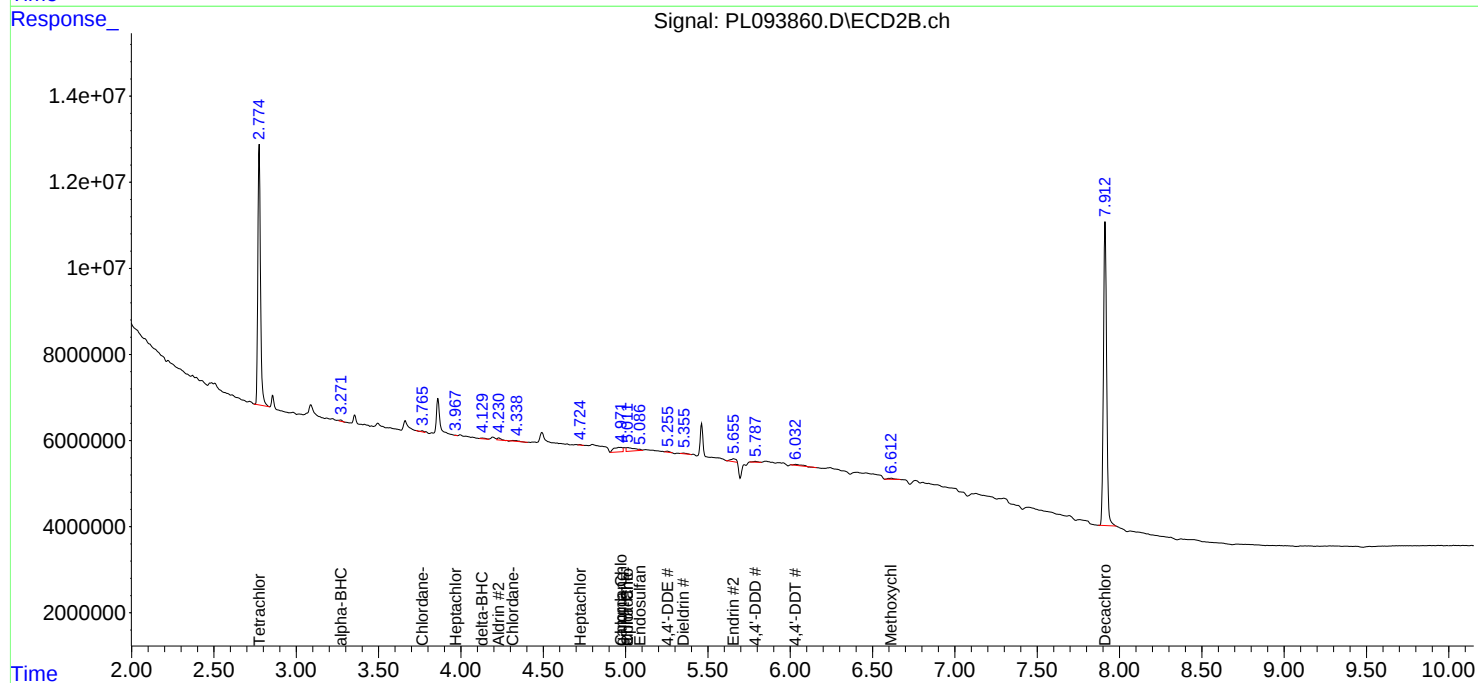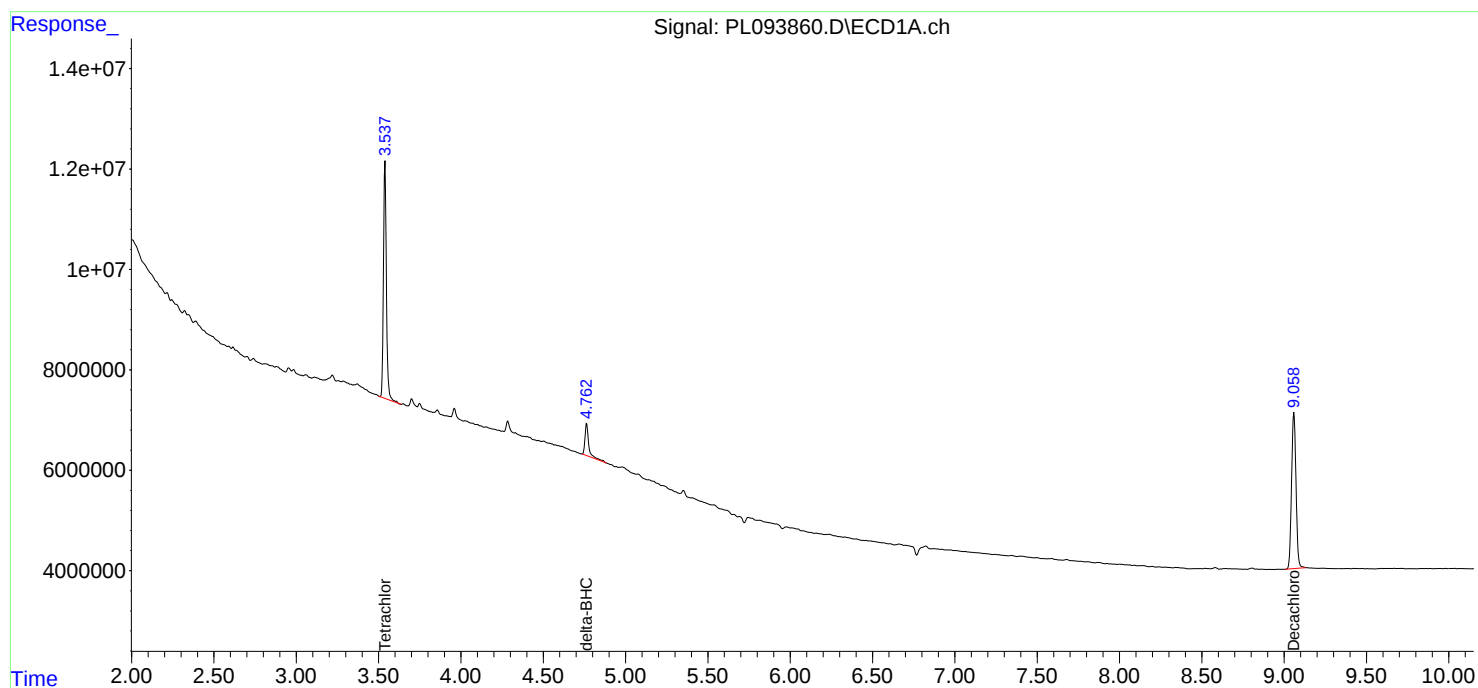


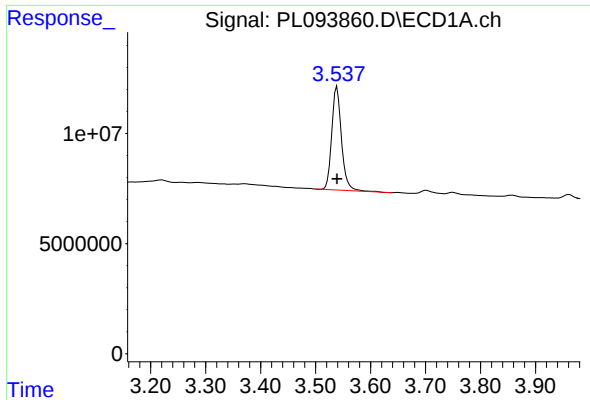

#1 Tetrachloro-m-xylene


R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 57894896
Conc: 21.50 ng/ml

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

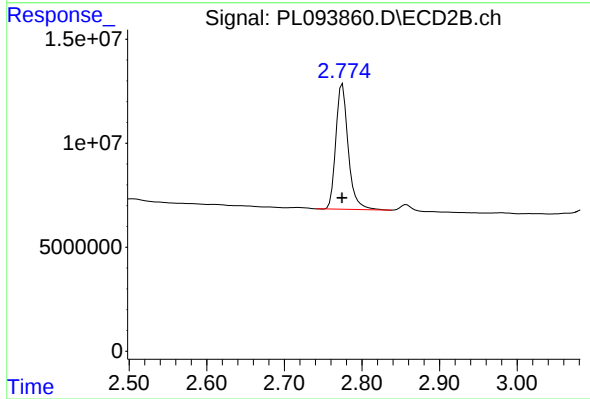


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: 0.000 min
Response: 66771965
Conc: 20.46 ng/ml

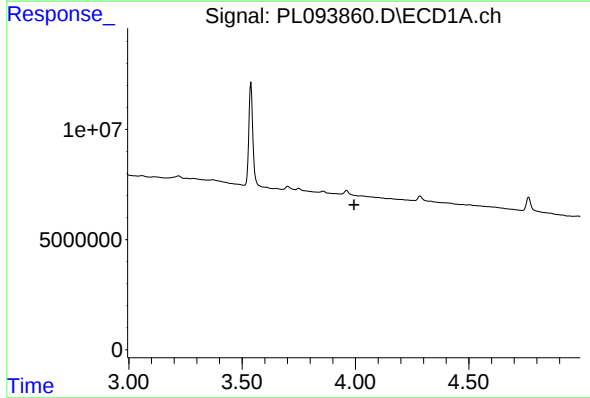


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.995 min
Response: 0
Conc: N.D.

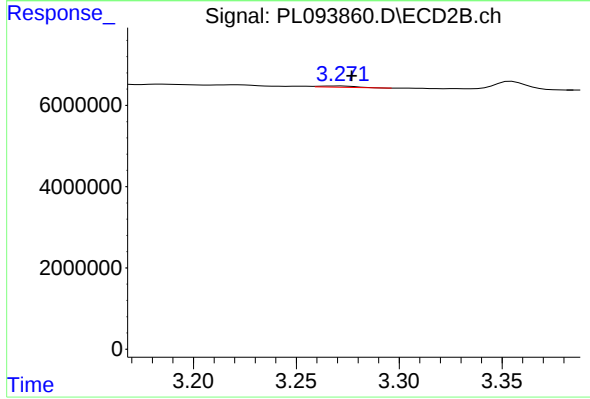

#2 alpha-BHC


R.T.: 3.271 min
Delta R.T.: -0.005 min
Response: 372306
Conc: 0.08 ng/ml

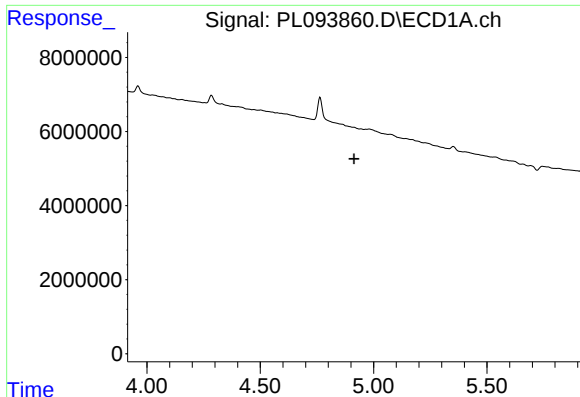

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.914 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

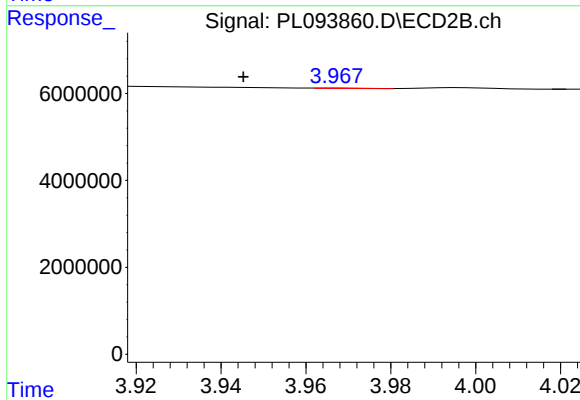


#4 Heptachlor

R.T.: 3.968 min
Delta R.T.: 0.022 min
Response: 76322
Conc: 0.02 ng/ml

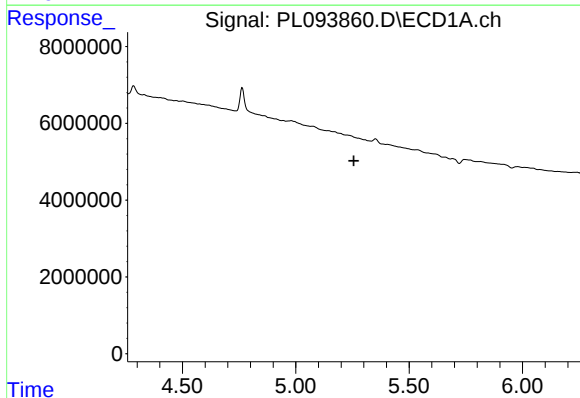


#5 Aldrin

R.T.: 0.000 min
Exp R.T.: 5.256 min
Response: 0
Conc: N.D.

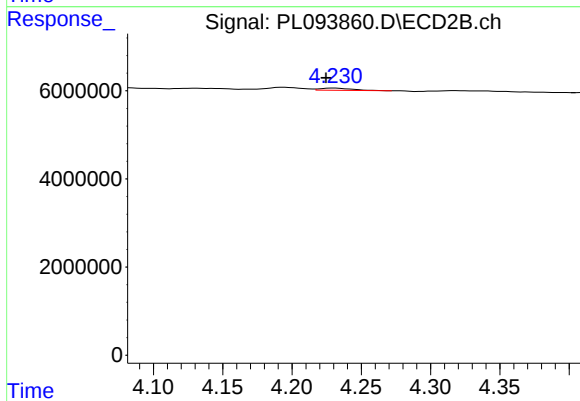

#5 Aldrin


R.T.: 4.231 min
Delta R.T.: 0.006 min
Response: 707454
Conc: 0.16 ng/ml

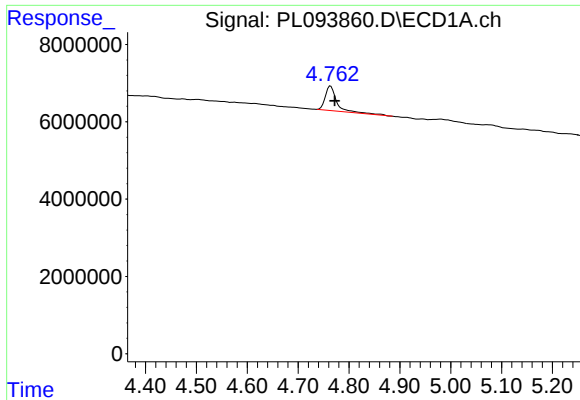

#7 delta-BHC


R.T.: 4.764 min
Delta R.T.: -0.008 min
Response: 9877223
Conc: 2.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

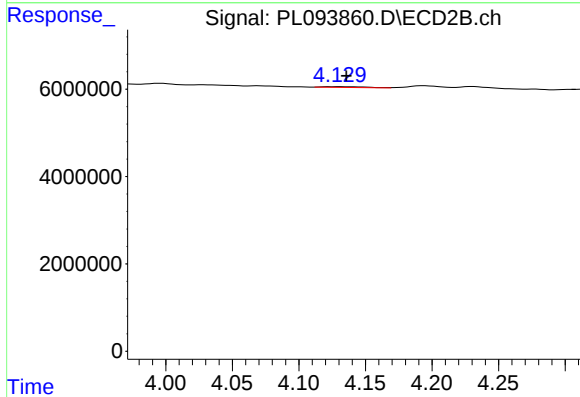


#7 delta-BHC

R.T.: 4.130 min
Delta R.T.: -0.005 min
Response: 370722
Conc: 0.08 ng/ml

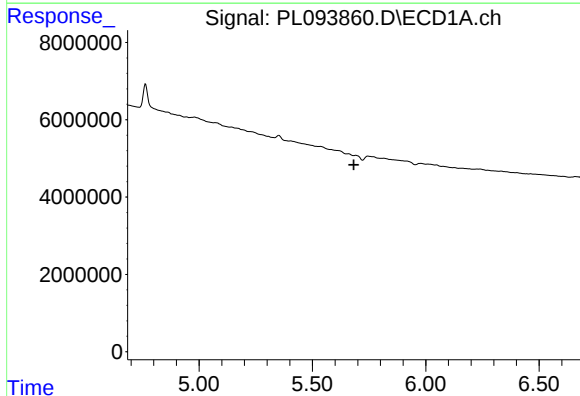


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.682 min
Response: 0
Conc: N.D.

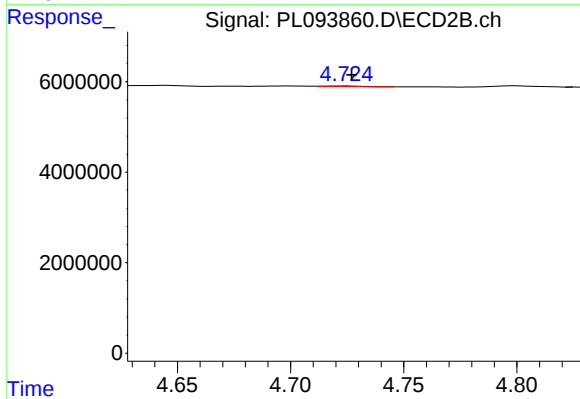

#8 Heptachlor epoxide


R.T.: 4.725 min
Delta R.T.: -0.002 min
Response: 97472
Conc: 0.02 ng/ml

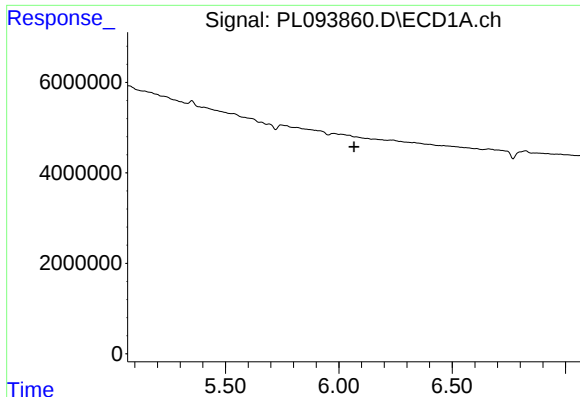

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.067 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

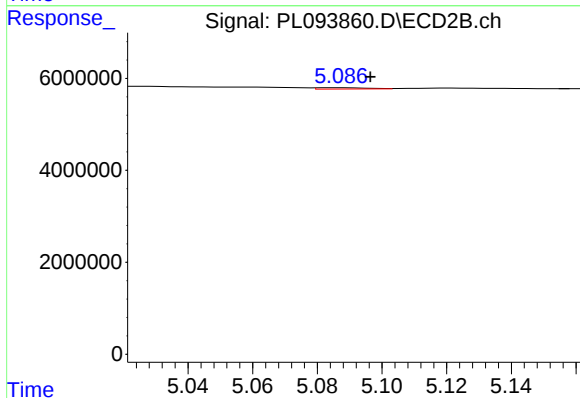


#9 Endosulfan I

R.T.: 5.087 min
Delta R.T.: -0.010 min
Response: 313239
Conc: 0.08 ng/ml

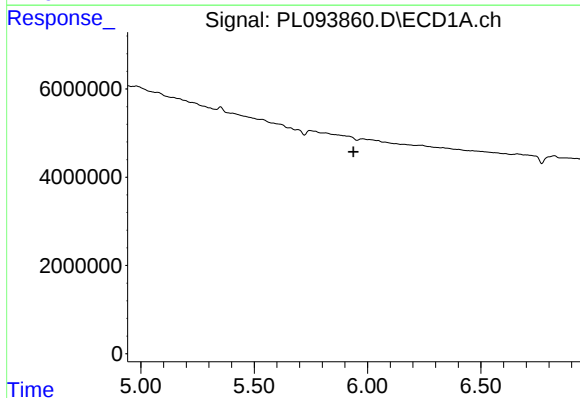


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.938 min
Response: 0
Conc: N.D.

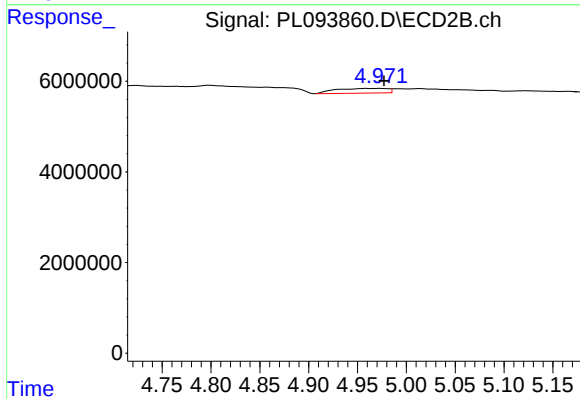

#10 gamma-Chlordane


R.T.: 4.973 min
Delta R.T.: -0.004 min
Response: 3840835
Conc: 0.91 ng/ml

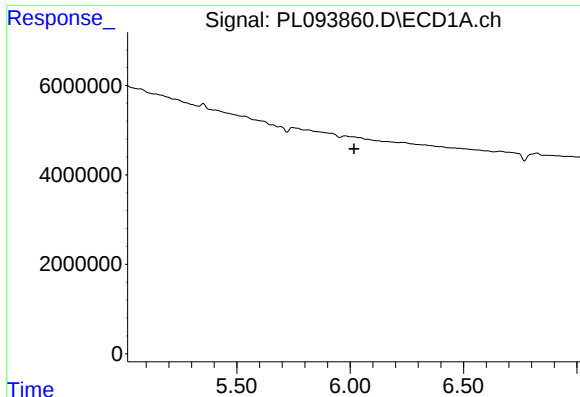

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.017 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

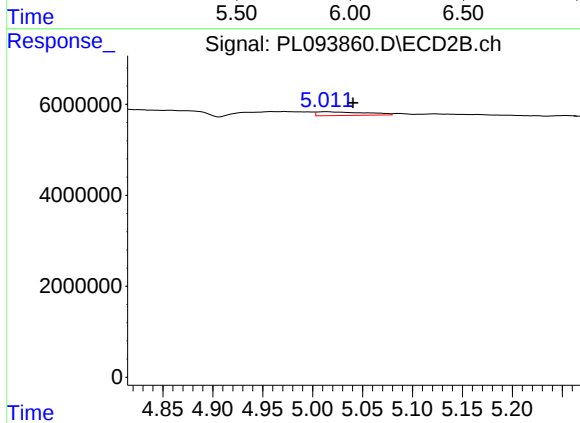


#11 alpha-Chlordane

R.T.: 5.014 min
Delta R.T.: -0.026 min
Response: 2787063
Conc: 0.67 ng/ml

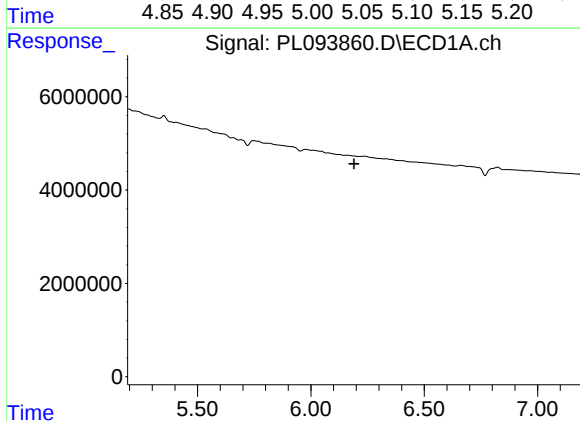


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 6.191 min
Response: 0
Conc: N.D.

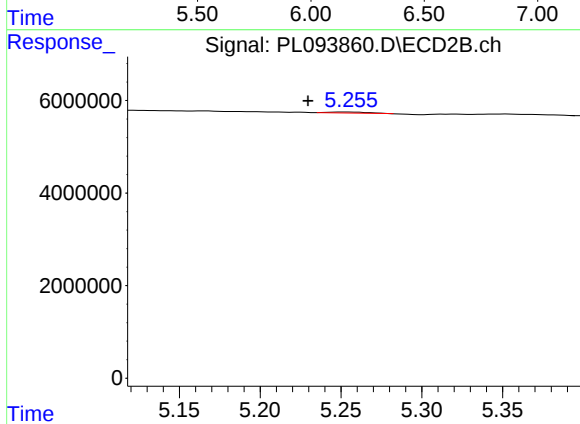

#12 4,4'-DDE


R.T.: 5.253 min
Delta R.T.: 0.024 min
Response: 337624
Conc: 0.08 ng/ml

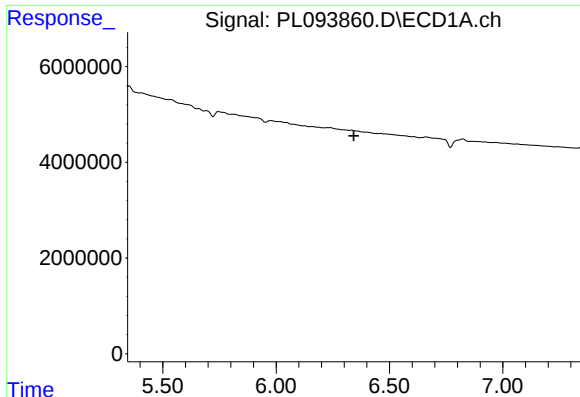

#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 6.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

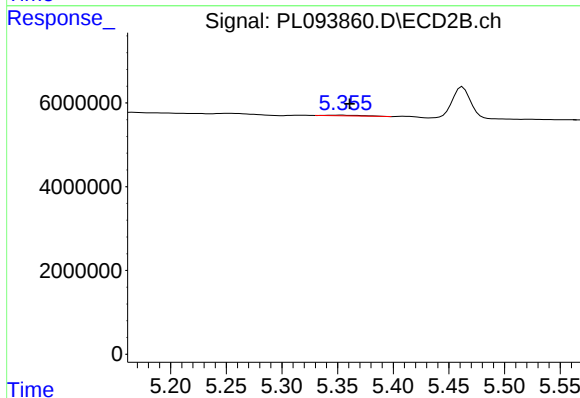


#13 Dieldrin

R.T.: 5.354 min
Delta R.T.: -0.007 min
Response: 376366
Conc: 0.09 ng/ml


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 6.572 min
Response: 0
Conc: N.D.

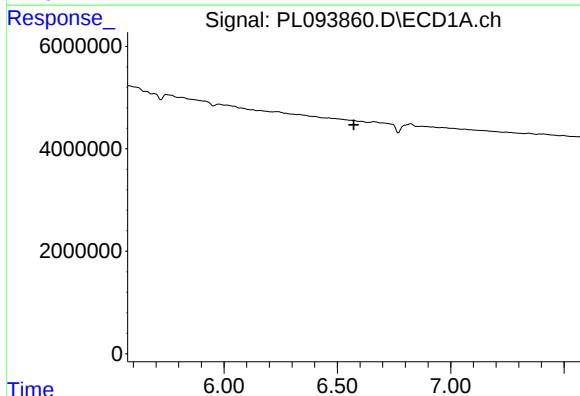

#14 Endrin


R.T.: 5.656 min
Delta R.T.: 0.019 min
Response: 1506631
Conc: 0.41 ng/ml

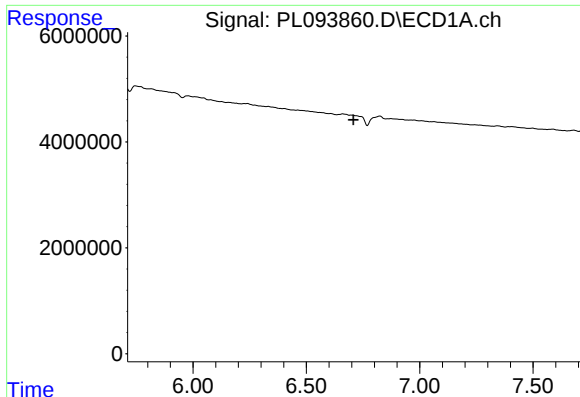

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.708 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

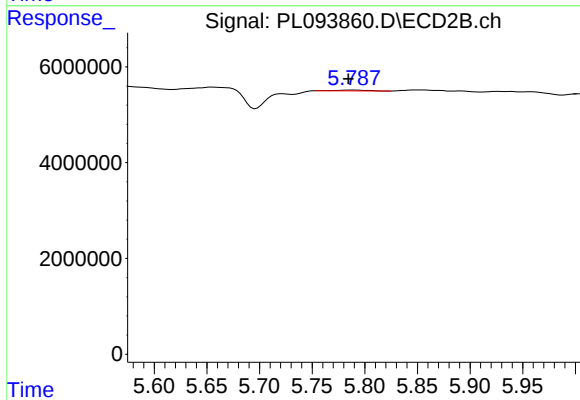


#16 4,4'-DDD

R.T.: 5.788 min
Delta R.T.: 0.004 min
Response: 350710
Conc: 0.11 ng/ml

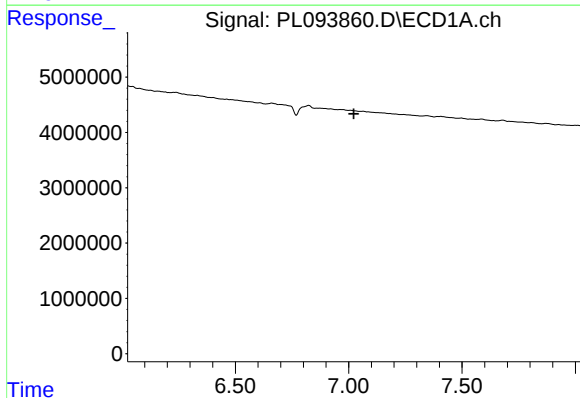


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 7.022 min
Response: 0
Conc: N.D.

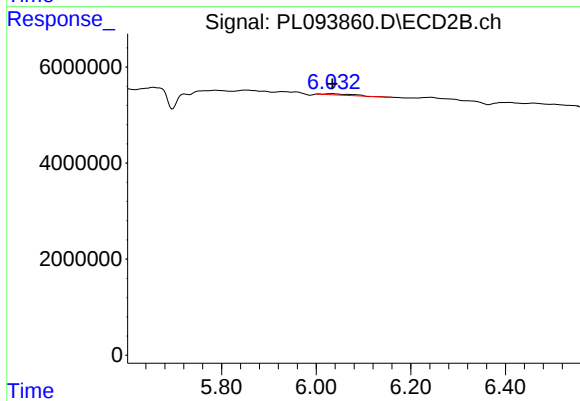

#17 4,4'-DDT


R.T.: 6.033 min
Delta R.T.: -0.001 min
Response: 859429
Conc: 0.26 ng/ml

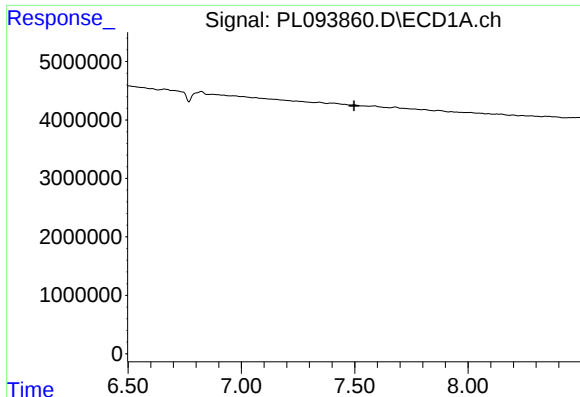

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.498 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

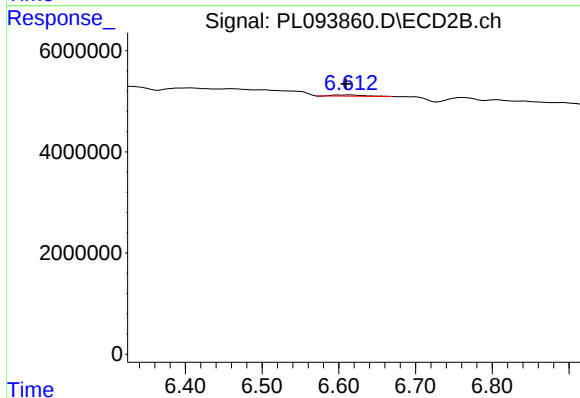


#20 Methoxychlor

R.T.: 6.614 min
Delta R.T.: 0.005 min
Response: 609215
Conc: 0.34 ng/ml

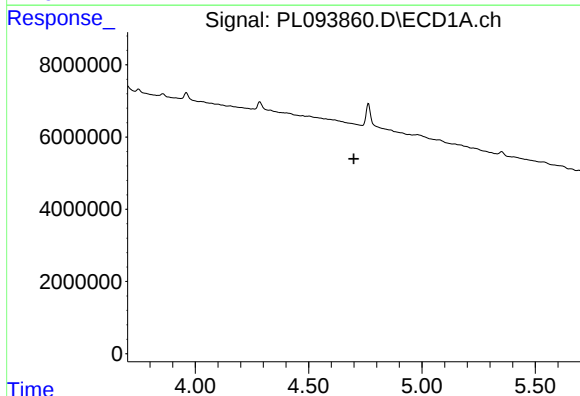


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

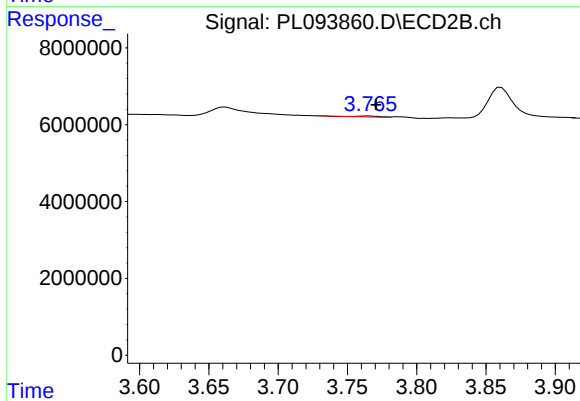

#23 Chlordane-1


R.T.: 3.765 min
Delta R.T.: -0.005 min
Response: 321214
Conc: 2.57 ng/ml

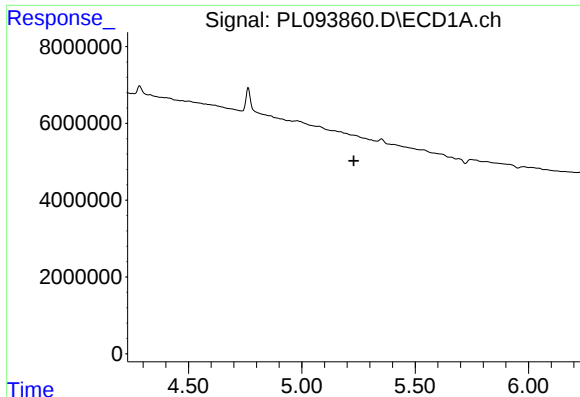

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 5.229 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

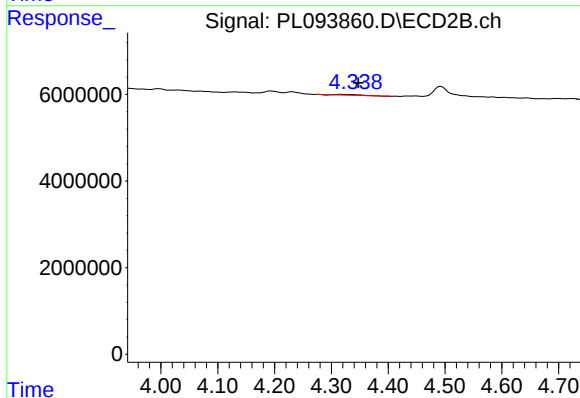


#24 Chlordane-2

R.T.: 4.317 min
Delta R.T.: -0.030 min
Response: 454744
Conc: 3.10 ng/ml

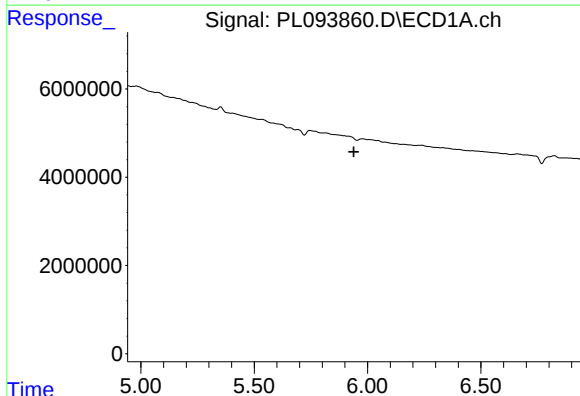


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.939 min
Response: 0
Conc: N.D.

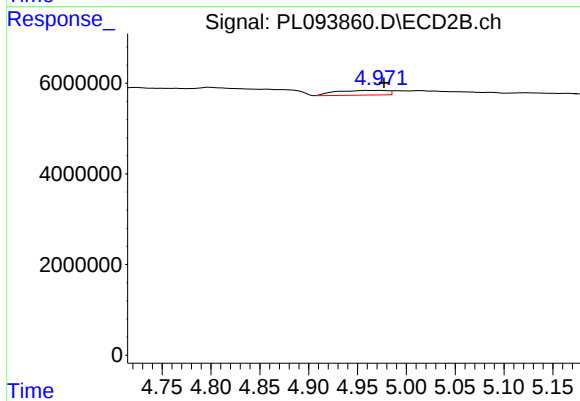

#25 Chlordane-3


R.T.: 4.973 min
Delta R.T.: -0.004 min
Response: 3840835
Conc: 8.83 ng/ml

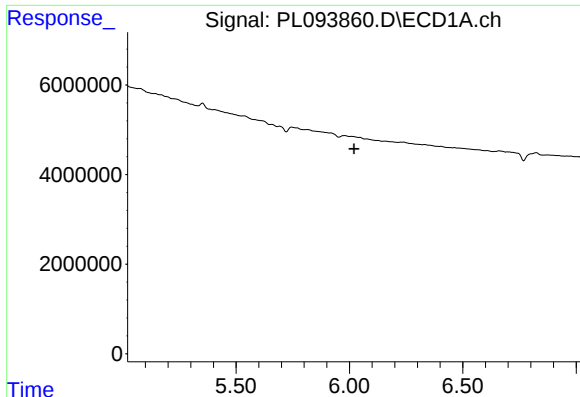

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 6.021 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JPP-20.1-012725

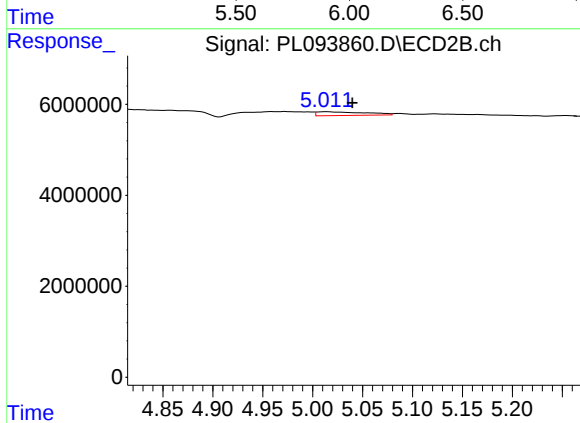


#26 Chlordane-4

R.T.: 5.014 min
Delta R.T.: -0.026 min
Response: 2787063
Conc: 6.58 ng/ml

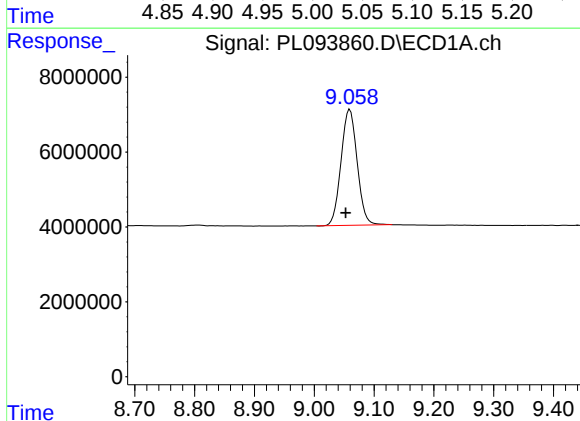

#28 Decachlorobiphenyl

R.T.: 9.060 min
Delta R.T.: 0.007 min
Response: 58124889
Conc: 27.79 ng/ml

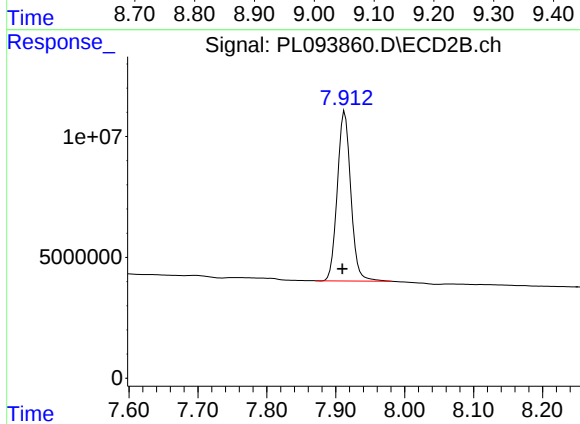

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.003 min
Response: 95383275
Conc: 27.22 ng/ml