

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013020\
 Data File : PL056214.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 13:41
 Operator : AJ\MA
 Sample : L1296-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 00:37:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	130.3E6	37756718	12.442	12.912
28)	SA Decachlor...	8.249	9.088	131.7E6	29093150	12.505	12.862
Target Compounds							
2)	A alpha-BHC	0.000	4.429f	0	37315704	N.D.	8.525 #
10)	B gamma-Chl...	5.461f	0.000	13668775	0	0.872	N.D. #
11)	B alpha-Chl...	0.000	6.197	0	7418047	N.D.	2.340 #
12)	B 4,4'-DDE	5.659	6.352	95427088	21900655	6.584	7.311
14)	MA Endrin	6.050	0.000	22580123	0	1.607	N.D. #
17)	MA 4,4'-DDT	6.416	7.143	84268137	16152585	7.711	7.036
20)	A Methoxychlor	6.947f	0.000	14504139	0	2.730	N.D. #
23)	Chlordane-1	4.372	0.000	12993452	0	34.325	N.D. #
24)	Chlordane-2	4.904f	0.000	12802400	0	29.222	N.D. #
25)	Chlordane-3	5.461f	0.000	13668775	0	10.826	N.D. #
26)	Chlordane-4	0.000	6.197	0	7418047	N.D.	16.884 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013020\
Data File : PL056214.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 13:41
Operator : AJ\MA
Sample : L1296-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 00:37:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

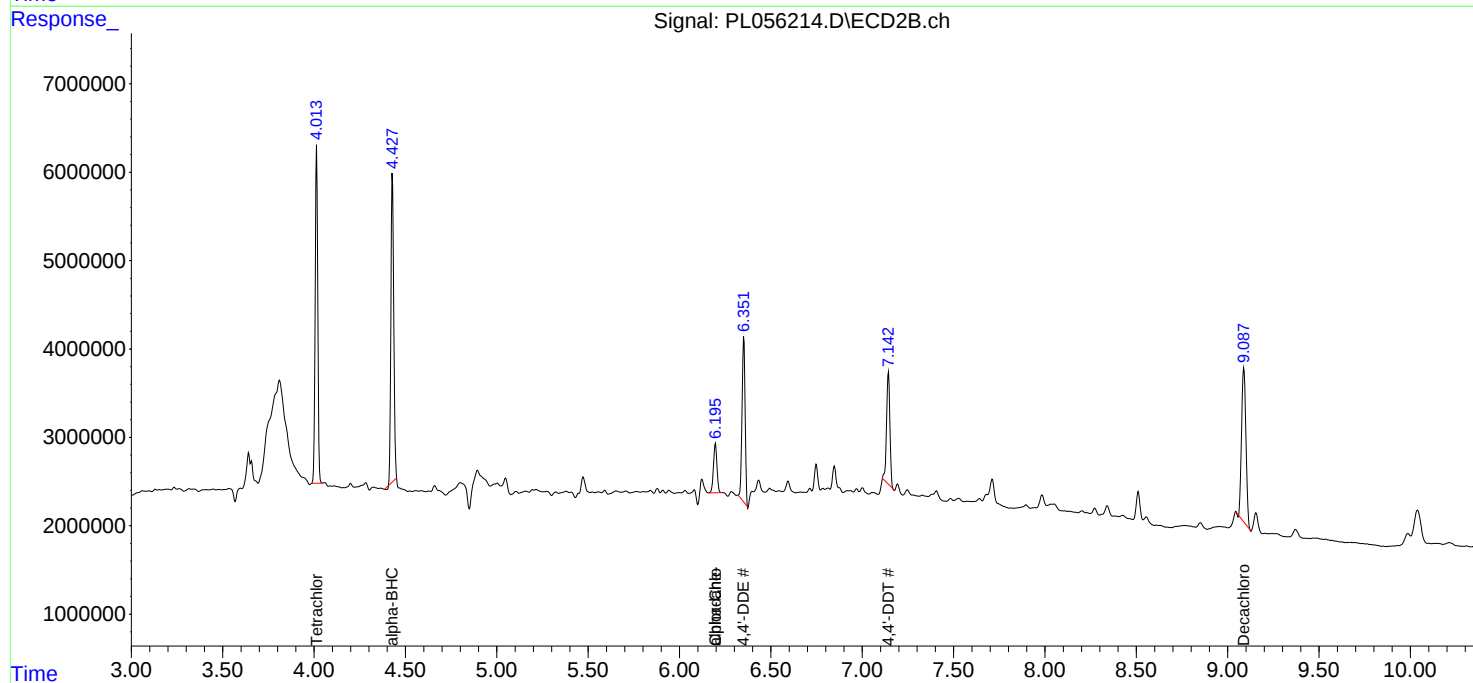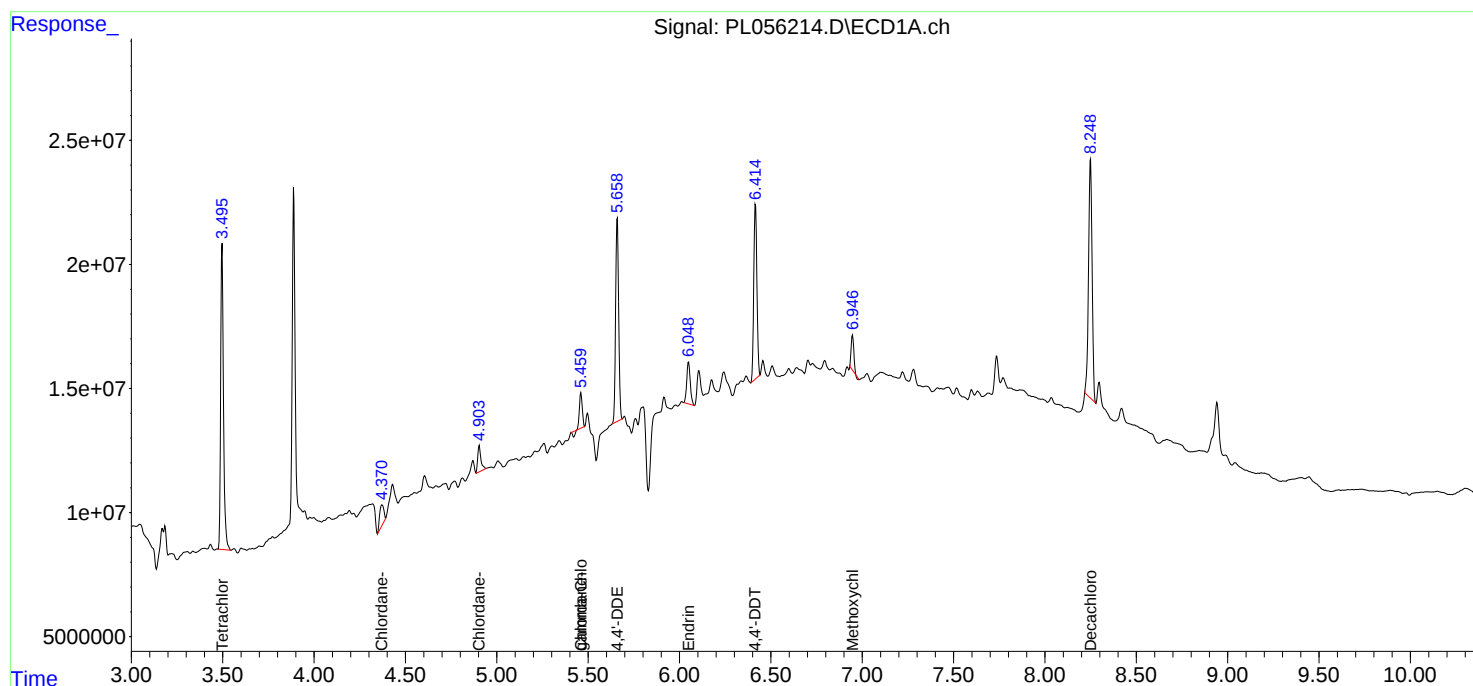


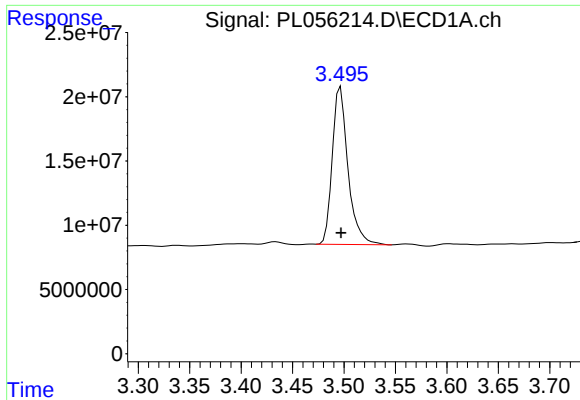

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 130305632
Conc: 12.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

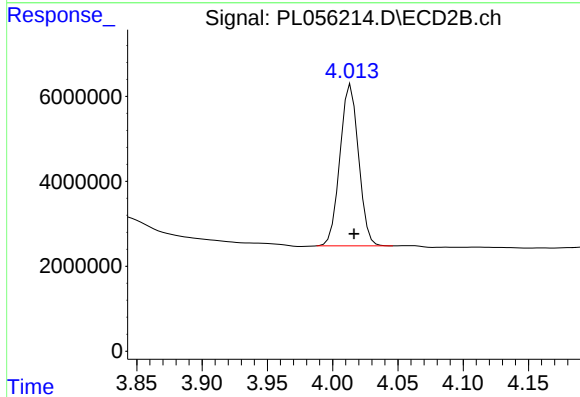


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: -0.002 min
Response: 37756718
Conc: 12.91 ng/ml

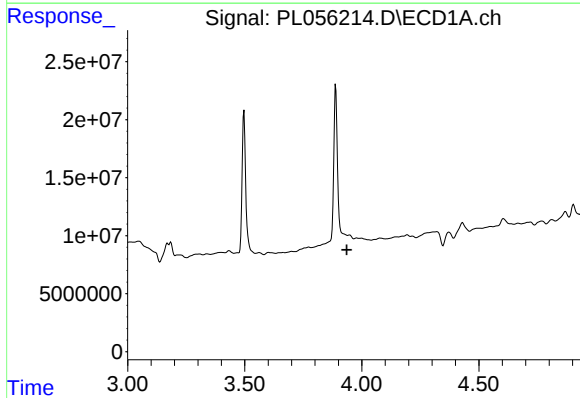


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

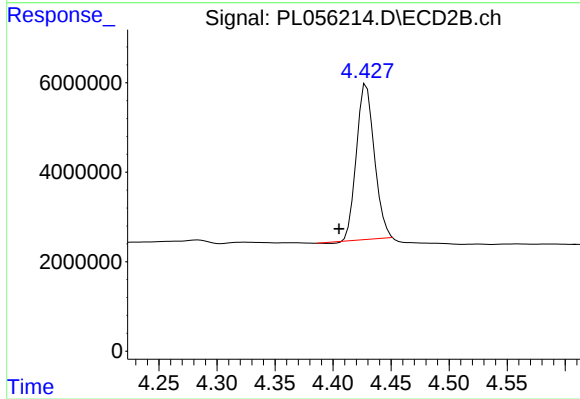

#2 alpha-BHC


R.T.: 4.429 min
Delta R.T.: 0.023 min
Response: 37315704
Conc: 8.52 ng/ml

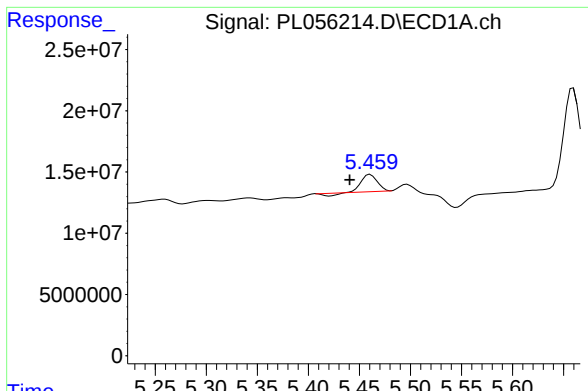

#10 gamma-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.020 min
Response: 13668775
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

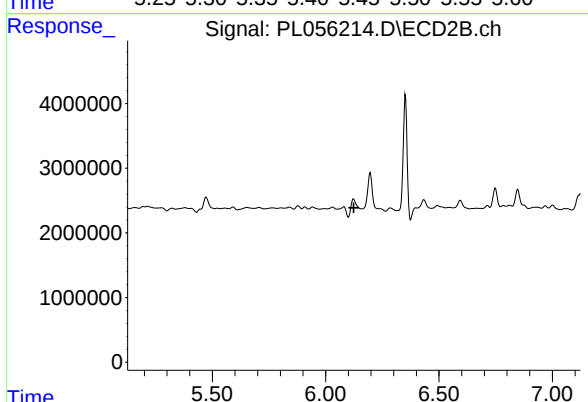


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.124 min
Response: 0
Conc: N.D.

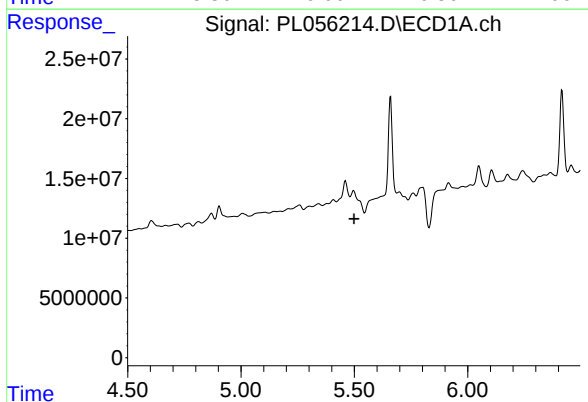


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

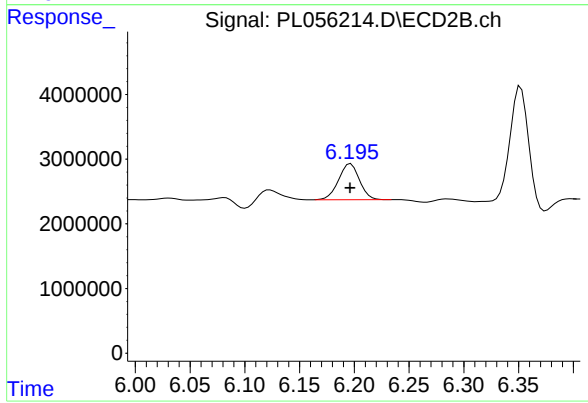

#11 alpha-Chlordane


R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 7418047
Conc: 2.34 ng/ml

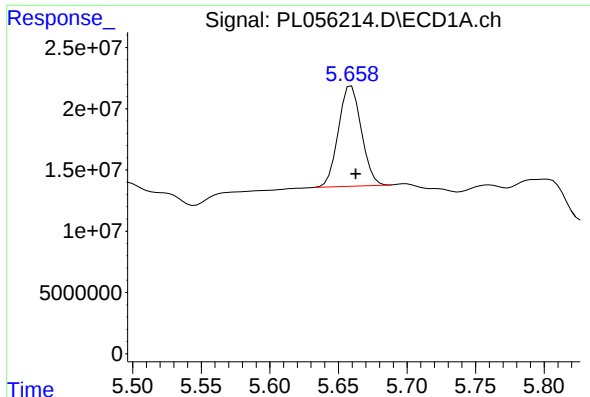

#12 4,4'-DDE


R.T.: 5.659 min
Delta R.T.: -0.003 min
Response: 95427088
Conc: 6.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

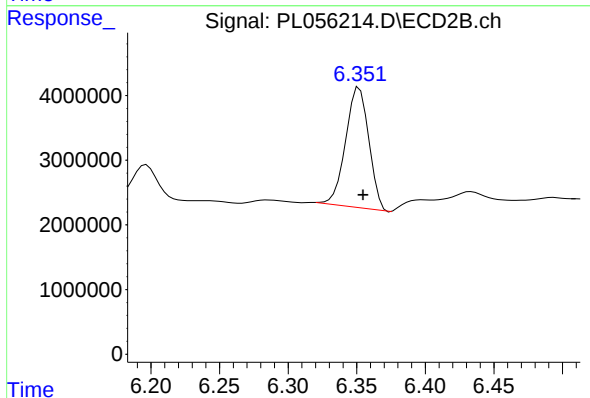


#12 4,4'-DDE

R.T.: 6.352 min
Delta R.T.: -0.003 min
Response: 21900655
Conc: 7.31 ng/ml

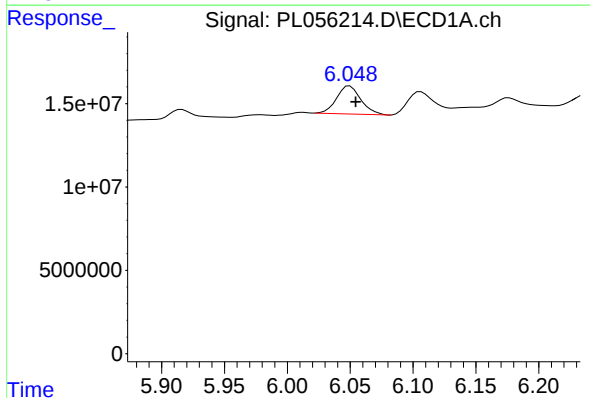


#14 Endrin

R.T.: 6.050 min
Delta R.T.: -0.005 min
Response: 22580123
Conc: 1.61 ng/ml

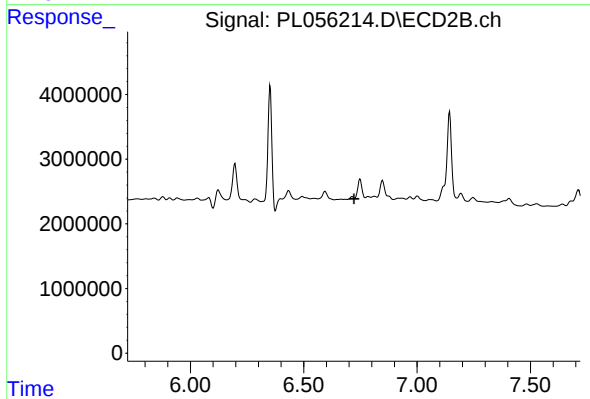

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.723 min
Response: 0
Conc: N.D.

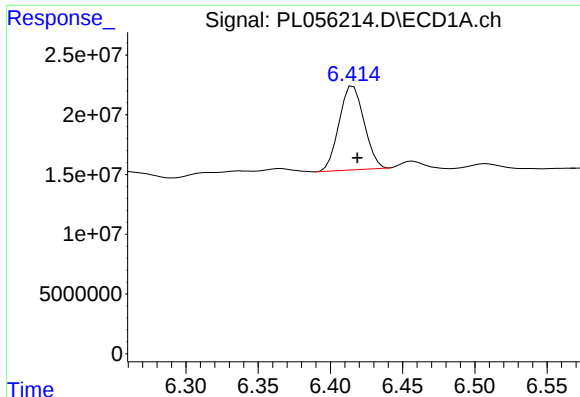

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: -0.003 min
Response: 84268137
Conc: 7.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

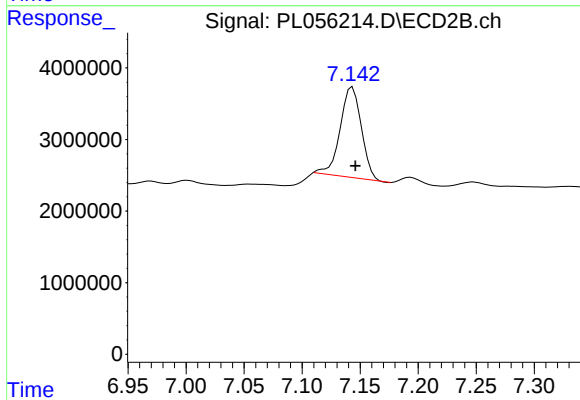


#17 4,4'-DDT

R.T.: 7.143 min
Delta R.T.: -0.003 min
Response: 16152585
Conc: 7.04 ng/ml

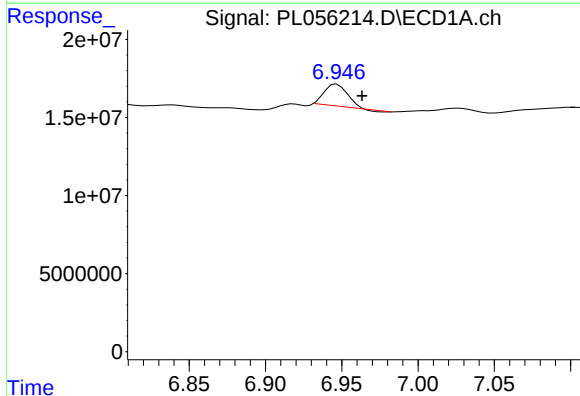


#20 Methoxychlor

R.T.: 6.947 min
Delta R.T.: -0.017 min
Response: 14504139
Conc: 2.73 ng/ml

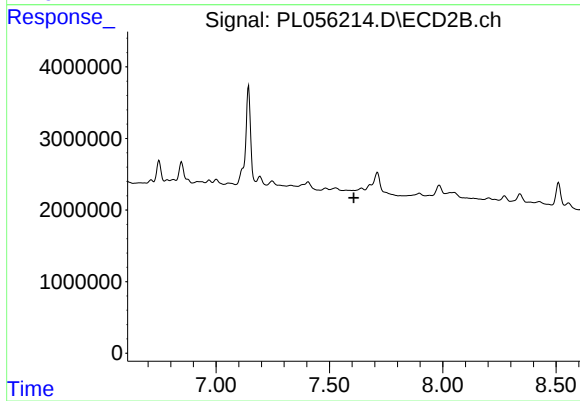

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 7.607 min
Response: 0
Conc: N.D.

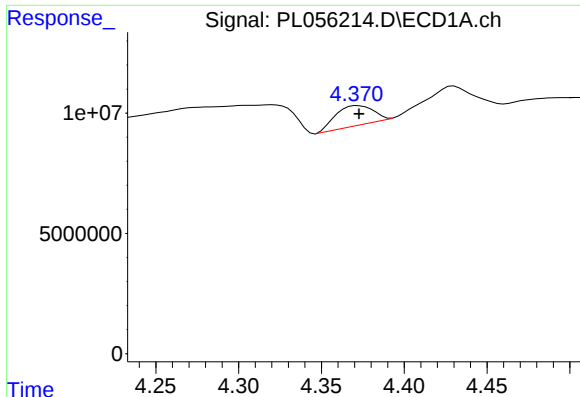

#23 Chlordane-1


R.T.: 4.372 min
Delta R.T.: 0.000 min
Response: 12993452
Conc: 34.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

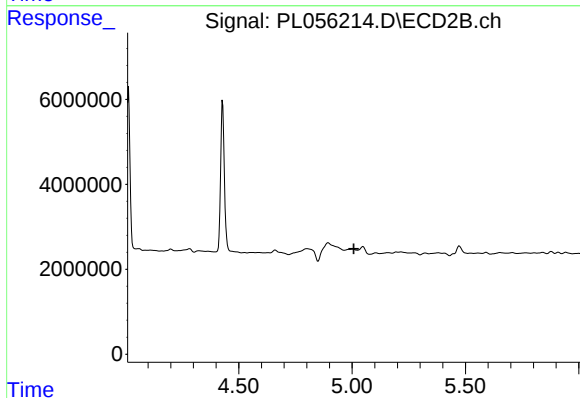


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

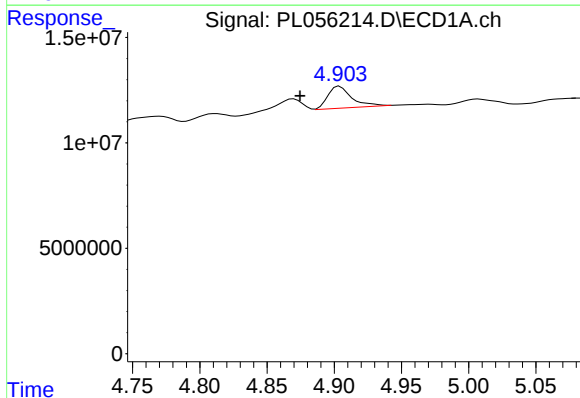


#24 Chlordane-2

R.T.: 4.904 min
Delta R.T.: 0.029 min
Response: 12802400
Conc: 29.22 ng/ml

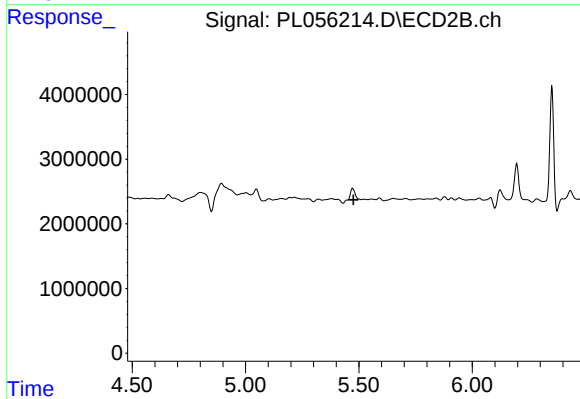

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

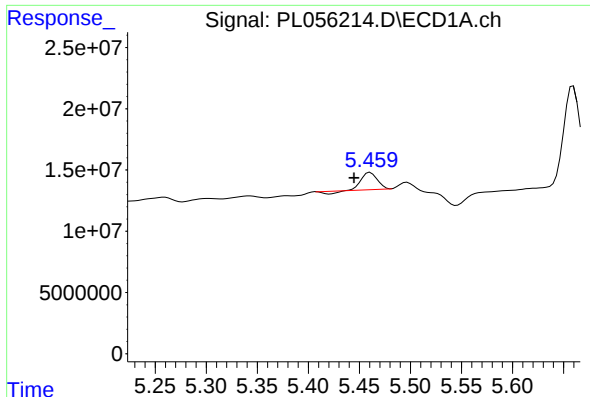

#25 Chlordane-3


R.T.: 5.461 min
Delta R.T.: 0.016 min
Response: 13668775
Conc: 10.83 ng/ml

Instrument :
ECD_L
ClientSampleId :

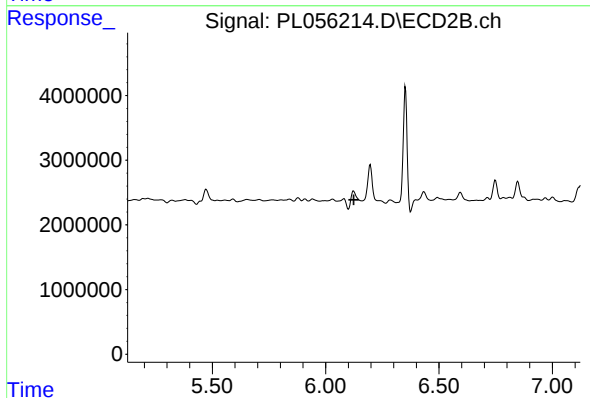


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

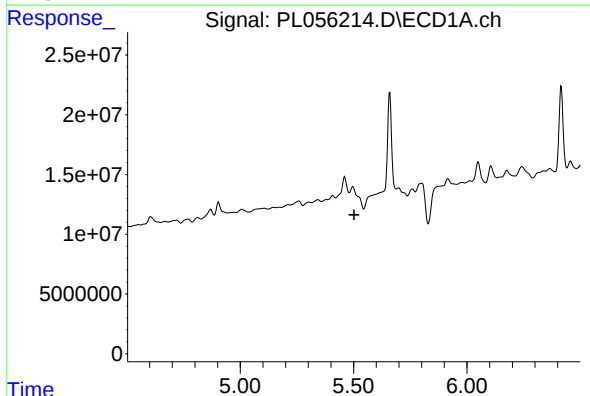


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

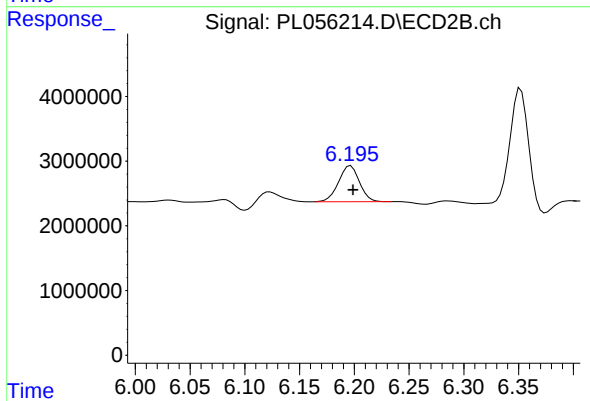

#26 Chlordane-4


R.T.: 6.197 min
Delta R.T.: -0.002 min
Response: 7418047
Conc: 16.88 ng/ml

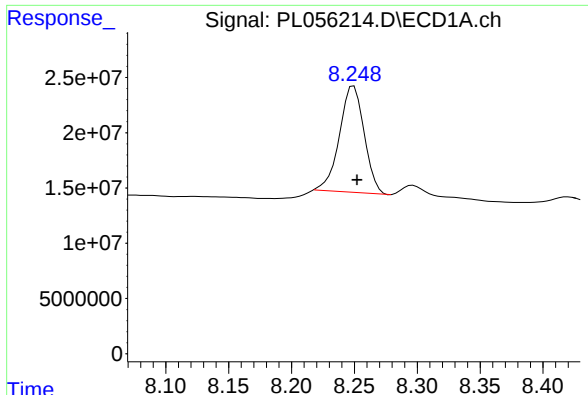

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 131658336
Conc: 12.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

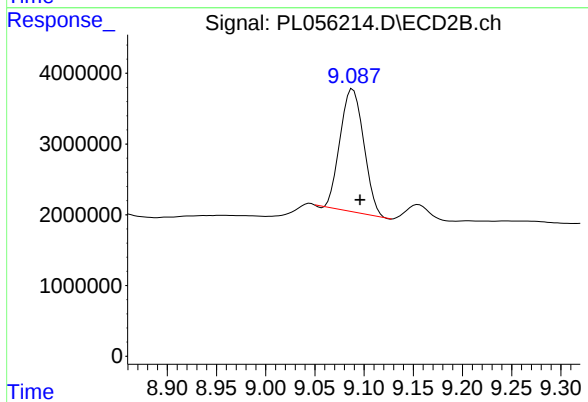

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.008 min
Response: 29093150
Conc: 12.86 ng/ml