

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013020\
 Data File : PL056221.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2020 15:20
 Operator : AJ\MA
 Sample : L1310-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CTY-SB-10102-0-80

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 00:39:19 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	122.5E6	36276464	11.697	12.406
28)	SA Decachlor...	8.250	9.088	112.1E6	26934669	10.647	11.908
Target Compounds							
12)	B 4,4'-DDE	5.659	0.000	12662371	0	0.874	N.D. #
17)	MA 4,4'-DDT	6.413	0.000	10972534	0	1.004	N.D. #
20)	A Methoxychlor	6.946f	0.000	11169478	0	2.103	N.D. #
23)	Chlordane-1	4.369	0.000	13198840	0	34.867	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013020\
Data File : PL056221.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2020 15:20
Operator : AJ\MA
Sample : L1310-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CTY-SB-10102-0-80

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 00:39:19 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

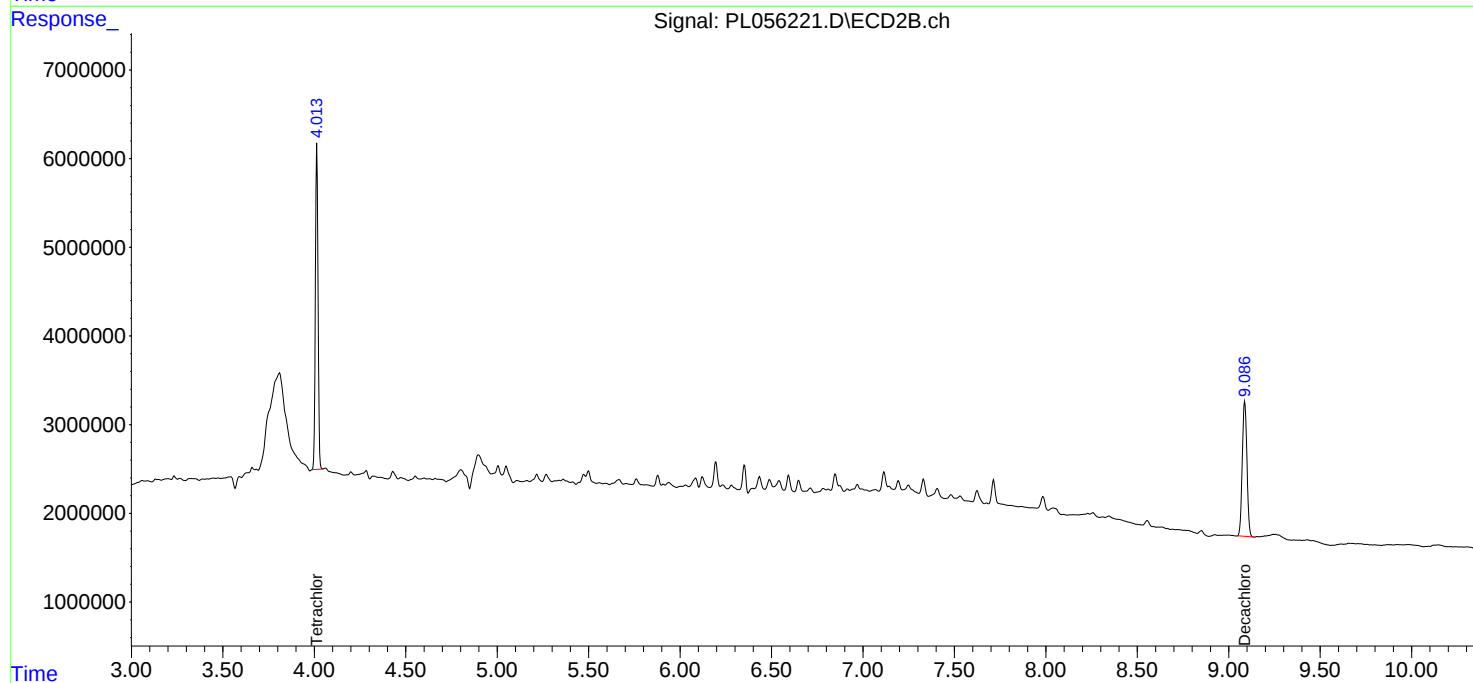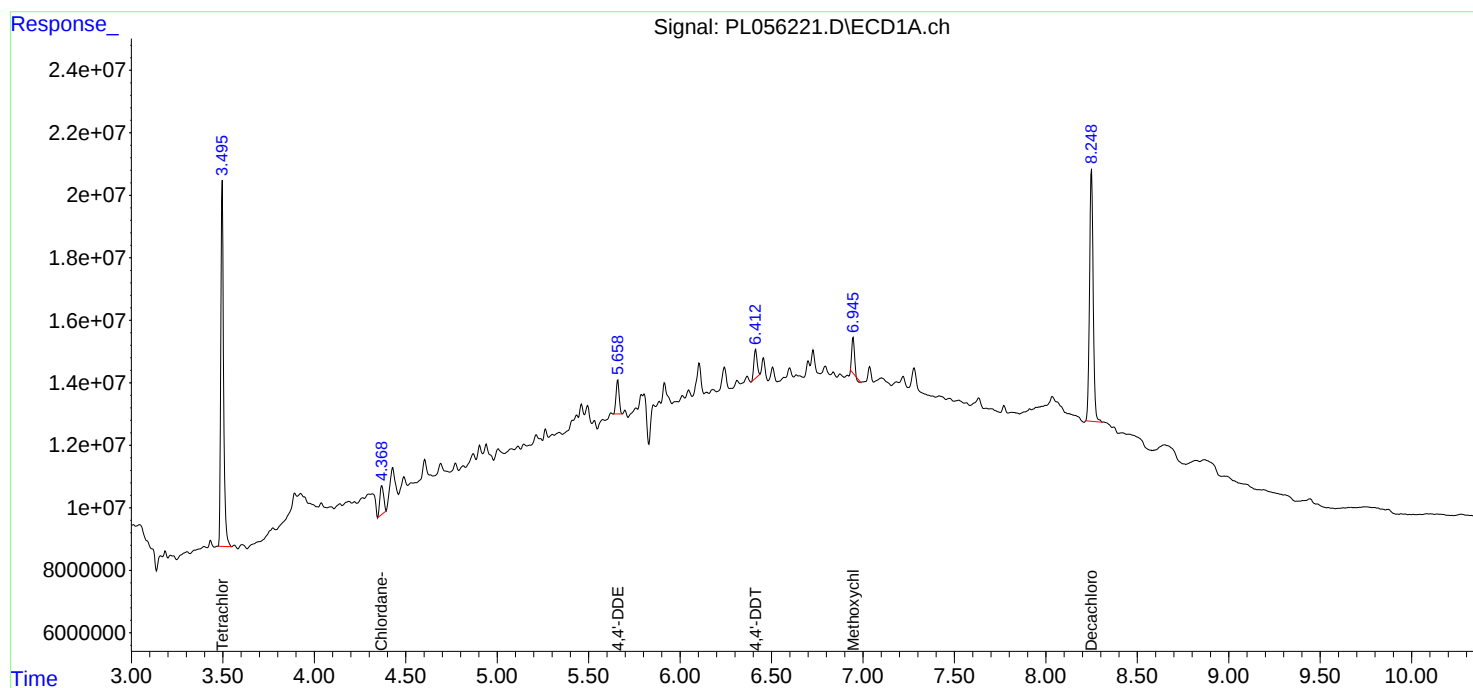


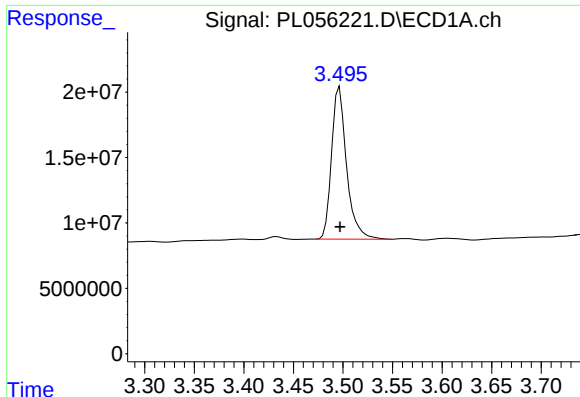

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 122498387
Conc: 11.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTY-SB-10102-0-80

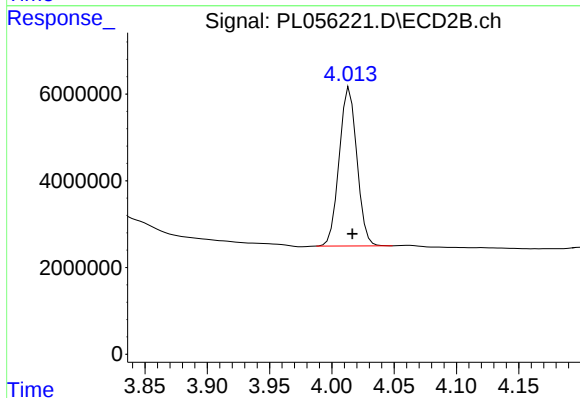


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: -0.002 min
Response: 36276464
Conc: 12.41 ng/ml

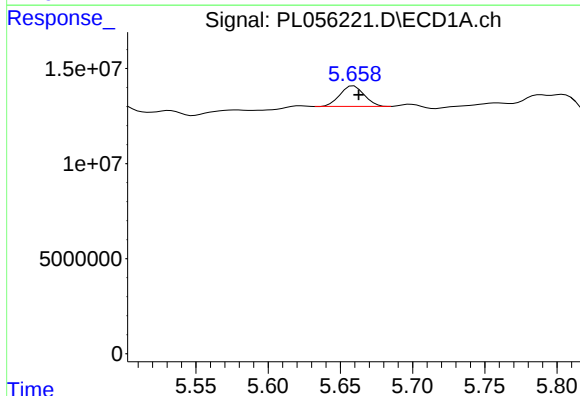


#12 4,4'-DDE

R.T.: 5.659 min
Delta R.T.: -0.003 min
Response: 12662371
Conc: 0.87 ng/ml

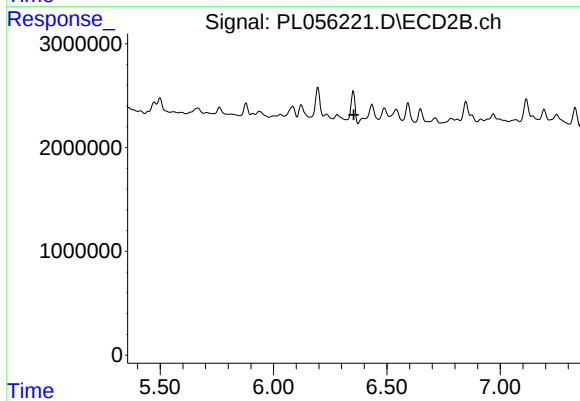

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.355 min
Response: 0
Conc: N.D.

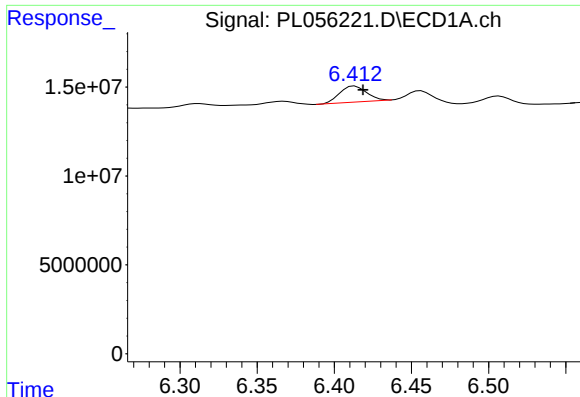

#17 4,4'-DDT


R.T.: 6.413 min
Delta R.T.: -0.005 min
Response: 10972534
Conc: 1.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTY-SB-10102-0-80

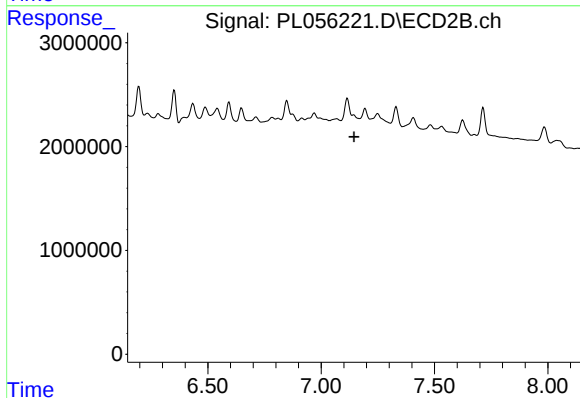


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

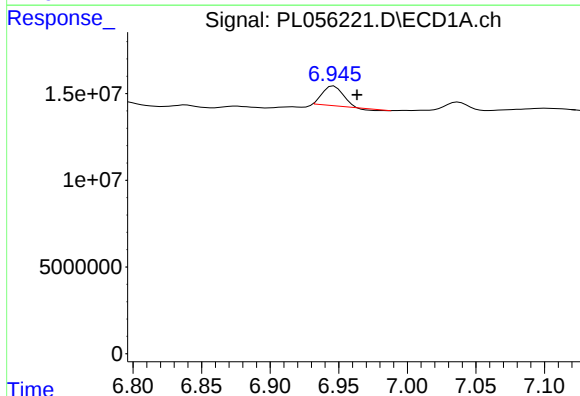


#20 Methoxychlor

R.T.: 6.946 min
Delta R.T.: -0.017 min
Response: 11169478
Conc: 2.10 ng/ml

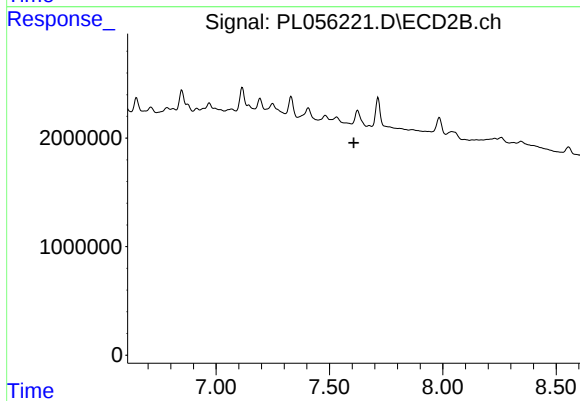

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.607 min
Response: 0
Conc: N.D.

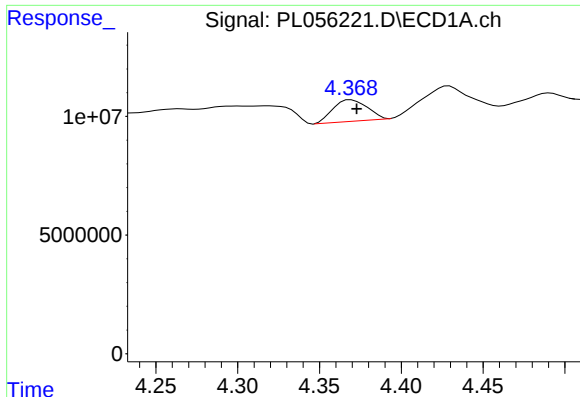

#23 Chlordane-1


R.T.: 4.369 min
Delta R.T.: -0.003 min
Response: 13198840
Conc: 34.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
CTY-SB-10102-0-80

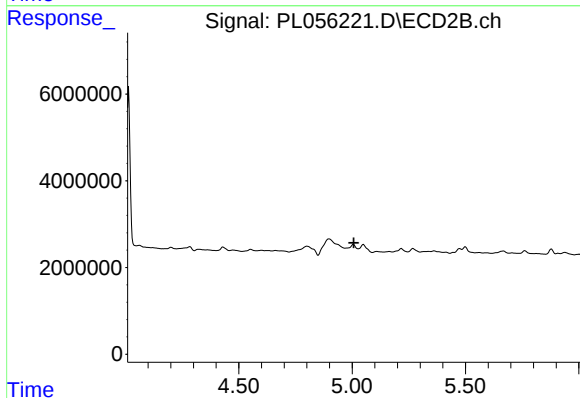


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.008 min
Response: 0
Conc: N.D.

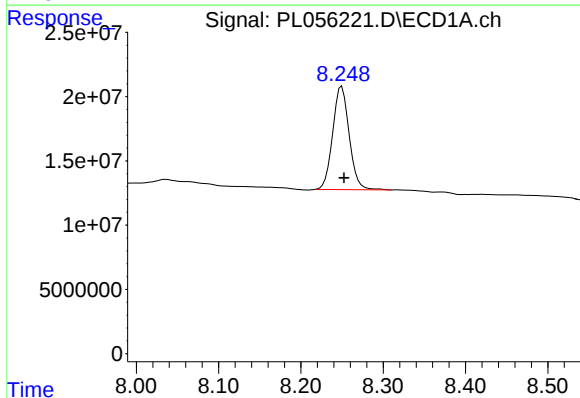

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: -0.003 min
Response: 112090451
Conc: 10.65 ng/ml

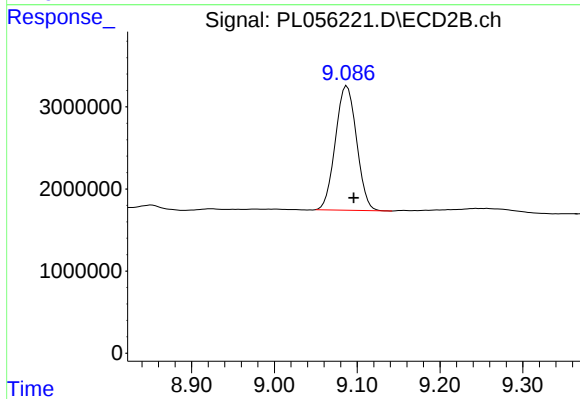

#28 Decachlorobiphenyl

R.T.: 9.088 min
Delta R.T.: -0.008 min
Response: 26934669
Conc: 11.91 ng/ml