

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064519.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 12:52
 Operator : AR\AJ
 Sample : M1251-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 400026

Manual Integrations
 APPROVED

Sohil
 2/1/2021 2:55:37 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:23:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.433	4.107	34290641	26504752	11.264	11.127
28) SA Decachlor...	8.164	9.269	31625744	19130079	10.036	9.344
Target Compounds						
12) B 4,4'-DDE	5.582	6.483	11405317	7904044	3.026	3.053
17) MA 4,4'-DDT	6.334	7.279	4552088	2104014	1.483	1.024m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064519.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 12:52
Operator : AR\AJ
Sample : M1251-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
400026


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:37 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:23:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

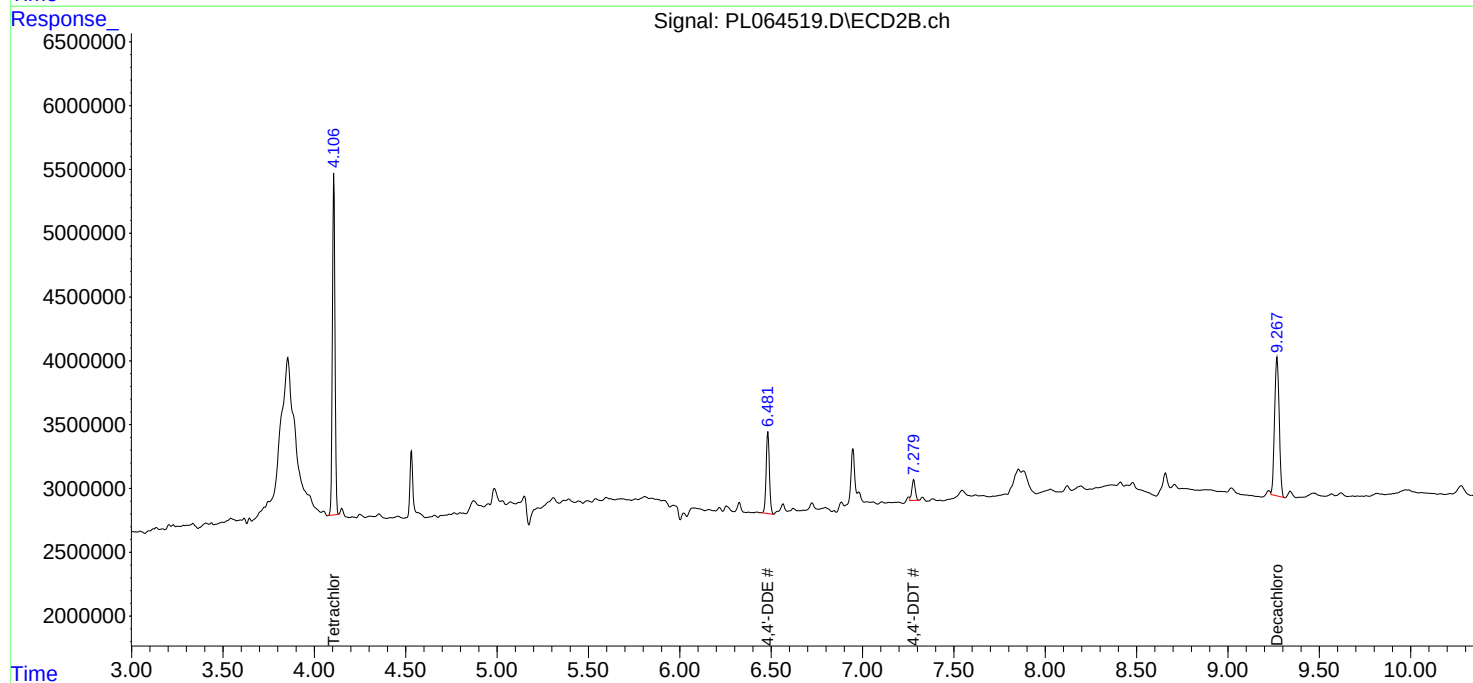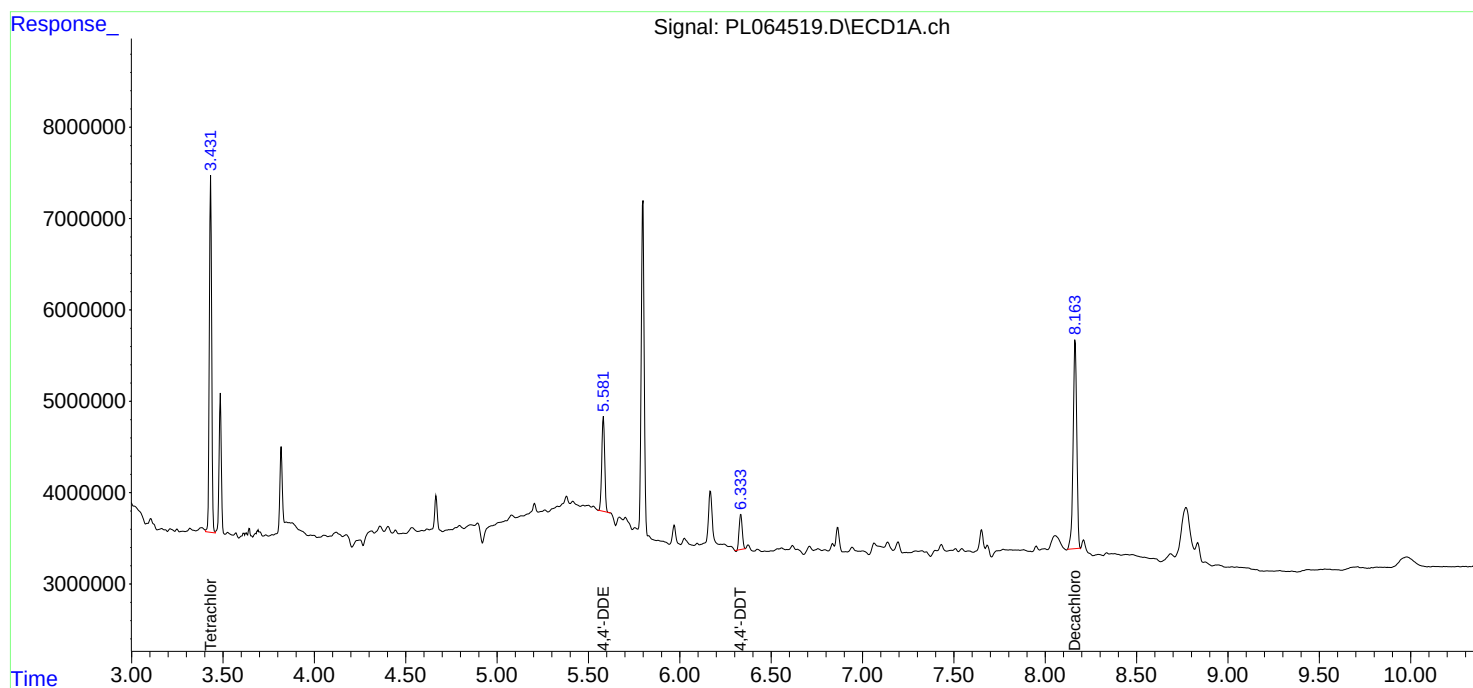

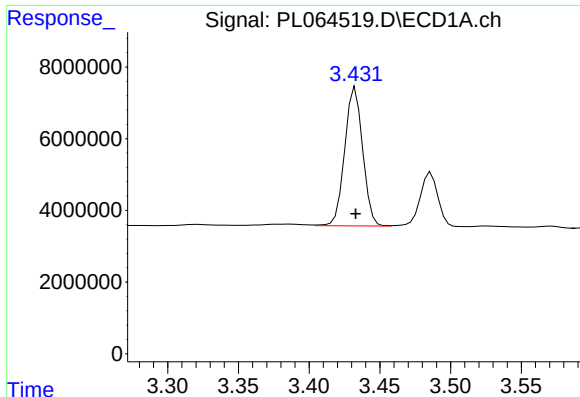


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 34290641
Conc: 11.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
400026


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:37 PM

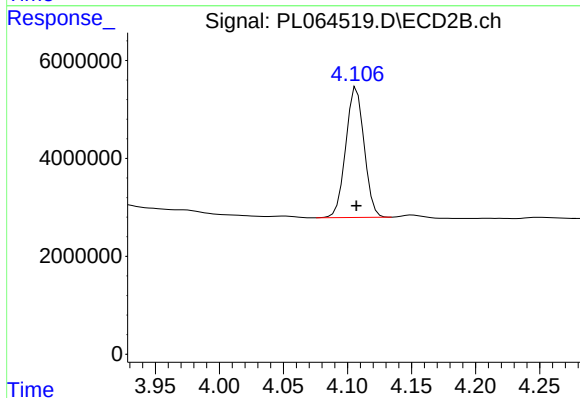


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 26504752
Conc: 11.13 ng/ml

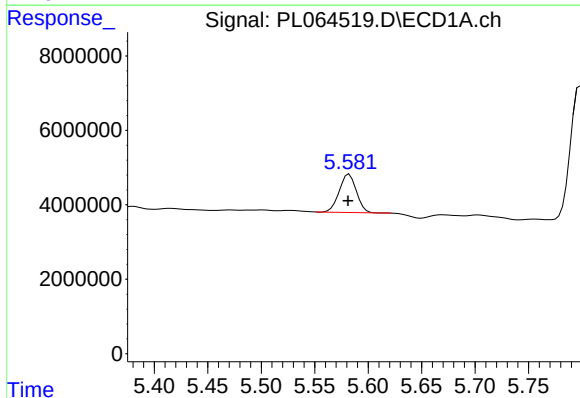


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 11405317
Conc: 3.03 ng/ml

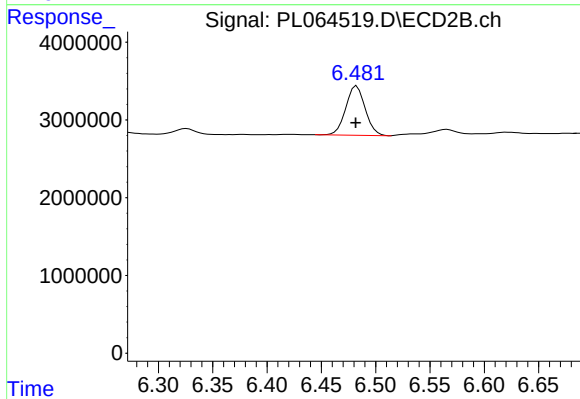

#12 4,4'-DDE

R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 7904044
Conc: 3.05 ng/ml

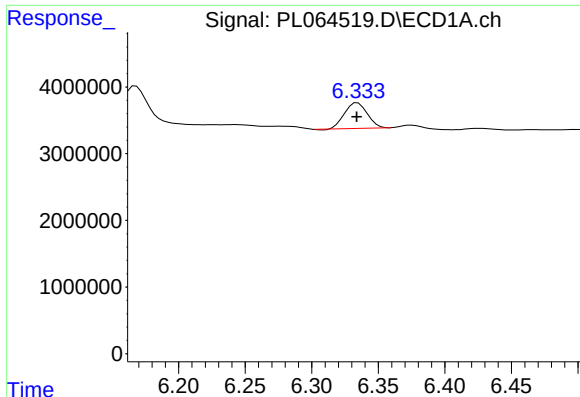


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 4552088
Conc: 1.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
400026


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:37 PM

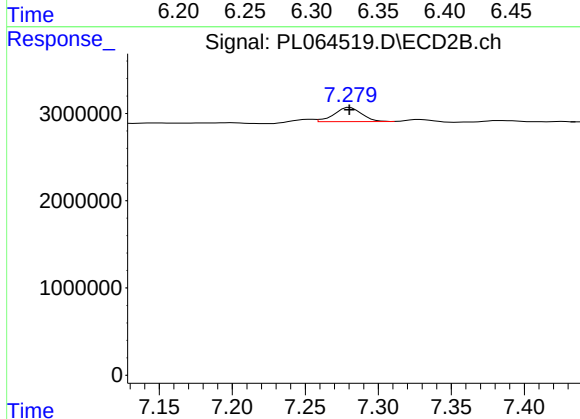


#17 4,4'-DDT

R.T.: 7.279 min
Delta R.T.: -0.001 min
Response: 2104014
Conc: 1.02 ng/ml m

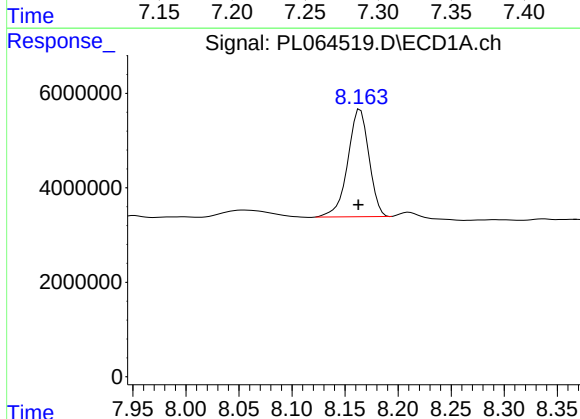

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 31625744
Conc: 10.04 ng/ml

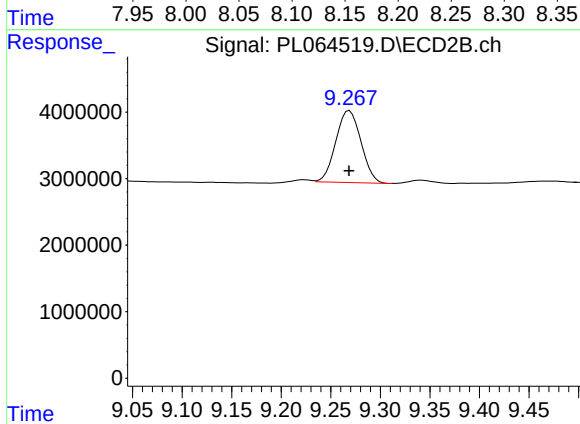

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.000 min
Response: 19130079
Conc: 9.34 ng/ml