

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064522.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 13:34
 Operator : AR\AJ
 Sample : M1251-07
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 400024

Manual Integrations
 APPROVED

Sohil
 2/1/2021 2:55:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:23:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.432	4.107	35302074	26655518	11.597	11.190
28) SA Decachlor...	8.162	9.268	36290077	20178197	11.516m	9.856m
Target Compounds						
12) B 4,4'-DDE	5.582	6.482	8211067	5650163	2.178	2.182
17) MA 4,4'-DDT	6.333	7.281	4575837	2140552	1.491	1.042 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064522.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 13:34
Operator : AR\AJ
Sample : M1251-07
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
400024


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:23:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

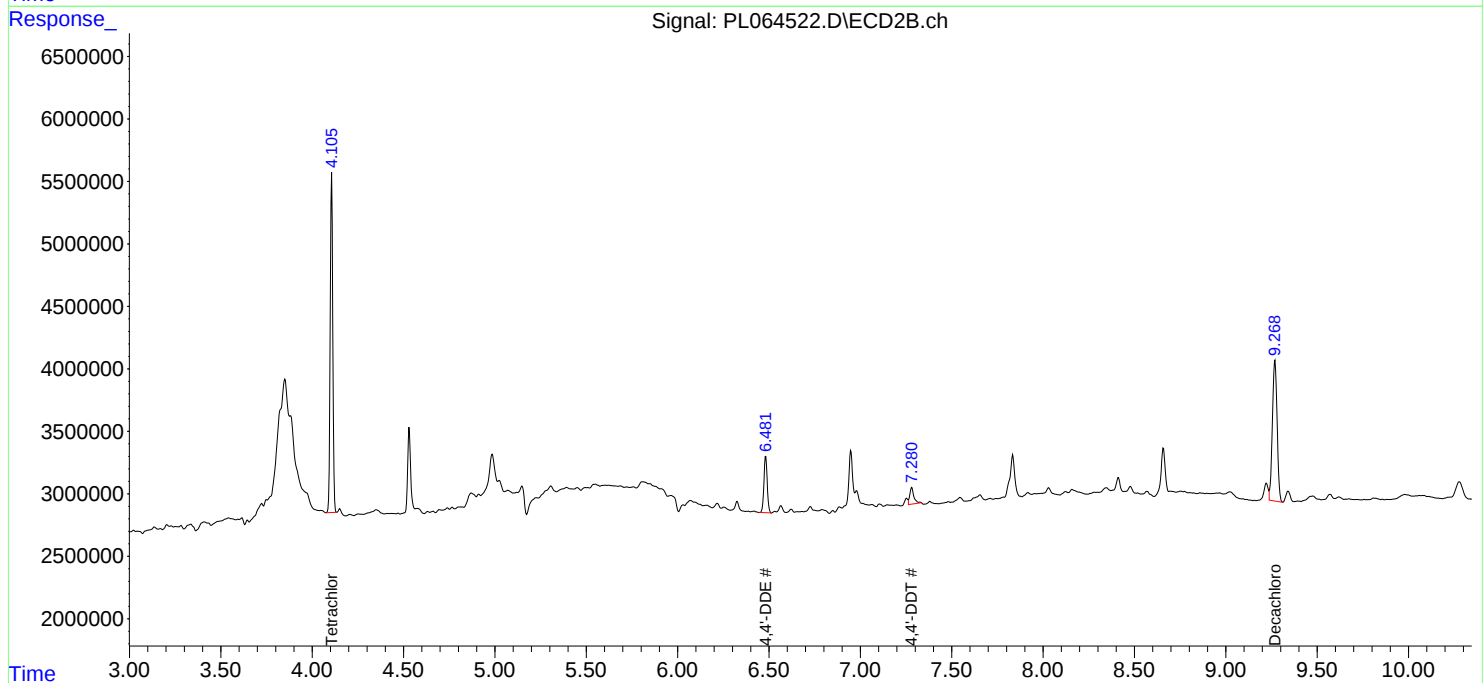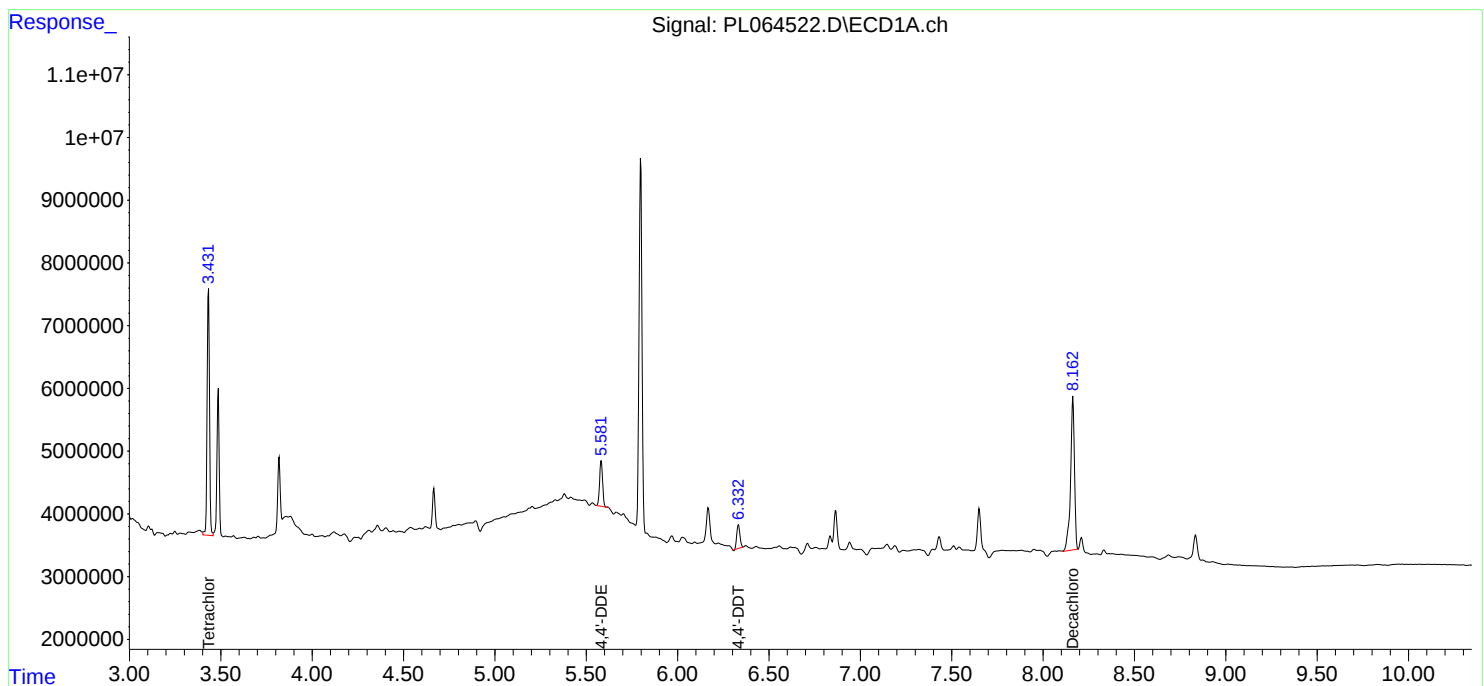

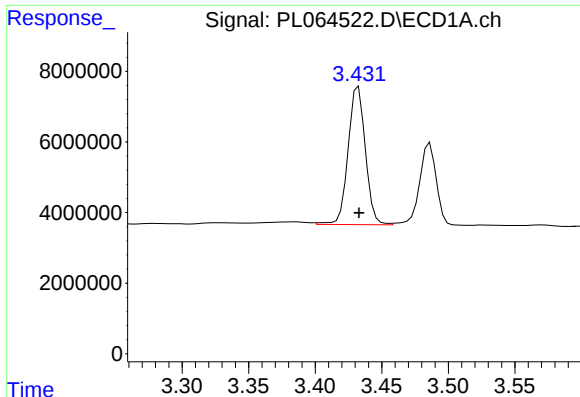


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 35302074
Conc: 11.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
400024


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:40 PM

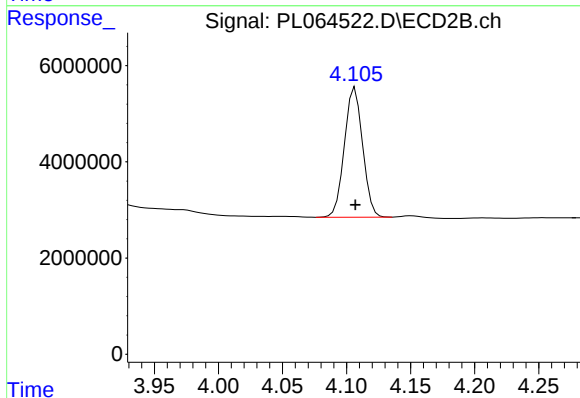


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 26655518
Conc: 11.19 ng/ml

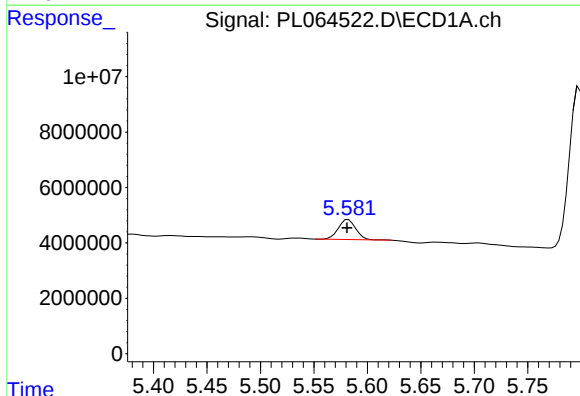


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 8211067
Conc: 2.18 ng/ml

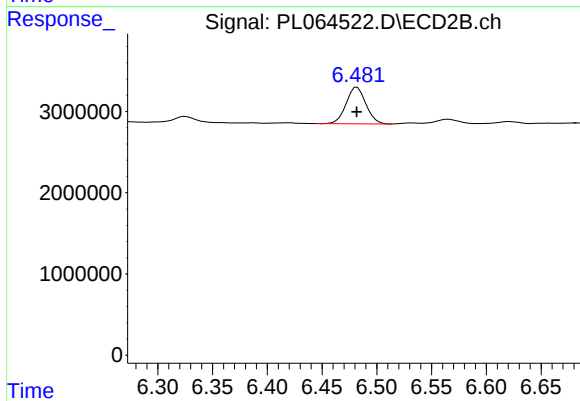

#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 5650163
Conc: 2.18 ng/ml

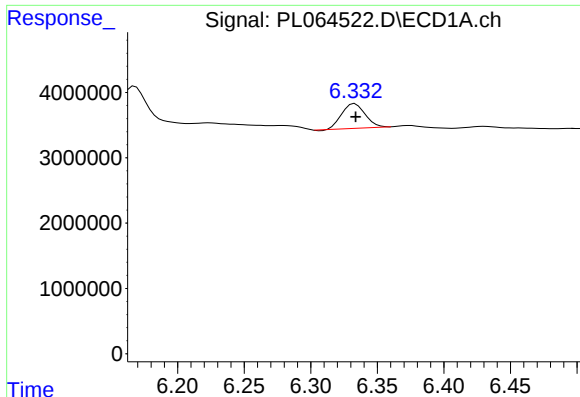


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 4575837
Conc: 1.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
400024


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:40 PM

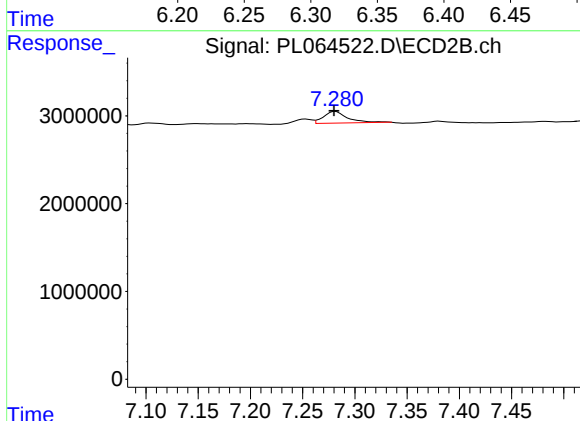


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.001 min
Response: 2140552
Conc: 1.04 ng/ml

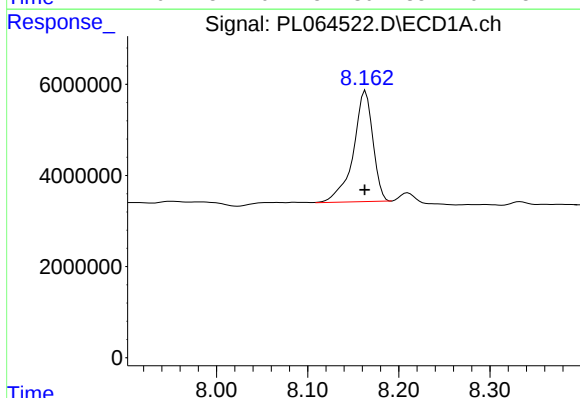

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 36290077
Conc: 11.52 ng/ml m

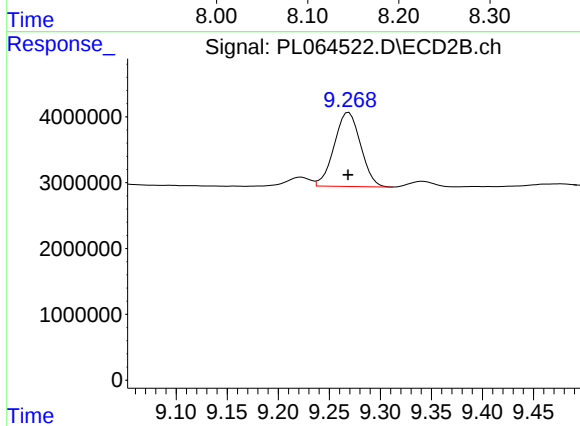

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 20178197
Conc: 9.86 ng/ml m