

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064523.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 13:49
 Operator : AR\AJ
 Sample : M1252-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BS-SP

Manual Integrations
 APPROVED

Sohil
 2/1/2021 2:55:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:24:10 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	62245499	47065457	20.448	19.759
28)	SA Decachlor...	8.163	9.268	64517326	41521219	20.473	20.280
Target Compounds							
12)	B 4,4'-DDE	5.582	6.482	51875278	35070502	13.762	13.544
16)	A 4,4'-DDD	6.094	6.980	7600413	10260465	2.415m	4.457 #
17)	MA 4,4'-DDT	6.334	7.279	8121095	8336676	2.646	4.059 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064523.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 13:49
Operator : AR\AJ
Sample : M1252-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BS-SP


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:24:10 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

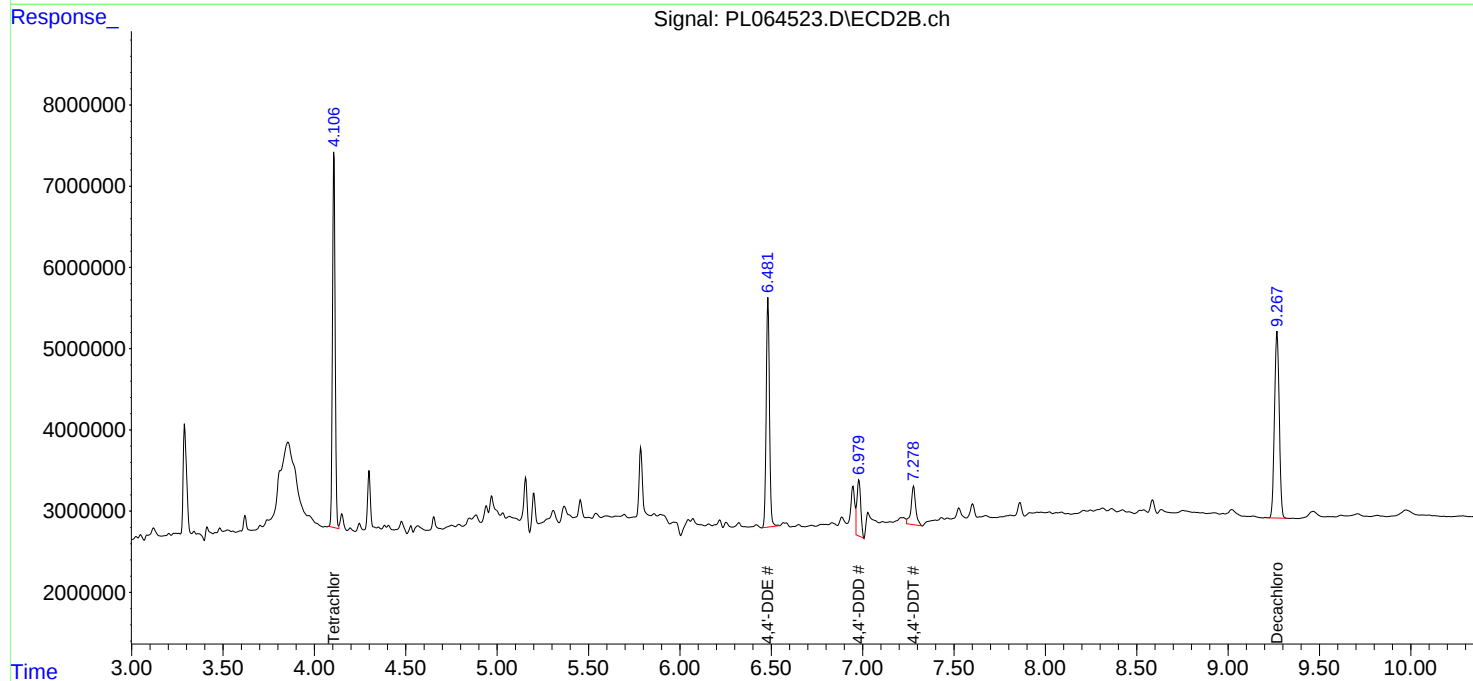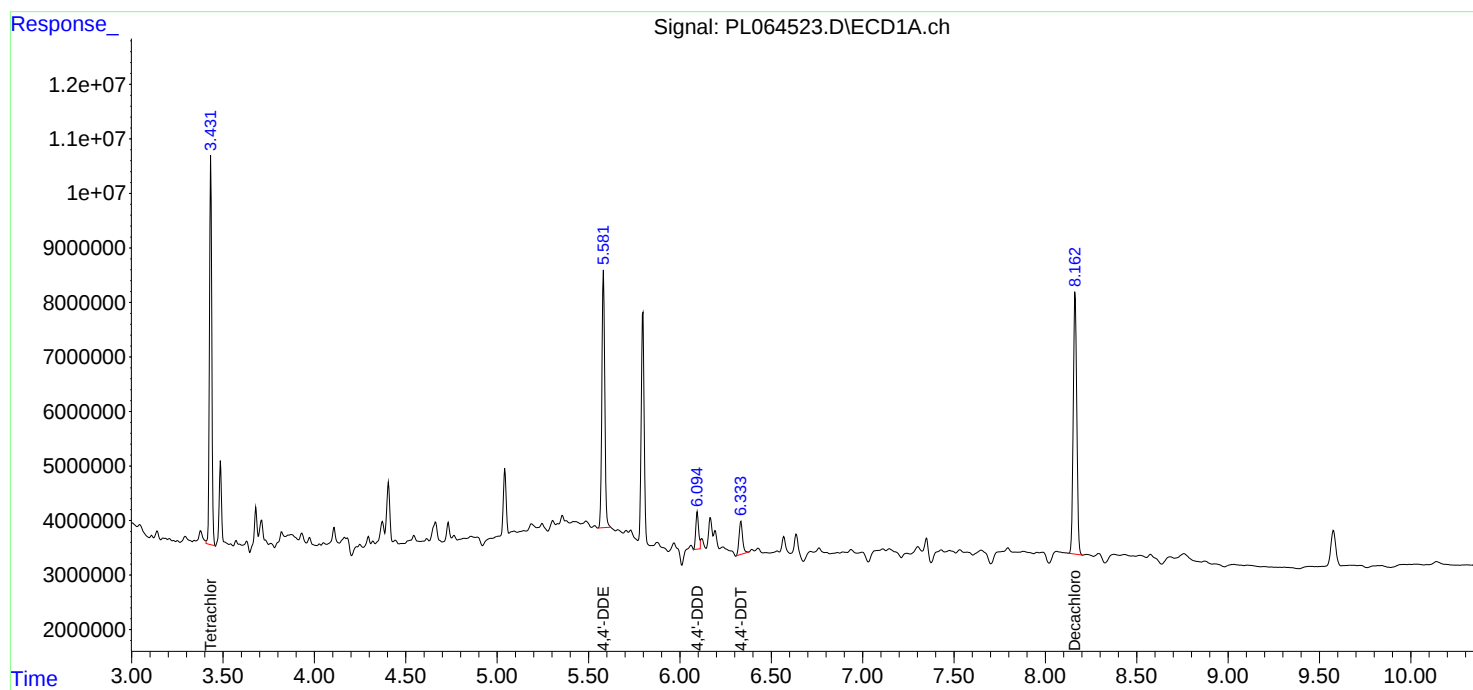

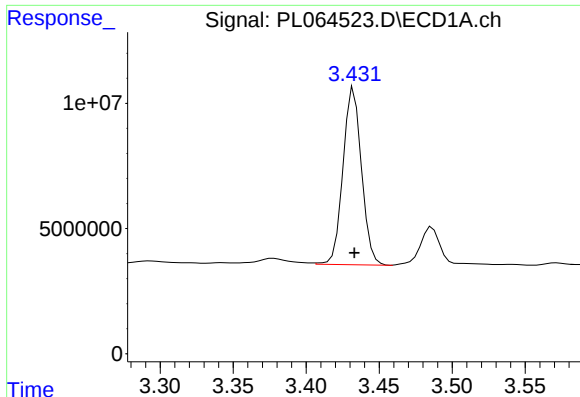


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 62245499
Conc: 20.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
BS-SP


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:42 PM

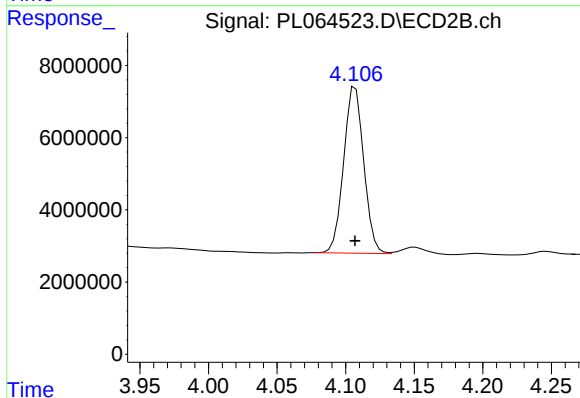


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 47065457
Conc: 19.76 ng/ml

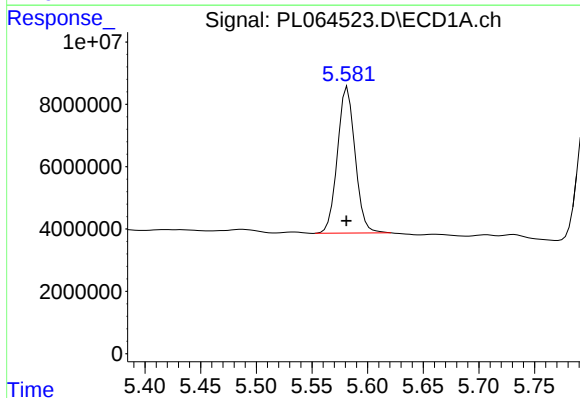


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 51875278
Conc: 13.76 ng/ml

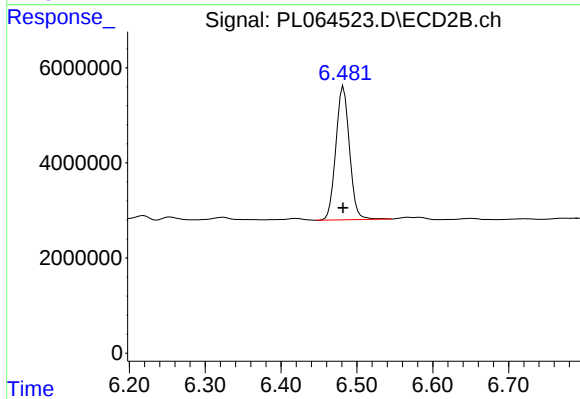

#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 35070502
Conc: 13.54 ng/ml

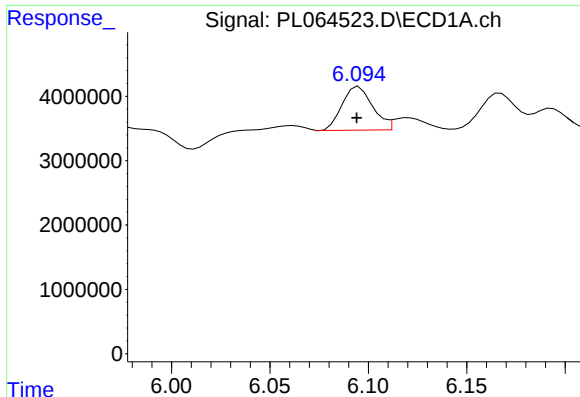


#16 4,4'-DDD

R.T.: 6.094 min
Delta R.T.: 0.000 min
Response: 7600413
Conc: 2.42 ng/ml m

Instrument :
ECD_L
ClientSampleId :
BS-SP


Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:42 PM

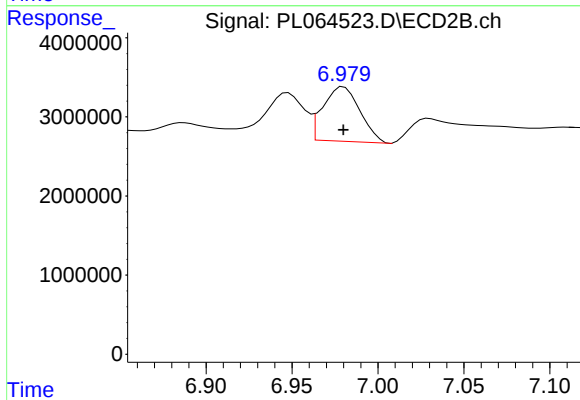


#16 4,4'-DDD

R.T.: 6.980 min
Delta R.T.: 0.000 min
Response: 10260465
Conc: 4.46 ng/ml

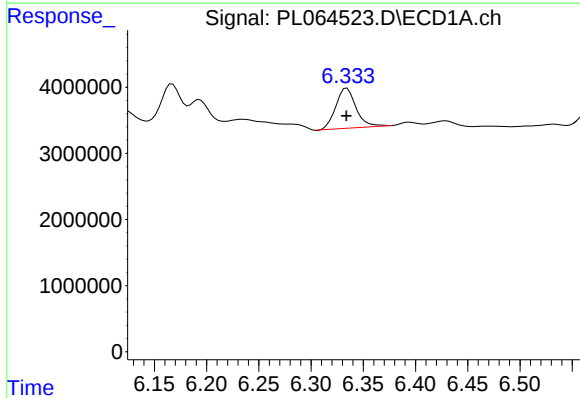


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 8121095
Conc: 2.65 ng/ml

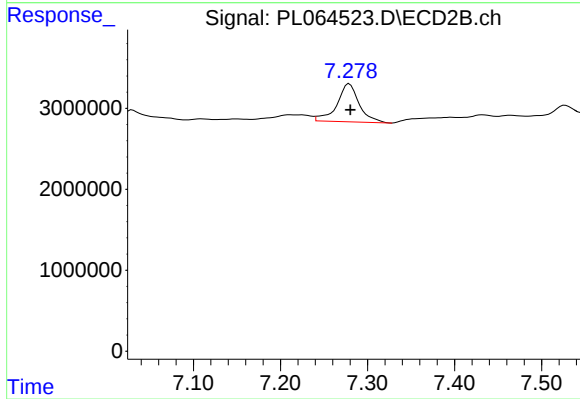

#17 4,4'-DDT

R.T.: 7.279 min
Delta R.T.: -0.001 min
Response: 8336676
Conc: 4.06 ng/ml

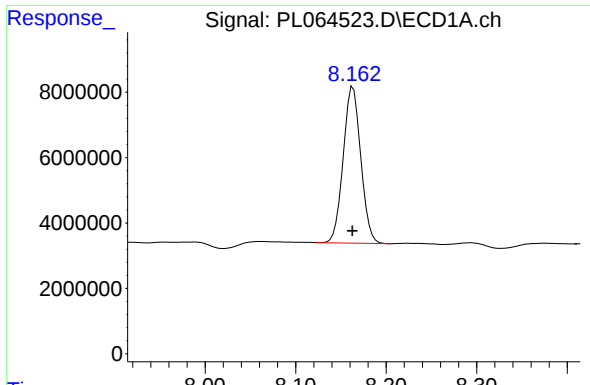


#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 64517326
Conc: 20.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
BS-SP

Manual Integrations
APPROVED

Sohil
2/1/2021 2:55:42 PM

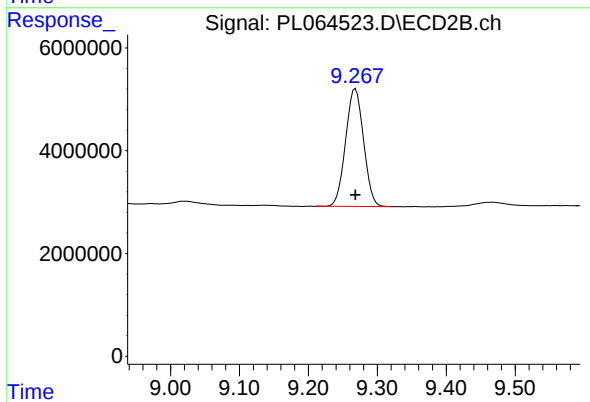

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 41521219
Conc: 20.28 ng/ml