

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064535.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 16:53
 Operator : AR\AJ
 Sample : M1254-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-15

Manual Integrations
 APPROVED

Ankita
 2/2/2021 1:22:05 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:28:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.430	4.107	34468213	27176194	11.323m	11.409
28) SA Decachlor...	8.149	9.267	123.7E6	22955479	39.260	11.212 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064535.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 16:53
Operator : AR\AJ
Sample : M1254-01
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT-15


Manual Integrations
APPROVED

Ankita
2/2/2021 1:22:05 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:28:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

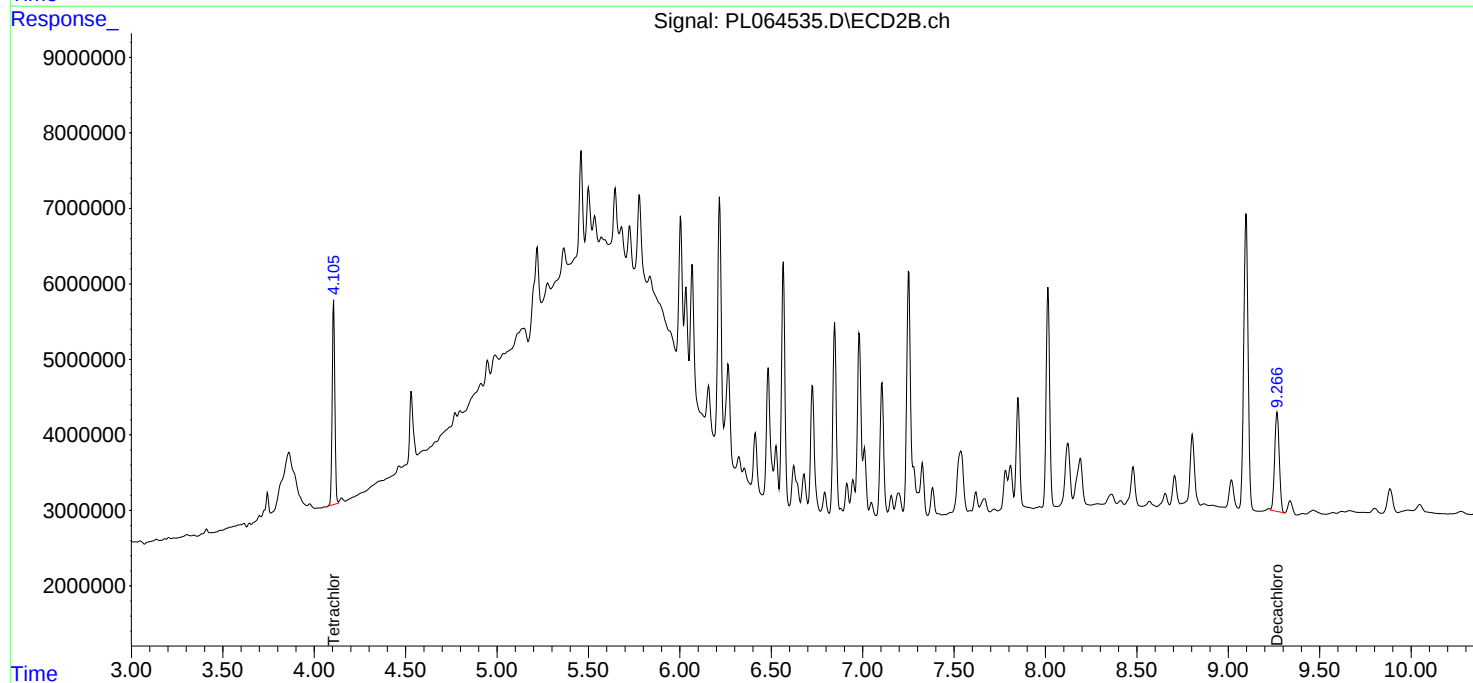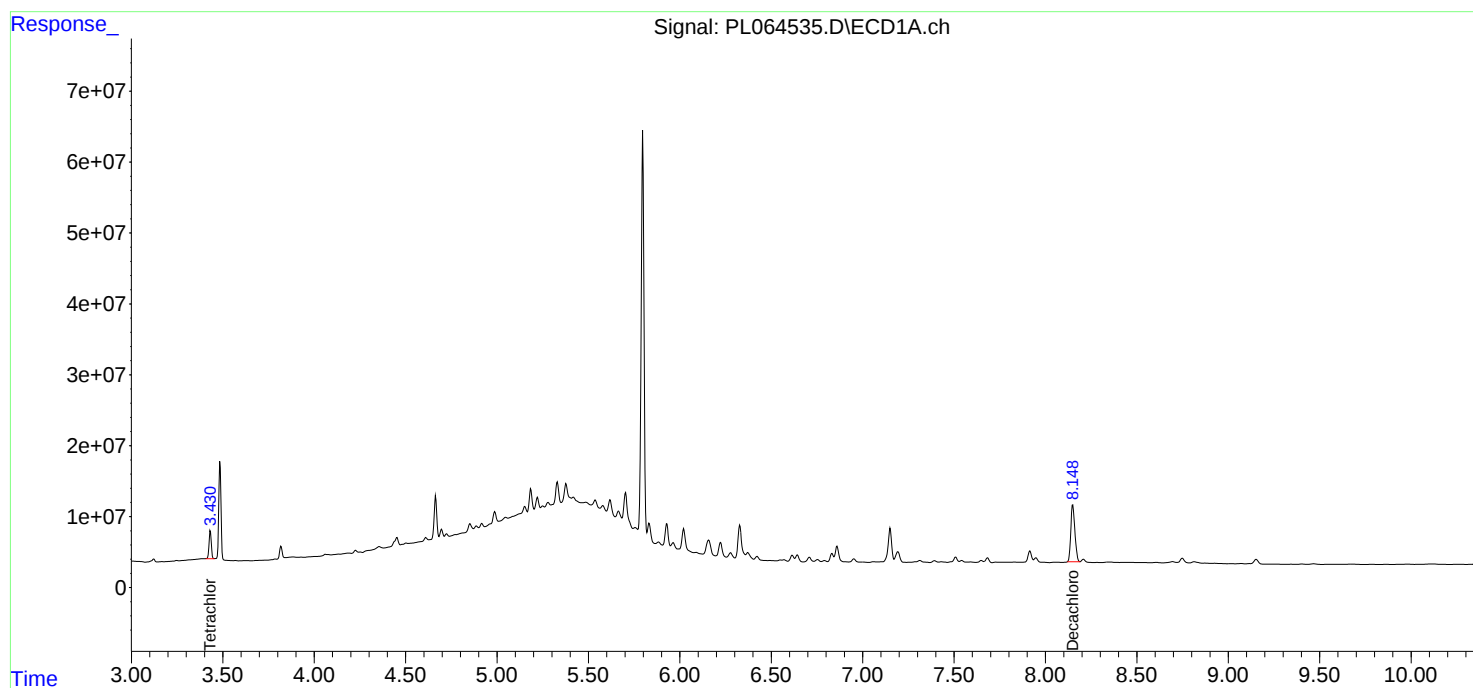

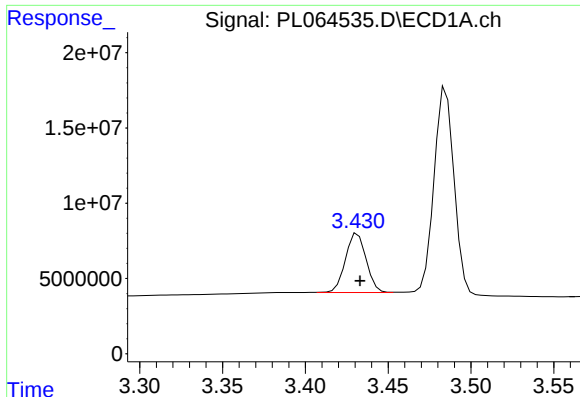


#1 Tetrachloro-m-xylene

R.T.: 3.430 min
Delta R.T.: -0.003 min
Response: 34468213
Conc: 11.32 ng/ml m

Instrument :
ECD_L
ClientSampleId :
CRT-15


Manual Integrations
APPROVED

Ankita
2/2/2021 1:22:05 PM

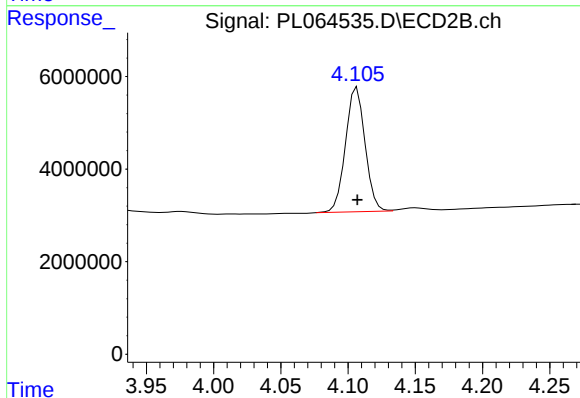


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 27176194
Conc: 11.41 ng/ml

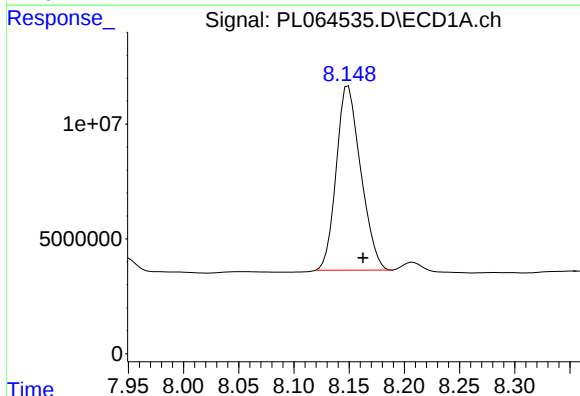

#28 Decachlorobiphenyl

R.T.: 8.149 min
Delta R.T.: -0.013 min
Response: 123721551
Conc: 39.26 ng/ml

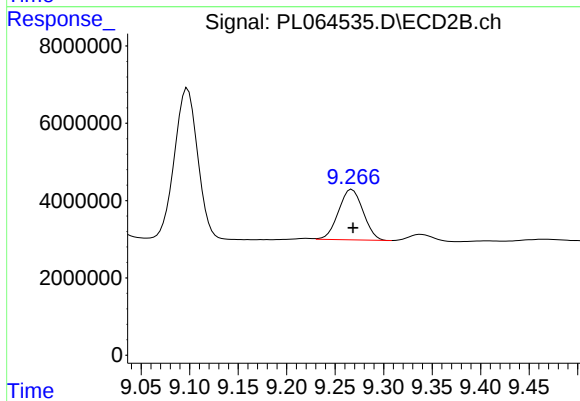

#28 Decachlorobiphenyl

R.T.: 9.267 min
Delta R.T.: -0.001 min
Response: 22955479
Conc: 11.21 ng/ml