

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 17:07
 Operator : AR\AJ
 Sample : M1254-06
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-5

Manual Integrations
 APPROVED

Ankita
 2/2/2021 1:22:07 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:28:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	46388132	30122789	15.238	12.646
28)	SA Decachlor...	8.162	9.268	48339269	33128522	15.339	16.181
Target Compounds							
12)	B 4,4'-DDE	5.579	6.482	7196385	4223792	1.909m	1.631m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 17:07
Operator : AR\AJ
Sample : M1254-06
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
CRT-5


Manual Integrations
APPROVED

Ankita
2/2/2021 1:22:07 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:28:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

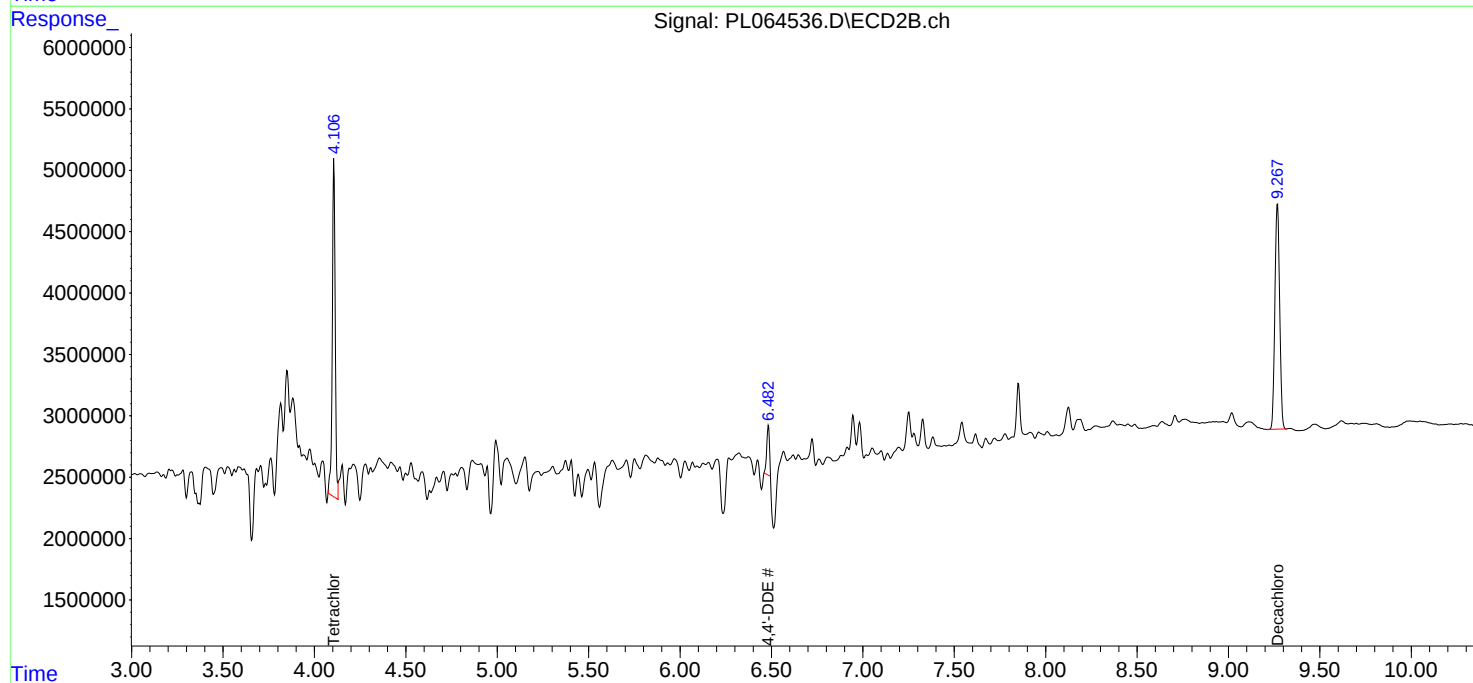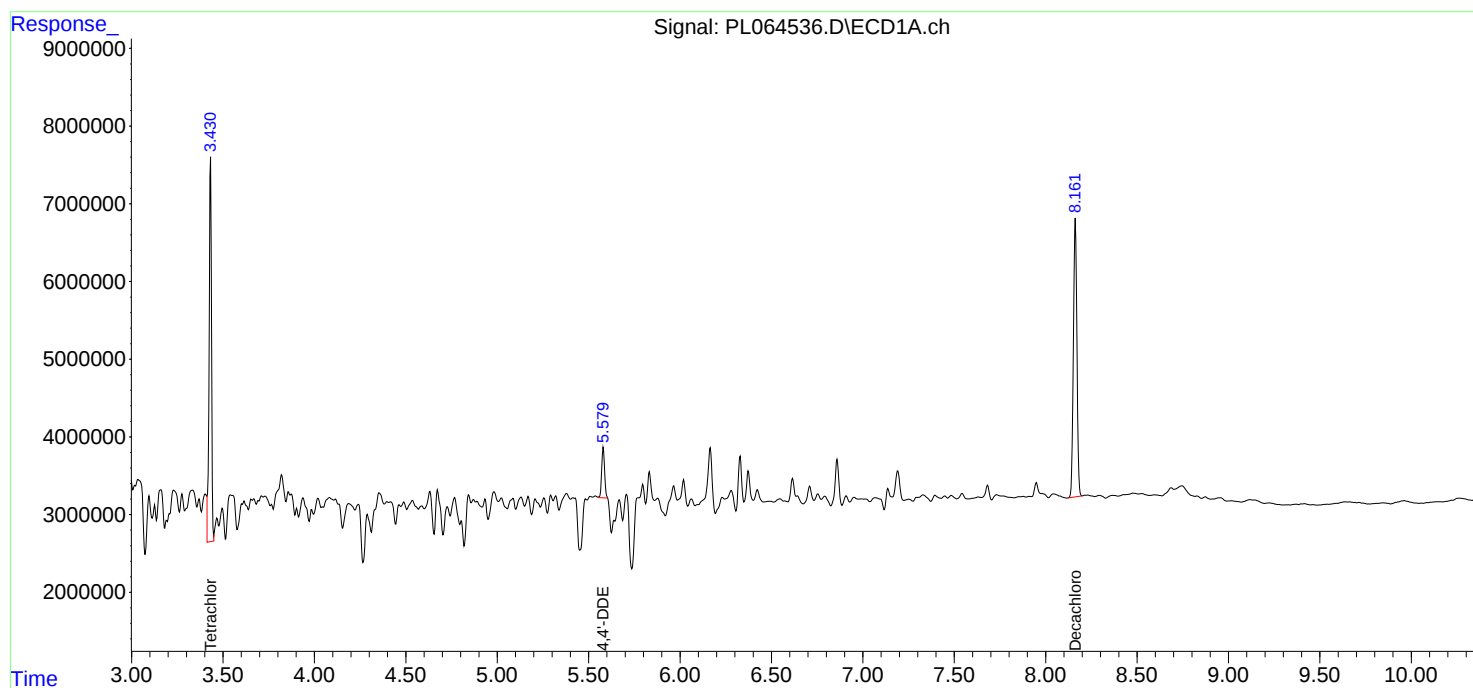

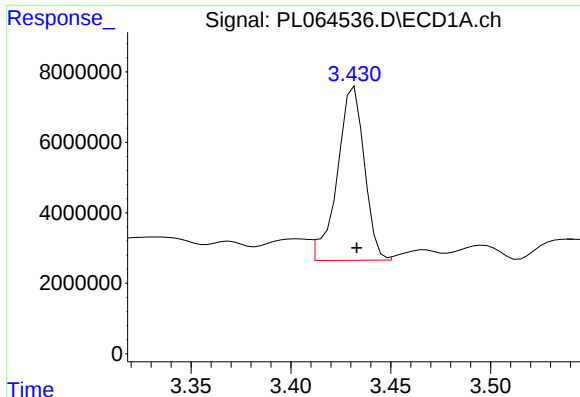


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: -0.001 min
Response: 46388132
Conc: 15.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-5


Manual Integrations
APPROVED

Ankita
2/2/2021 1:22:07 PM

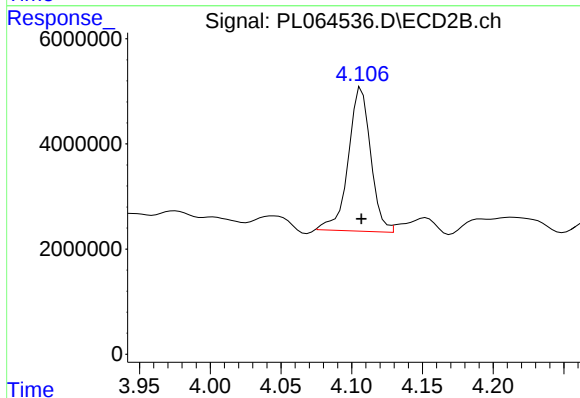


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 30122789
Conc: 12.65 ng/ml

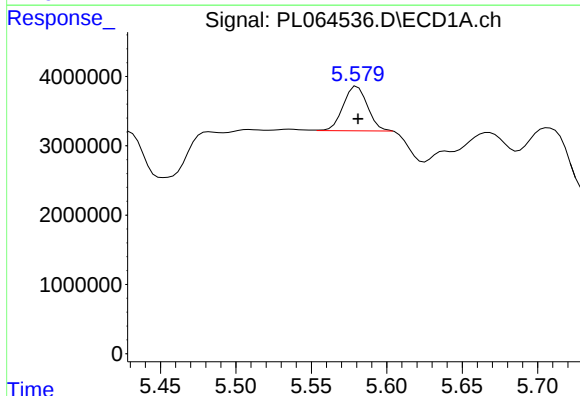


#12 4,4'-DDE

R.T.: 5.579 min
Delta R.T.: -0.002 min
Response: 7196385
Conc: 1.91 ng/ml m

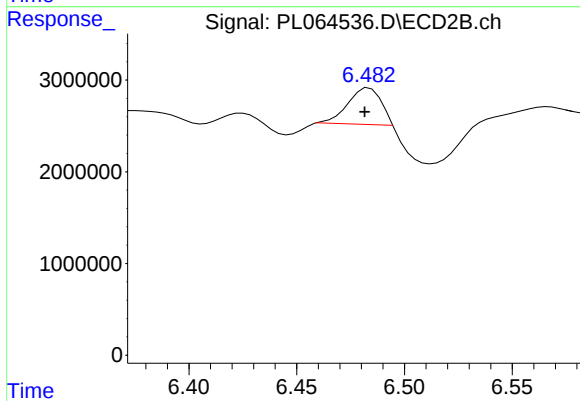

#12 4,4'-DDE

R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 4223792
Conc: 1.63 ng/ml m

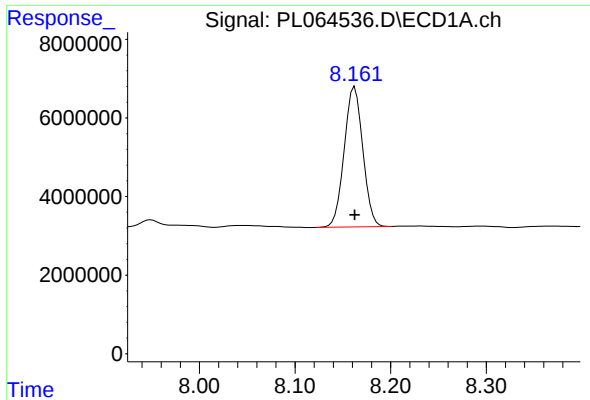


#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 48339269
Conc: 15.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-5

Manual Integrations
APPROVED

Ankita
2/2/2021 1:22:07 PM

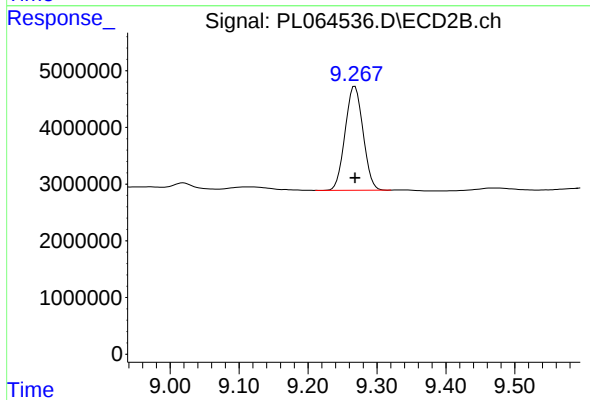

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 33128522
Conc: 16.18 ng/ml