

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
 Data File : PL064537.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 29 Jan 2021 17:21
 Operator : AR\AJ
 Sample : M1255-01
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CRT-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 03:28:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.106	35126743	26527151	11.539	11.136
28)	SA Decachlor...	8.163	9.268	37337313	23956972	11.848	11.701
Target Compounds							
12)	B 4,4'-DDE	5.580	6.482	7902890	6207697	2.097	2.397
17)	MA 4,4'-DDT	6.332	7.280	7557259	2630888	2.462	1.281 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013021\
Data File : PL064537.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 29 Jan 2021 17:21
Operator : AR\AJ
Sample : M1255-01
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CRT-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 03:28:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

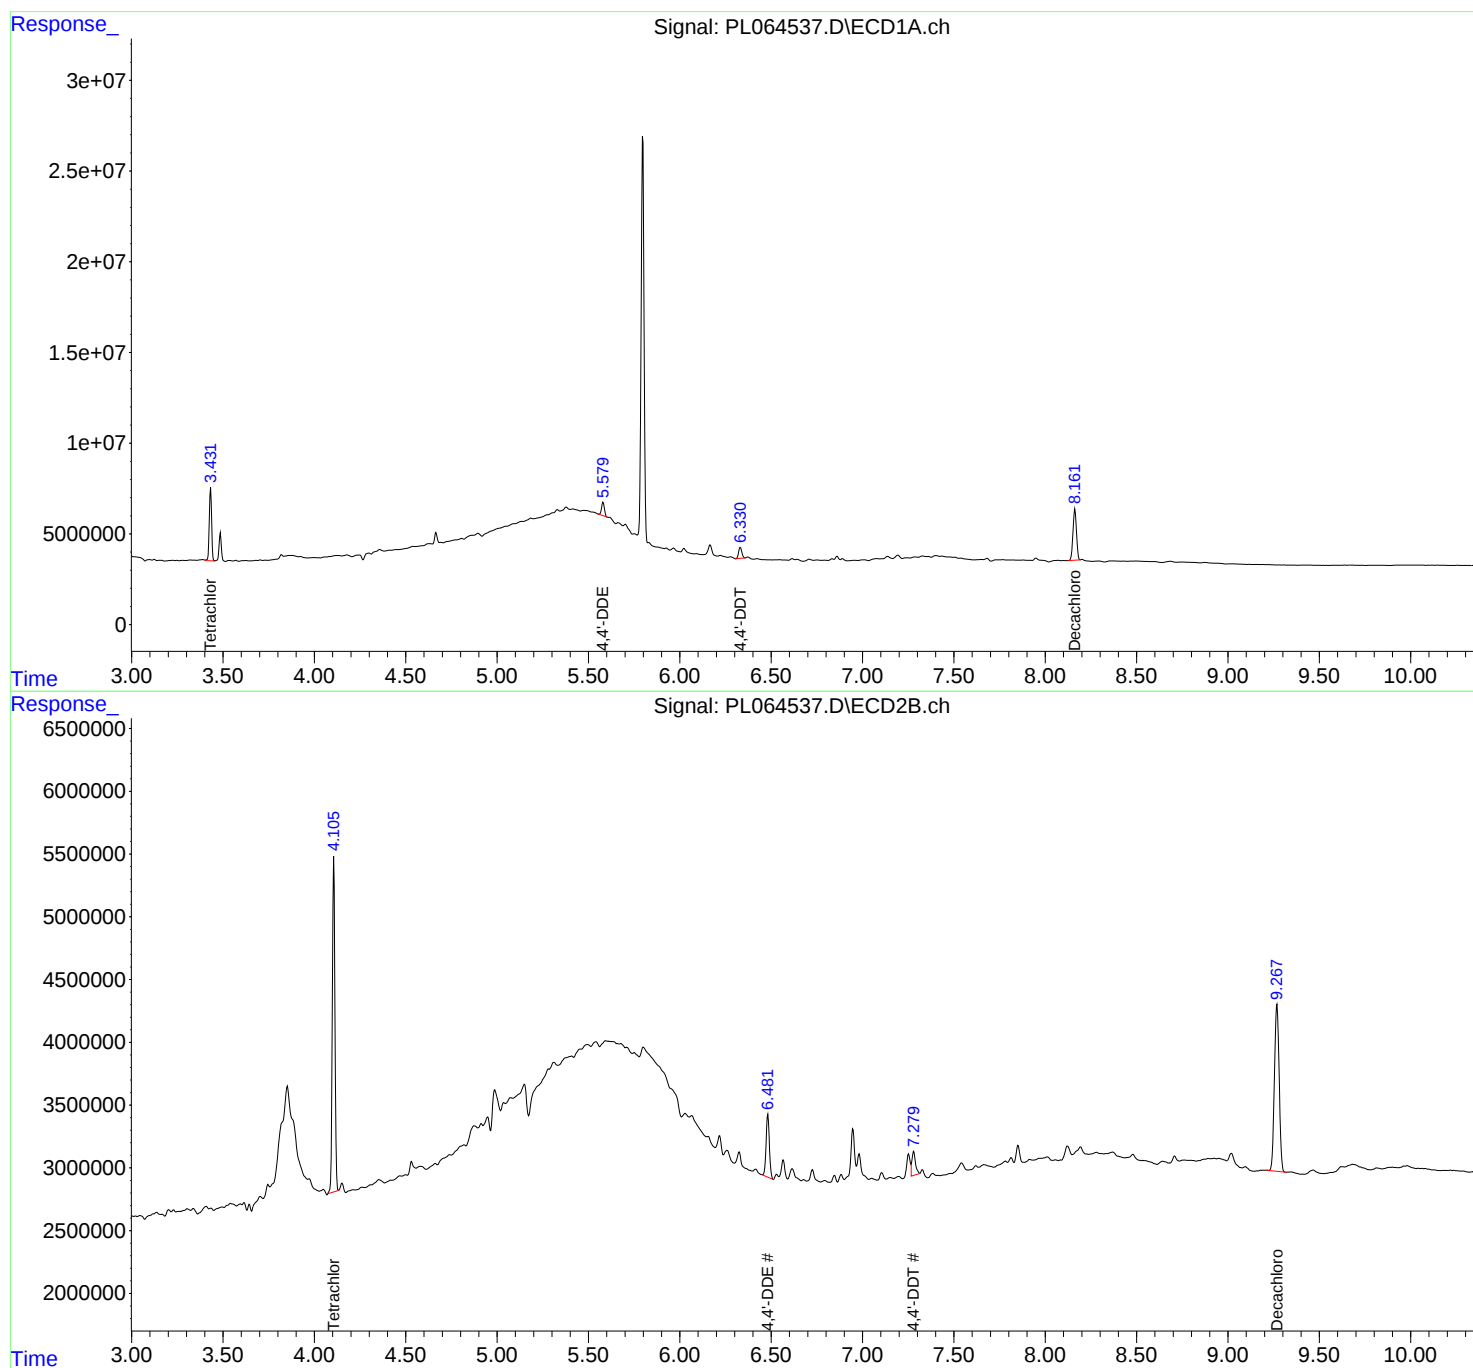


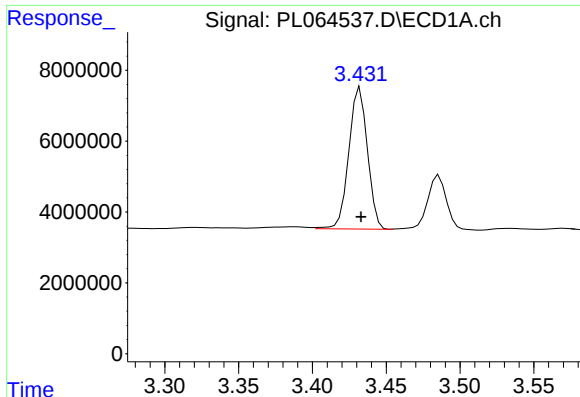

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 35126743
Conc: 11.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-3

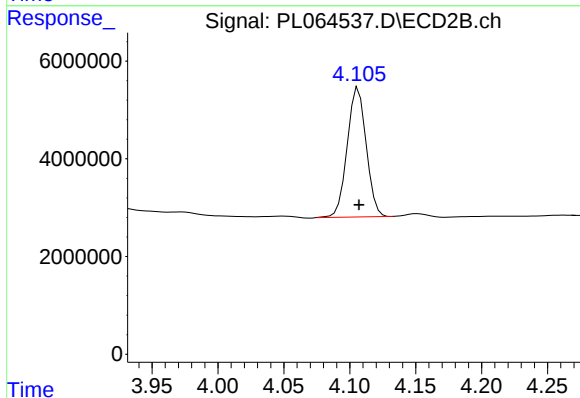


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.000 min
Response: 26527151
Conc: 11.14 ng/ml

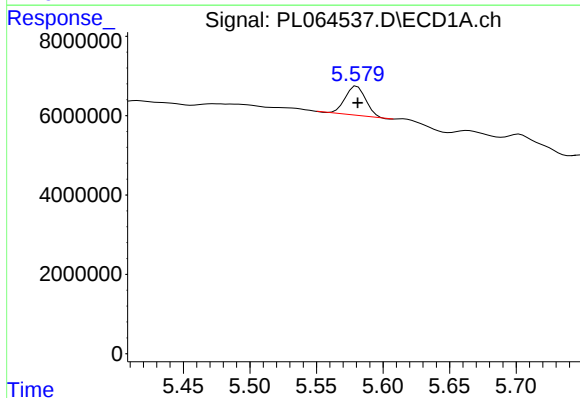


#12 4,4'-DDE

R.T.: 5.580 min
Delta R.T.: 0.000 min
Response: 7902890
Conc: 2.10 ng/ml

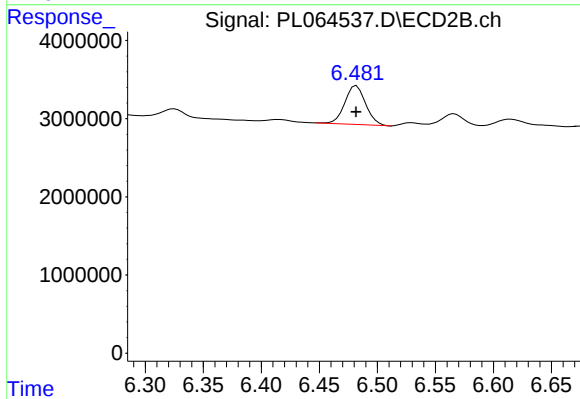

#12 4,4'-DDE


R.T.: 6.482 min
Delta R.T.: 0.000 min
Response: 6207697
Conc: 2.40 ng/ml

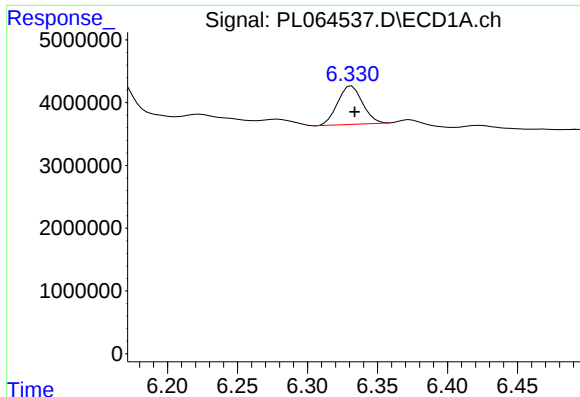

#17 4,4'-DDT


R.T.: 6.332 min
Delta R.T.: -0.002 min
Response: 7557259
Conc: 2.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
CRT-3

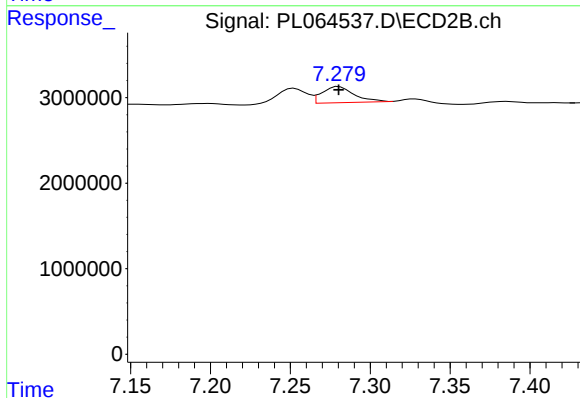


#17 4,4'-DDT

R.T.: 7.280 min
Delta R.T.: 0.000 min
Response: 2630888
Conc: 1.28 ng/ml

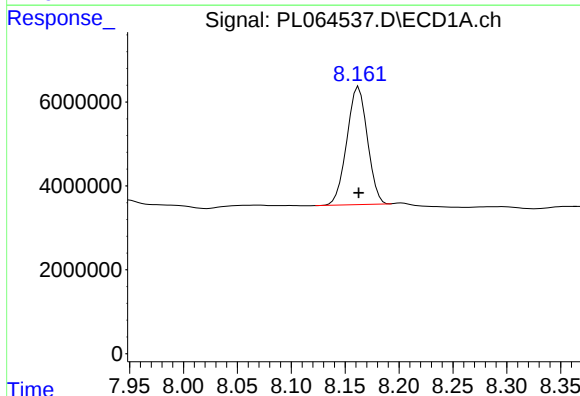

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 37337313
Conc: 11.85 ng/ml

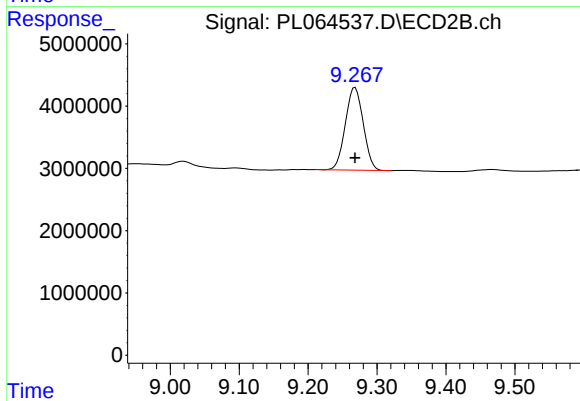

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.000 min
Response: 23956972
Conc: 11.70 ng/ml