

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013024\
 Data File : PL088037.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2024 11:08
 Operator : AR\AJ
 Sample : P1234-01DL 100X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 293DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/31/2024
 Supervised By :Ankita Jodhani 01/31/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 30 21:14:37 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 29 12:34:13 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
10) B	gamma-Chl...	5.831	4.887	117.8E6	46196029	31.829m 29.928
11) B	alpha-Chl...	5.913	4.952	140.6E6	53334199	38.358m 34.224

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013024\
Data File : PL088037.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2024 11:08
Operator : AR\AJ
Sample : P1234-01DL 100X
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
293DL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/31/2024
Supervised By : Ankita Jodhani 01/31/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 30 21:14:37 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012724.M
Quant Title : GC Extractables
QLast Update : Mon Jan 29 12:34:13 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

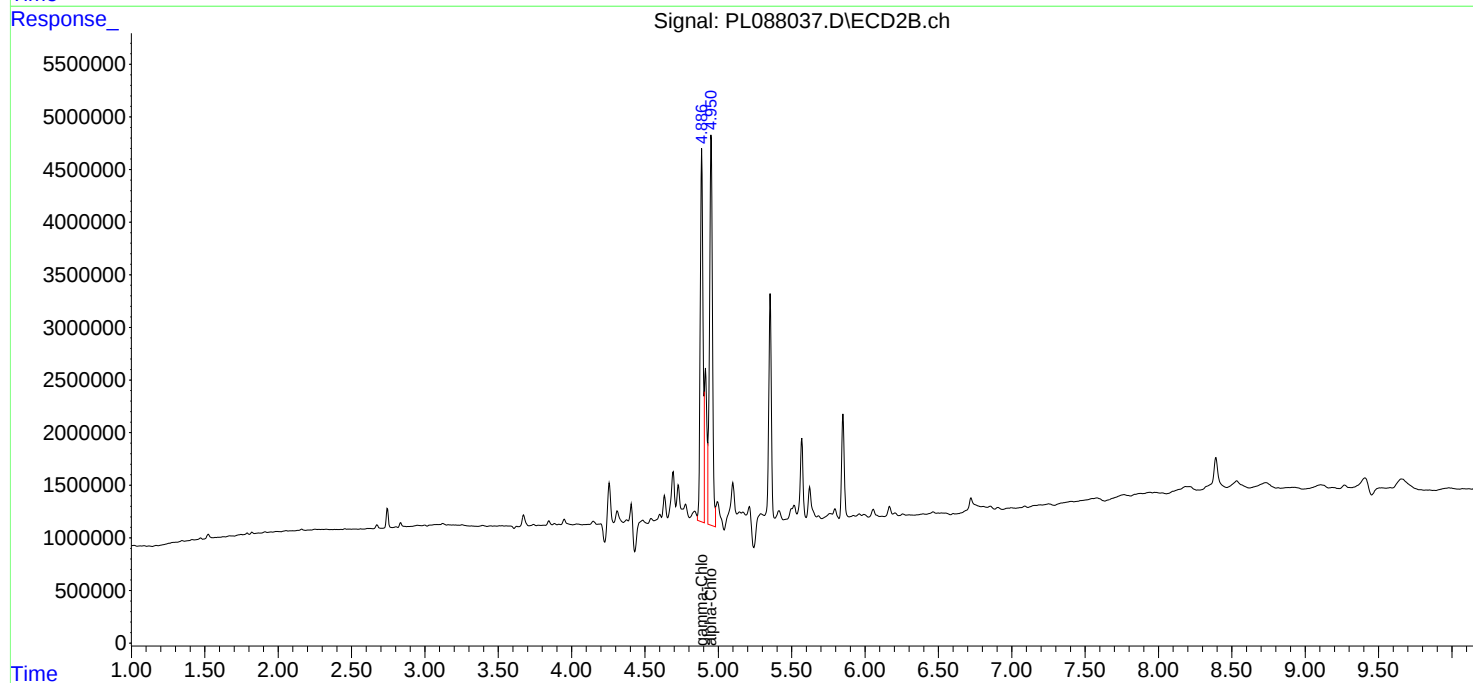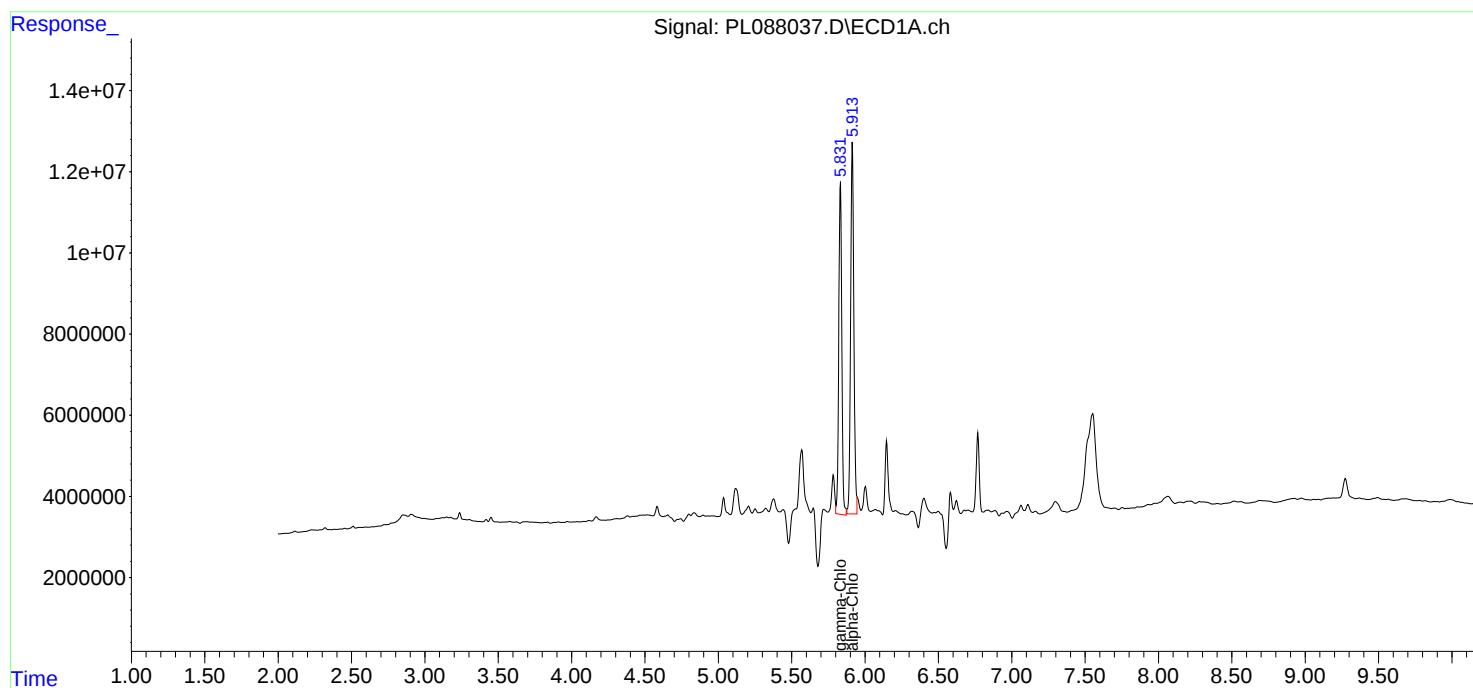

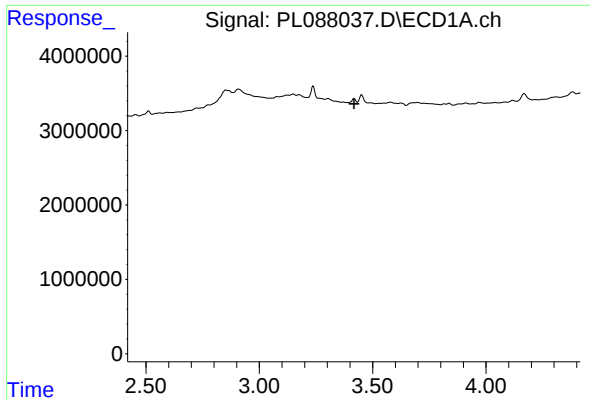


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 3.418 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
293DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2024
Supervised By :Ankita Jodhani 01/31/2024

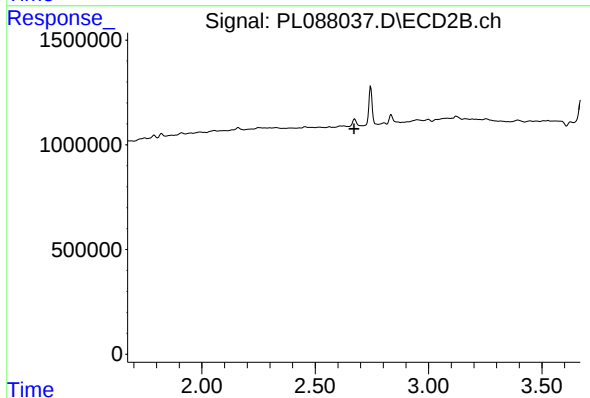


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 2.671 min
Response: 0
Conc: N.D.

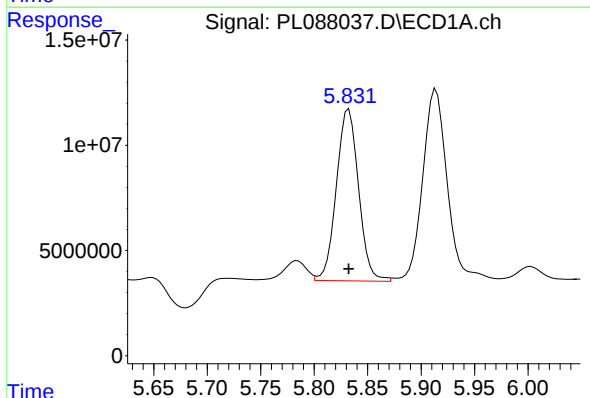


#10 gamma-Chlordane

R.T.: 5.831 min
Delta R.T.: -0.001 min
Response: 117839187
Conc: 31.83 ng/ml m

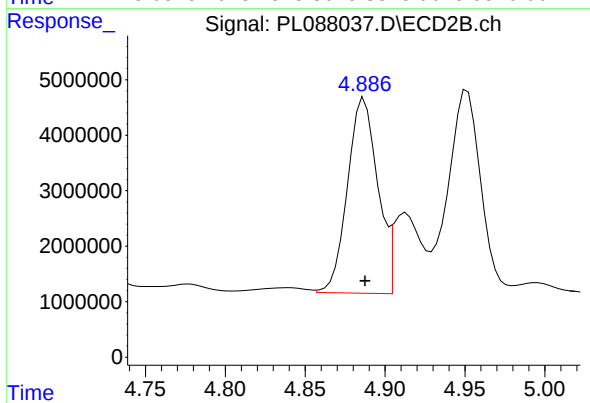

#10 gamma-Chlordane

R.T.: 4.887 min
Delta R.T.: 0.000 min
Response: 46196029
Conc: 29.93 ng/ml

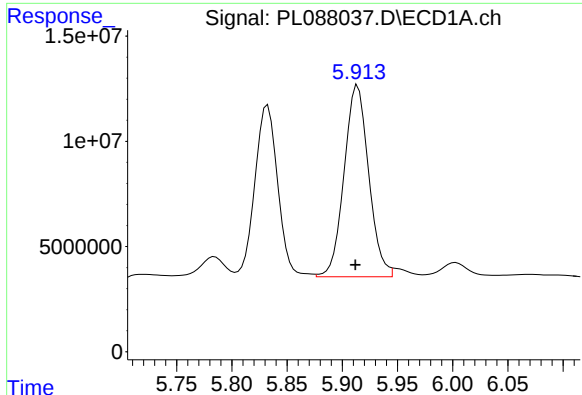


#11 alpha-Chlordane

R.T.: 5.913 min
Delta R.T.: 0.000 min
Response: 140645117
Conc: 38.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
293DL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2024
Supervised By :Ankita Jodhani 01/31/2024

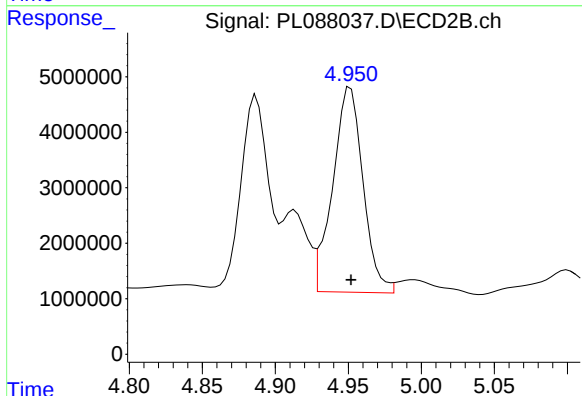


#11 alpha-Chlordane

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 53334199
Conc: 34.22 ng/ml

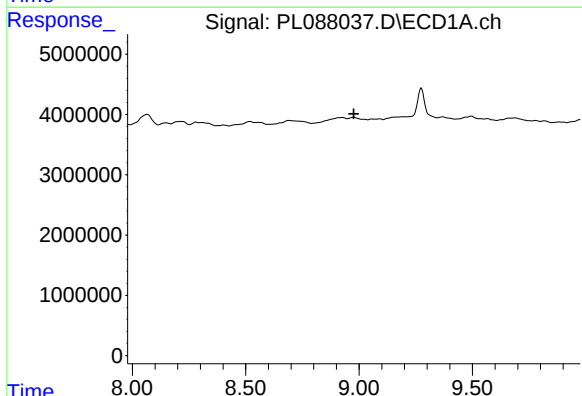

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.977 min
Response: 0
Conc: N.D.

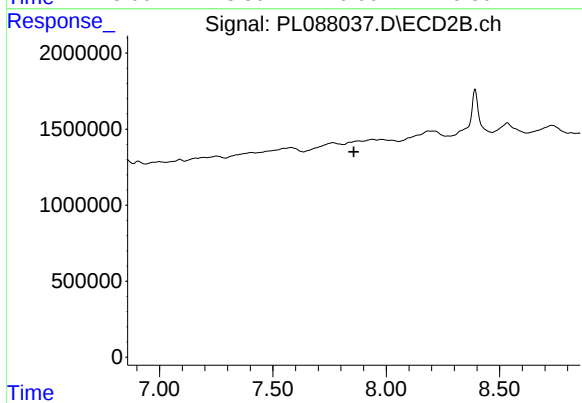

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 7.857 min
Response: 0
Conc: N.D.