

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013025\
 Data File : PL093924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 30 Jan 2025 23:30
 Operator : AR\AJ
 Sample : Q1219-01 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LAW-25-0015

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/31/2025
 Supervised By : Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 01:44:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.536	2.773	3128542	6413990	1.162m	1.965m#
28) SA Decachlor...	9.054	7.911	18009921	3486620	8.609m	0.995m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013025\
Data File : PL093924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 30 Jan 2025 23:30
Operator : AR\AJ
Sample : Q1219-01 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LAW-25-0015


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 01:44:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

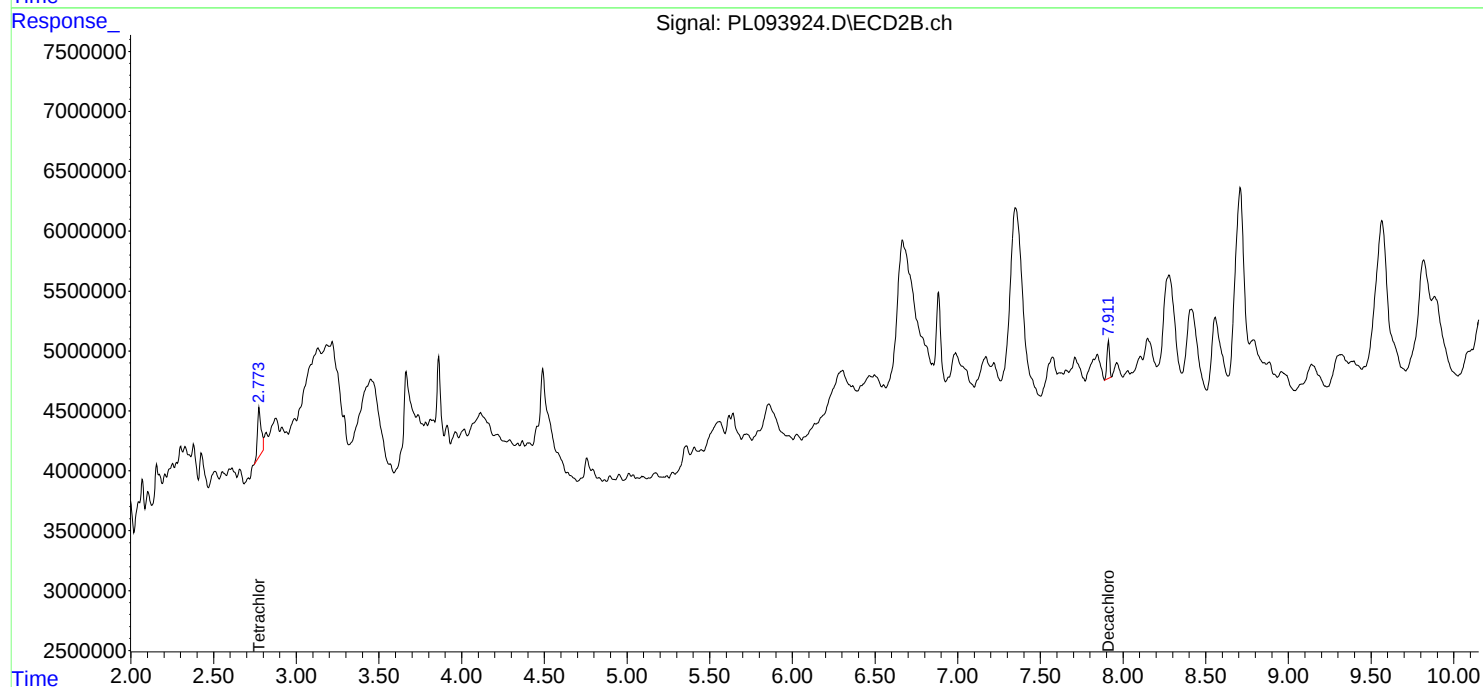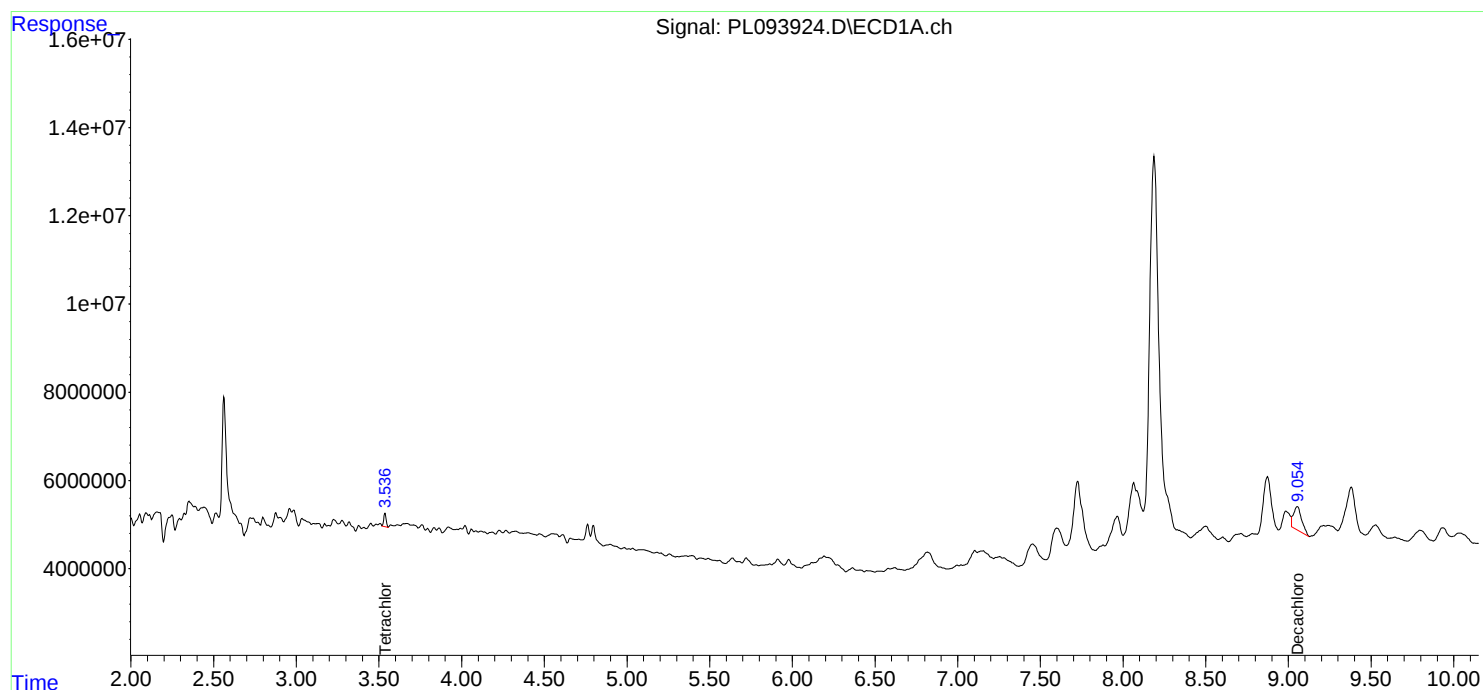

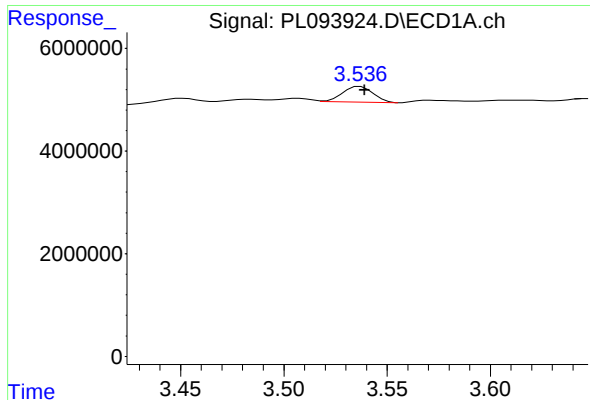


#1 Tetrachloro-m-xylene

R.T.: 3.536 min
Delta R.T.: -0.003 min
Response: 3128542
Conc: 1.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0015


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/31/2025
Supervised By :Ankita Jodhani 01/31/2025

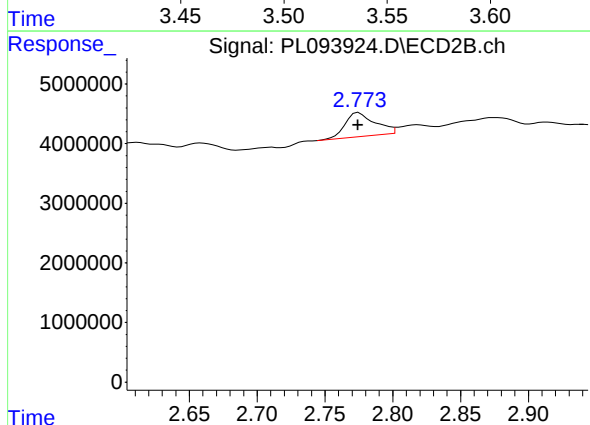


#1 Tetrachloro-m-xylene

R.T.: 2.773 min
Delta R.T.: 0.000 min
Response: 6413990
Conc: 1.96 ng/ml

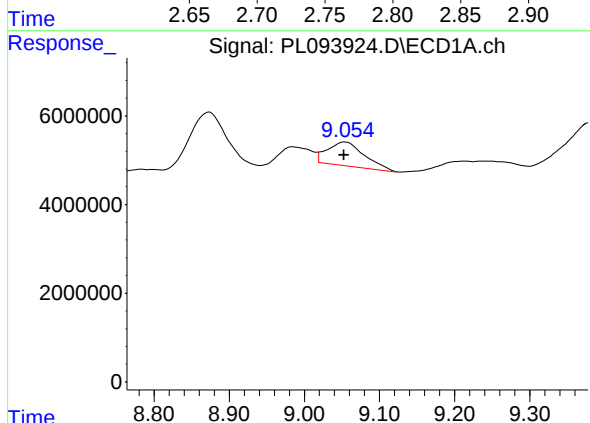

#28 Decachlorobiphenyl

R.T.: 9.054 min
Delta R.T.: 0.001 min
Response: 18009921
Conc: 8.61 ng/ml

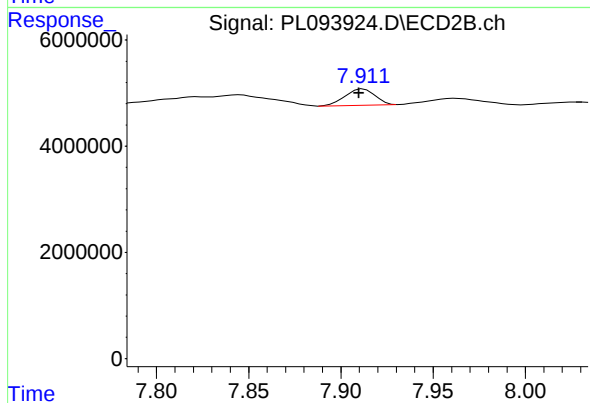

#28 Decachlorobiphenyl

R.T.: 7.911 min
Delta R.T.: 0.000 min
Response: 3486620
Conc: 1.00 ng/ml