

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL013120\  
 Data File : PL056236.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 31 Jan 2020 14:29  
 Operator : AJ\MA  
 Sample : L1325-03  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :  
 200029

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Jan 31 22:11:10 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL012820.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jan 28 13:10:37 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|--------|
| -----                       |                 |        |       |          |          |        |        |
| System Monitoring Compounds |                 |        |       |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.497  | 4.014 | 121.7E6  | 36782421 | 11.620 | 12.579 |
| 28)                         | SA Decachlor... | 8.250  | 9.087 | 109.7E6  | 25514857 | 10.417 | 11.280 |
| Target Compounds            |                 |        |       |          |          |        |        |
| 10)                         | B gamma-Chl...  | 5.461f | 0.000 | 9698626  | 0        | 0.618  | N.D. # |
| 12)                         | B 4,4'-DDE      | 5.660  | 0.000 | 17011290 | 0        | 1.174  | N.D. # |
| 17)                         | MA 4,4'-DDT     | 6.415  | 0.000 | 10872219 | 0        | 0.995  | N.D. # |
| 25)                         | Chlordane-3     | 5.461f | 0.000 | 9698626  | 0        | 7.682  | N.D. # |
| -----                       |                 |        |       |          |          |        |        |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL013120\  
Data File : PL056236.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 31 Jan 2020 14:29  
Operator : AJ\MA  
Sample : L1325-03  
Misc :  
ALS Vial : 11 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :  
200029

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Jan 31 22:11:10 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL012820.M  
Quant Title : GC Extractables  
QLast Update : Tue Jan 28 13:10:37 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

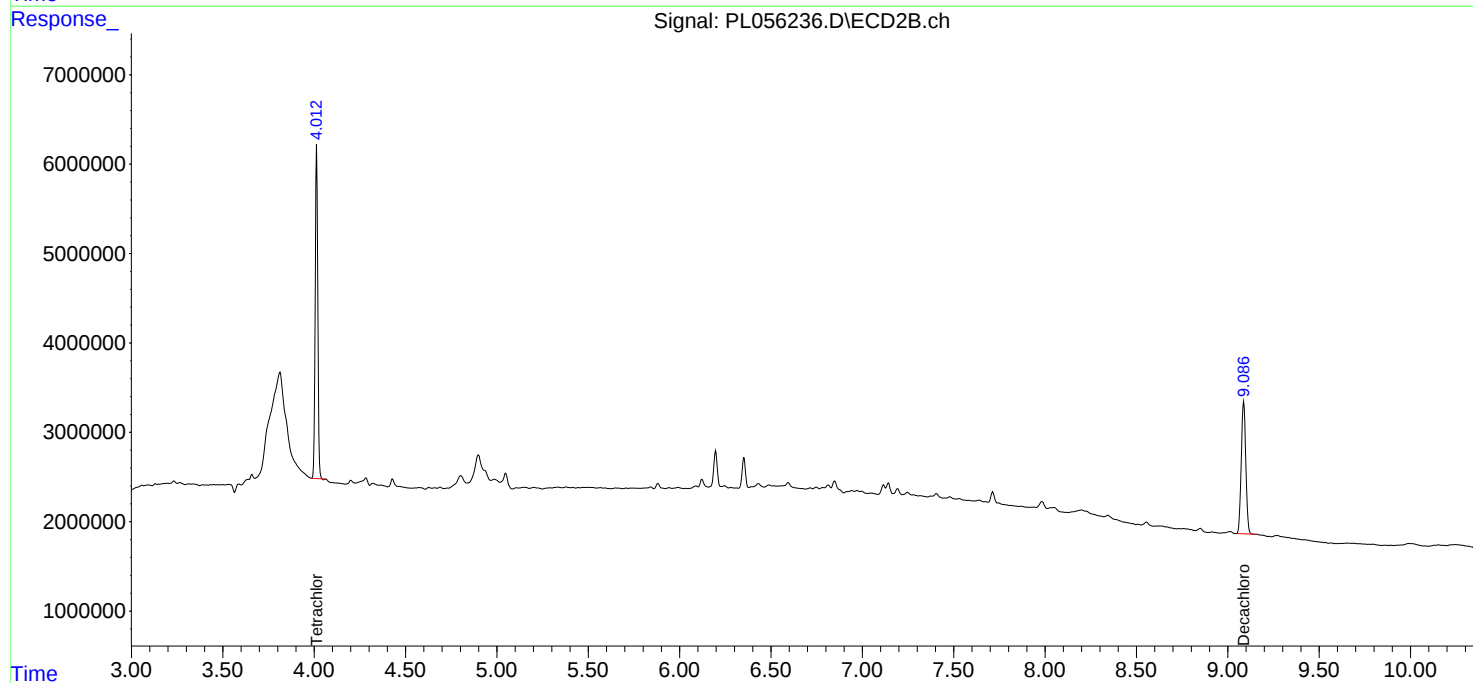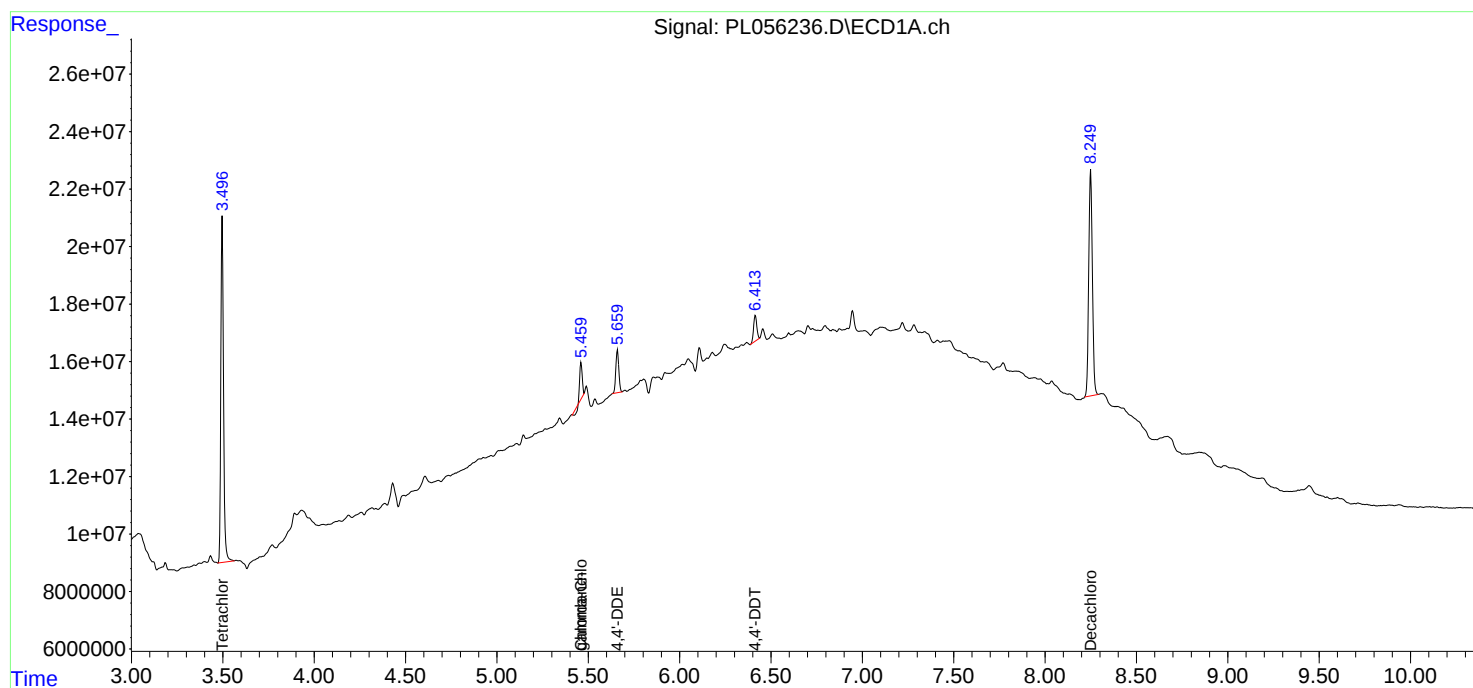


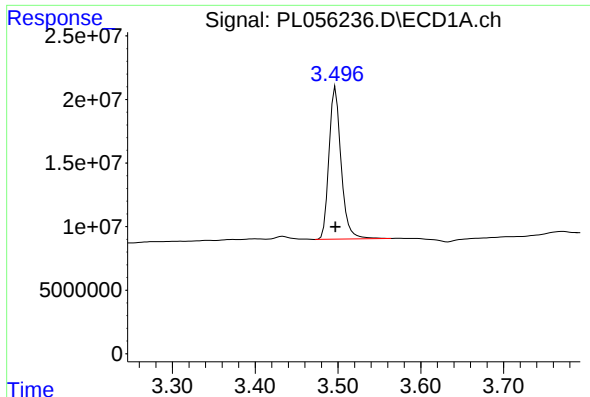

#1 Tetrachloro-m-xylene


R.T.: 3.497 min  
Delta R.T.: 0.000 min  
Response: 121691192  
Conc: 11.62 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
200029

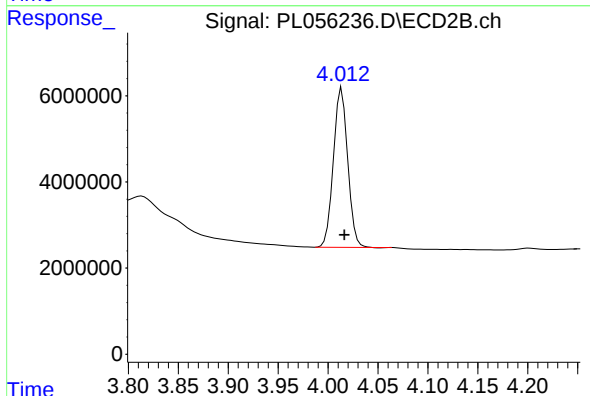


#1 Tetrachloro-m-xylene

R.T.: 4.014 min  
Delta R.T.: -0.003 min  
Response: 36782421  
Conc: 12.58 ng/ml

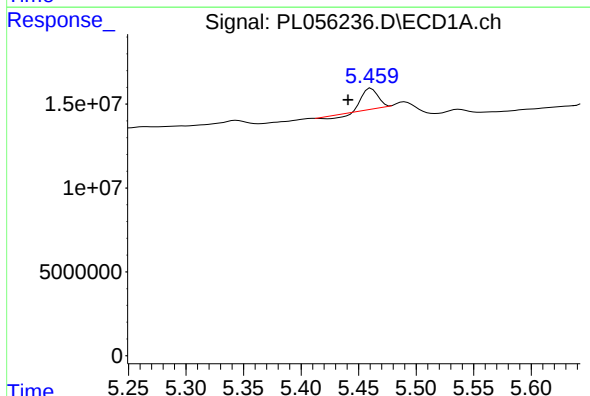


#10 gamma-Chlordane

R.T.: 5.461 min  
Delta R.T.: 0.020 min  
Response: 9698626  
Conc: 0.62 ng/ml

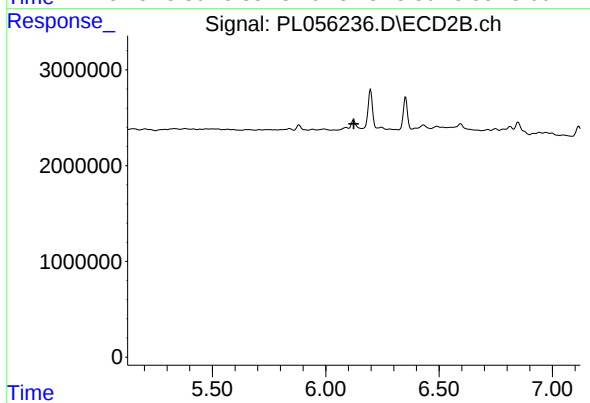

#10 gamma-Chlordane


R.T.: 0.000 min  
Exp R.T.: 6.124 min  
Response: 0  
Conc: N.D.

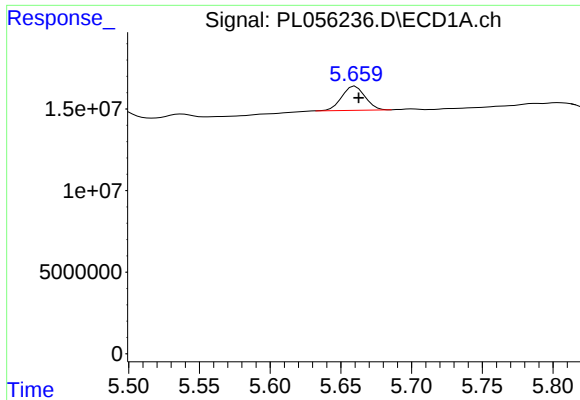

#12 4,4'-DDE


R.T.: 5.660 min  
Delta R.T.: -0.003 min  
Response: 17011290  
Conc: 1.17 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
200029

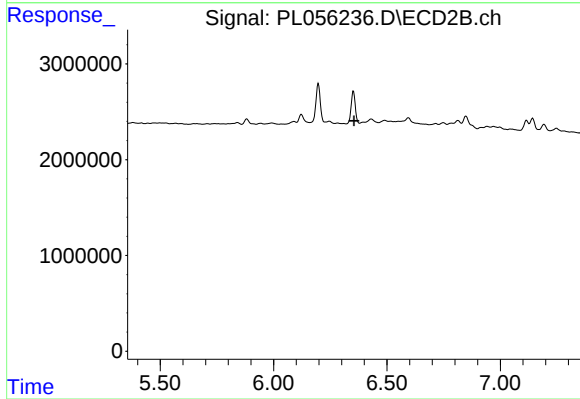


#12 4,4'-DDE

R.T.: 0.000 min  
Exp R.T. : 6.355 min  
Response: 0  
Conc: N.D.

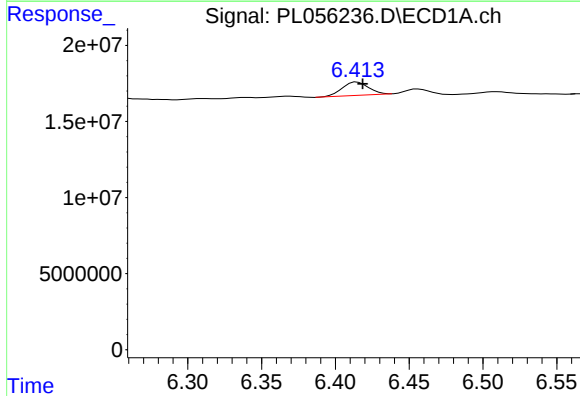


#17 4,4'-DDT

R.T.: 6.415 min  
Delta R.T.: -0.004 min  
Response: 10872219  
Conc: 0.99 ng/ml

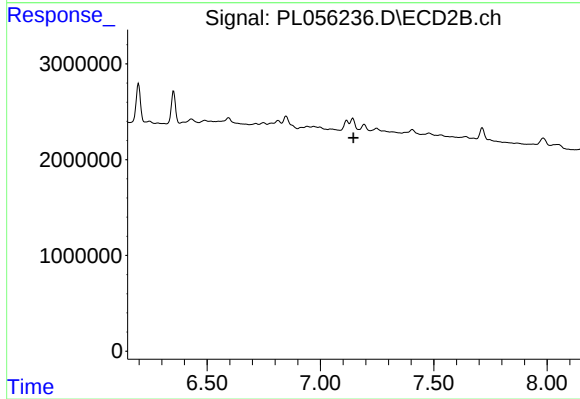

#17 4,4'-DDT


R.T.: 0.000 min  
Exp R.T. : 7.146 min  
Response: 0  
Conc: N.D.

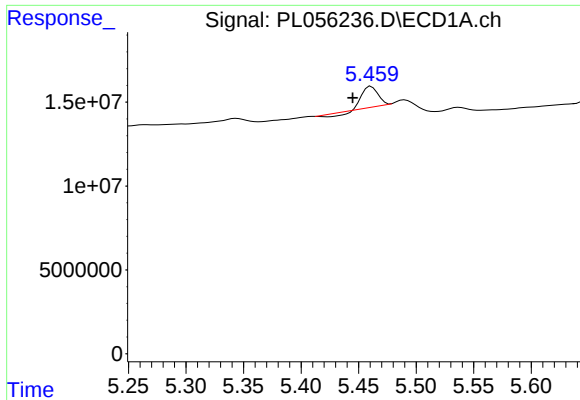

#25 Chlordane-3


R.T.: 5.461 min  
Delta R.T.: 0.016 min  
Response: 9698626  
Conc: 7.68 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :  
200029

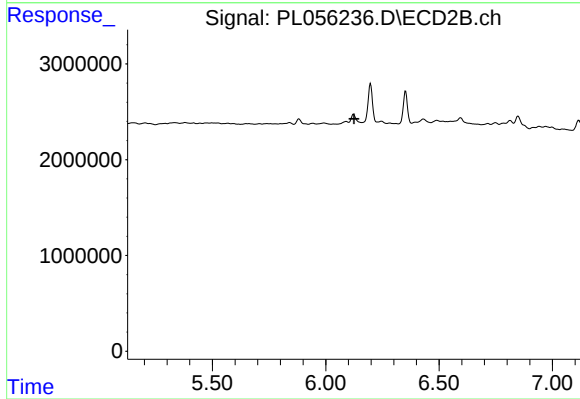


#25 Chlordane-3

R.T.: 0.000 min  
Exp R.T.: 6.125 min  
Response: 0  
Conc: N.D.

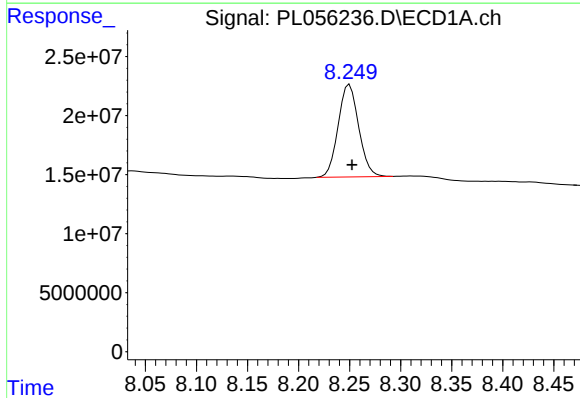

#28 Decachlorobiphenyl

R.T.: 8.250 min  
Delta R.T.: -0.002 min  
Response: 109671624  
Conc: 10.42 ng/ml

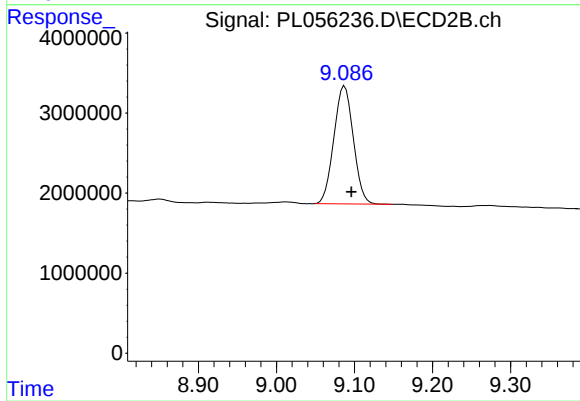

#28 Decachlorobiphenyl

R.T.: 9.087 min  
Delta R.T.: -0.009 min  
Response: 25514857  
Conc: 11.28 ng/ml