

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
 Data File : PL056245.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 16:35
 Operator : AJ\MA
 Sample : L1325-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 346

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 22:13:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.014	222.8E6	65653454	21.272	22.453
28)	SA Decachlor...	8.249	9.087	205.1E6	46489917	19.484	20.553
Target Compounds							
10)	B gamma-Chl...	5.439	6.121	37877970	11994174	2.415	3.772 #
11)	B alpha-Chl...	5.496	6.195	41001373	14643200	2.665	4.620 #
17)	MA 4,4'-DDT	6.413	0.000	8314398	0	0.761	N.D. #
23)	Chlordane-1	4.370	0.000	8238740	0	21.764	N.D. #
24)	Chlordane-2	4.870	0.000	15433951	0	35.229	N.D. #
25)	Chlordane-3	5.439	6.121	37877970	11994174	30.001	31.913
26)	Chlordane-4	5.496	6.195	41001373	14643200	37.893	33.329


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
Data File : PL056245.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 16:35
Operator : AJ\MA
Sample : L1325-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
346

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 22:13:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

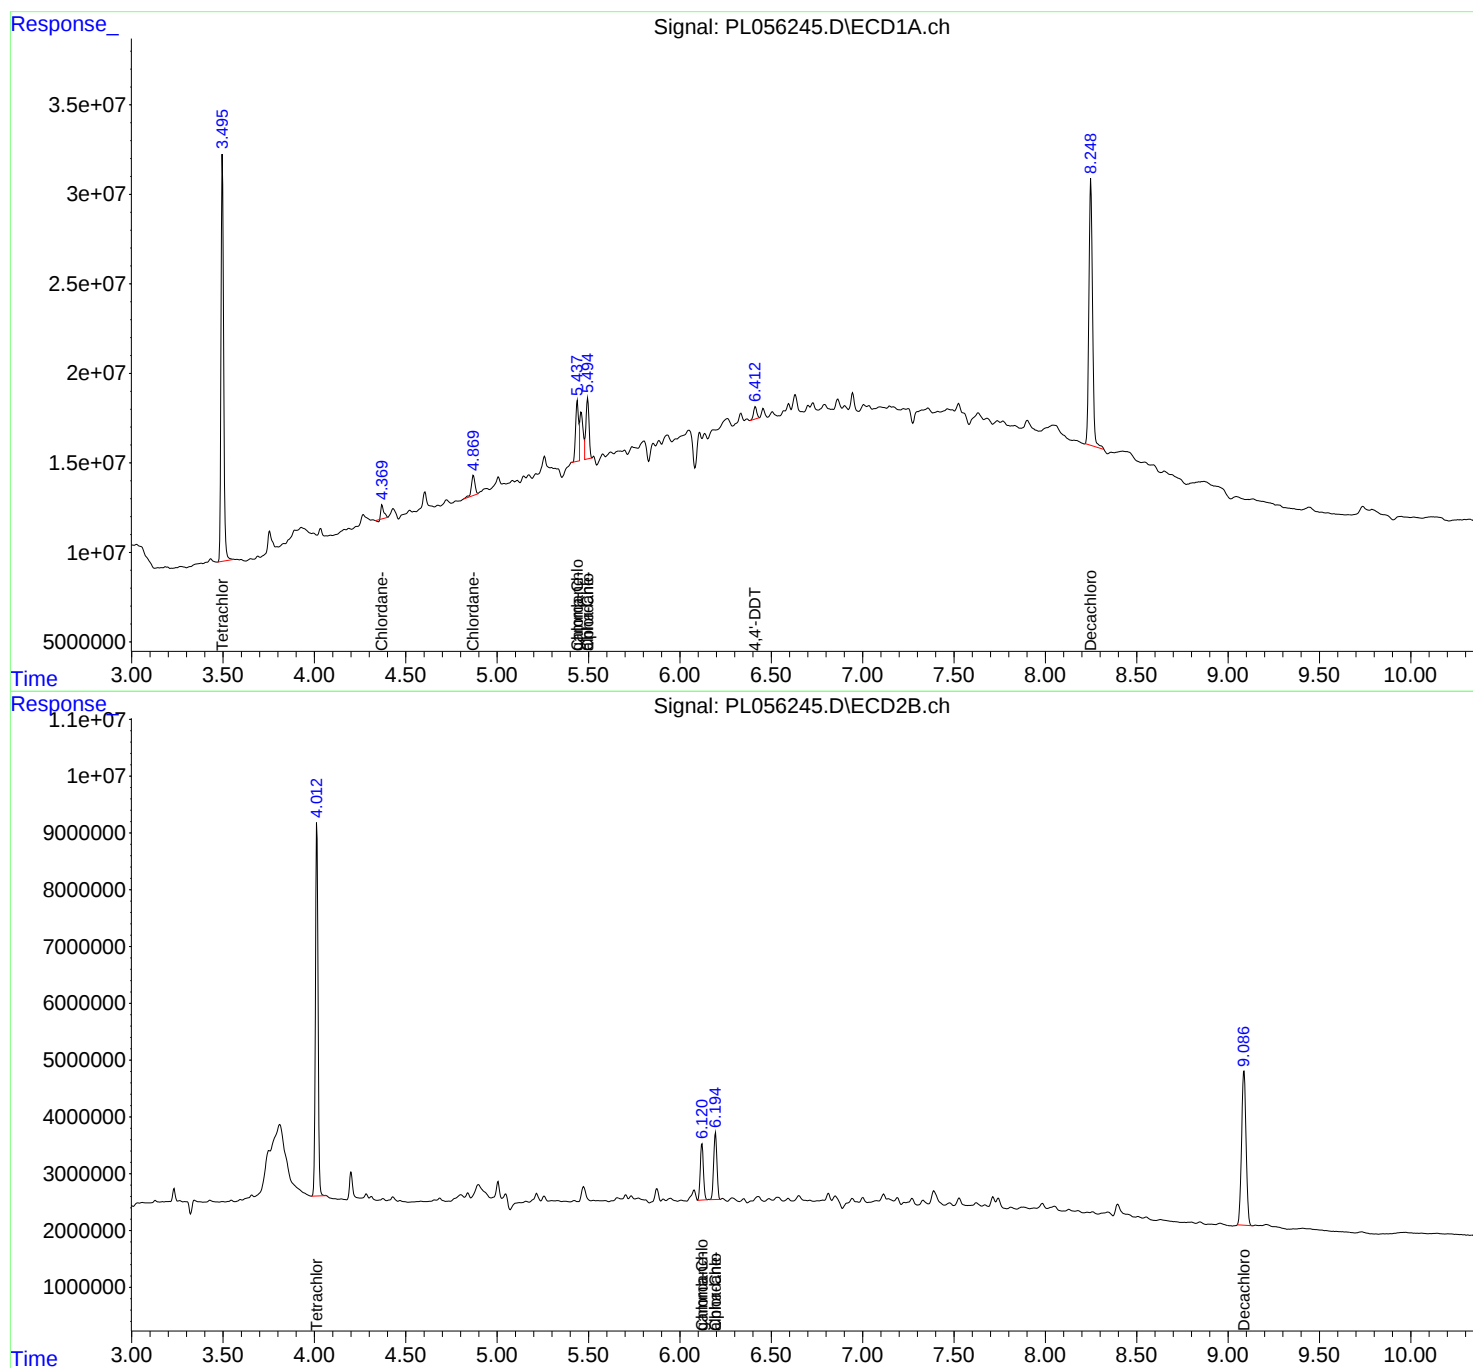


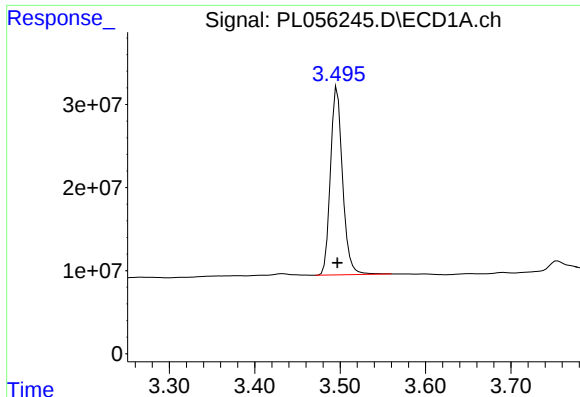

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 222779410
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
346

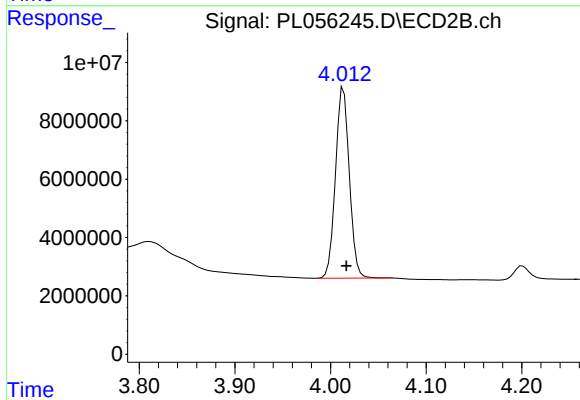


#1 Tetrachloro-m-xylene

R.T.: 4.014 min
Delta R.T.: -0.003 min
Response: 65653454
Conc: 22.45 ng/ml

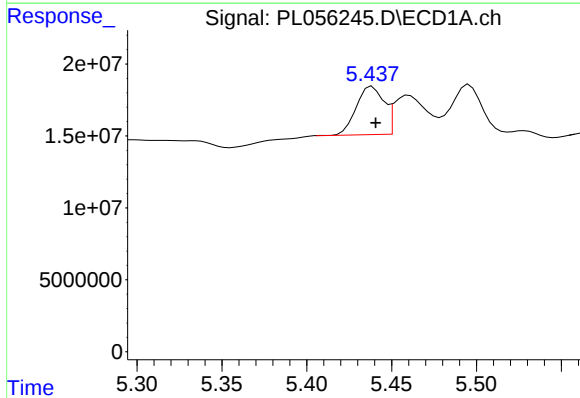


#10 gamma-Chlordane

R.T.: 5.439 min
Delta R.T.: -0.002 min
Response: 37877970
Conc: 2.42 ng/ml

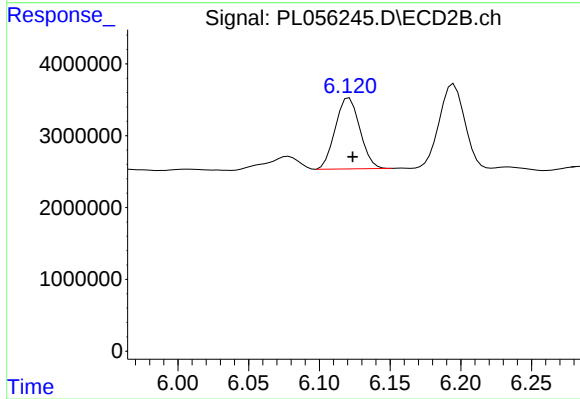

#10 gamma-Chlordane


R.T.: 6.121 min
Delta R.T.: -0.002 min
Response: 11994174
Conc: 3.77 ng/ml

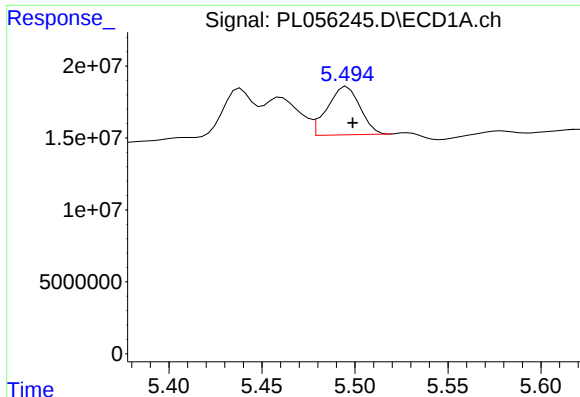

#11 alpha-Chlordane


R.T.: 5.496 min
Delta R.T.: -0.003 min
Response: 41001373
Conc: 2.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
346

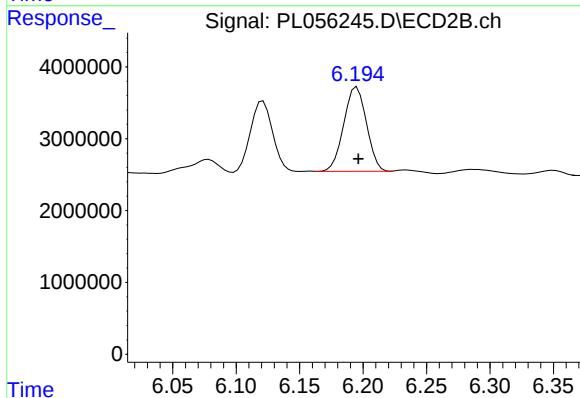


#11 alpha-Chlordane

R.T.: 6.195 min
Delta R.T.: -0.001 min
Response: 14643200
Conc: 4.62 ng/ml

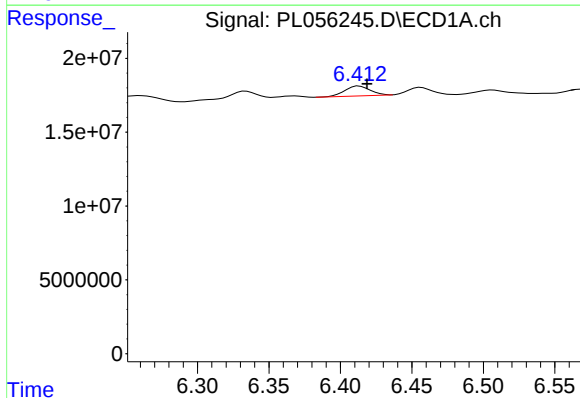


#17 4,4'-DDT

R.T.: 6.413 min
Delta R.T.: -0.005 min
Response: 8314398
Conc: 0.76 ng/ml

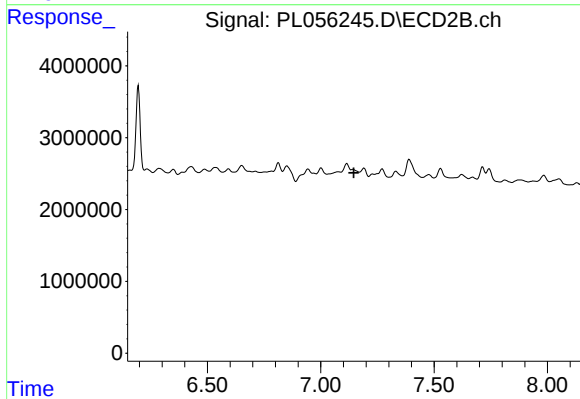

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.146 min
Response: 0
Conc: N.D.

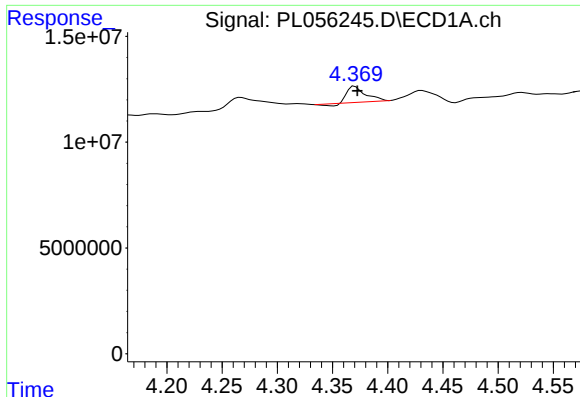

#23 Chlordane-1


R.T.: 4.370 min
Delta R.T.: -0.002 min
Response: 8238740
Conc: 21.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
346

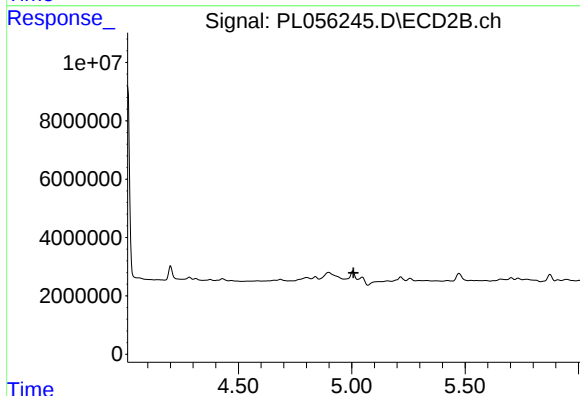


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

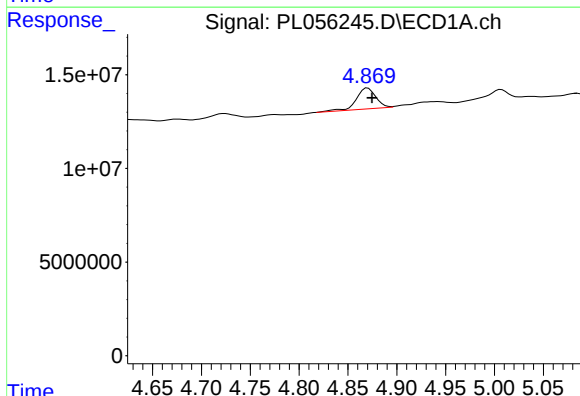


#24 Chlordane-2

R.T.: 4.870 min
Delta R.T.: -0.004 min
Response: 15433951
Conc: 35.23 ng/ml

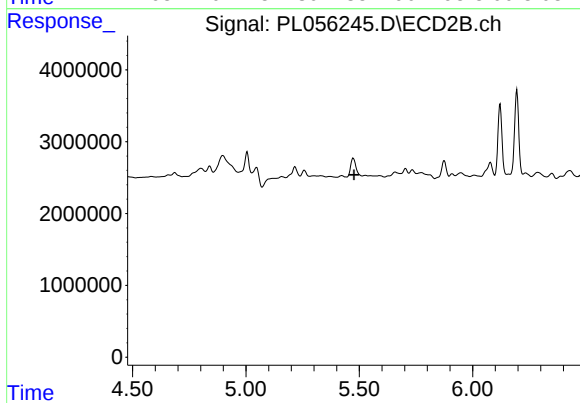

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.477 min
Response: 0
Conc: N.D.

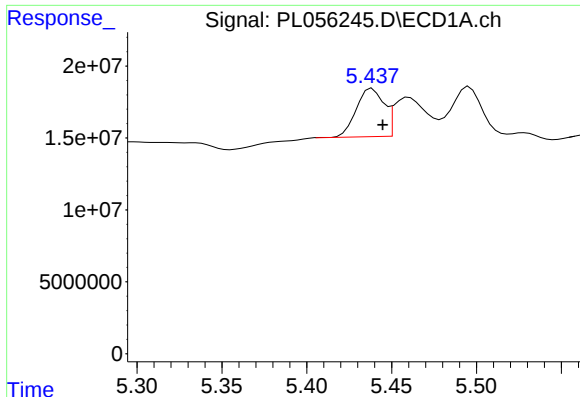

#25 Chlordane-3


R.T.: 5.439 min
Delta R.T.: -0.006 min
Response: 37877970
Conc: 30.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
346

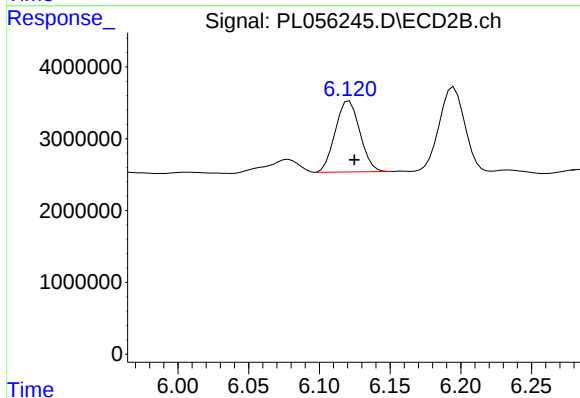


#25 Chlordane-3

R.T.: 6.121 min
Delta R.T.: -0.004 min
Response: 11994174
Conc: 31.91 ng/ml

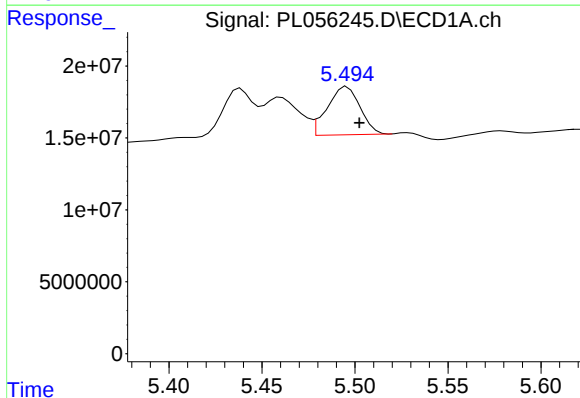


#26 Chlordane-4

R.T.: 5.496 min
Delta R.T.: -0.007 min
Response: 41001373
Conc: 37.89 ng/ml

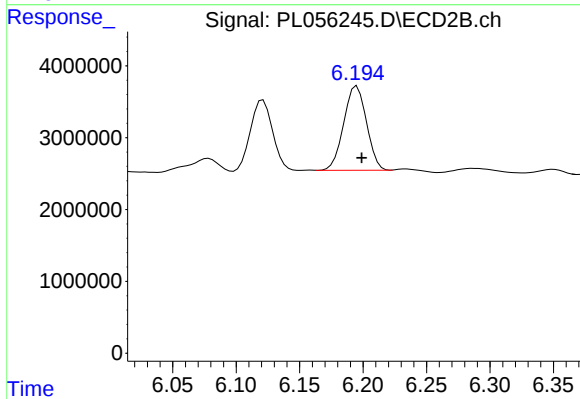

#26 Chlordane-4


R.T.: 6.195 min
Delta R.T.: -0.004 min
Response: 14643200
Conc: 33.33 ng/ml

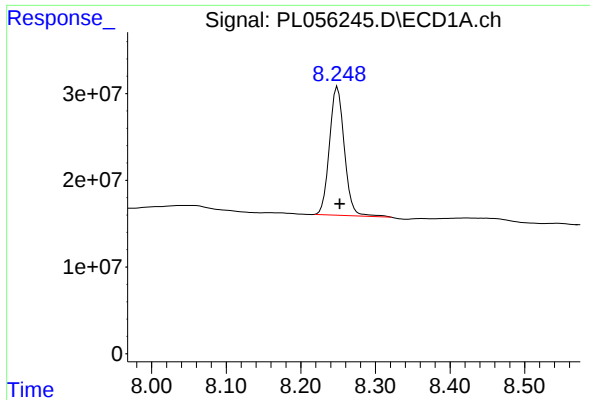

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 205133695
Conc: 19.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
346

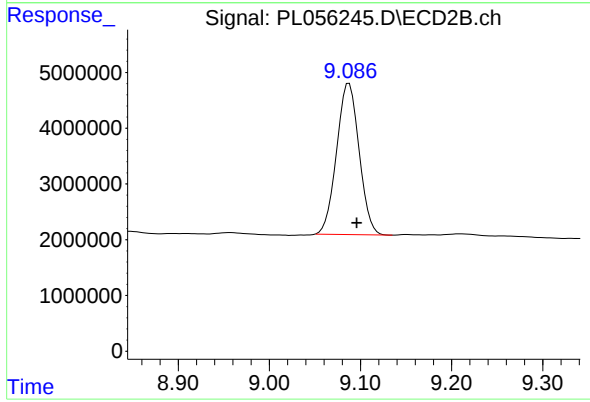

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.008 min
Response: 46489917
Conc: 20.55 ng/ml