

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
 Data File : PL056252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 18:14
 Operator : AJ\MA
 Sample : L1319-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 RAINEY-PARK-BH-02-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 22:15:25 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	218.0E6	66276898	20.820	22.666
28)	SA Decachlor...	8.249	9.086	184.9E6	40070254	17.560	17.715
Target Compounds							
9)	A Endosulfan I	5.577f	0.000	20618808	0	1.421	N.D. #
12)	B 4,4'-DDE	5.660	6.351	142.1E6	29207360	9.807	9.751
14)	MA Endrin	6.050	0.000	48546774	0	3.455	N.D. #
15)	B Endosulfa...	6.333	6.945	13430605	13807015	1.027	5.129 #
16)	A 4,4'-DDD	6.177	0.000	11158039	0	1.038	N.D. #
17)	MA 4,4'-DDT	6.416	7.142	115.1E6	21417309	10.531	9.329
27)	Chlordane-5	6.333	0.000	13430605	0	32.376	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
Data File : PL056252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 18:14
Operator : AJ\MA
Sample : L1319-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 22:15:25 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

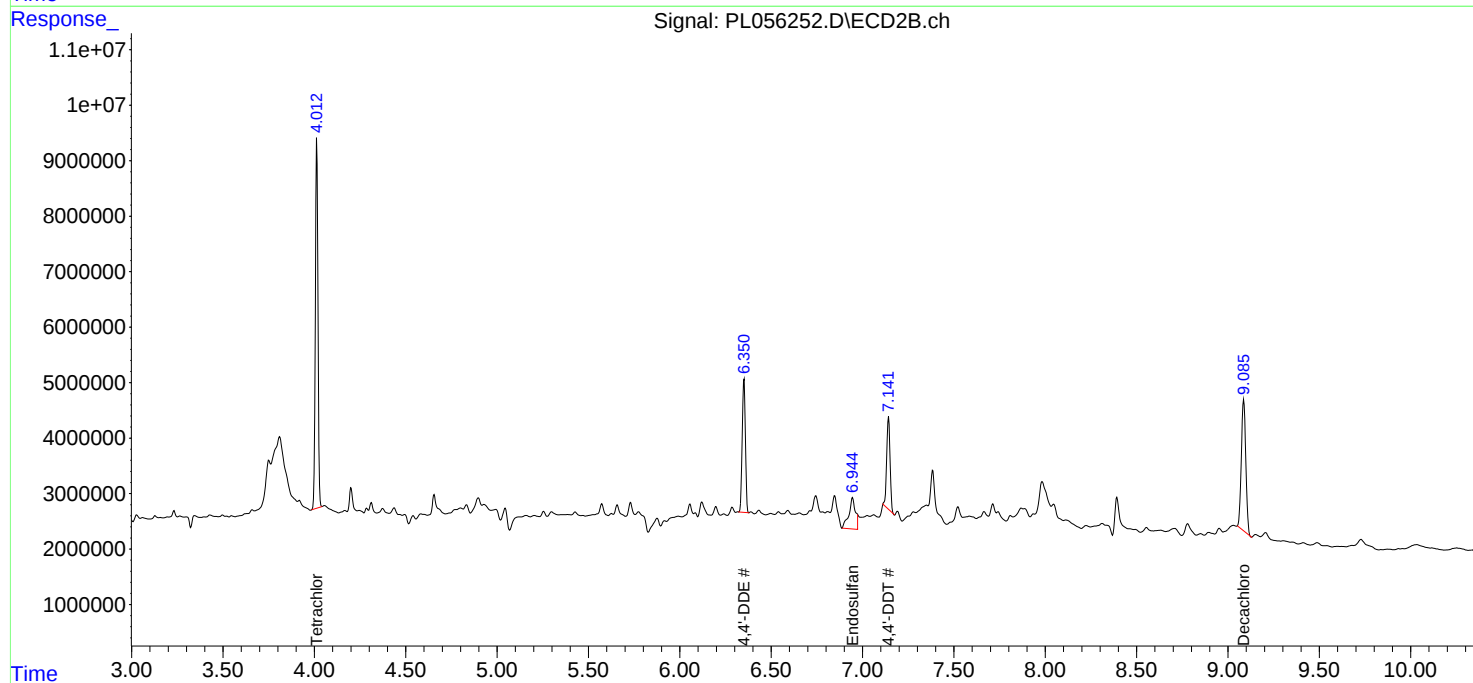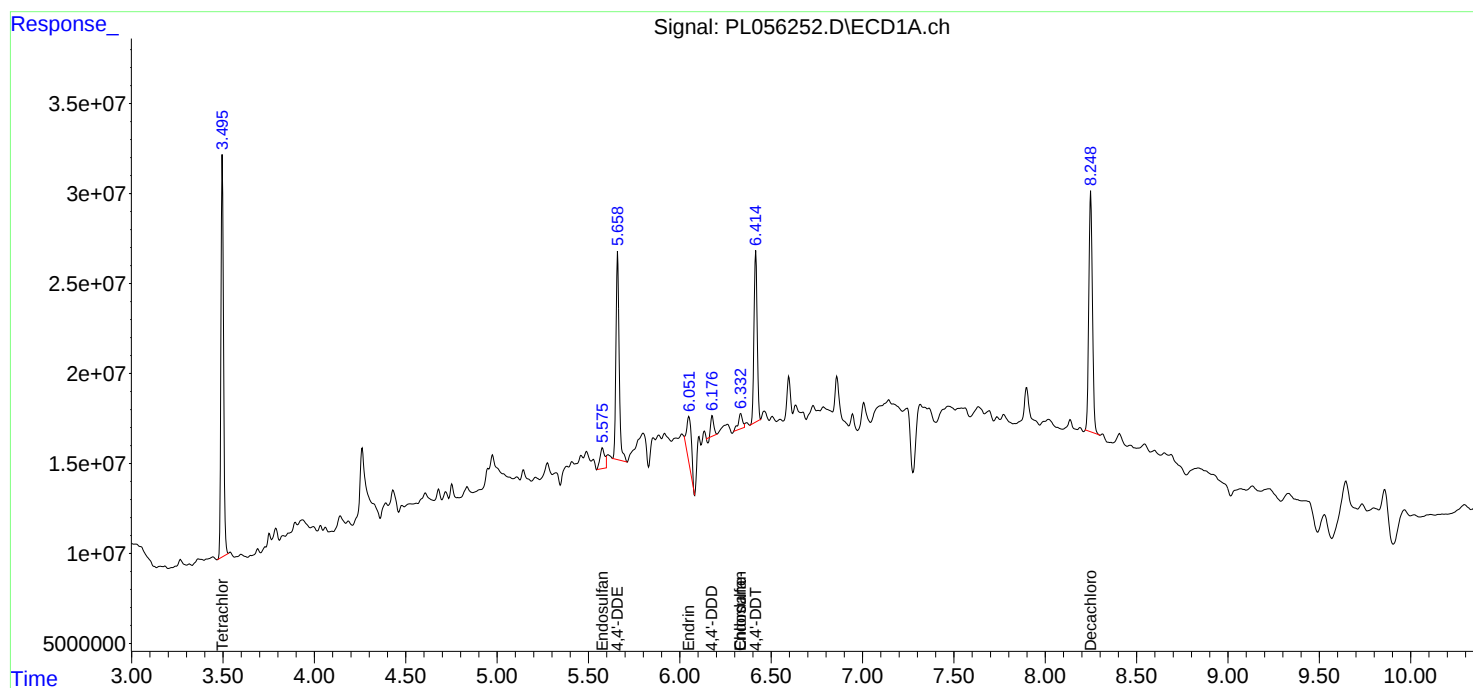


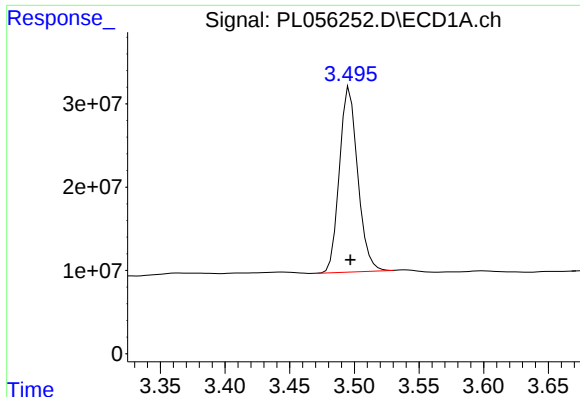

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 218044750
Conc: 20.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

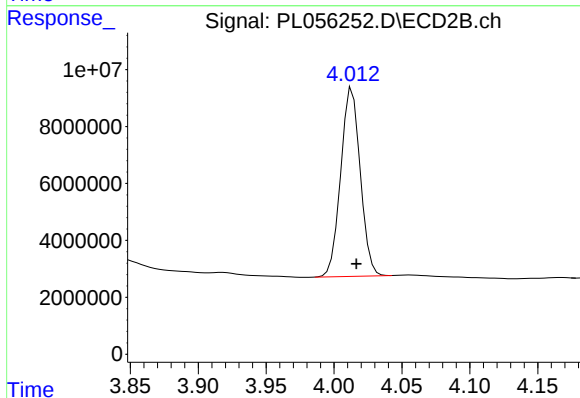


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.003 min
Response: 66276898
Conc: 22.67 ng/ml

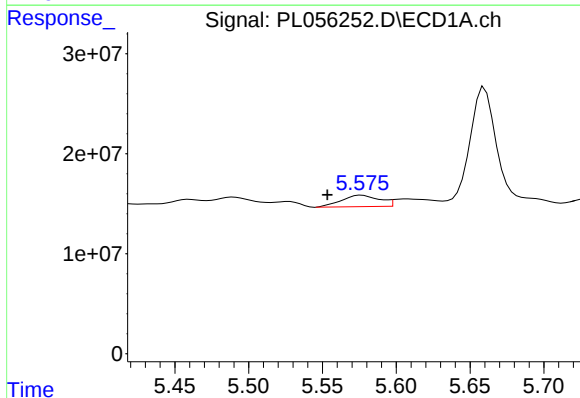


#9 Endosulfan I

R.T.: 5.577 min
Delta R.T.: 0.023 min
Response: 20618808
Conc: 1.42 ng/ml

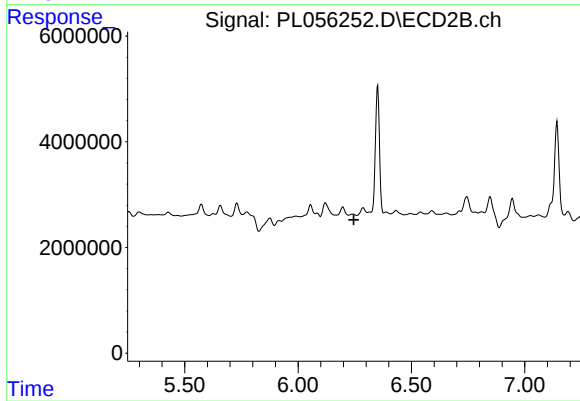

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

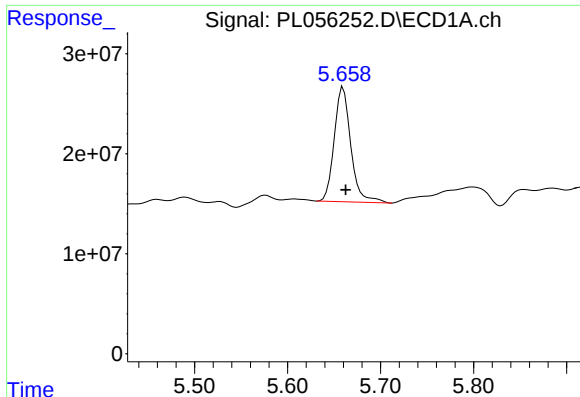

#12 4,4'-DDE


R.T.: 5.660 min
Delta R.T.: -0.003 min
Response: 142141853
Conc: 9.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

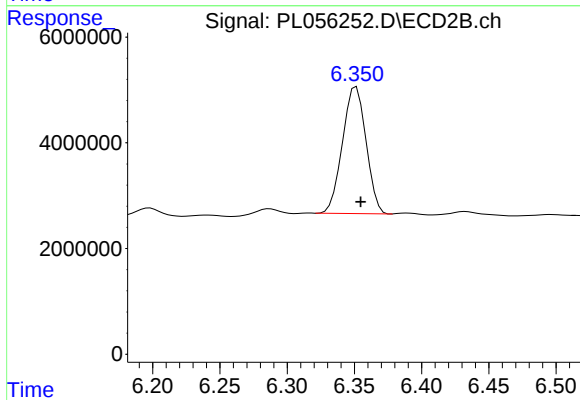


#12 4,4'-DDE

R.T.: 6.351 min
Delta R.T.: -0.003 min
Response: 29207360
Conc: 9.75 ng/ml

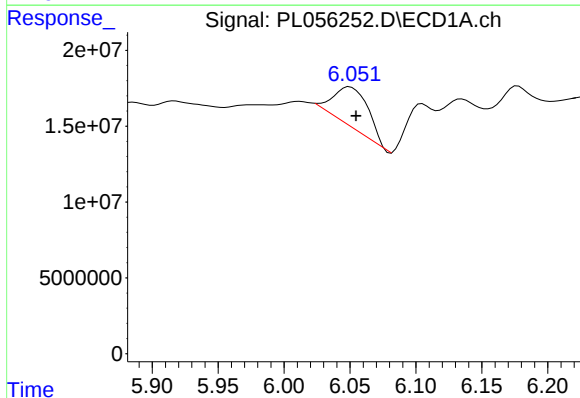


#14 Endrin

R.T.: 6.050 min
Delta R.T.: -0.005 min
Response: 48546774
Conc: 3.45 ng/ml

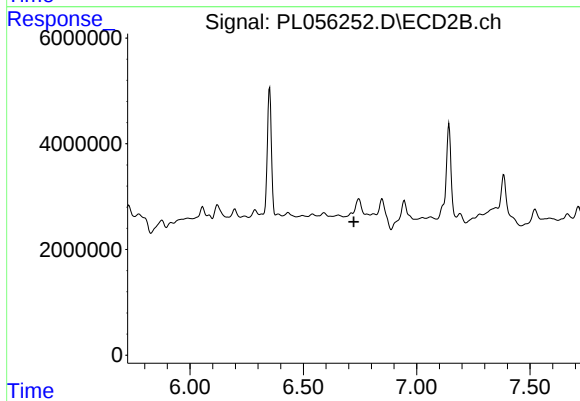

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 6.723 min
Response: 0
Conc: N.D.

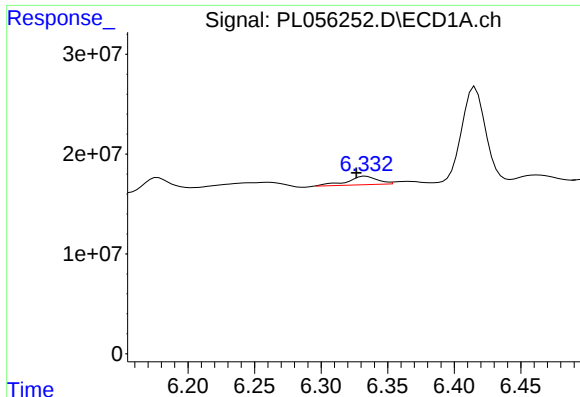

#15 Endosulfan II


R.T.: 6.333 min
Delta R.T.: 0.007 min
Response: 13430605
Conc: 1.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

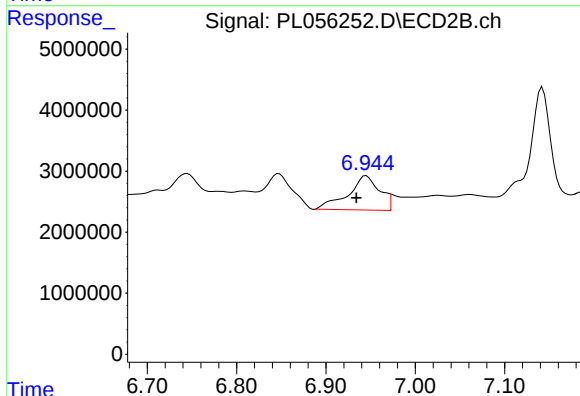


#15 Endosulfan II

R.T.: 6.945 min
Delta R.T.: 0.011 min
Response: 13807015
Conc: 5.13 ng/ml

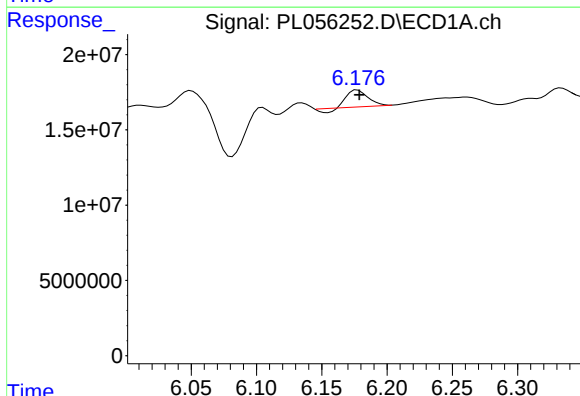


#16 4,4'-DDD

R.T.: 6.177 min
Delta R.T.: -0.001 min
Response: 11158039
Conc: 1.04 ng/ml

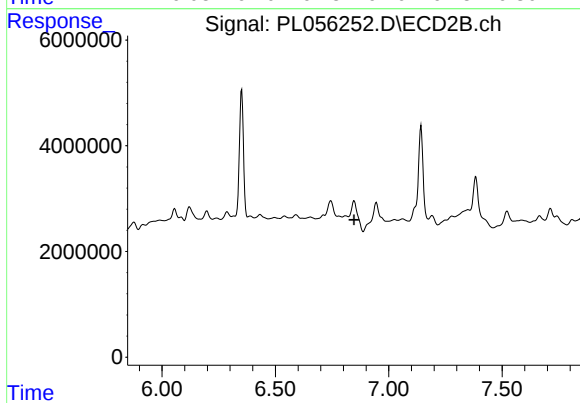

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.847 min
Response: 0
Conc: N.D.

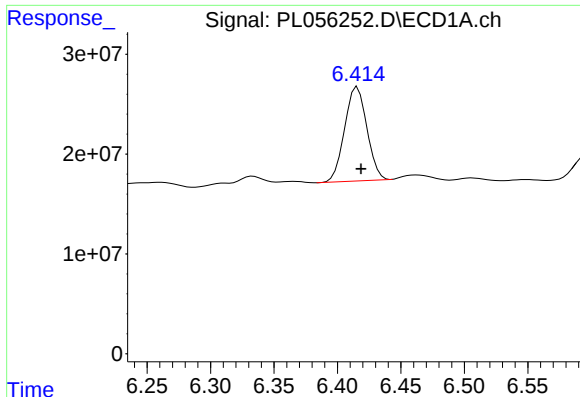

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: -0.003 min
Response: 115088283
Conc: 10.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

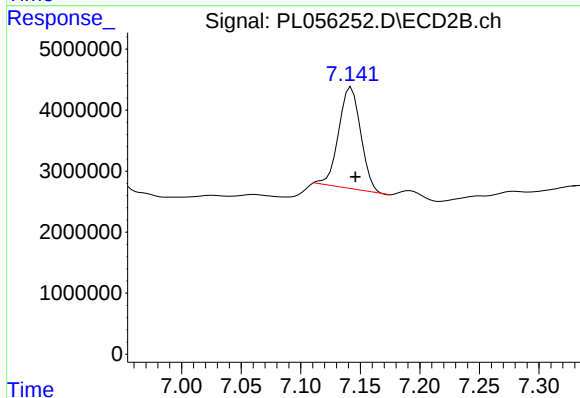


#17 4,4'-DDT

R.T.: 7.142 min
Delta R.T.: -0.004 min
Response: 21417309
Conc: 9.33 ng/ml

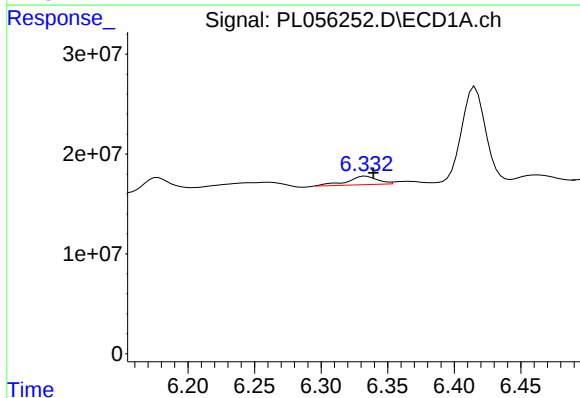


#27 Chlordane-5

R.T.: 6.333 min
Delta R.T.: -0.006 min
Response: 13430605
Conc: 32.38 ng/ml

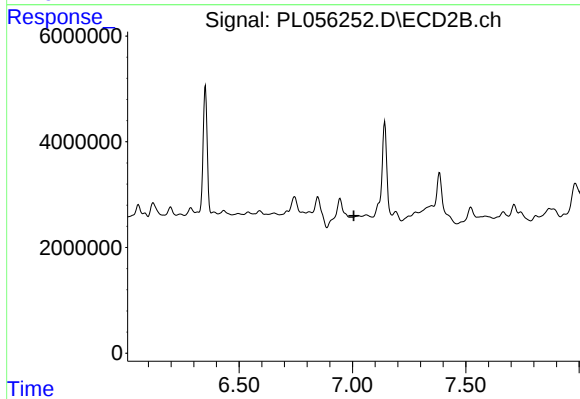

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

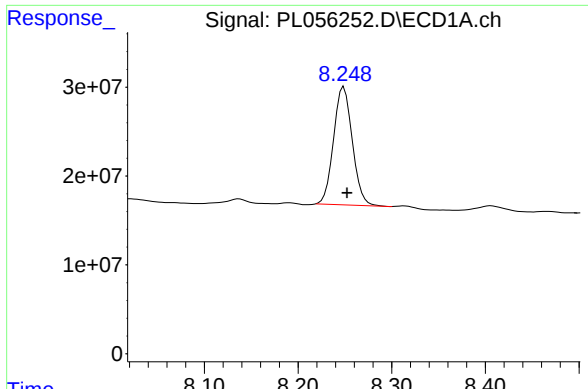

#28 Decachlorobiphenyl

R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 184871542
Conc: 17.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
RAINEY-PARK-BH-02-A

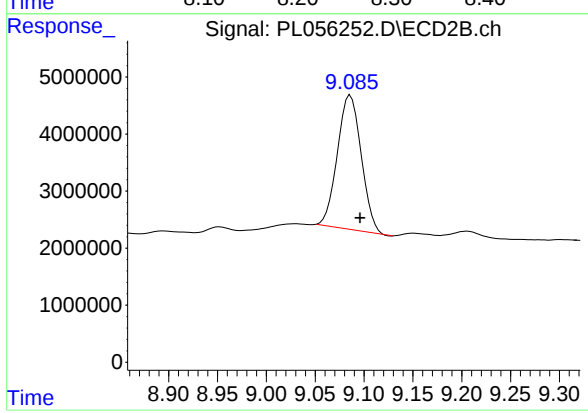

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: -0.010 min
Response: 40070254
Conc: 17.71 ng/ml