

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
 Data File : PL056253.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2020 18:28
 Operator : AJ\MA
 Sample : L1320-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 ETGI-367

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 22:15:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.496	4.013	217.5E6	65575896	20.769	22.426
28)	SA Decachlor...	8.250	9.087	216.7E6	46869994	20.583	20.721
Target Compounds							
9)	A Endosulfan I	5.577f	0.000	10785302	0	0.743	N.D. #
11)	B alpha-Chl...	5.492	0.000	32511924	0	2.113	N.D. #
15)	B Endosulfa...	6.333	0.000	12404652	0	0.948	N.D. #
19)	B Endosulfa...	6.723f	0.000	84676425	0	6.965	N.D. #
26)	Chlordane-4	5.492	0.000	32511924	0	30.047	N.D. #
27)	Chlordane-5	6.333	0.000	12404652	0	29.903	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013120\
Data File : PL056253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2020 18:28
Operator : AJ\MA
Sample : L1320-01
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
ETGI-367

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 22:15:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

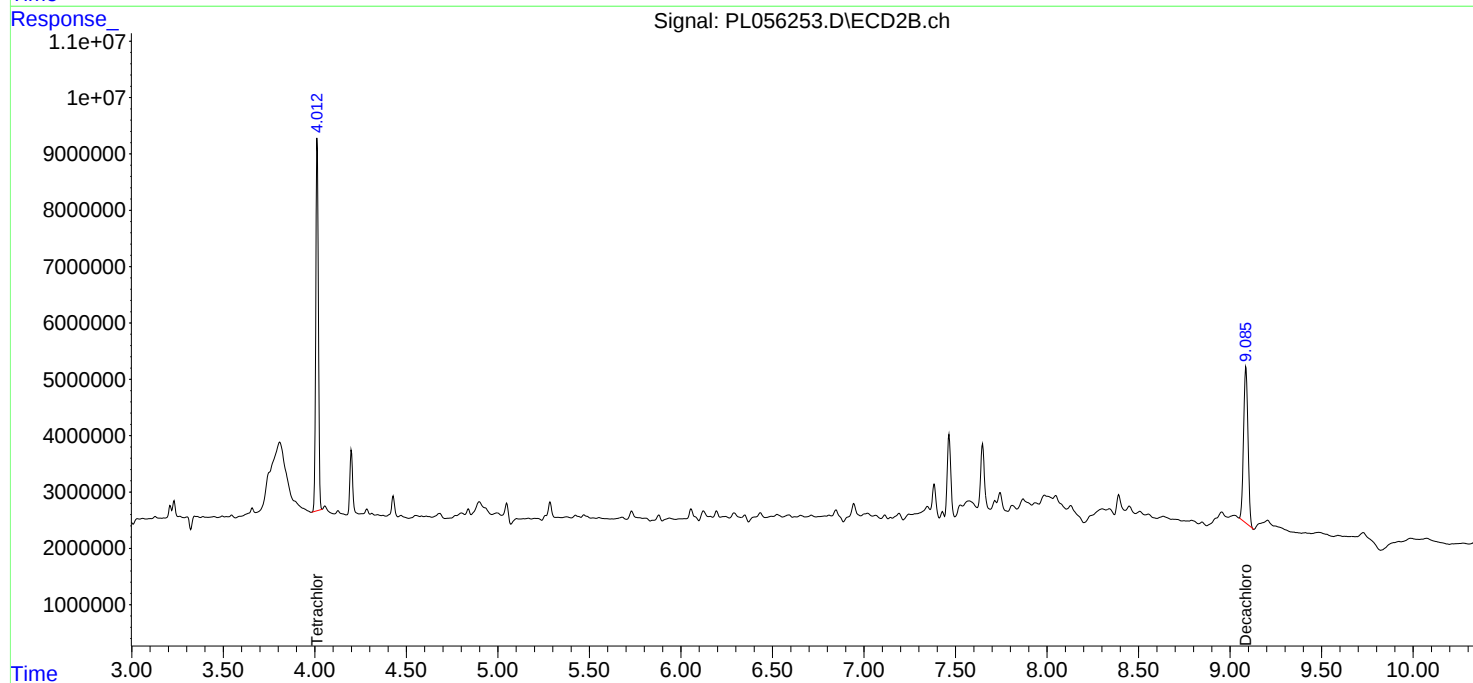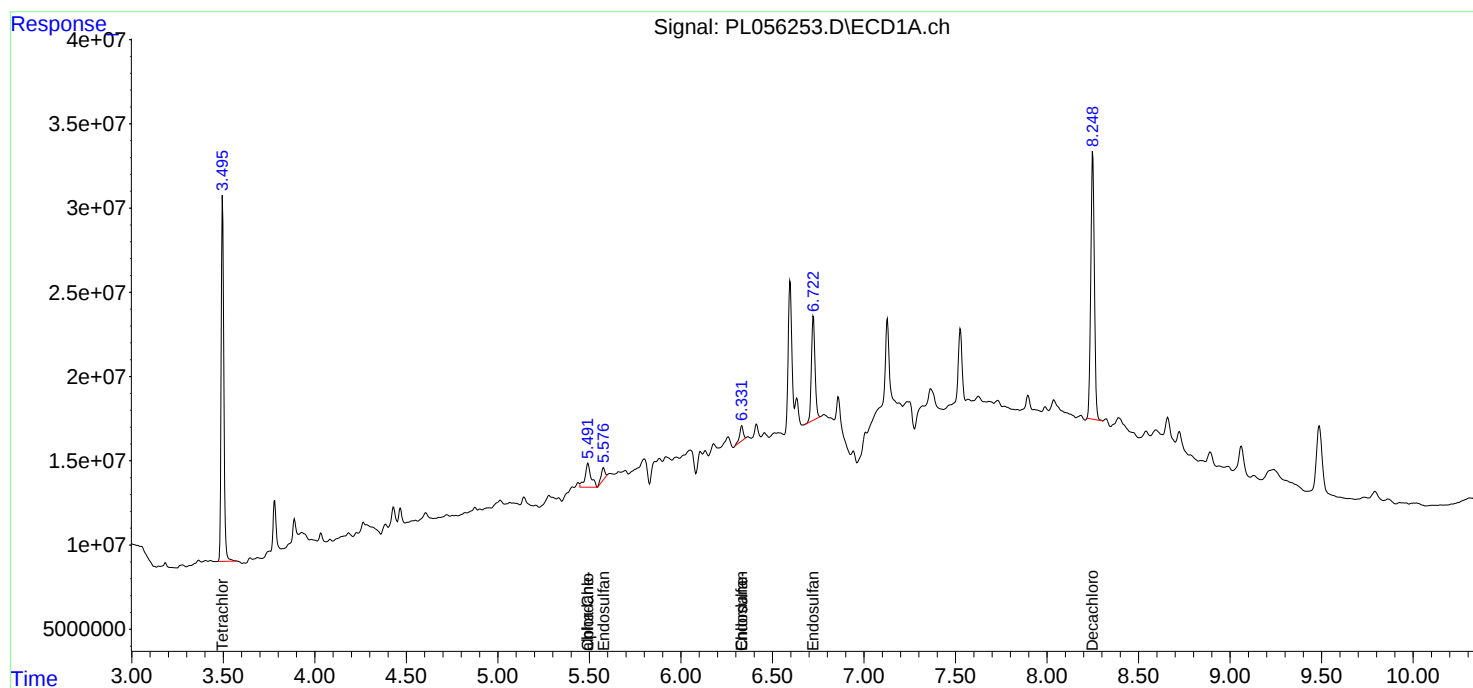


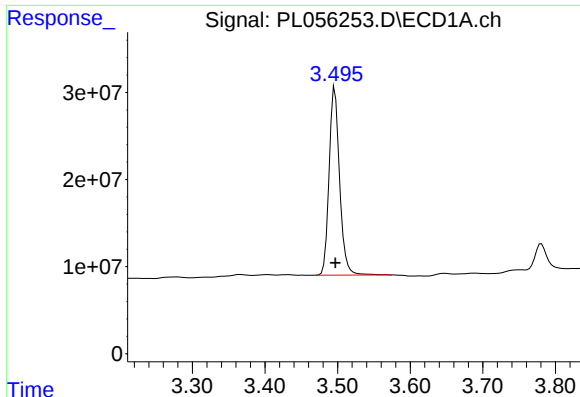

#1 Tetrachloro-m-xylene


R.T.: 3.496 min
Delta R.T.: 0.000 min
Response: 217513360
Conc: 20.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-367

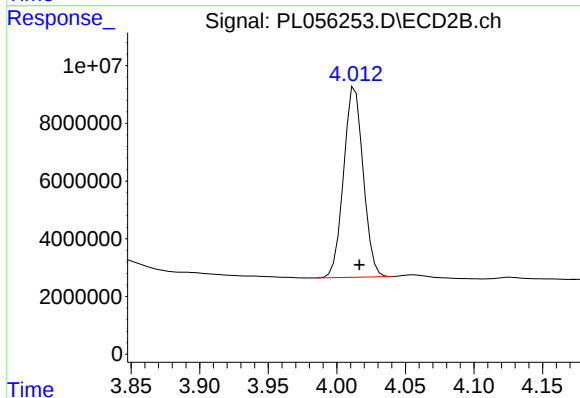


#1 Tetrachloro-m-xylene

R.T.: 4.013 min
Delta R.T.: -0.003 min
Response: 65575896
Conc: 22.43 ng/ml

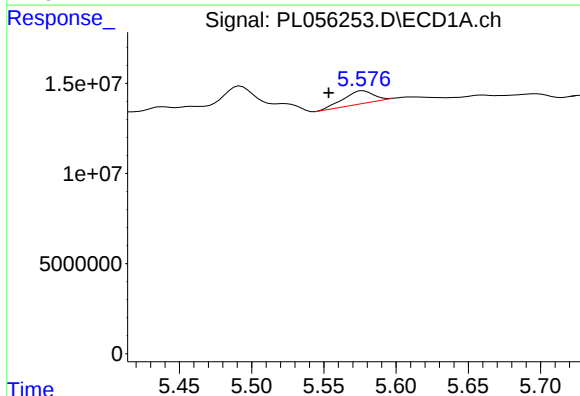


#9 Endosulfan I

R.T.: 5.577 min
Delta R.T.: 0.024 min
Response: 10785302
Conc: 0.74 ng/ml

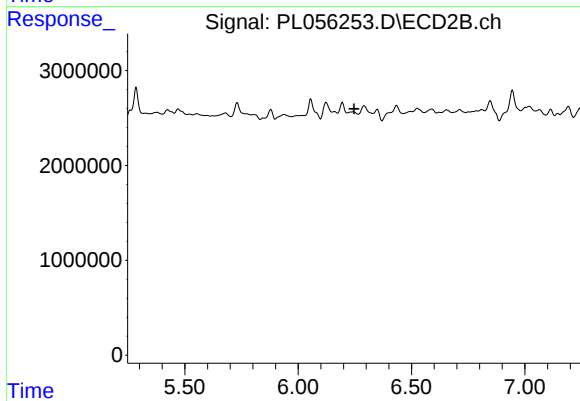

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.246 min
Response: 0
Conc: N.D.

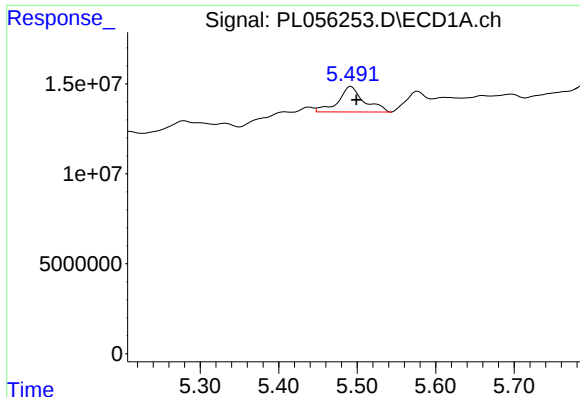

#11 alpha-Chlordane


R.T.: 5.492 min
Delta R.T.: -0.007 min
Response: 32511924
Conc: 2.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-367

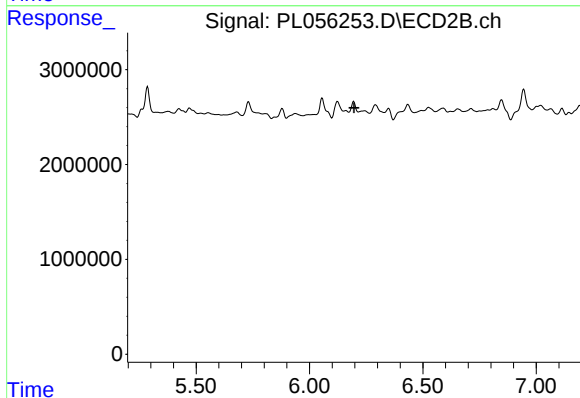


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.196 min
Response: 0
Conc: N.D.

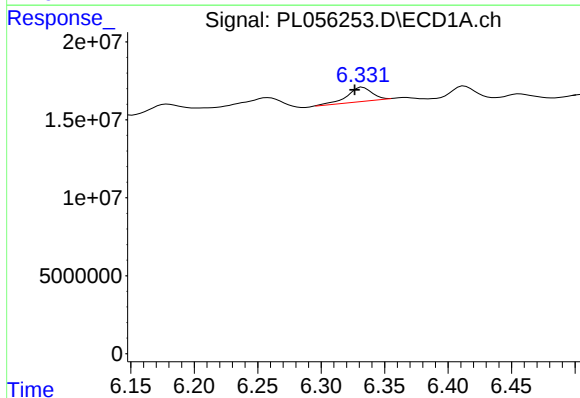


#15 Endosulfan II

R.T.: 6.333 min
Delta R.T.: 0.006 min
Response: 12404652
Conc: 0.95 ng/ml

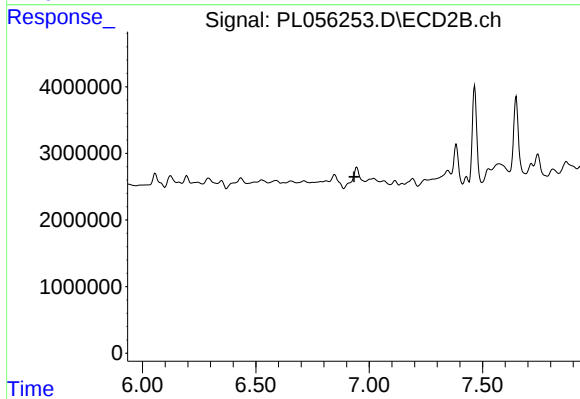

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.934 min
Response: 0
Conc: N.D.

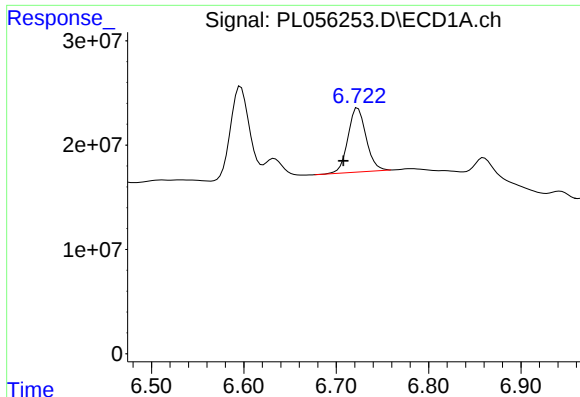

#19 Endosulfan Sulfate


R.T.: 6.723 min
Delta R.T.: 0.016 min
Response: 84676425
Conc: 6.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-367

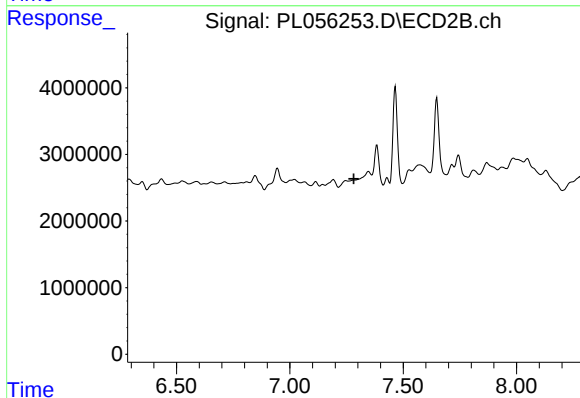


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.282 min
Response: 0
Conc: N.D.

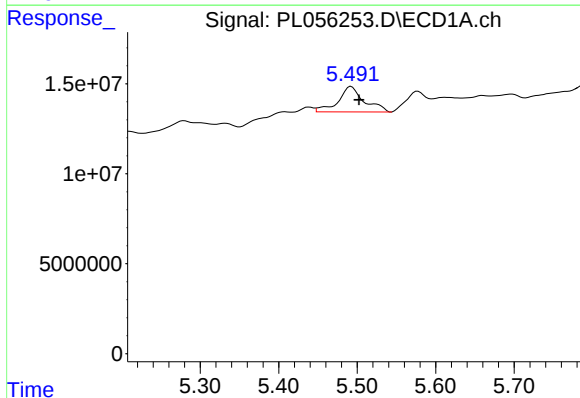


#26 Chlordane-4

R.T.: 5.492 min
Delta R.T.: -0.010 min
Response: 32511924
Conc: 30.05 ng/ml

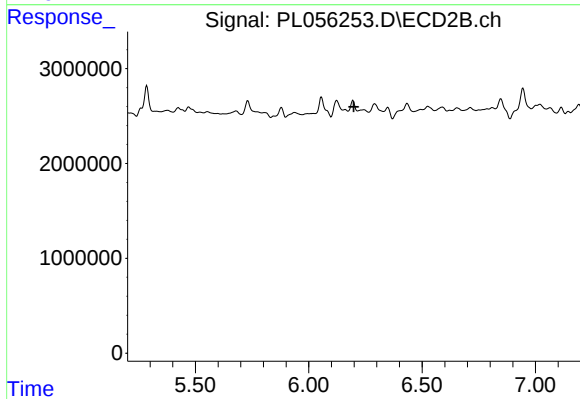

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T. : 6.199 min
Response: 0
Conc: N.D.

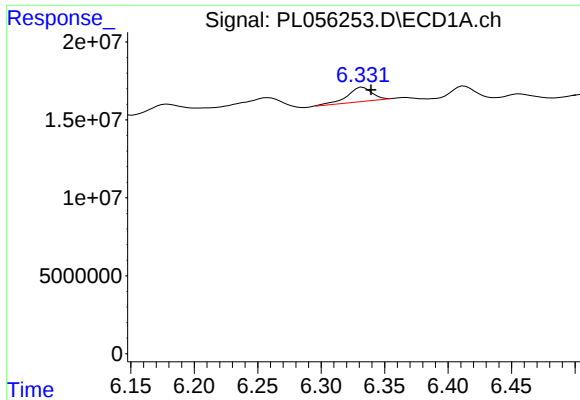

#27 Chlordane-5


R.T.: 6.333 min
Delta R.T.: -0.007 min
Response: 12404652
Conc: 29.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
ETGI-367

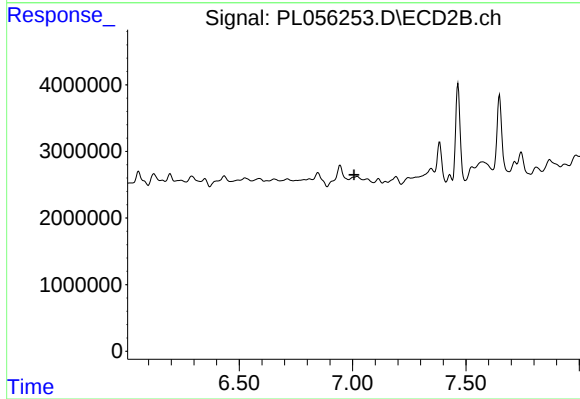


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

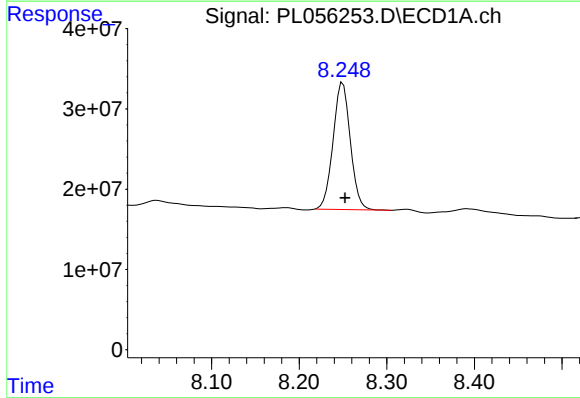

#28 Decachlorobiphenyl

R.T.: 8.250 min
Delta R.T.: -0.002 min
Response: 216695288
Conc: 20.58 ng/ml

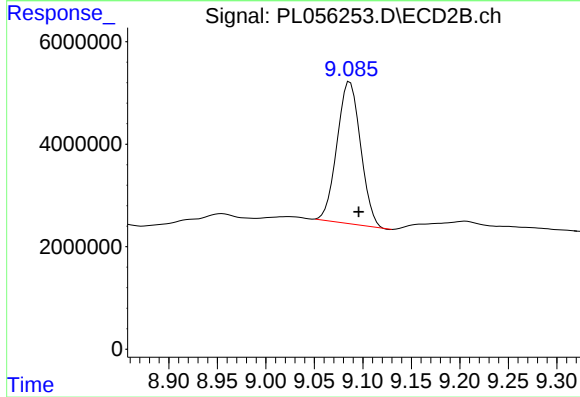

#28 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.009 min
Response: 46869994
Conc: 20.72 ng/ml