

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013123\
 Data File : PL080643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jan 2023 19:22
 Operator : AR\AJ
 Sample : 01348-02
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 E-H5(31.5-33.5)

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/01/2023
 Supervised By :Ankita Jodhani 02/01/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 31 21:00:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.349	2.688	45386276	44479007	21.161m	20.250
2) SA Decachlor...	8.787	7.835	35807910	46922652	20.453	19.694

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013123\
Data File : PL080643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jan 2023 19:22
Operator : AR\AJ
Sample : 01348-02
Misc :
ALS Vial : 33 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
E-H5(31.5-33.5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/01/2023
Supervised By : Ankita Jodhani 02/01/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 31 21:00:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

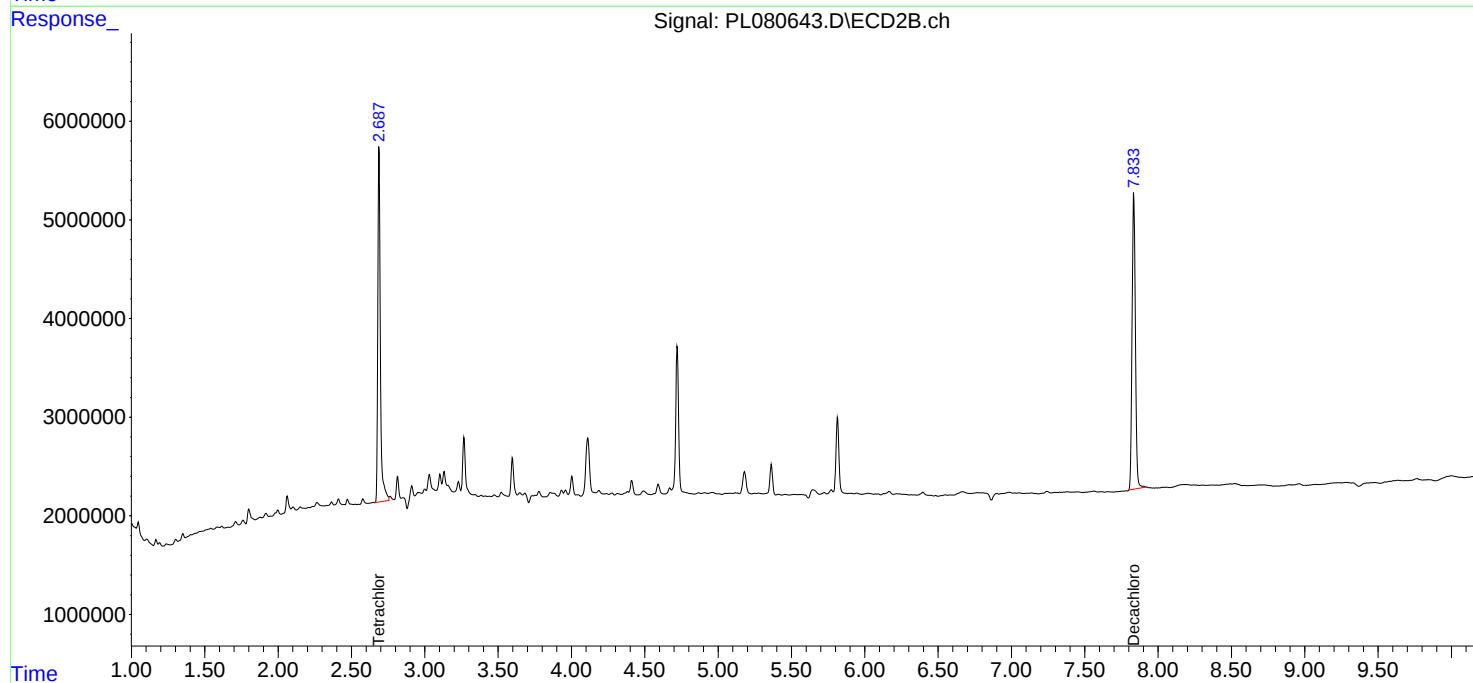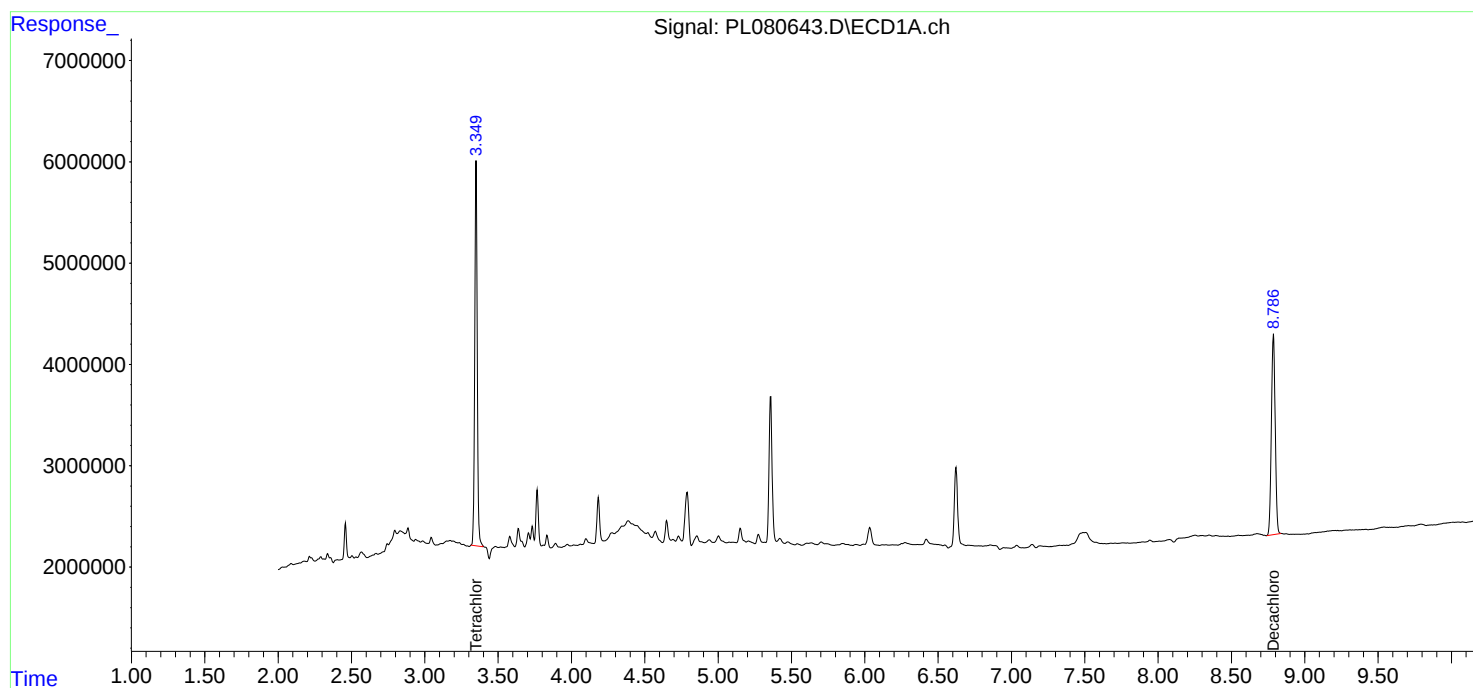

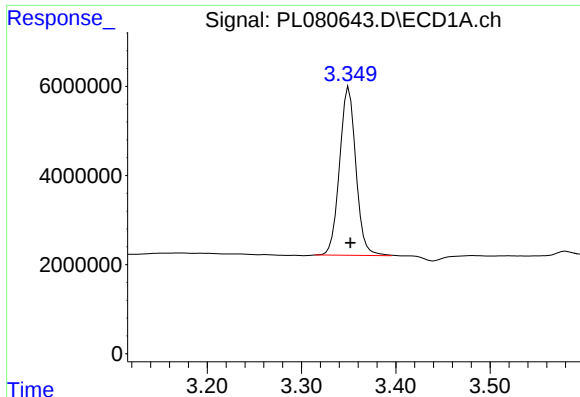


#1 Tetrachloro-m-xylene

R.T.: 3.349 min
Delta R.T.: -0.003 min
Response: 45386276
Conc: 21.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
E-H5(31.5-33.5)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/01/2023
Supervised By :Ankita Jodhani 02/01/2023

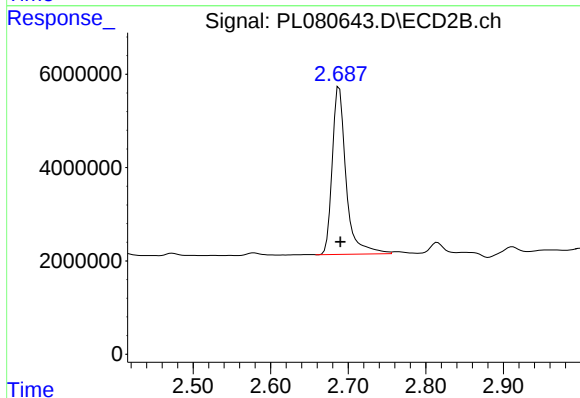


#1 Tetrachloro-m-xylene

R.T.: 2.688 min
Delta R.T.: -0.001 min
Response: 44479007
Conc: 20.25 ng/ml

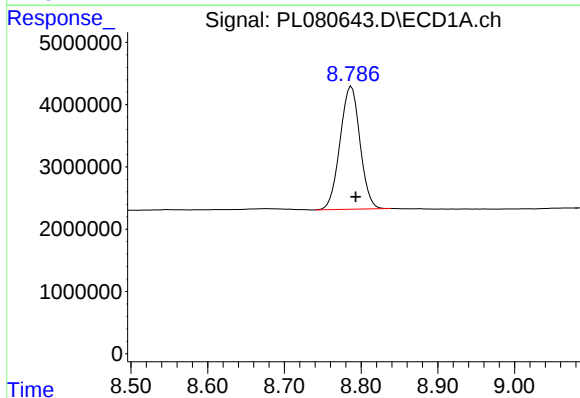

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 35807910
Conc: 20.45 ng/ml

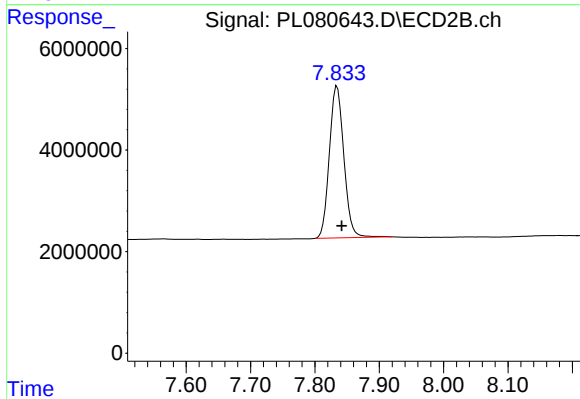

#28 Decachlorobiphenyl

R.T.: 7.835 min
Delta R.T.: -0.007 min
Response: 46922652
Conc: 19.69 ng/ml