

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013125\
 Data File : PL093976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2025 02:03
 Operator : AR\AJ
 Sample : Q1219-01 10X
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 LAW-25-0015

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 02/03/2025
 Supervised By : Ankita Jodhani 02/03/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 06:45:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 21 14:58:05 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.774	3428454	8308694	1.273m	2.545m#
28) SA Decachlor...	9.059	7.913	17389598	3990480	8.313m	1.139m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL013125\
Data File : PL093976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2025 02:03
Operator : AR\AJ
Sample : Q1219-01 10X
Misc :
ALS Vial : 41 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
LAW-25-0015


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/03/2025
Supervised By : Ankita Jodhani 02/03/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 06:45:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012125.M
Quant Title : GC Extractables
QLast Update : Tue Jan 21 14:58:05 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

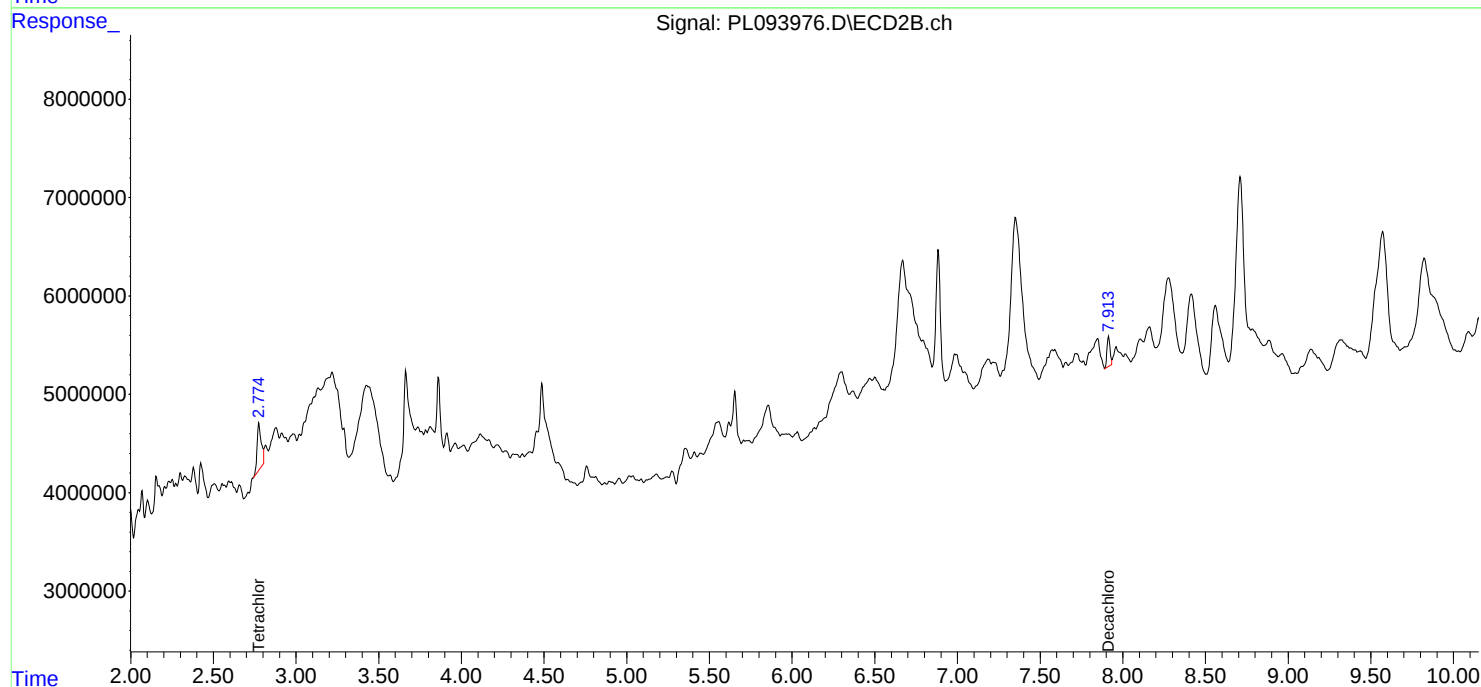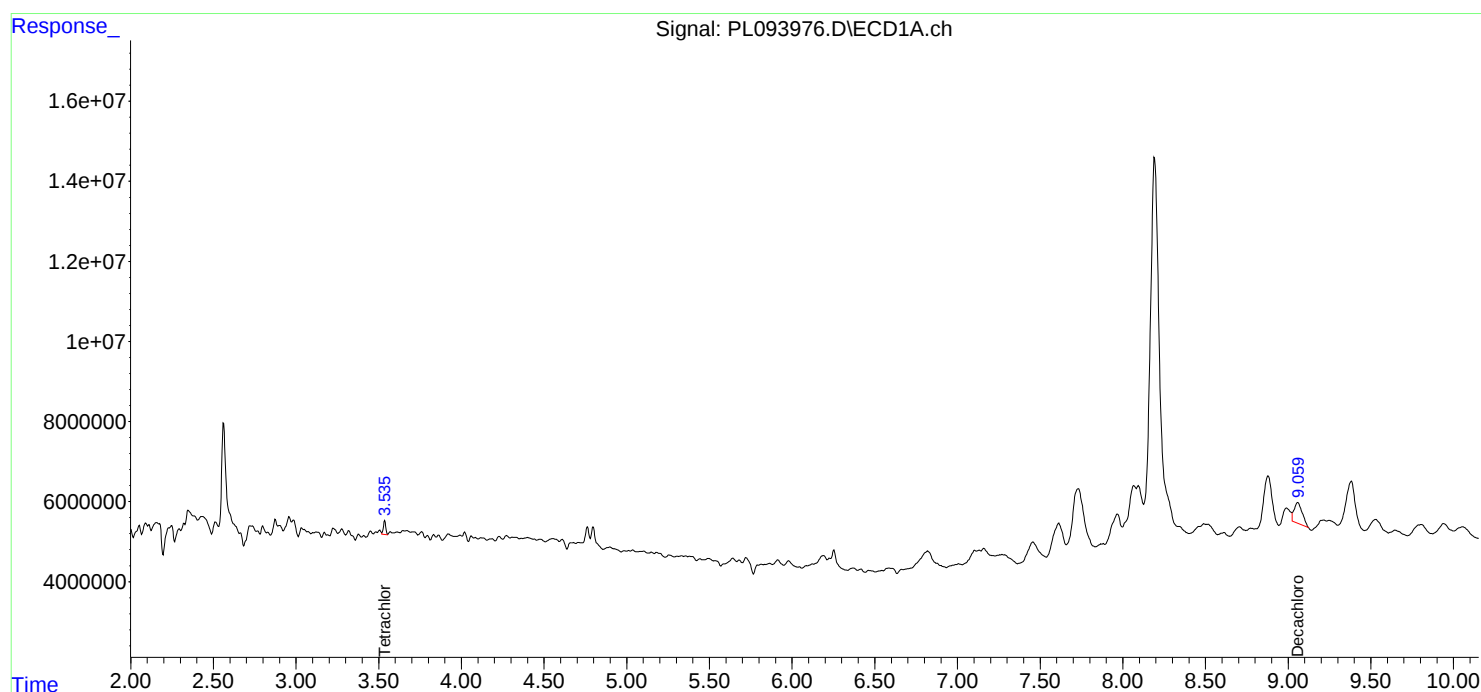

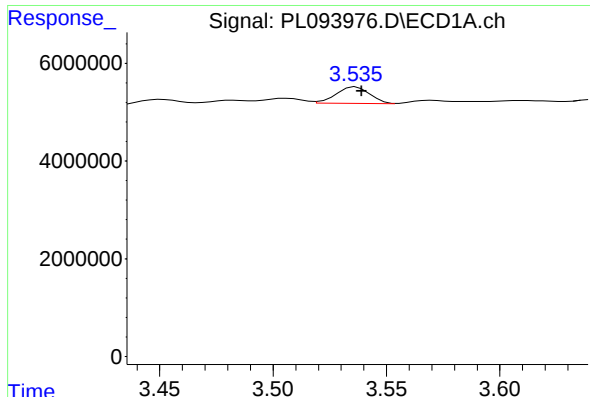


#1 Tetrachloro-m-xylene

R.T.: 3.535 min
Delta R.T.: -0.004 min
Response: 3428454
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
LAW-25-0015


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/03/2025
Supervised By :Ankita Jodhani 02/03/2025

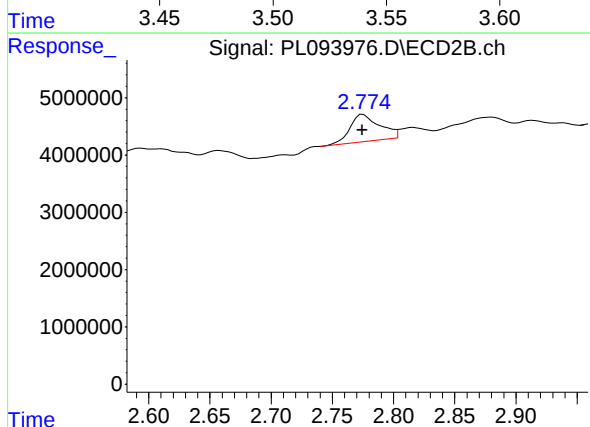


#1 Tetrachloro-m-xylene

R.T.: 2.774 min
Delta R.T.: 0.000 min
Response: 8308694
Conc: 2.55 ng/ml

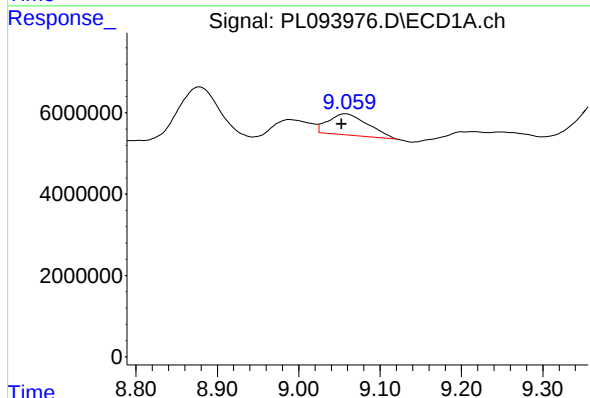

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: 0.006 min
Response: 17389598
Conc: 8.31 ng/ml

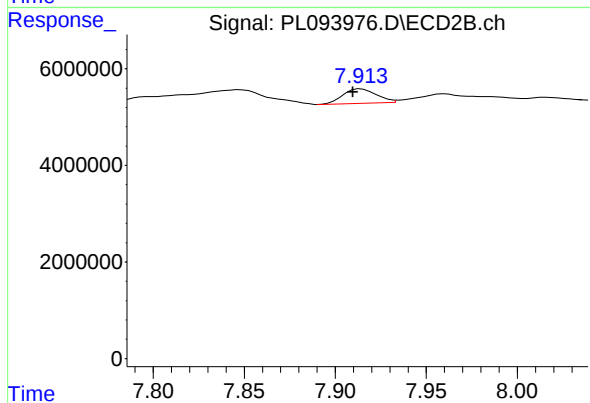

#28 Decachlorobiphenyl

R.T.: 7.913 min
Delta R.T.: 0.003 min
Response: 3990480
Conc: 1.14 ng/ml