

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
 Data File : PL044388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2019 19:00
 Operator : AJ\SJ
 Sample : K1299-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-LEACH-AMND-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 23:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.985	113.9E6	49315049	18.802	22.608
28)	SA Decachlor...	8.049	9.042	84774244	24921454	12.224	11.234
Target Compounds							
3)	MA gamma-BHC...	4.068	4.680	6004256	4141462	0.747	1.566 #
5)	MB Aldrin	4.591	5.482	389.5E6	120.1E6	49.880	47.740
6)	B beta-BHC	4.286f	0.000	83348256	0	24.041	N.D. #
8)	B Heptachlo...	0.000	5.814f	0	20607588	N.D.	8.910 #
9)	A Endosulfan I	5.387	6.239	77736853	17065240	11.035	7.371 #
10)	B gamma-Chl...	5.294	0.000	168.8E6	0	21.789	N.D. #
11)	B alpha-Chl...	5.320	0.000	139.7E6	0	18.335	N.D. #
20)	A Methoxychlor	6.784	0.000	30100403	0	10.151	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
Data File : PL044388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2019 19:00
Operator : AJ\SJ
Sample : K1299-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 23:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

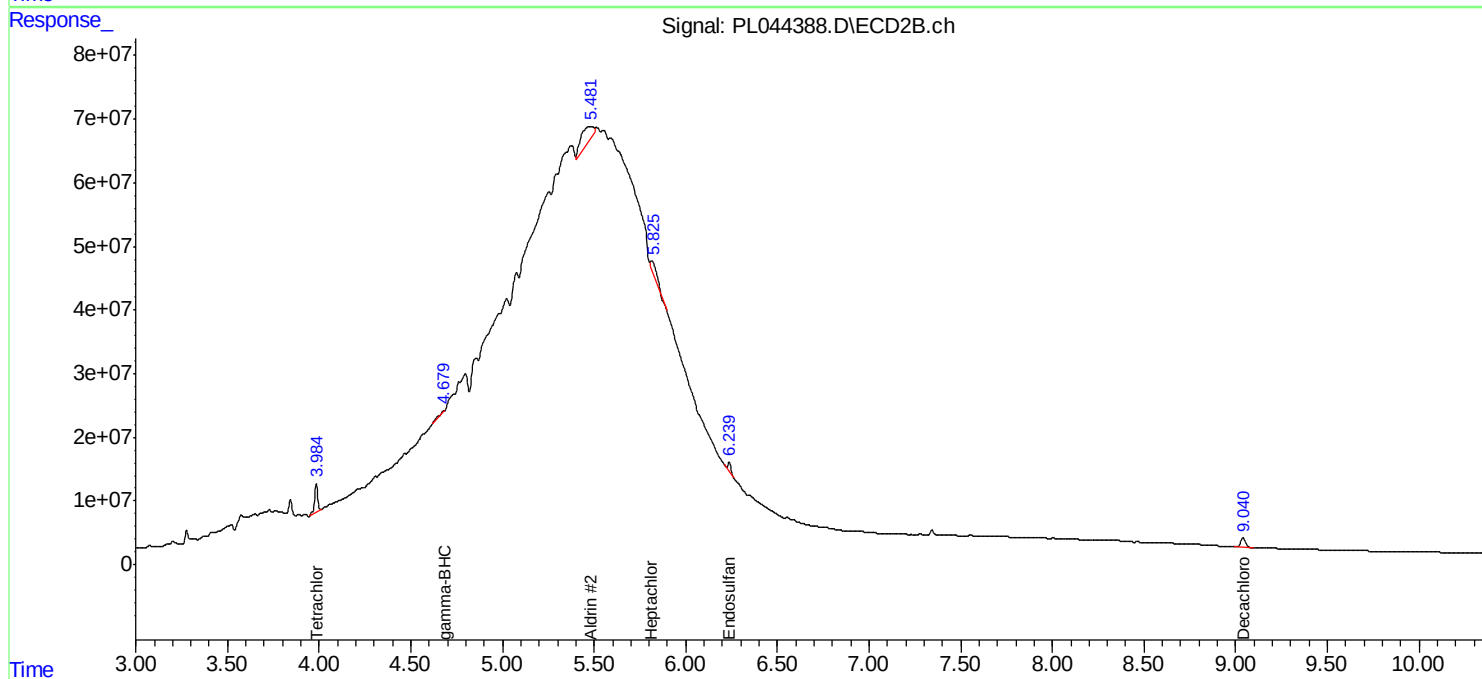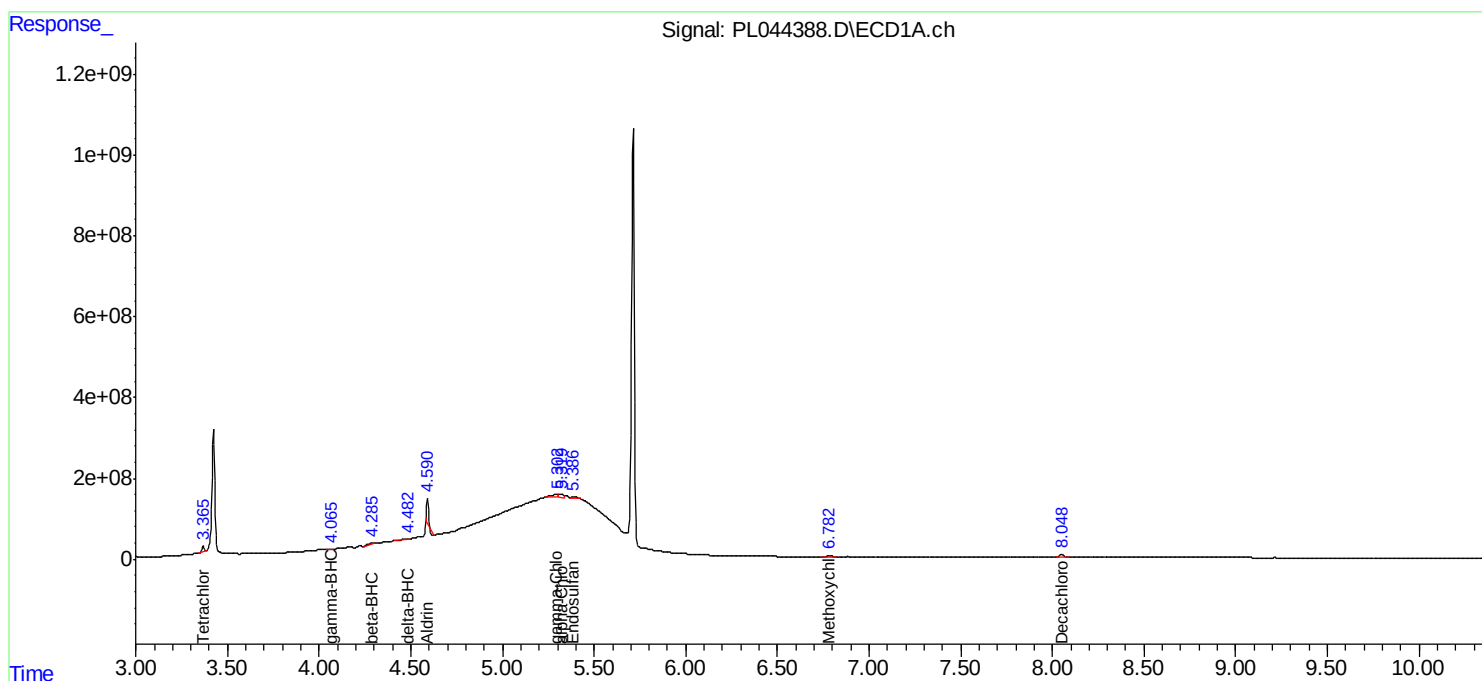


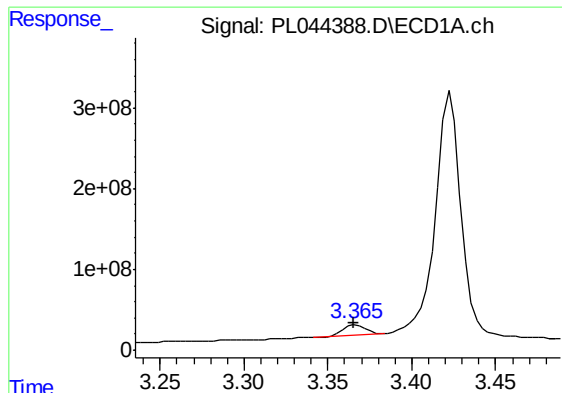

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.002 min
Response: 113945192
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

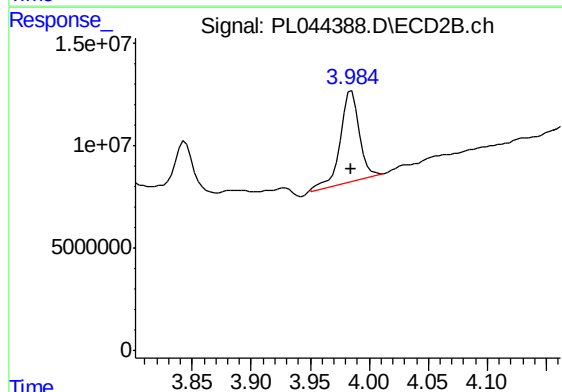


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 49315049
Conc: 22.61 ng/ml

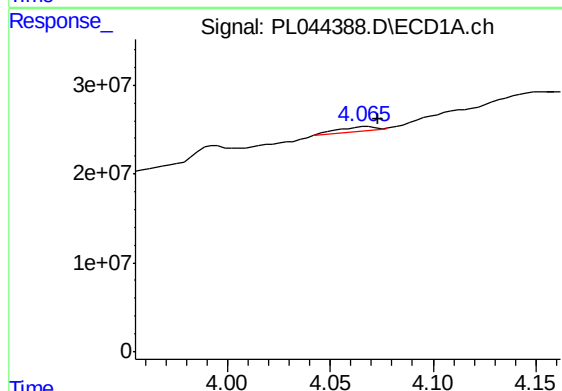


#3 gamma-BHC (Lindane)

R.T.: 4.068 min
Delta R.T.: -0.005 min
Response: 6004256
Conc: 0.75 ng/ml

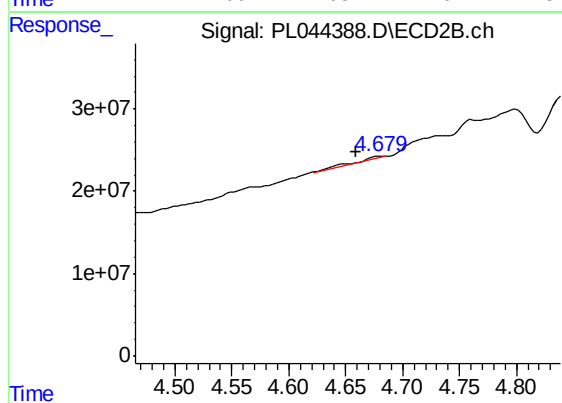

#3 gamma-BHC (Lindane)


R.T.: 4.680 min
Delta R.T.: 0.021 min
Response: 4141462
Conc: 1.57 ng/ml

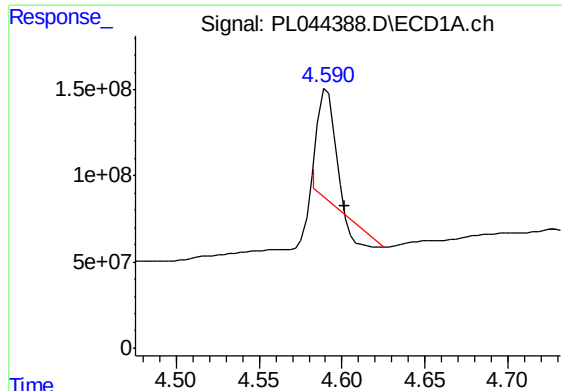

#5 Aldrin


R.T.: 4.591 min
Delta R.T.: -0.010 min
Response: 389458507
Conc: 49.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

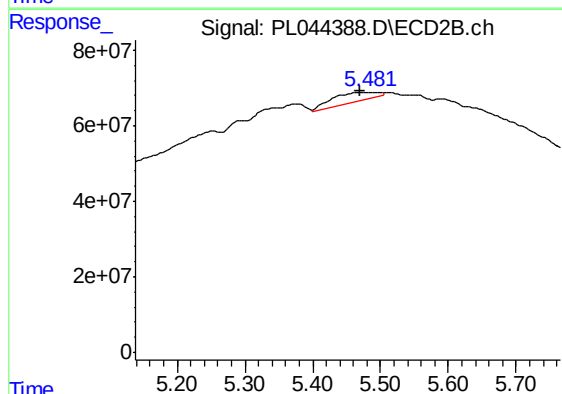


#5 Aldrin

R.T.: 5.482 min
Delta R.T.: 0.011 min
Response: 120111776
Conc: 47.74 ng/ml

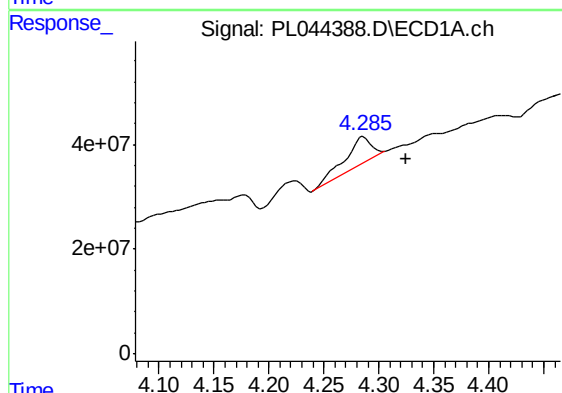


#6 beta-BHC

R.T.: 4.286 min
Delta R.T.: -0.039 min
Response: 83348256
Conc: 24.04 ng/ml

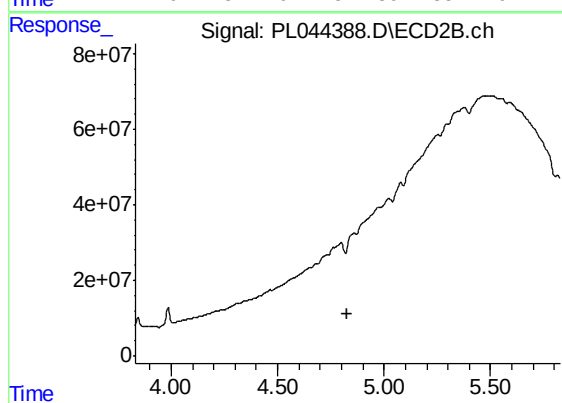

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.830 min
Response: 0
Conc: N.D.

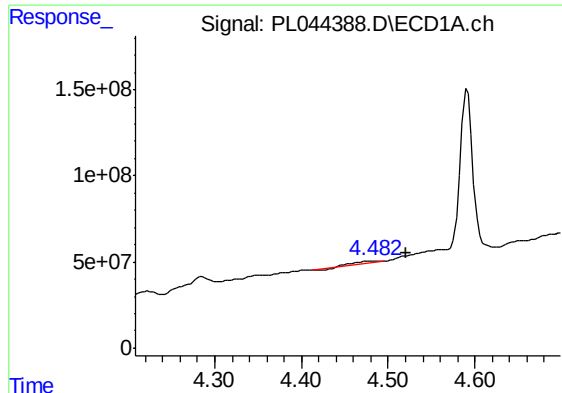

#7 delta-BHC


R.T.: 4.483 min
Delta R.T.: -0.038 min
Response: 13428887
Conc: 2.07 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

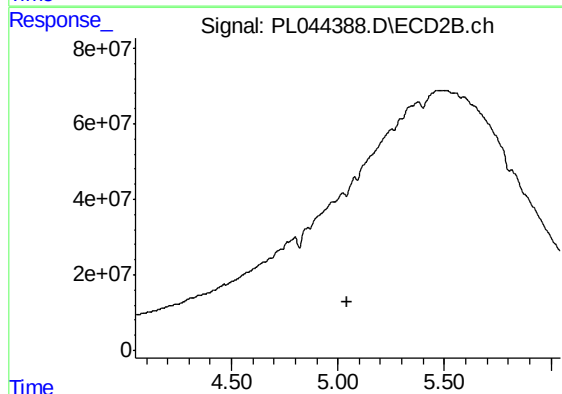


#7 delta-BHC

R.T.: 5.079 min
Delta R.T.: 0.033 min
Response: -4115981
Conc: N.D.

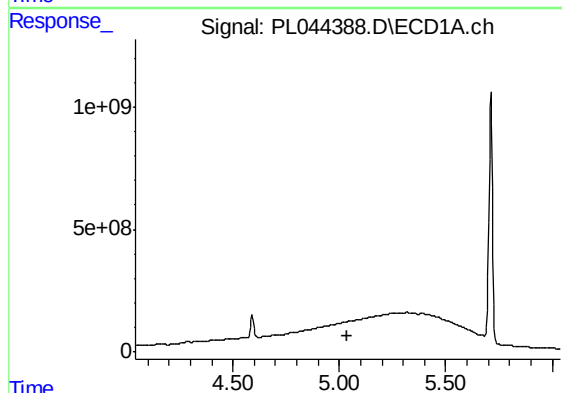


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.039 min
Response: 0
Conc: N.D.

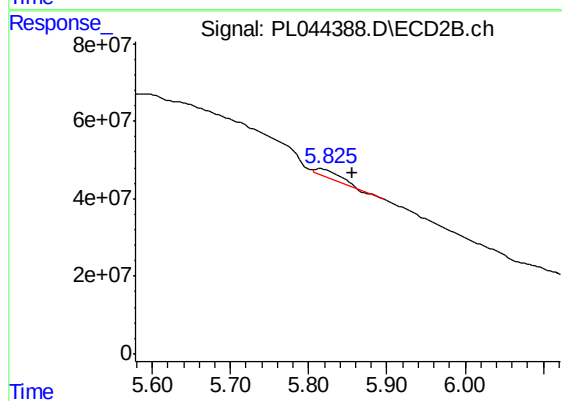

#8 Heptachlor epoxide


R.T.: 5.814 min
Delta R.T.: -0.042 min
Response: 20607588
Conc: 8.91 ng/ml

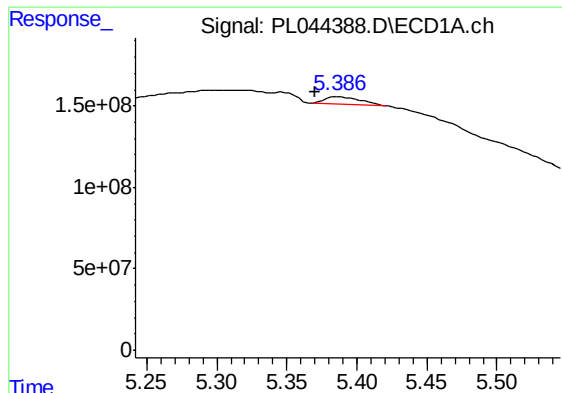

#9 Endosulfan I


R.T.: 5.387 min
Delta R.T.: 0.017 min
Response: 77736853
Conc: 11.03 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

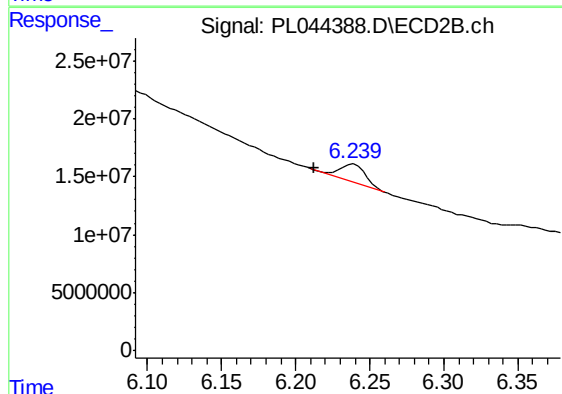


#9 Endosulfan I

R.T.: 6.239 min
Delta R.T.: 0.027 min
Response: 17065240
Conc: 7.37 ng/ml

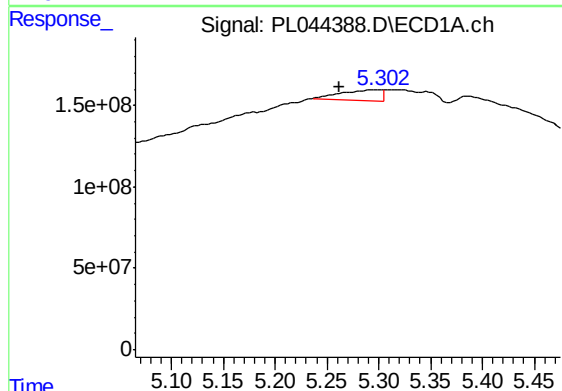


#10 gamma-Chlordane

R.T.: 5.294 min
Delta R.T.: 0.032 min
Response: 168764875
Conc: 21.79 ng/ml

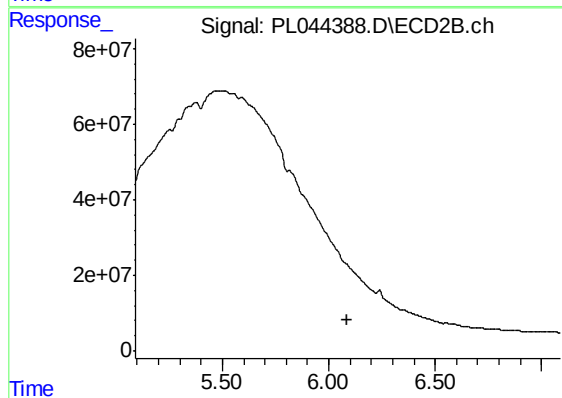

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.090 min
Response: 0
Conc: N.D.

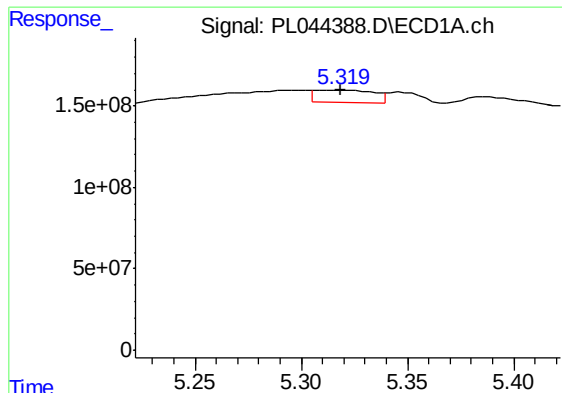

#11 alpha-Chlordane


R.T.: 5.320 min
Delta R.T.: 0.001 min
Response: 139719427
Conc: 18.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

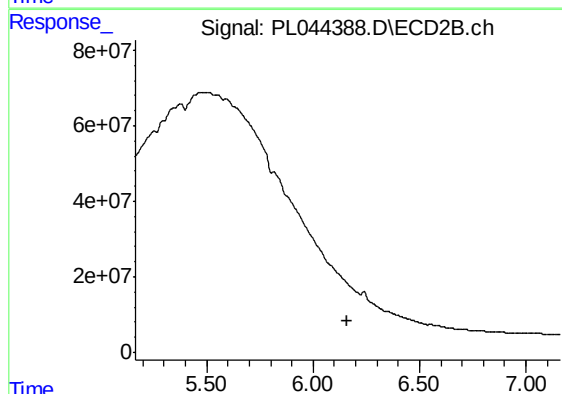


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.162 min
Response: 0
Conc: N.D.

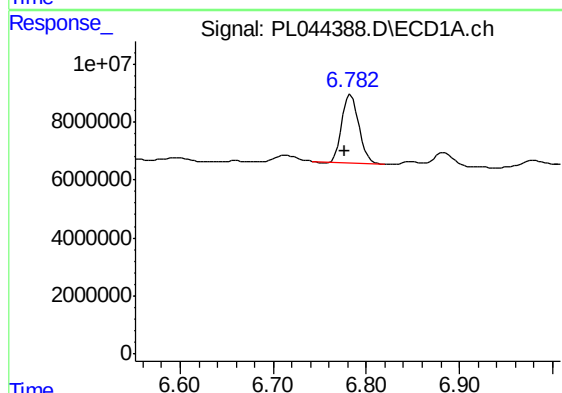


#20 Methoxychlor

R.T.: 6.784 min
Delta R.T.: 0.007 min
Response: 30100403
Conc: 10.15 ng/ml

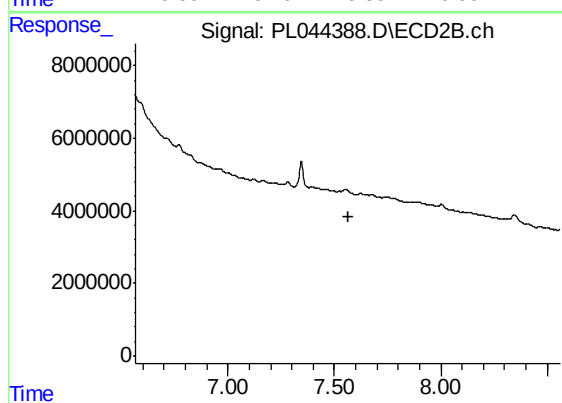

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.565 min
Response: 0
Conc: N.D.

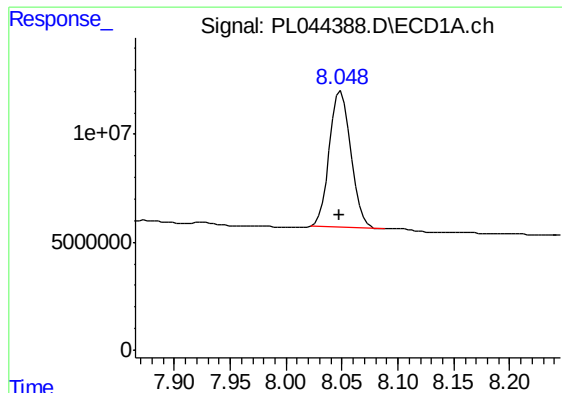

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 84774244
Conc: 12.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

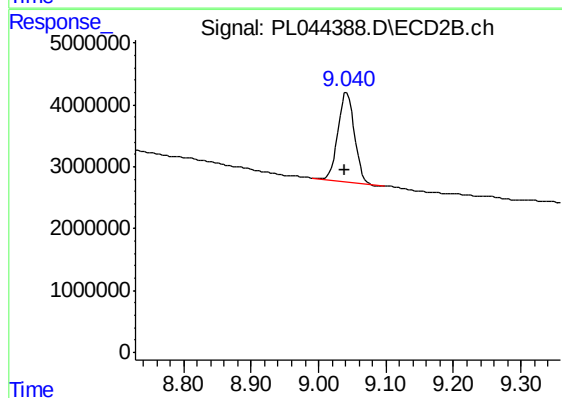

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 24921454
Conc: 11.23 ng/ml