

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
 Data File : PL044380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2019 17:08
 Operator : AJ\SJ
 Sample : K1299-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 0038-AMND-COMP-1

Manual Integrations
 APPROVED

Sohil
 2/4/2019 10:14:53 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 23:12:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.366	3.985	51032543	19089026	8.421	8.751
28) SA Decachlor...	8.048	9.042	55585832	18141681	8.015m	8.178
Target Compounds						
17) MA 4,4'-DDT	6.230	7.108	2575929	1006162	0.505m	0.613m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
Data File : PL044380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2019 17:08
Operator : AJ\SJ
Sample : K1299-05
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
0038-AMND-COMP-1


Manual Integrations
APPROVED

Sohil
2/4/2019 10:14:53 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 23:12:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

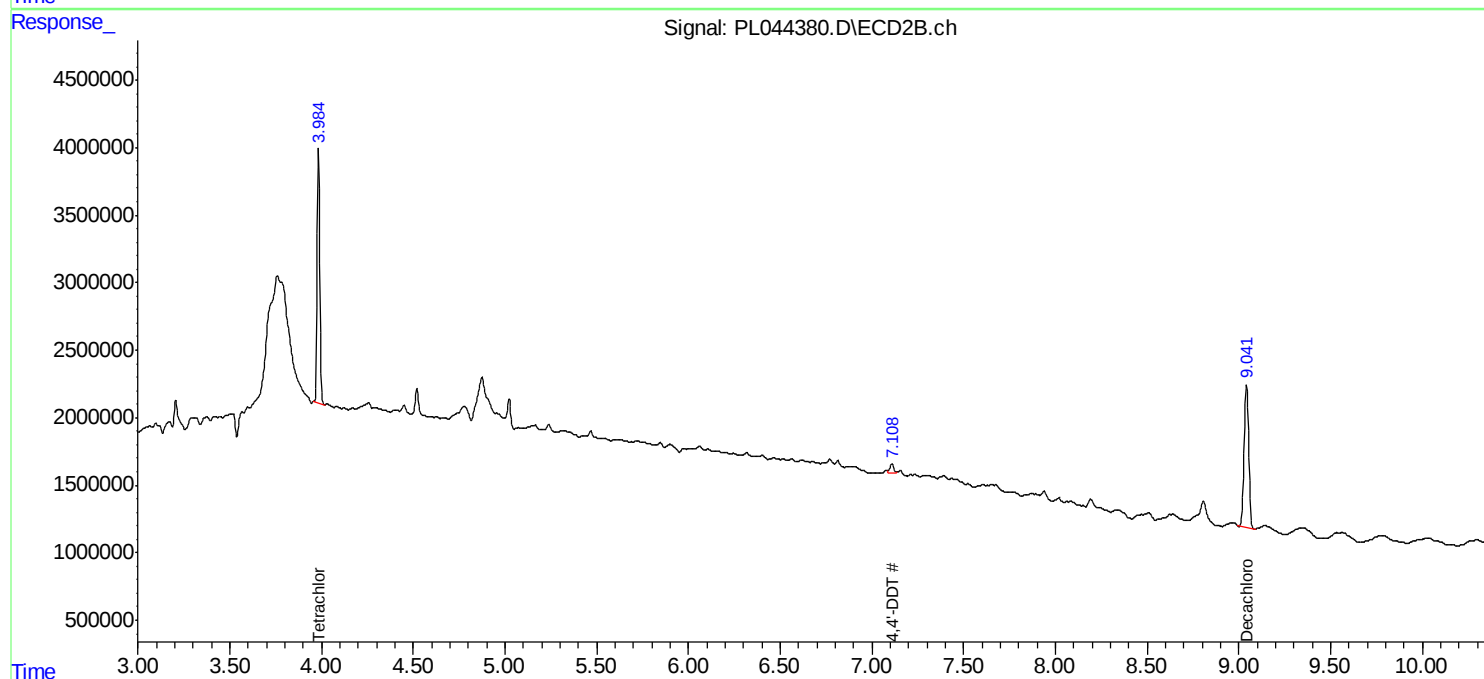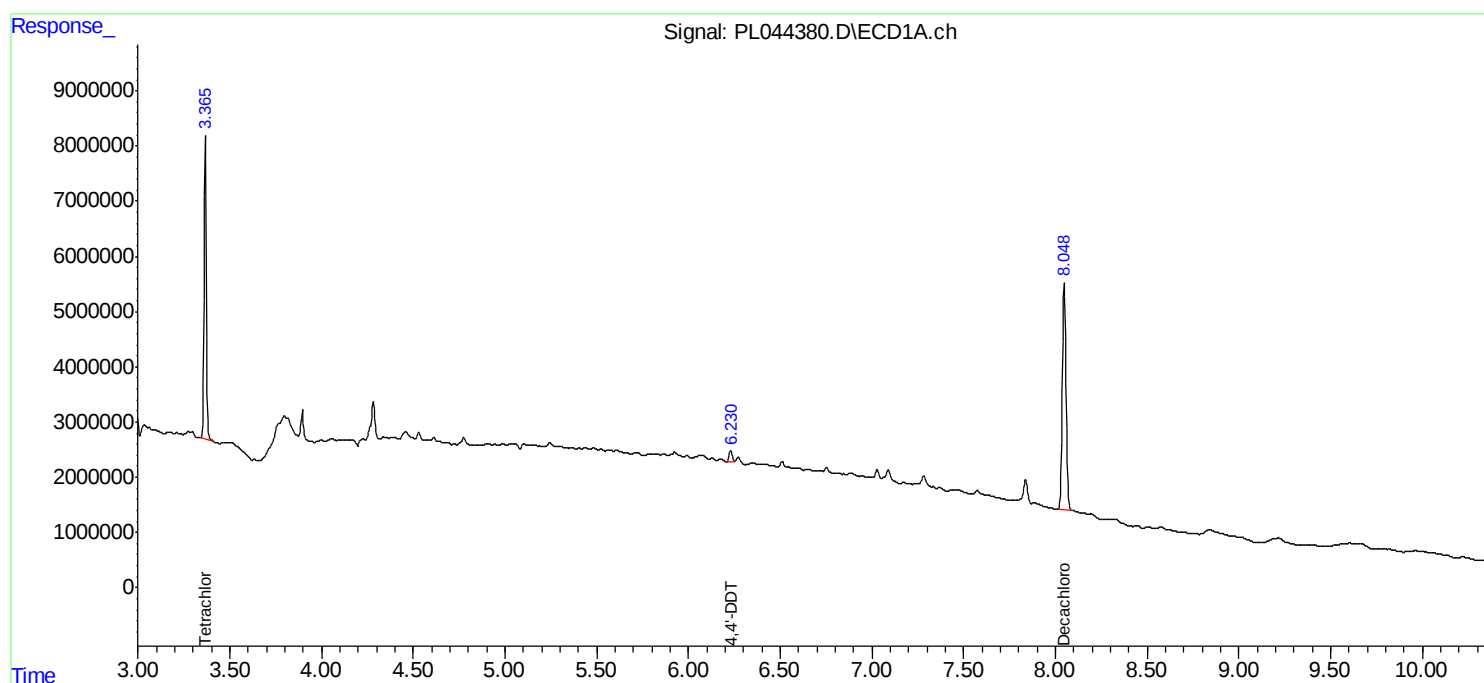

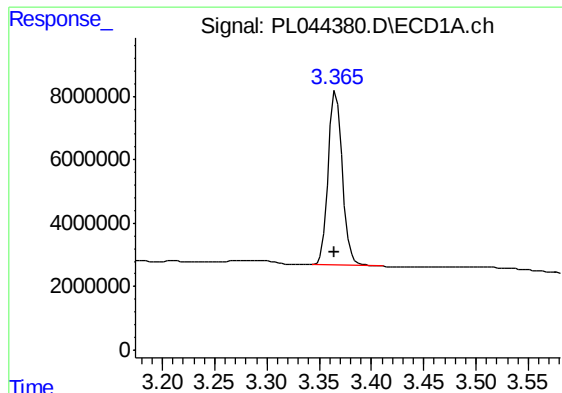


#1 Tetrachloro-m-xylene

R.T.: 3.366 min
Delta R.T.: 0.001 min
Response: 51032543
Conc: 8.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
0038-AMND-COMP-1


Manual Integrations
APPROVED

Sohil
2/4/2019 10:14:53 AM

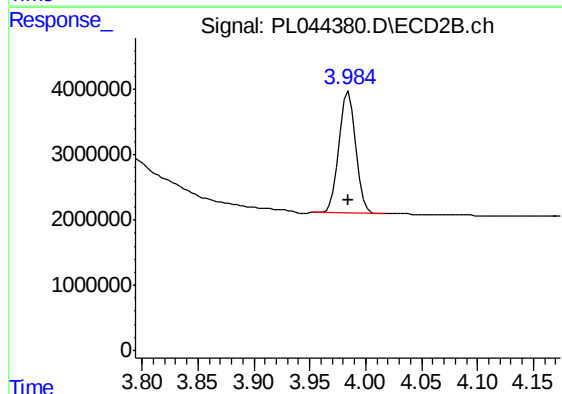


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 19089026
Conc: 8.75 ng/ml

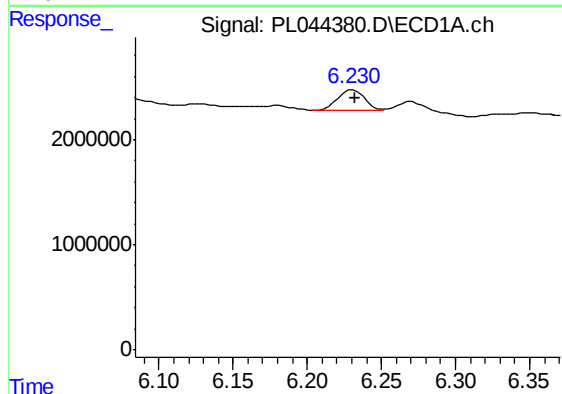


#17 4,4'-DDT

R.T.: 6.230 min
Delta R.T.: -0.003 min
Response: 2575929
Conc: 0.51 ng/ml m

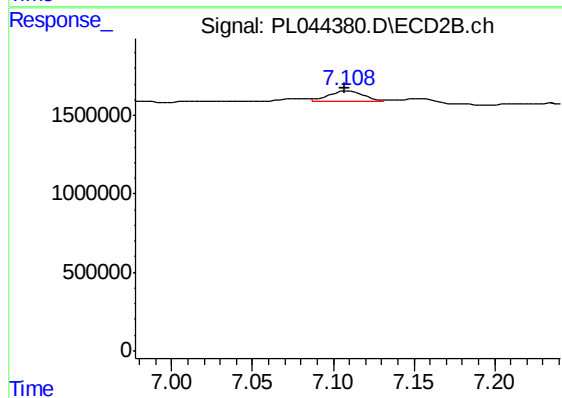

#17 4,4'-DDT

R.T.: 7.108 min
Delta R.T.: 0.000 min
Response: 1006162
Conc: 0.61 ng/ml m

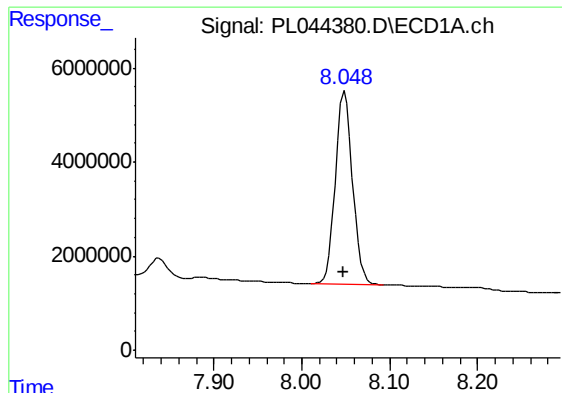


#28 Decachlorobiphenyl

R.T.: 8.048 min
Delta R.T.: 0.000 min
Response: 55585832
Conc: 8.02 ng/ml m

Instrument :
ECD_L
ClientSampleId :
0038-AMND-COMP-1

Manual Integrations
APPROVED

Sohil
2/4/2019 10:14:53 AM

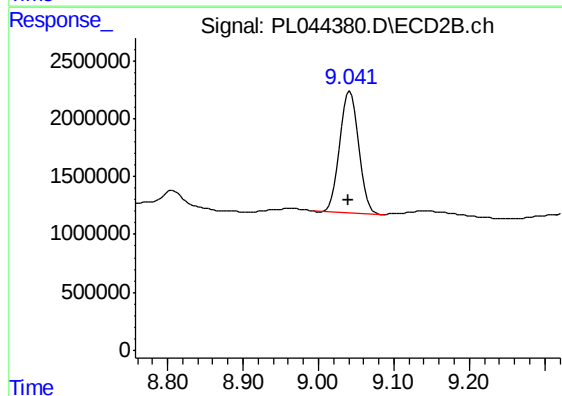

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 18141681
Conc: 8.18 ng/ml