

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
 Data File : PL044388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2019 19:00
 Operator : AJ\SJ
 Sample : K1299-10
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SPLP-LEACH-AMND-COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 01 23:13:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 28 01:20:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.367	3.985	113.9E6	49315049	18.802	22.608
28)	SA Decachlor...	8.049	9.042	84774244	24921454	12.224	11.234

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020119\
Data File : PL044388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2019 19:00
Operator : AJ\SJ
Sample : K1299-10
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 01 23:13:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012219.M
Quant Title : GC Extractables
QLast Update : Mon Jan 28 01:20:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

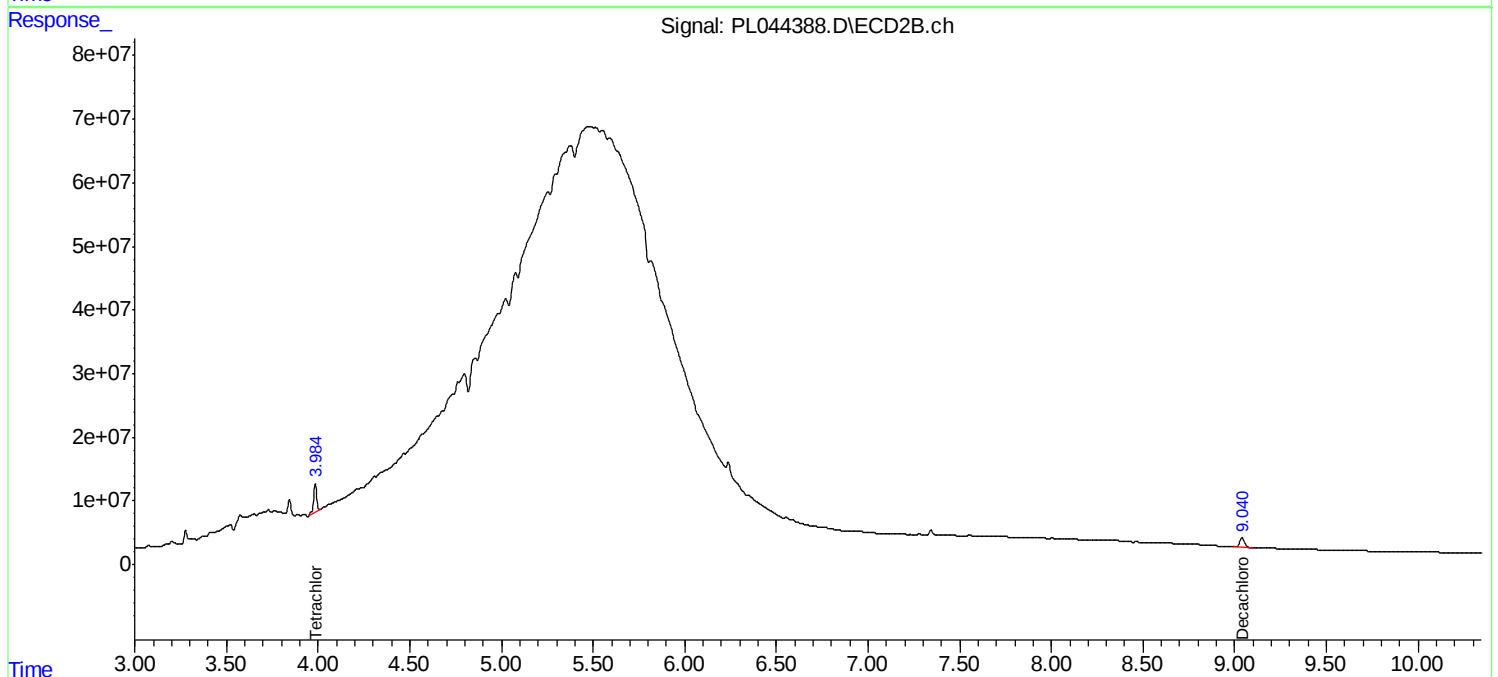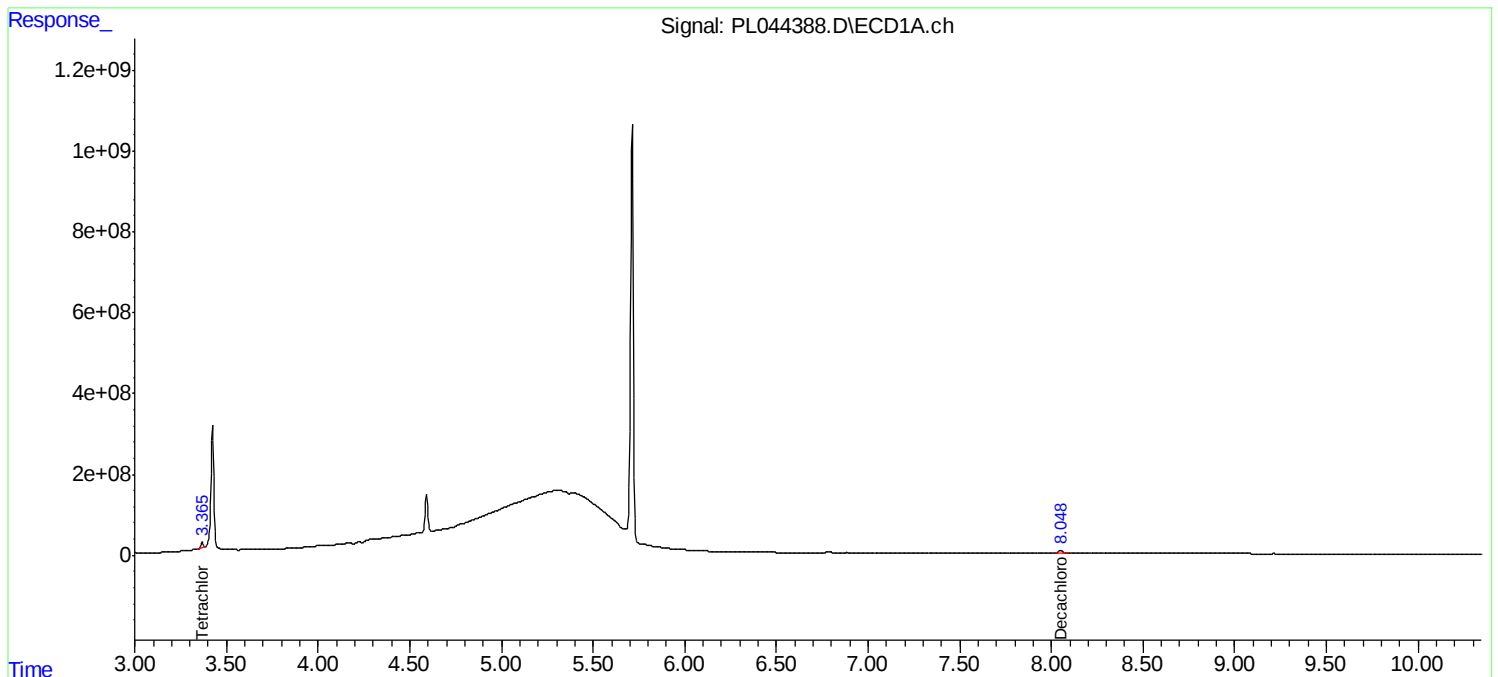


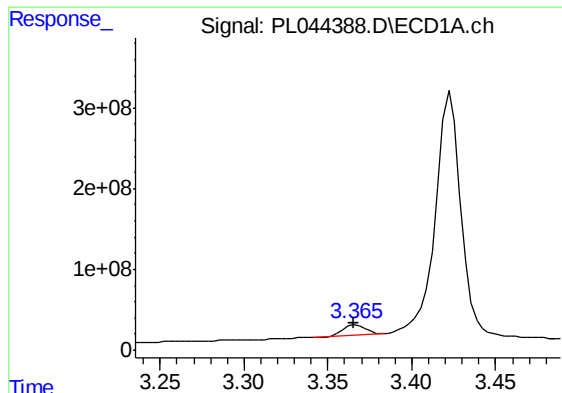

#1 Tetrachloro-m-xylene


R.T.: 3.367 min
Delta R.T.: 0.002 min
Response: 113945192
Conc: 18.80 ng/ml

Instrument :
ECD_L
ClientSampleId :
SPLP-LEACH-AMND-COMP-3

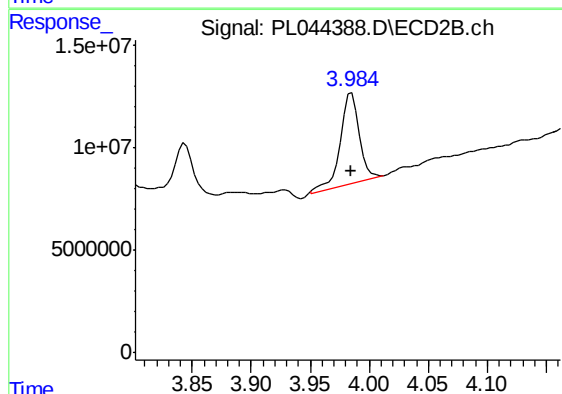


#1 Tetrachloro-m-xylene

R.T.: 3.985 min
Delta R.T.: 0.000 min
Response: 49315049
Conc: 22.61 ng/ml

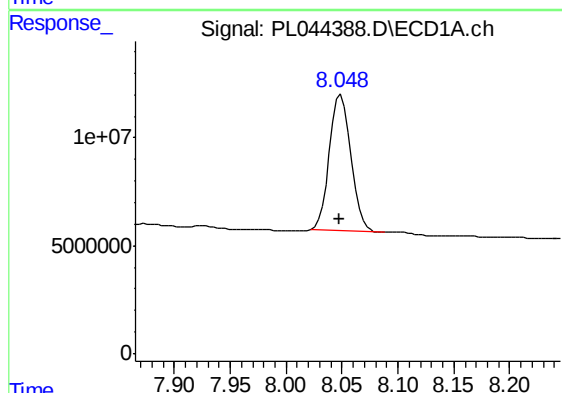

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.002 min
Response: 84774244
Conc: 12.22 ng/ml

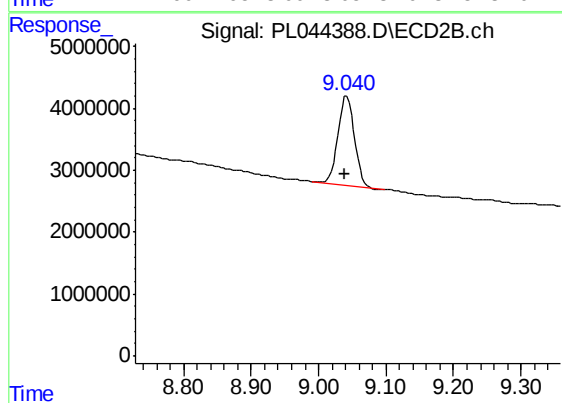

#28 Decachlorobiphenyl

R.T.: 9.042 min
Delta R.T.: 0.002 min
Response: 24921454
Conc: 11.23 ng/ml