

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
 Data File : PL072376.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 09:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:49:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.491	9728051	29501703	17.522	18.165
28)	SA Decachlor...	10.317	11.382	12987727	22175567	14.619	13.744
Target Compounds							
2)	A alpha-BHC	5.285f	0.000	227836	0	0.295	N.D. #
7)	B delta-BHC	0.000	7.017f	0	334817	N.D.	0.136 #
8)	B Heptachlo...	0.000	7.962	0	741378	N.D.	0.370 #
9)	A Endosulfan I	0.000	8.346f	0	27953	N.D.	0.015 #
11)	B alpha-Chl...	0.000	8.317	0	195029	N.D.	0.098 #
14)	MA Endrin	8.000f	0.000	181833	0	0.260	N.D. #
15)	B Endosulfa...	0.000	9.146f	0	1003940	N.D.	0.585 #
18)	B Endrin al...	0.000	9.285f	0	64658	N.D.	0.052 #
26)	Chlordane-4	0.000	8.317	0	195029	N.D.	0.587 #
27)	Chlordane-5	0.000	9.191	0	104792	N.D.	1.717 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
Data File : PL072376.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 09:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:49:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

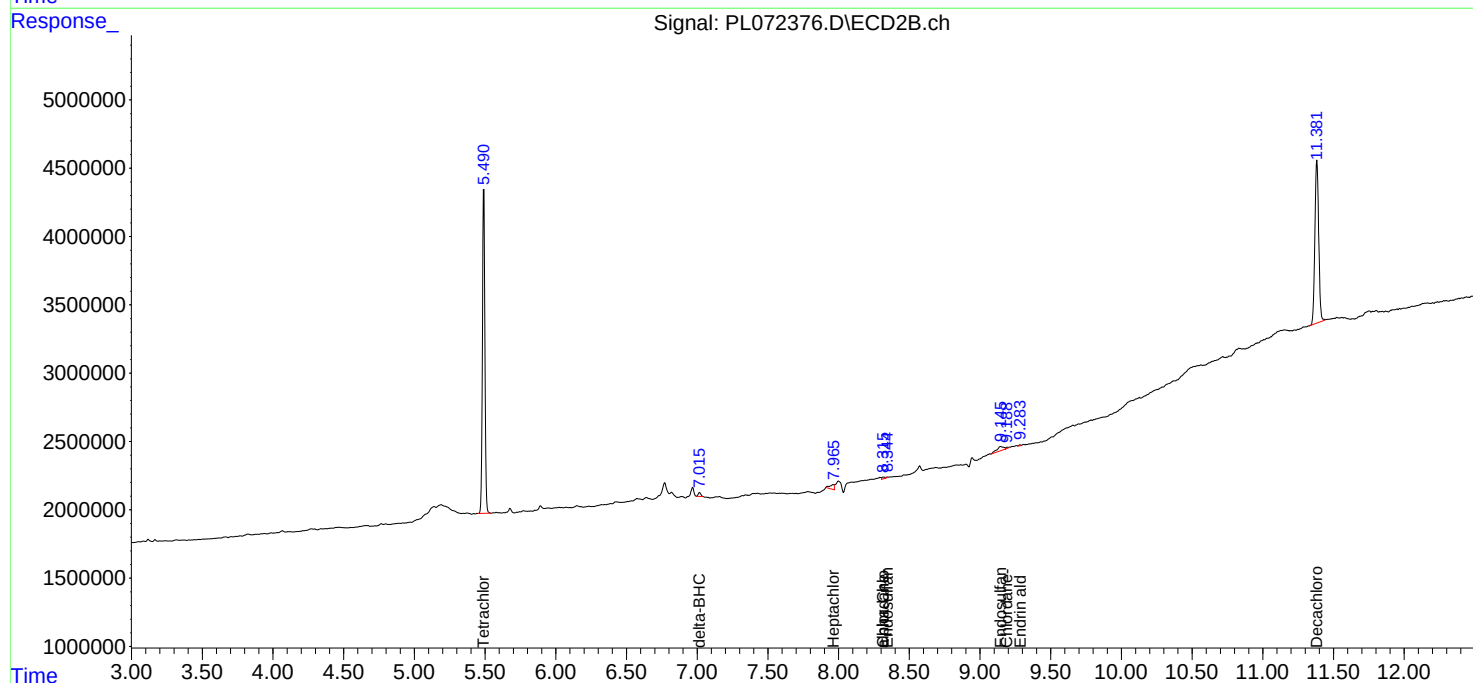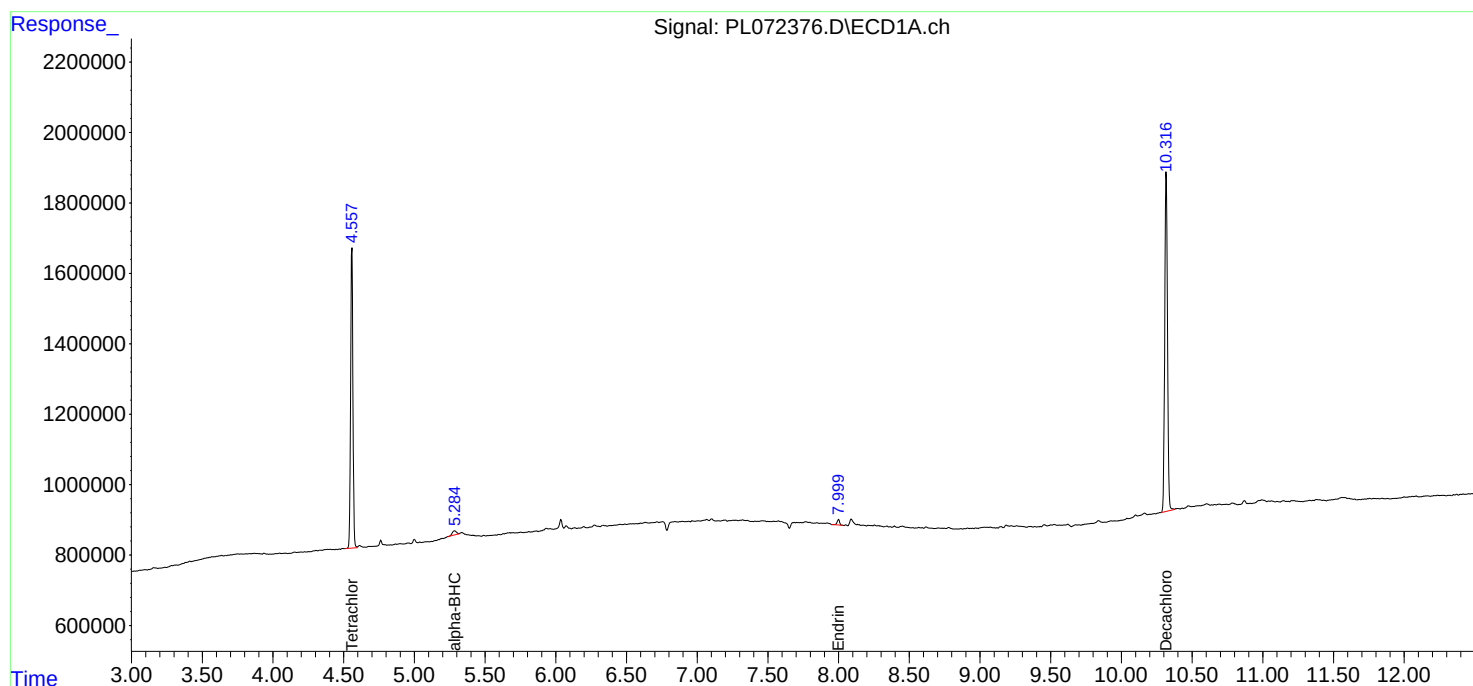


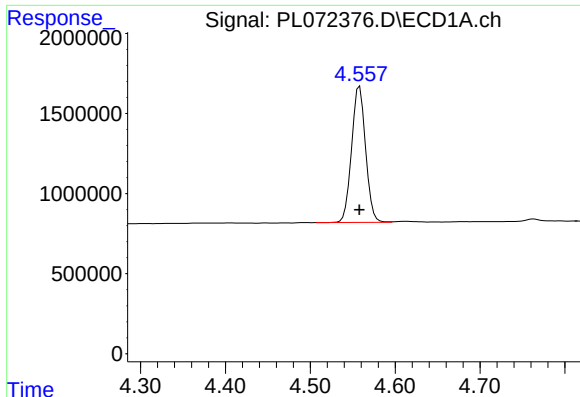

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.000 min
Response: 9728051
Conc: 17.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

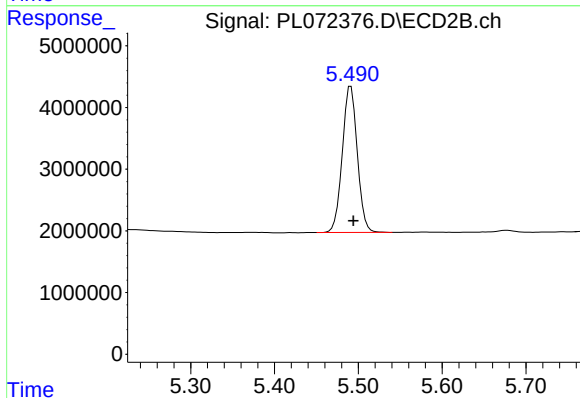


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 29501703
Conc: 18.16 ng/ml

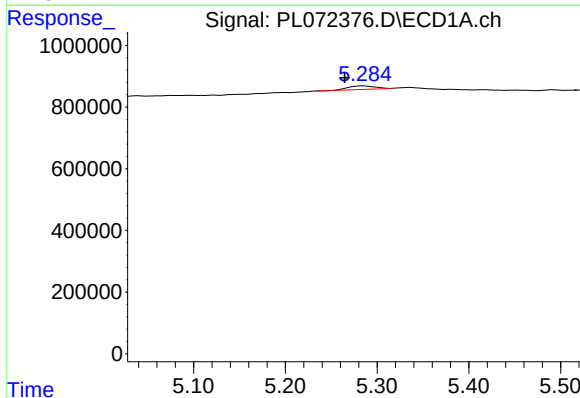


#2 alpha-BHC

R.T.: 5.285 min
Delta R.T.: 0.021 min
Response: 227836
Conc: 0.29 ng/ml

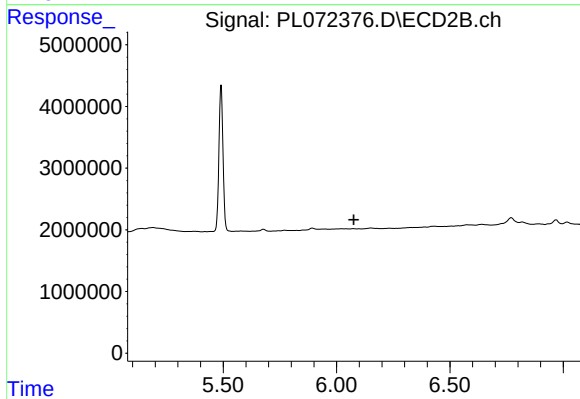

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 6.076 min
Response: 0
Conc: N.D.

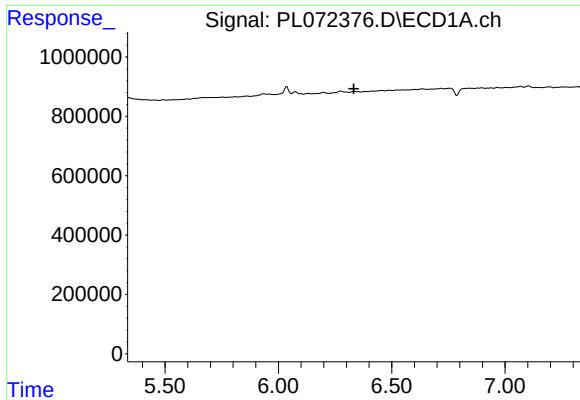

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

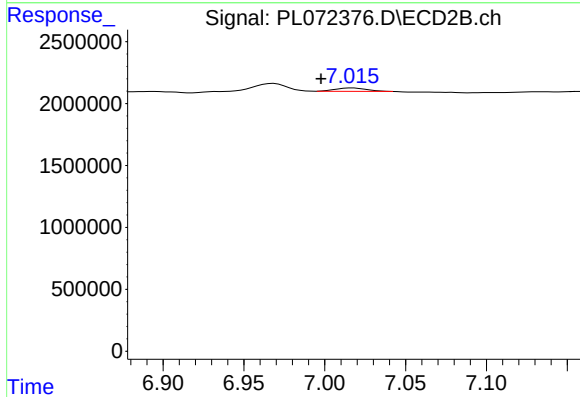


#7 delta-BHC

R.T.: 7.017 min
Delta R.T.: 0.019 min
Response: 334817
Conc: 0.14 ng/ml

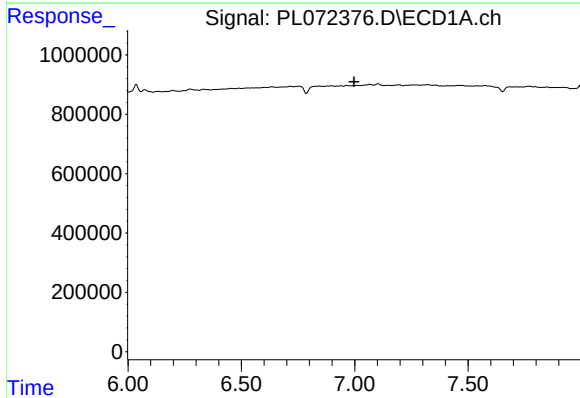


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

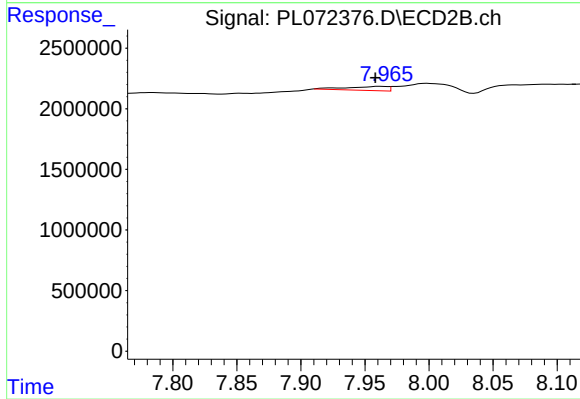

#8 Heptachlor epoxide


R.T.: 7.962 min
Delta R.T.: 0.004 min
Response: 741378
Conc: 0.37 ng/ml

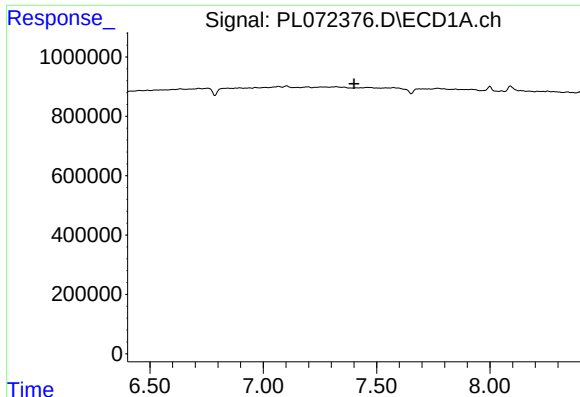

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

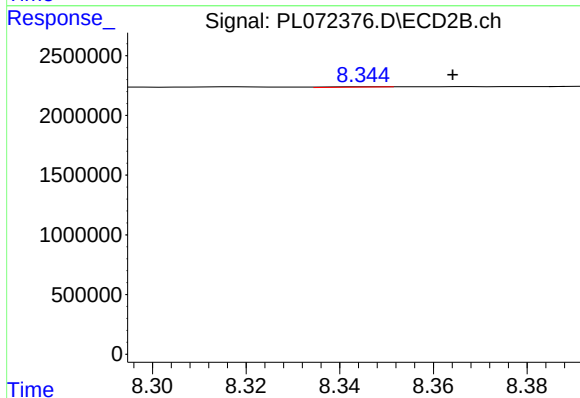


#9 Endosulfan I

R.T.: 8.346 min
Delta R.T.: -0.019 min
Response: 27953
Conc: 0.02 ng/ml

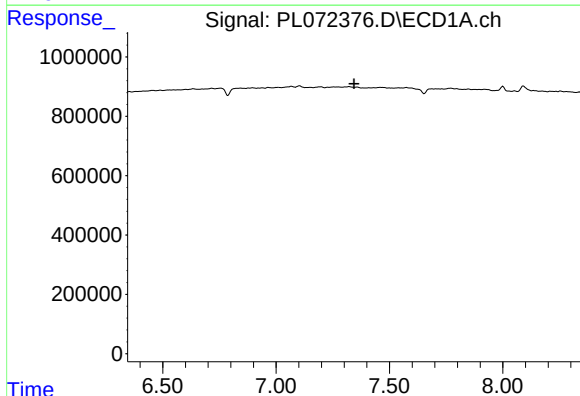


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

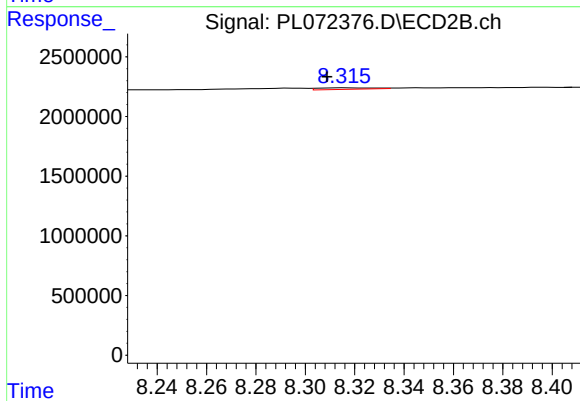

#11 alpha-Chlordane


R.T.: 8.317 min
Delta R.T.: 0.008 min
Response: 195029
Conc: 0.10 ng/ml

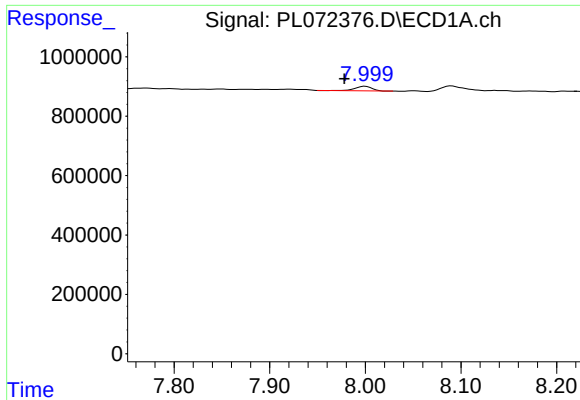

#14 Endrin


R.T.: 8.000 min
Delta R.T.: 0.022 min
Response: 181833
Conc: 0.26 ng/ml

Instrument :
ECD_L
ClientSampleId :

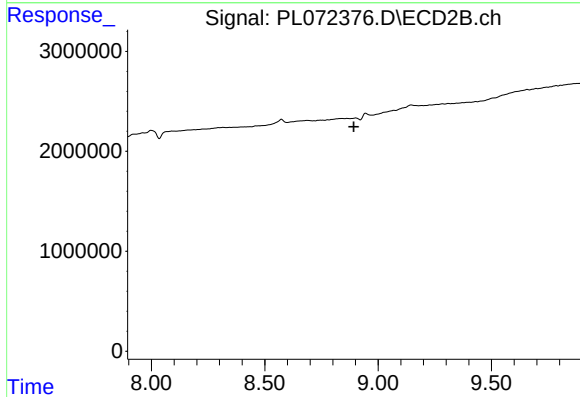


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 8.893 min
Response: 0
Conc: N.D.

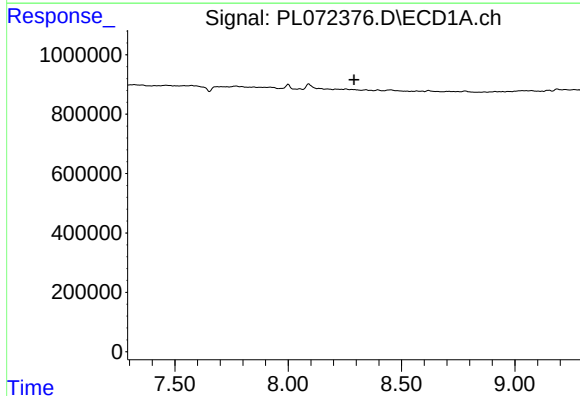


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 8.291 min
Response: 0
Conc: N.D.

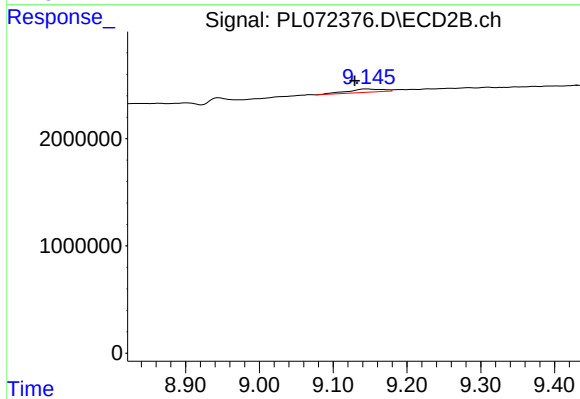

#15 Endosulfan II


R.T.: 9.146 min
Delta R.T.: 0.017 min
Response: 1003940
Conc: 0.59 ng/ml

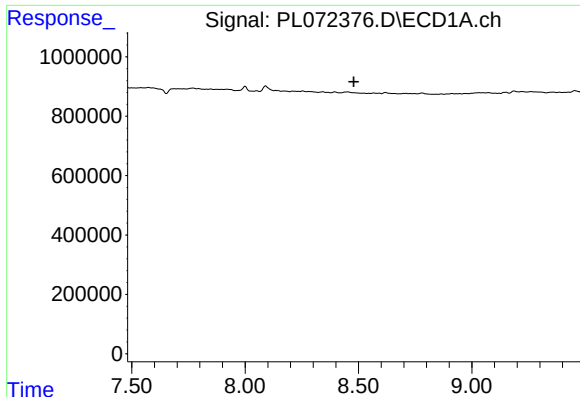

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

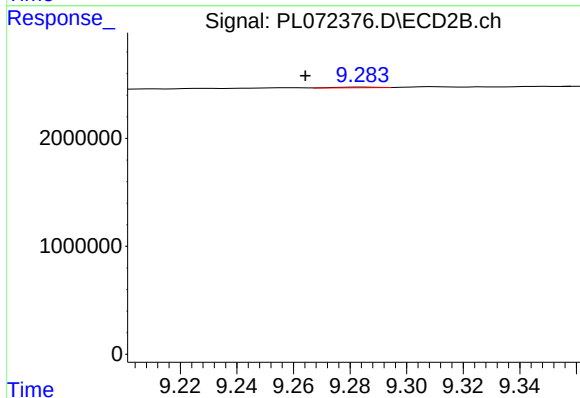


#18 Endrin aldehyde

R.T.: 9.285 min
Delta R.T.: 0.020 min
Response: 64658
Conc: 0.05 ng/ml

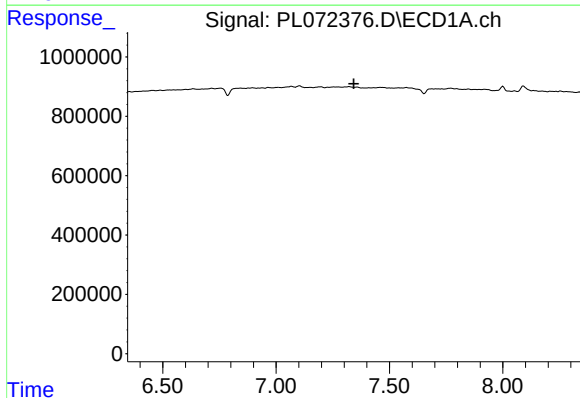


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

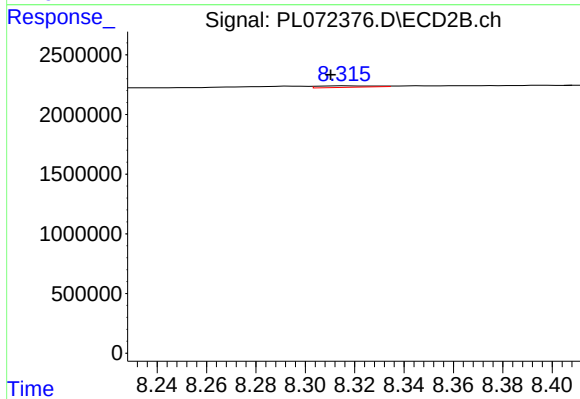

#26 Chlordane-4


R.T.: 8.317 min
Delta R.T.: 0.006 min
Response: 195029
Conc: 0.59 ng/ml

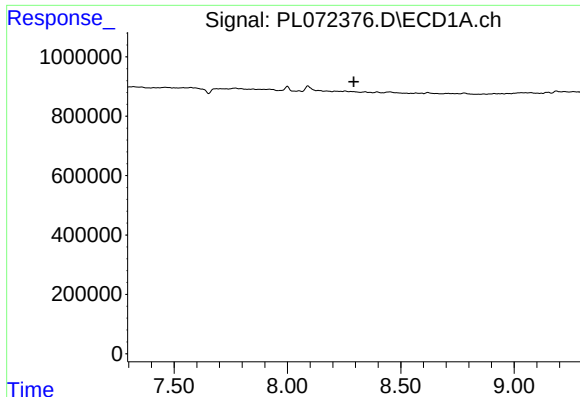

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

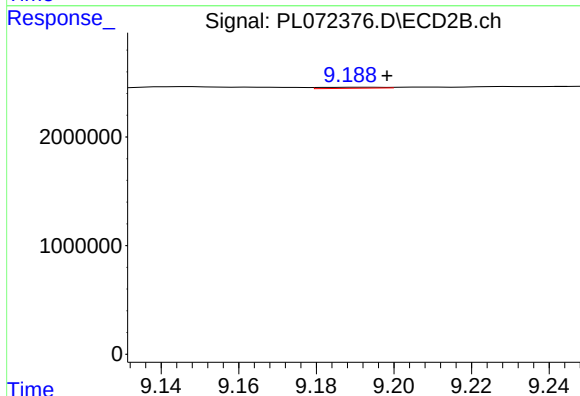


#27 Chlordane-5

R.T.: 9.191 min
Delta R.T.: -0.007 min
Response: 104792
Conc: 1.72 ng/ml

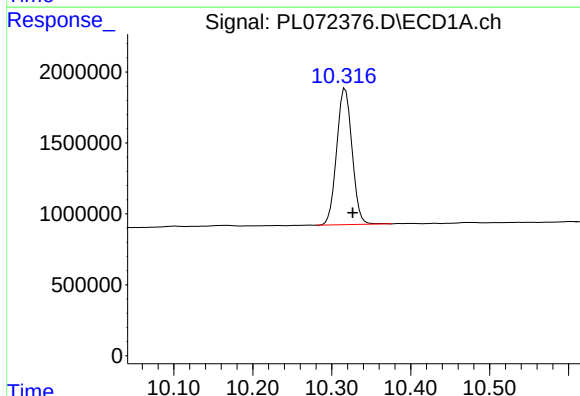

#28 Decachlorobiphenyl

R.T.: 10.317 min
Delta R.T.: -0.009 min
Response: 12987727
Conc: 14.62 ng/ml

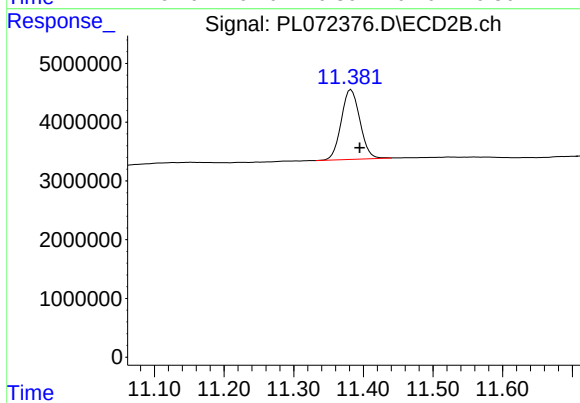

#28 Decachlorobiphenyl

R.T.: 11.382 min
Delta R.T.: -0.012 min
Response: 22175567
Conc: 13.74 ng/ml