

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
 Data File : PL072394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 17:35
 Operator : AR\AJ
 Sample : PB142378BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:57:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.490	8863152	28154420	15.964	17.335
28)	SA Decachlor...	10.315	11.381	15078053	24245457	16.971	15.027
Target Compounds							
5)	MB Aldrin	0.000	7.484	0	1046680	N.D.	0.473 #
7)	B delta-BHC	0.000	7.014f	0	2216334	N.D.	0.901 #
10)	B gamma-Chl...	0.000	8.240	0	55378	N.D.	0.027 #
11)	B alpha-Chl...	0.000	8.333f	0	106271	N.D.	0.054 #
13)	MA Dieldrin	0.000	8.656	0	32032	N.D.	0.016 #
15)	B Endosulfa...	0.000	9.146f	0	412434	N.D.	0.240 #
17)	MA 4,4'-DDT	0.000	9.362	0	207830	N.D.	0.131 #
20)	A Methoxychlor	0.000	9.874f	0	185467	N.D.	0.224 #
24)	Chlordane-2	0.000	7.484	0	1046680	N.D.	14.975 #
25)	Chlordane-3	0.000	8.240	0	55378	N.D.	0.199 #
26)	Chlordane-4	0.000	8.333f	0	106271	N.D.	0.320 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
Data File : PL072394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 17:35
Operator : AR\AJ
Sample : PB142378BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:57:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

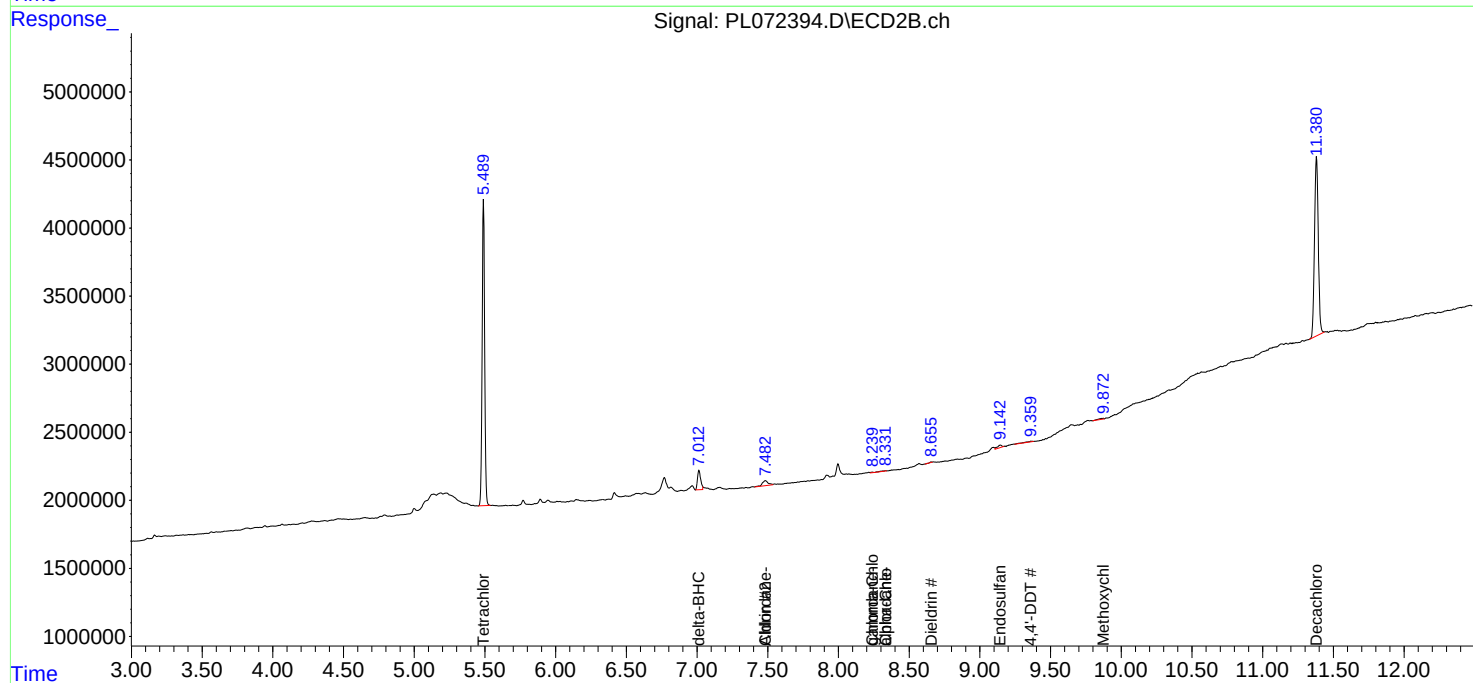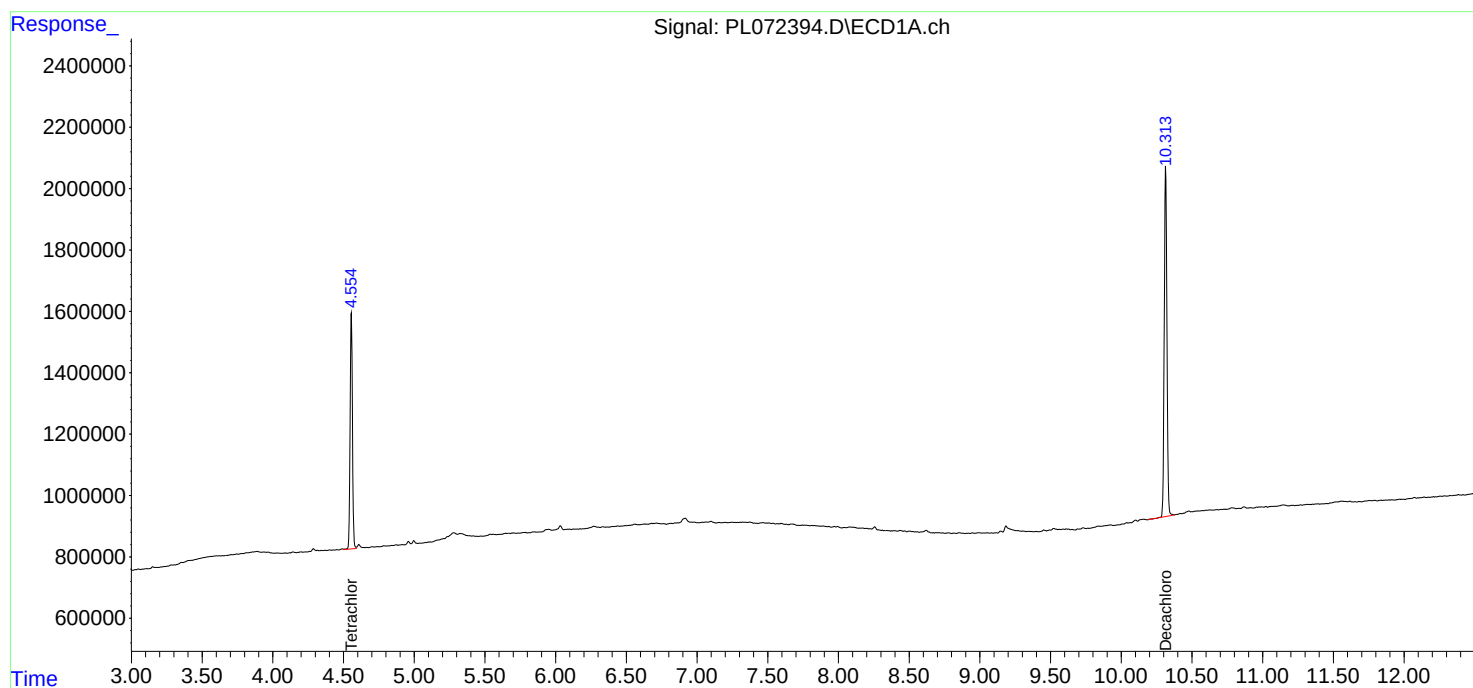


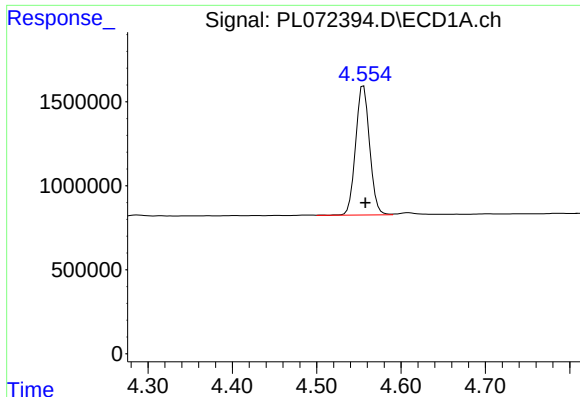

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 8863152
Conc: 15.96 ng/ml

Instrument :
ECD_L
ClientSampleId :

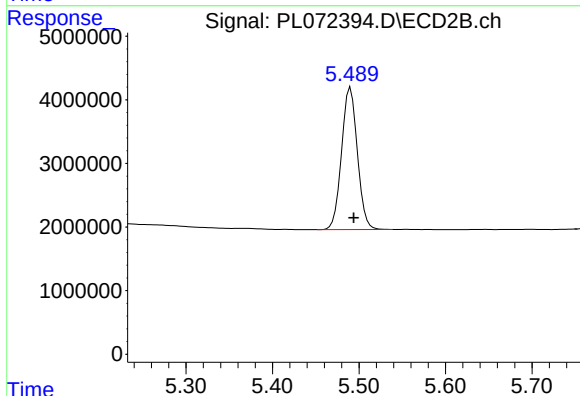


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.004 min
Response: 28154420
Conc: 17.34 ng/ml

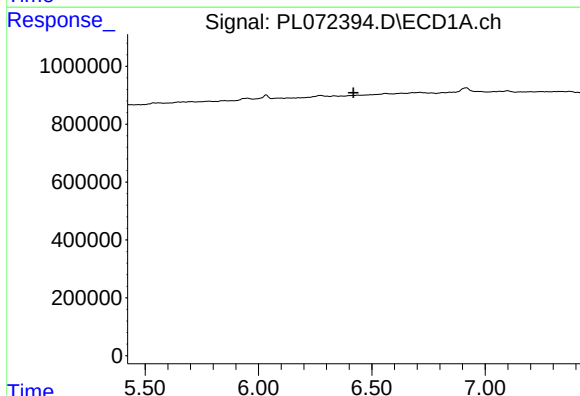


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.419 min
Response: 0
Conc: N.D.

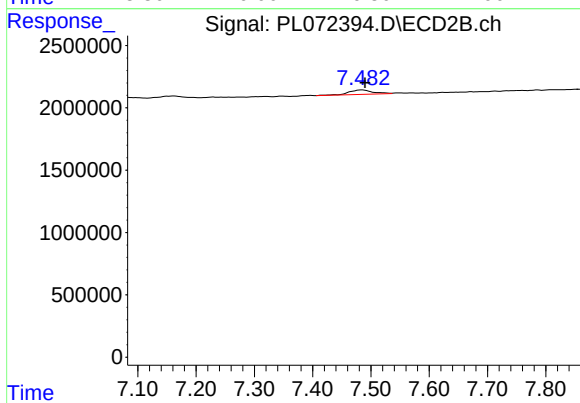

#5 Aldrin


R.T.: 7.484 min
Delta R.T.: -0.006 min
Response: 1046680
Conc: 0.47 ng/ml

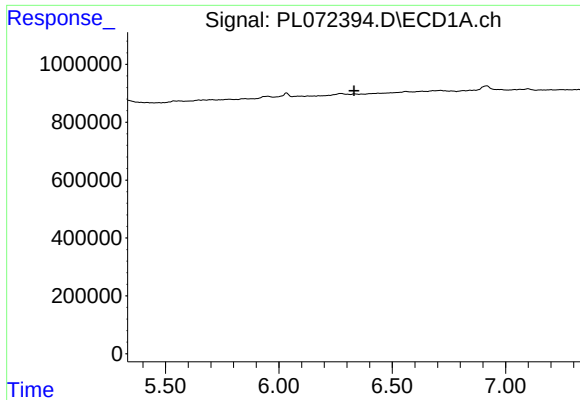

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.332 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

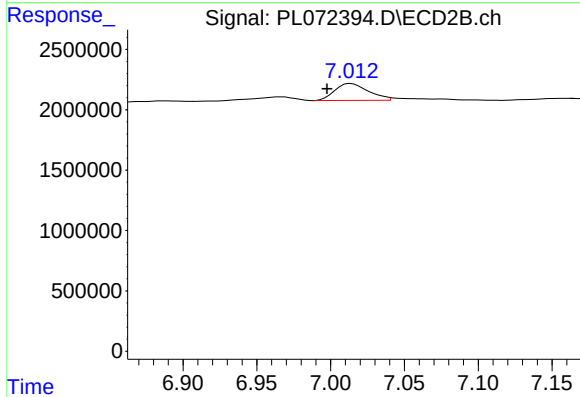


#7 delta-BHC

R.T.: 7.014 min
Delta R.T.: 0.016 min
Response: 2216334
Conc: 0.90 ng/ml

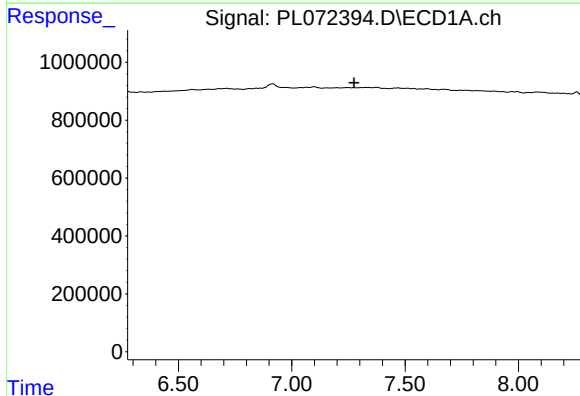


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

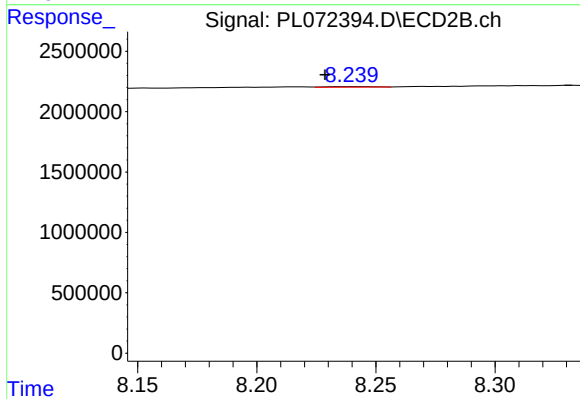

#10 gamma-Chlordane


R.T.: 8.240 min
Delta R.T.: 0.011 min
Response: 55378
Conc: 0.03 ng/ml

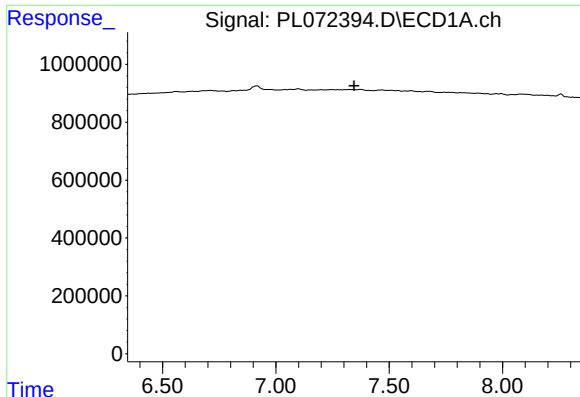

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

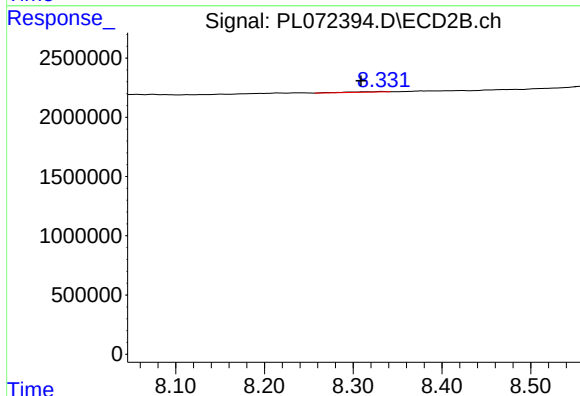


#11 alpha-Chlordane

R.T.: 8.333 min
Delta R.T.: 0.024 min
Response: 106271
Conc: 0.05 ng/ml

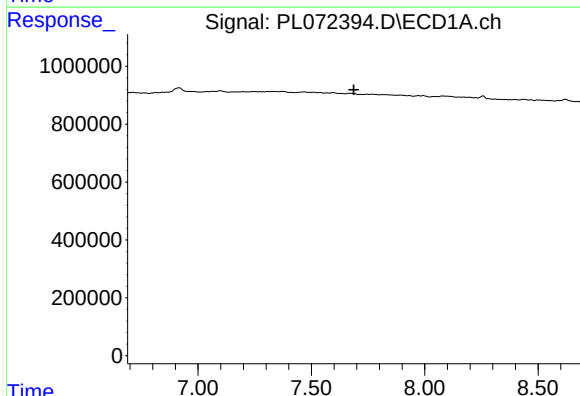


#13 Dieldrin

R.T.: 0.000 min
Exp R.T.: 7.686 min
Response: 0
Conc: N.D.

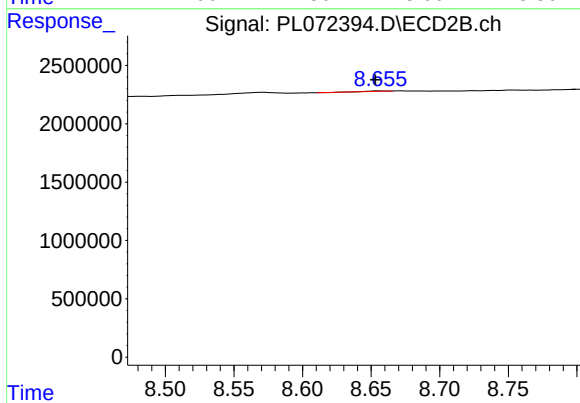

#13 Dieldrin


R.T.: 8.656 min
Delta R.T.: 0.003 min
Response: 32032
Conc: 0.02 ng/ml

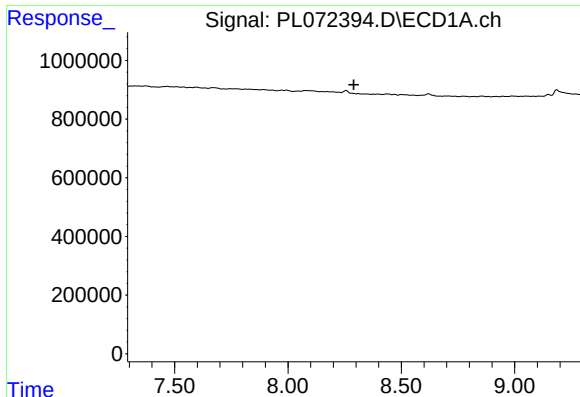

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

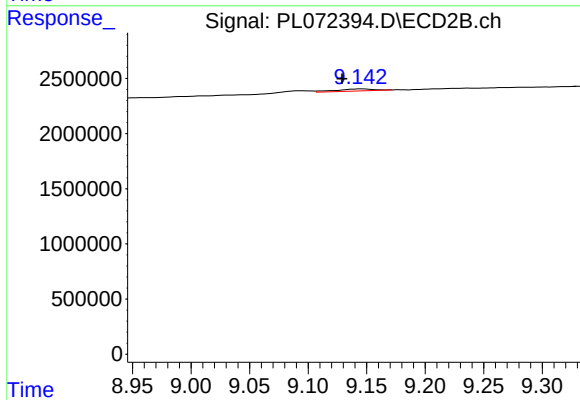


#15 Endosulfan II

R.T.: 9.146 min
Delta R.T.: 0.016 min
Response: 412434
Conc: 0.24 ng/ml

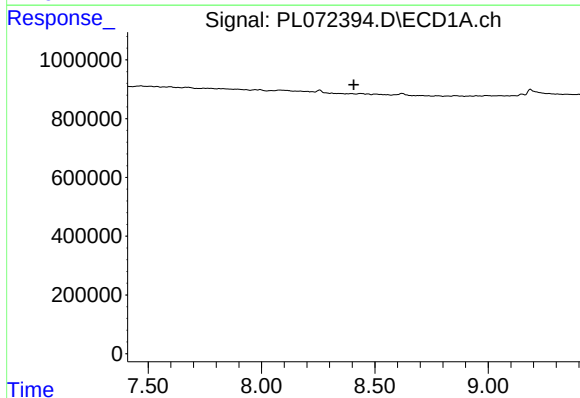


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

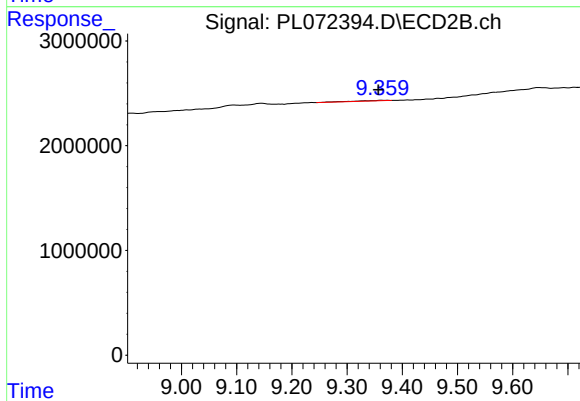

#17 4,4'-DDT


R.T.: 9.362 min
Delta R.T.: 0.005 min
Response: 207830
Conc: 0.13 ng/ml

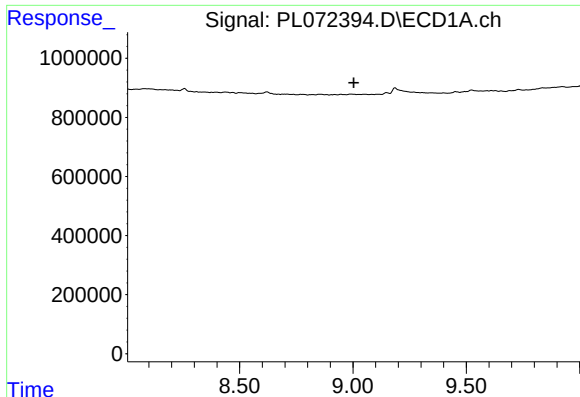

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.004 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

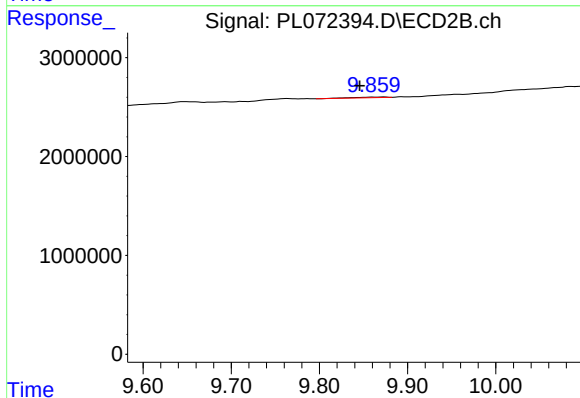


#20 Methoxychlor

R.T.: 9.874 min
Delta R.T.: 0.028 min
Response: 185467
Conc: 0.22 ng/ml

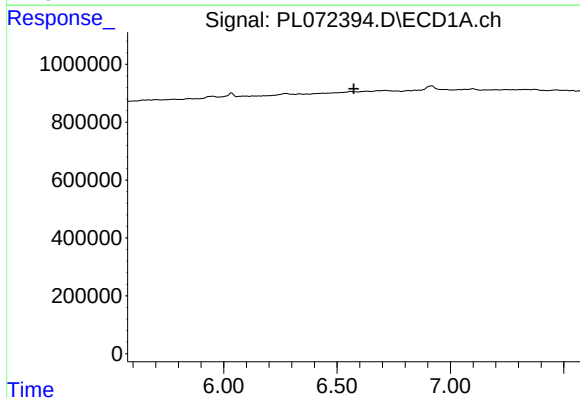


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.574 min
Response: 0
Conc: N.D.

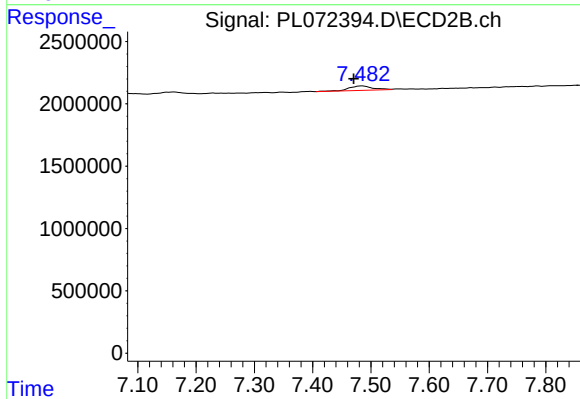

#24 Chlordane-2


R.T.: 7.484 min
Delta R.T.: 0.014 min
Response: 1046680
Conc: 14.98 ng/ml

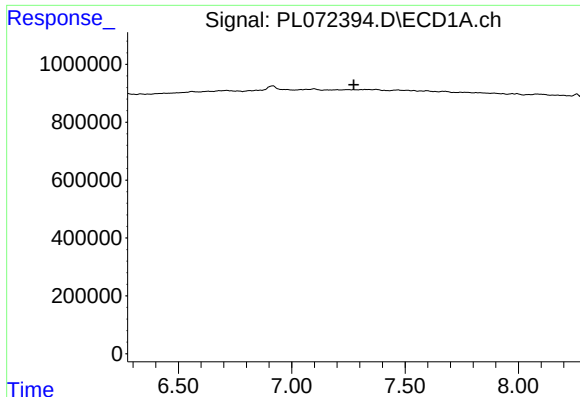

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

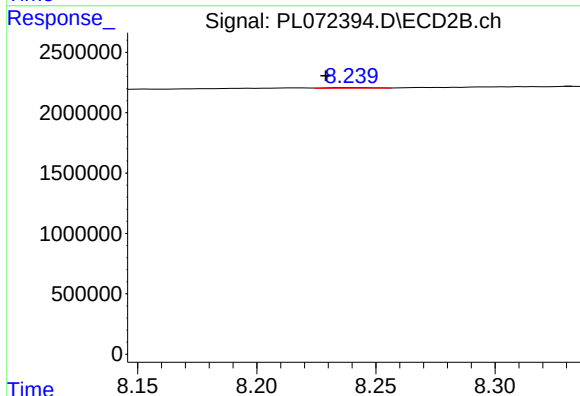


#25 Chlordane-3

R.T.: 8.240 min
Delta R.T.: 0.011 min
Response: 55378
Conc: 0.20 ng/ml

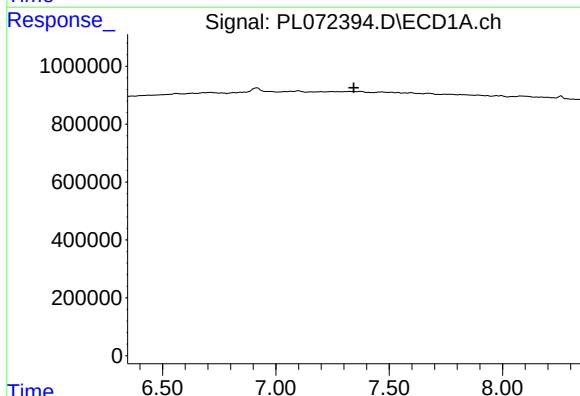


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

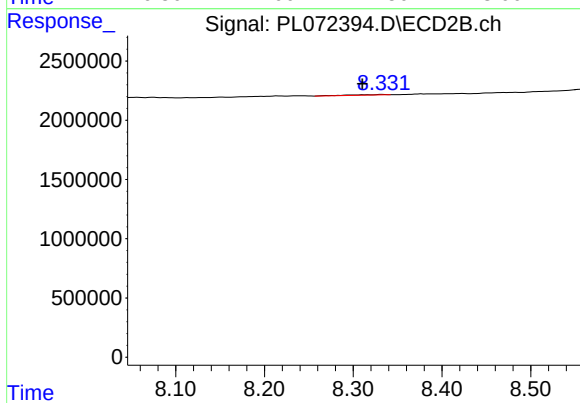

#26 Chlordane-4


R.T.: 8.333 min
Delta R.T.: 0.023 min
Response: 106271
Conc: 0.32 ng/ml

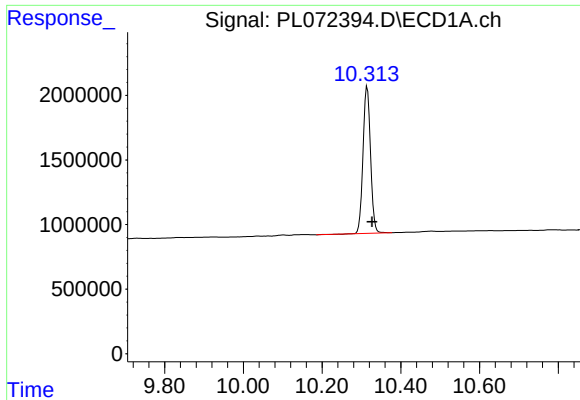

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: -0.012 min
Response: 15078053
Conc: 16.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

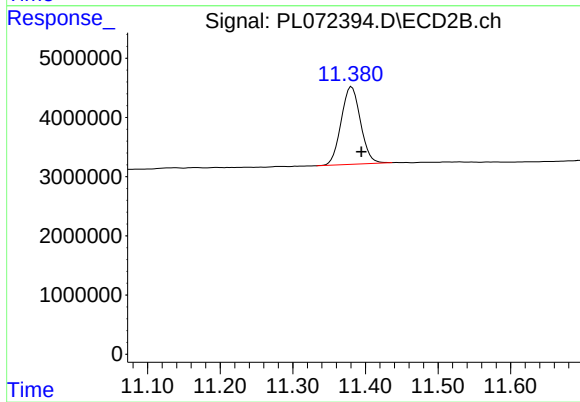

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: -0.014 min
Response: 24245457
Conc: 15.03 ng/ml