

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
 Data File : PL072380.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 13:11
 Operator : AR\AJ
 Sample : N1303-03 (Sig #1); N1303-+03 (Sig #2)
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 CC-6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:51:14 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.490	3830168	11542833	6.899m	7.107
28)	SA Decachlor...	10.315	11.381	7559312	11745016	8.509	7.279
Target Compounds							
12)	B 4,4'-DDE	7.554	8.490	777027	1575341	1.076	0.833



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
Data File : PL072380.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 13:11
Operator : AR\AJ
Sample : N1303-03 (Sig #1); N1303-+03 (Sig #2)
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CC-6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:51:14 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

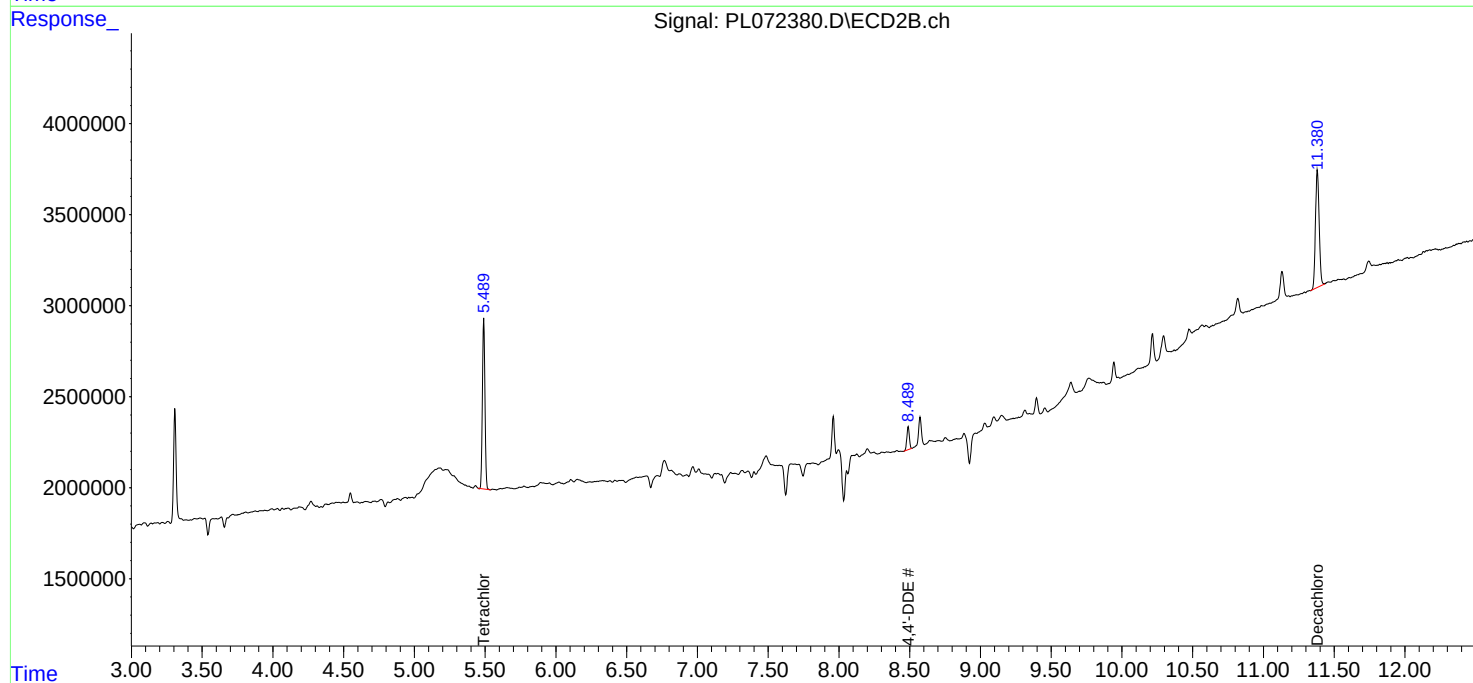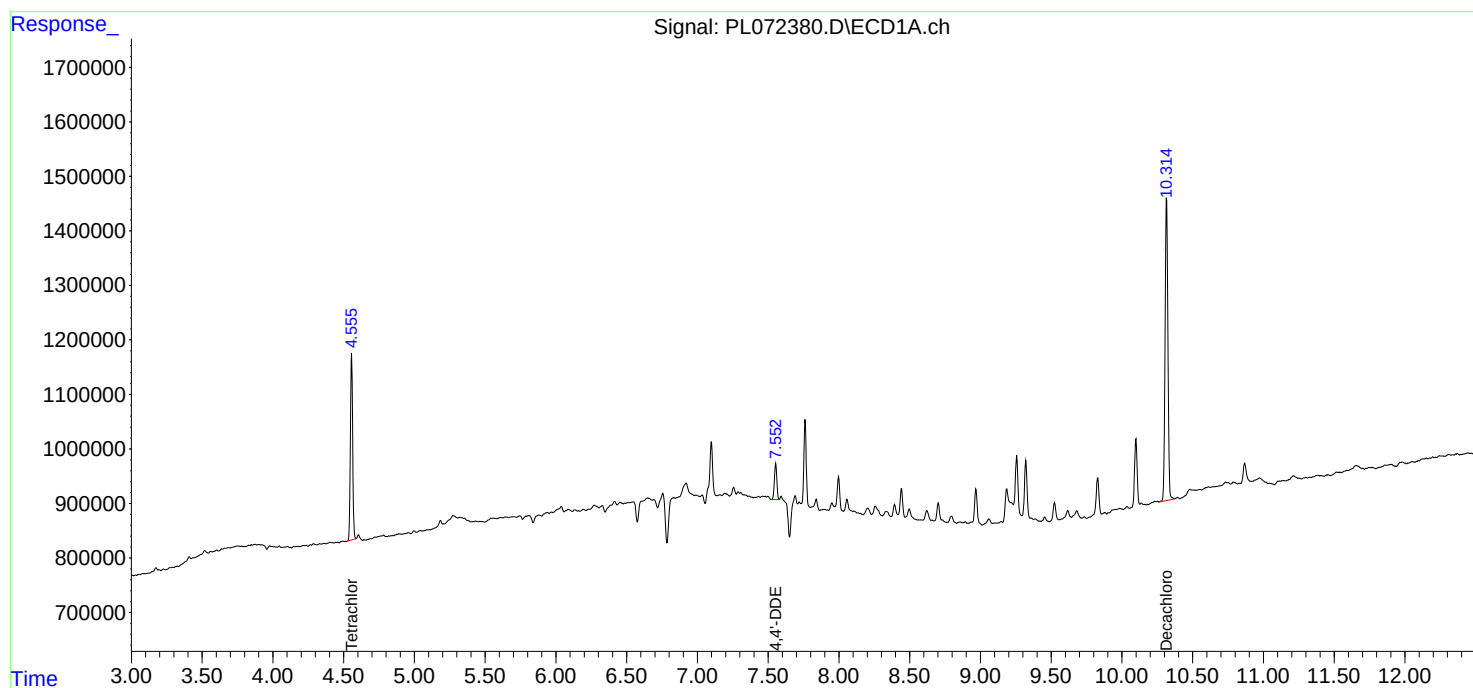


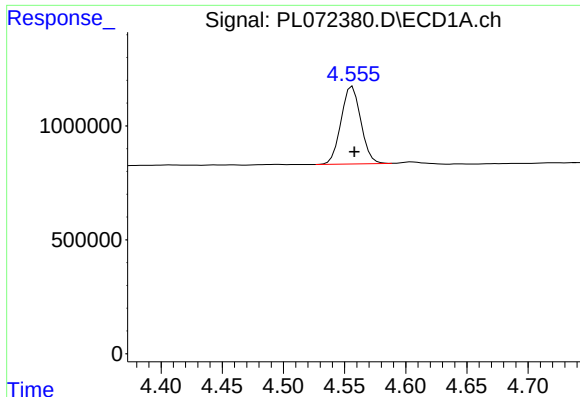

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 3830168
Conc: 6.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
CC-6

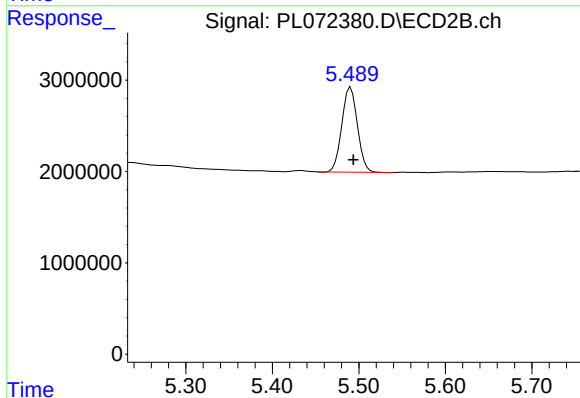


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.003 min
Response: 11542833
Conc: 7.11 ng/ml

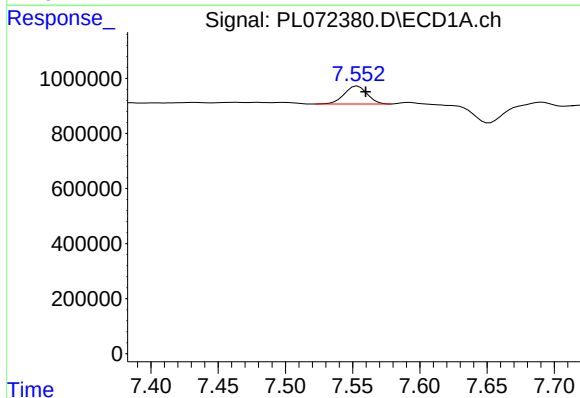


#12 4,4'-DDE

R.T.: 7.554 min
Delta R.T.: -0.006 min
Response: 777027
Conc: 1.08 ng/ml

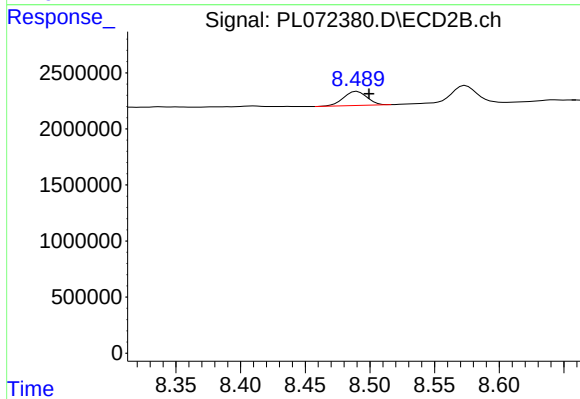

#12 4,4'-DDE


R.T.: 8.490 min
Delta R.T.: -0.009 min
Response: 1575341
Conc: 0.83 ng/ml

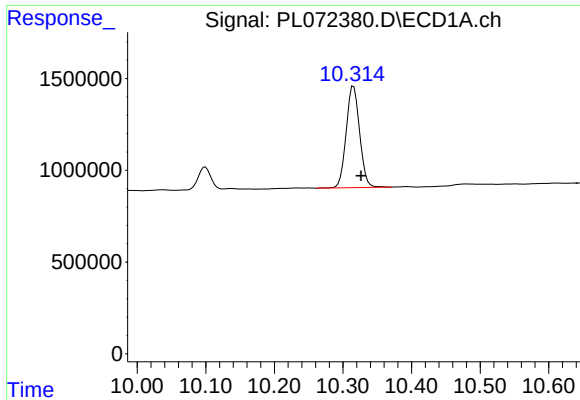

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: -0.011 min
Response: 7559312
Conc: 8.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
CC-6

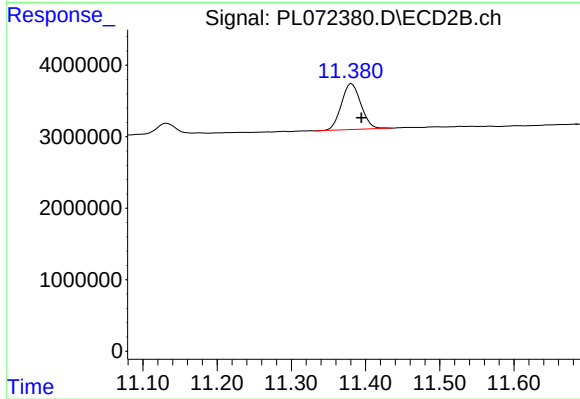

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: -0.013 min
Response: 11745016
Conc: 7.28 ng/ml