

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
 Data File : PL072385.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Feb 2022 14:38
 Operator : AR\AJ
 Sample : N1325-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TES-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 02 01:53:43 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.556	5.491	8850976	28523906	15.942	17.563
28)	SA Decachlor...	10.315	11.381	12776321	21928627	14.381	13.591
Target Compounds							
17)	MA 4,4'-DDT	8.396	9.349	345950	509782	0.521m	0.323 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020122\
Data File : PL072385.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Feb 2022 14:38
Operator : AR\AJ
Sample : N1325-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TES-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 02 01:53:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

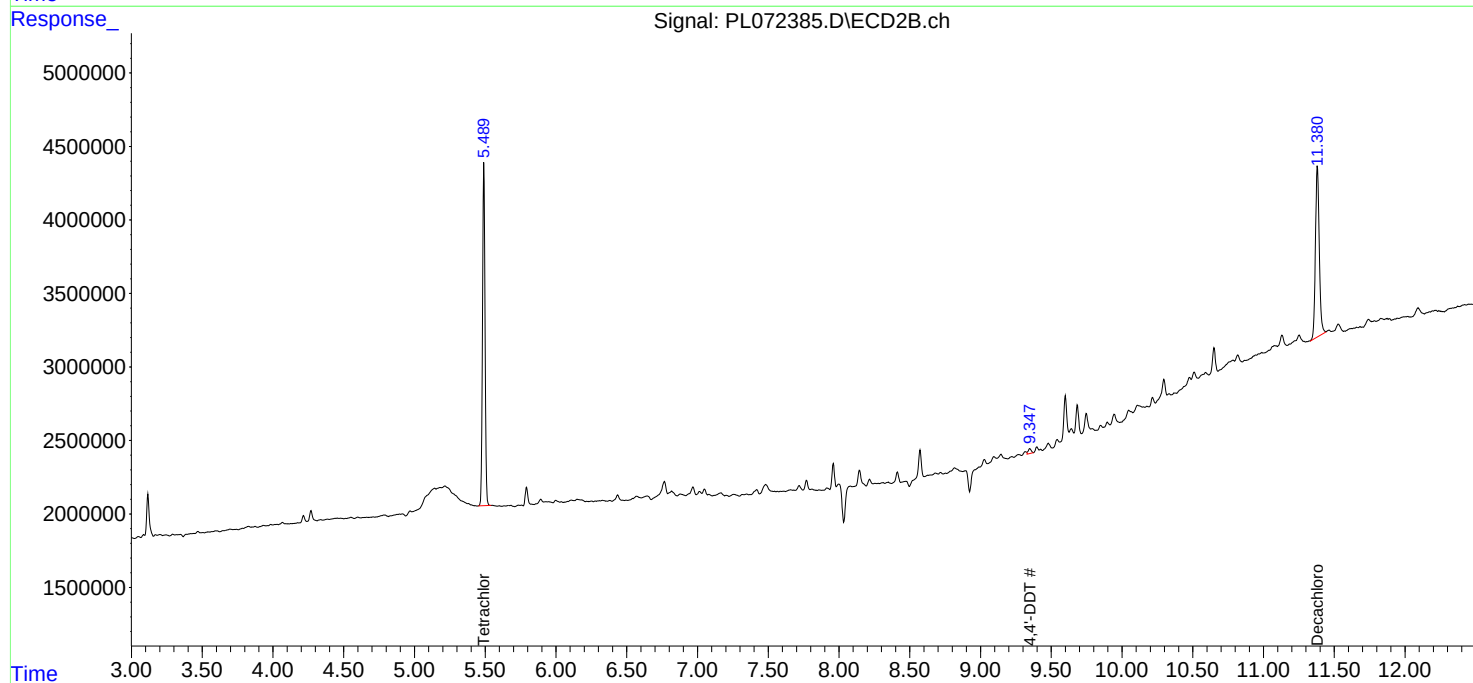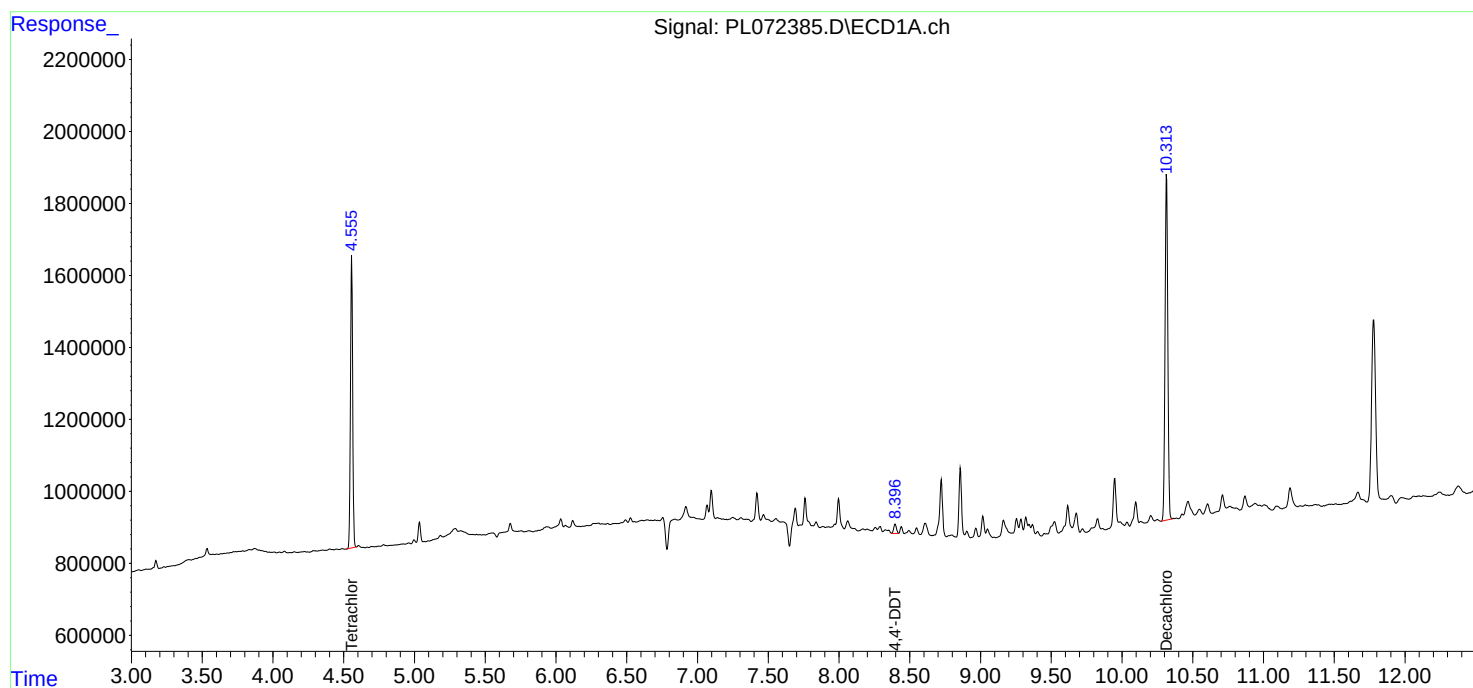


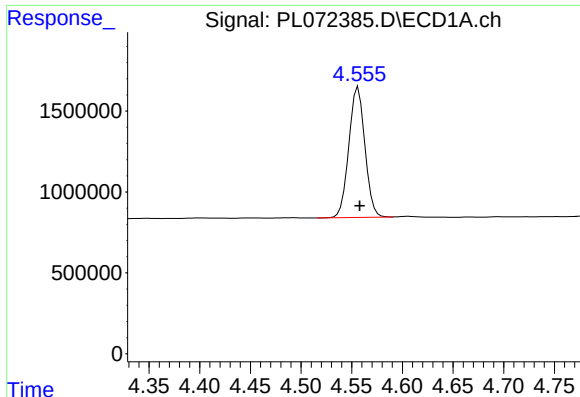

#1 Tetrachloro-m-xylene


R.T.: 4.556 min
Delta R.T.: -0.002 min
Response: 8850976
Conc: 15.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
TES-1

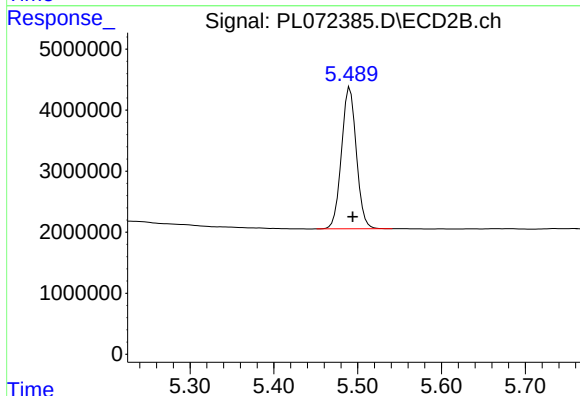


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: -0.003 min
Response: 28523906
Conc: 17.56 ng/ml

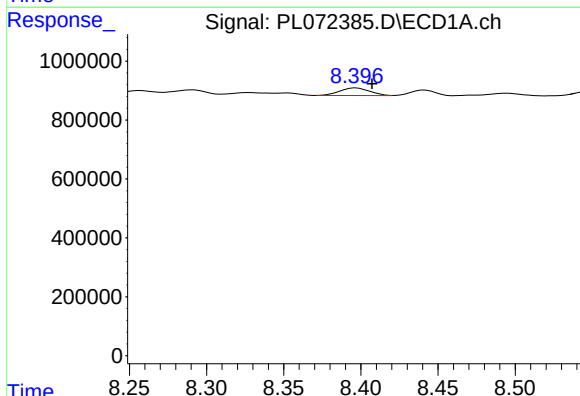


#17 4,4'-DDT

R.T.: 8.396 min
Delta R.T.: -0.012 min
Response: 345950
Conc: 0.52 ng/ml m

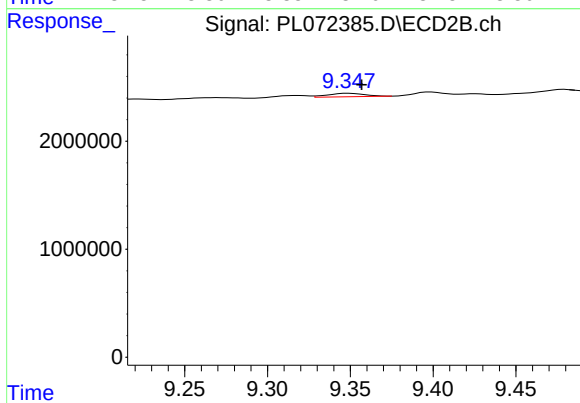

#17 4,4'-DDT


R.T.: 9.349 min
Delta R.T.: -0.008 min
Response: 509782
Conc: 0.32 ng/ml

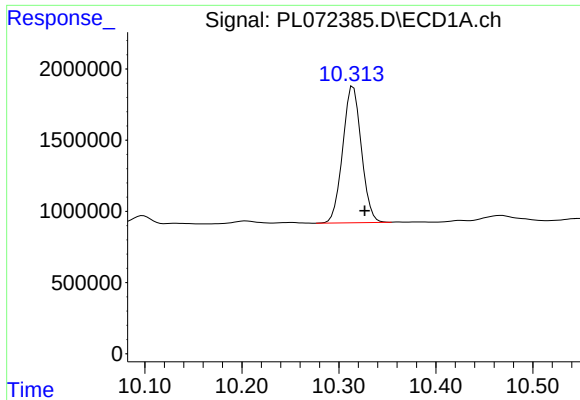

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: -0.012 min
Response: 12776321
Conc: 14.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
TES-1

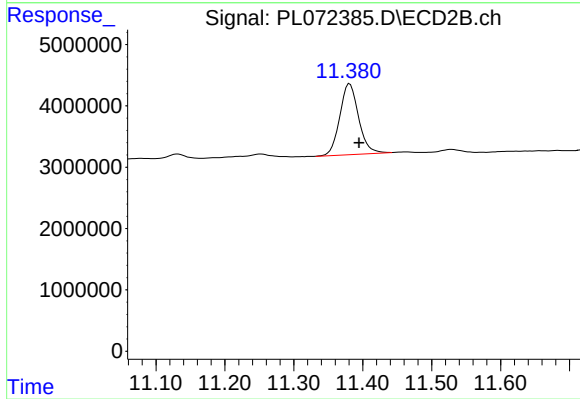

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: -0.014 min
Response: 21928627
Conc: 13.59 ng/ml