

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020222\
 Data File : PL072418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2022 17:06
 Operator : AR\AJ
 Sample : PB142436BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 00:36:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.555	5.490	9579245	31371026	17.254	19.316
28)	SA Decachlor...	10.315	11.381	14133712	21783944	15.909	13.501
Target Compounds							
7)	B delta-BHC	0.000	7.013f	0	3318466	N.D.	1.349 #
9)	A Endosulfan I	0.000	8.357	0	46244	N.D.	0.026 #
10)	B gamma-Chl...	0.000	8.229	0	172416	N.D.	0.085 #
11)	B alpha-Chl...	0.000	8.322	0	54298	N.D.	0.027 #
15)	B Endosulfa...	0.000	9.145f	0	1075209	N.D.	0.627 #
17)	MA 4,4'-DDT	0.000	9.363	0	72553	N.D.	0.046 #
18)	B Endrin al...	0.000	9.274	0	176127	N.D.	0.142 #
25)	Chlordane-3	0.000	8.229	0	172416	N.D.	0.621 #
26)	Chlordane-4	0.000	8.322	0	54298	N.D.	0.164 #
27)	Chlordane-5	0.000	9.182f	0	31587	N.D.	0.518 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020222\
Data File : PL072418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2022 17:06
Operator : AR\AJ
Sample : PB142436BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 00:36:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

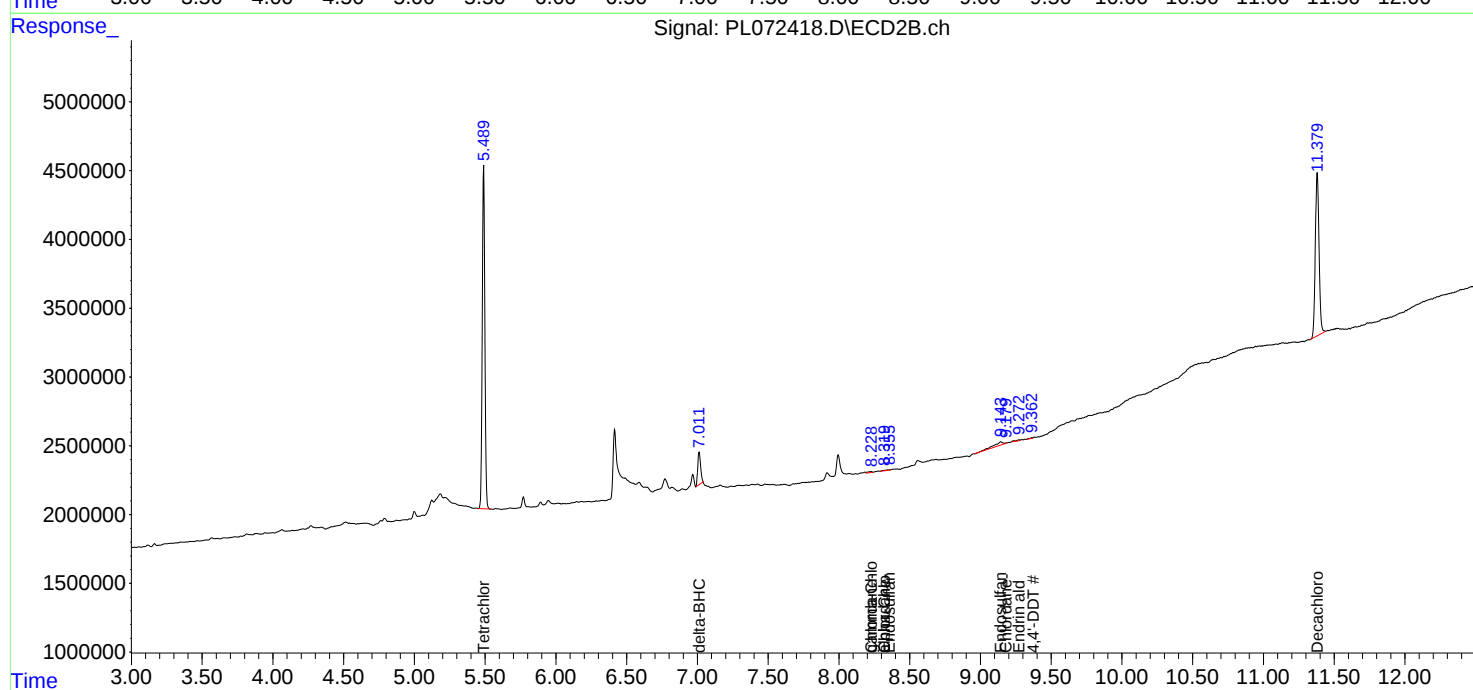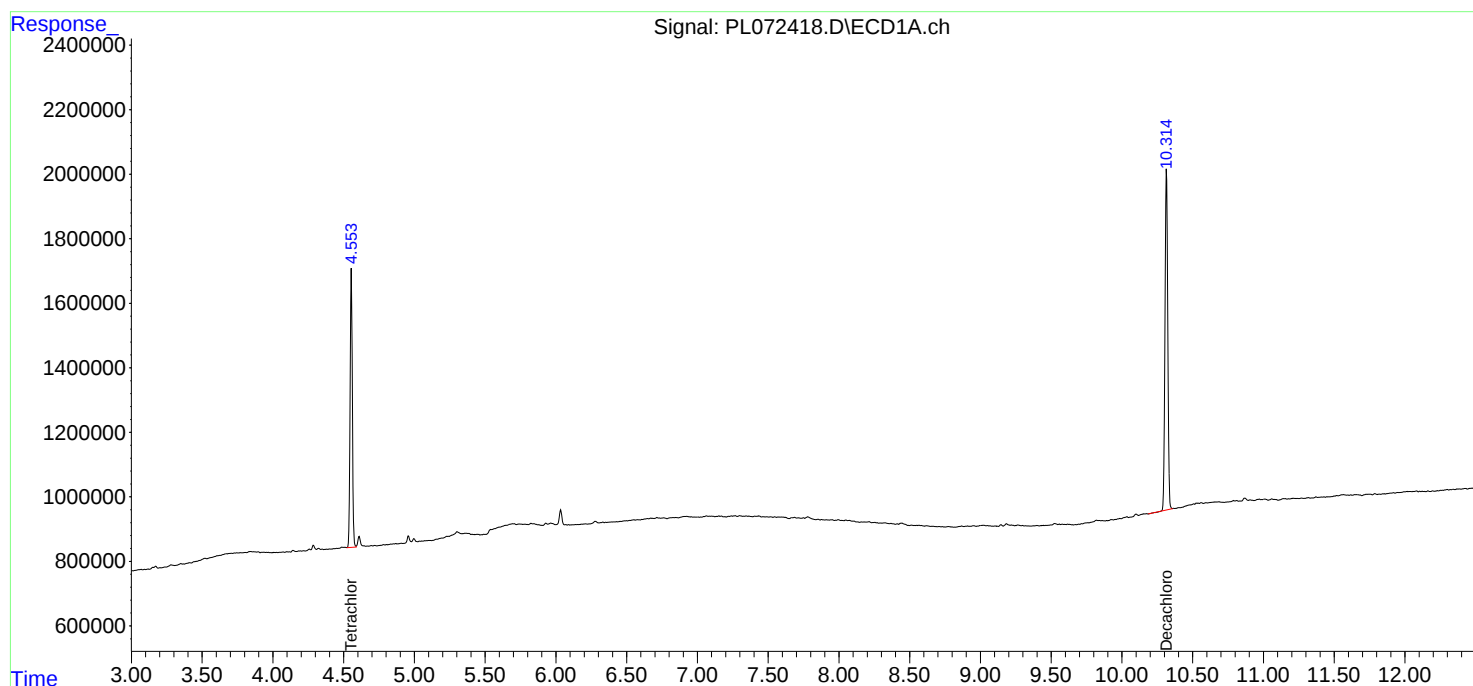


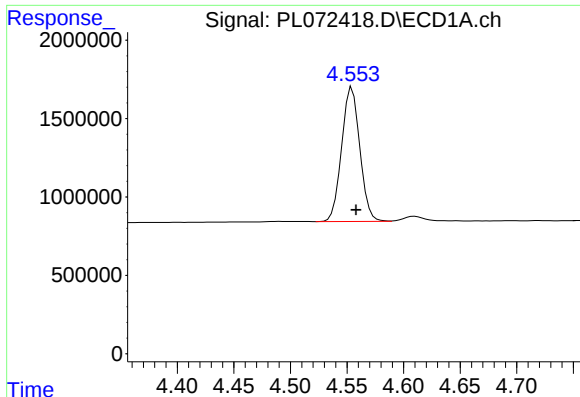

#1 Tetrachloro-m-xylene


R.T.: 4.555 min
Delta R.T.: -0.003 min
Response: 9579245
Conc: 17.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

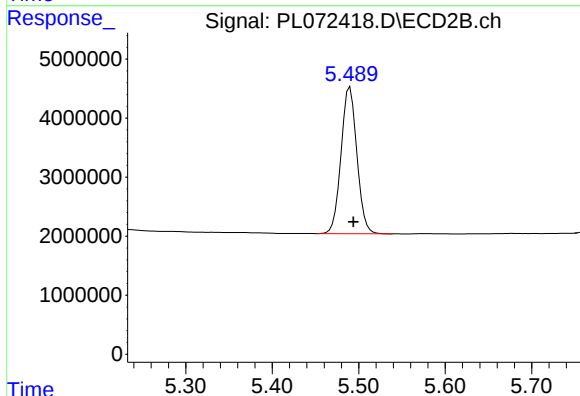


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.004 min
Response: 31371026
Conc: 19.32 ng/ml

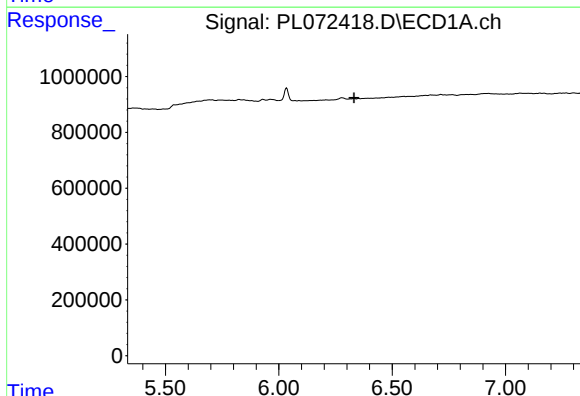


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

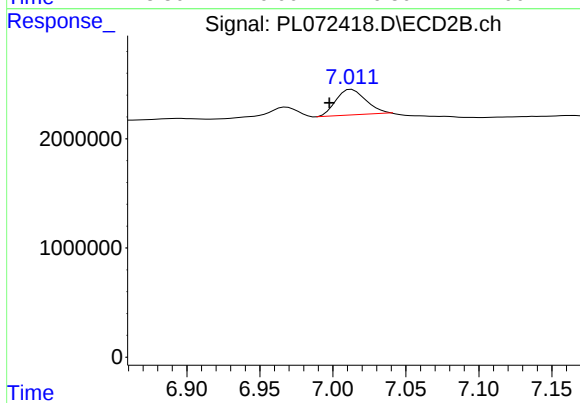

#7 delta-BHC


R.T.: 7.013 min
Delta R.T.: 0.015 min
Response: 3318466
Conc: 1.35 ng/ml

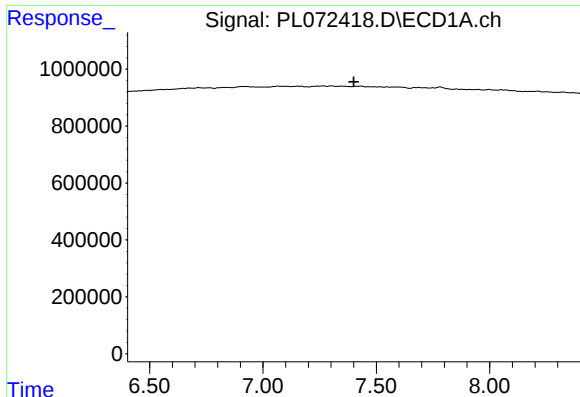

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.400 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

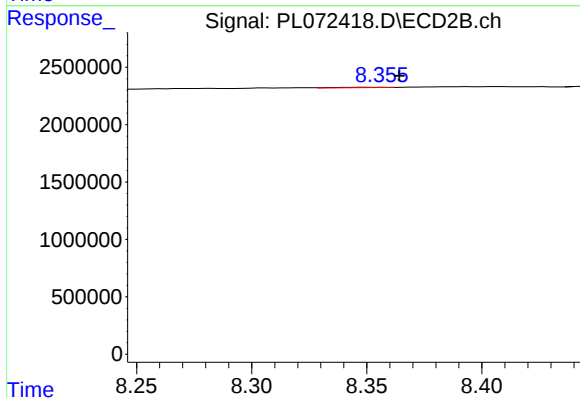


#9 Endosulfan I

R.T.: 8.357 min
Delta R.T.: -0.008 min
Response: 46244
Conc: 0.03 ng/ml

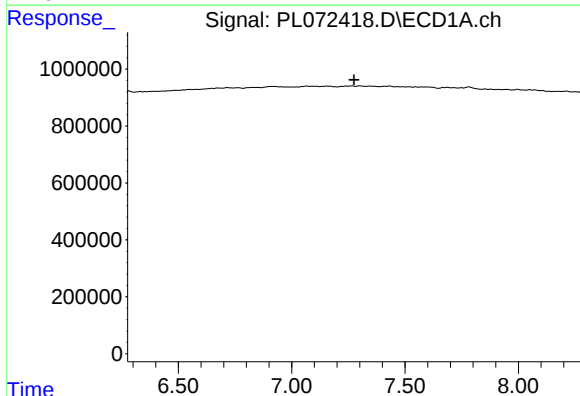


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

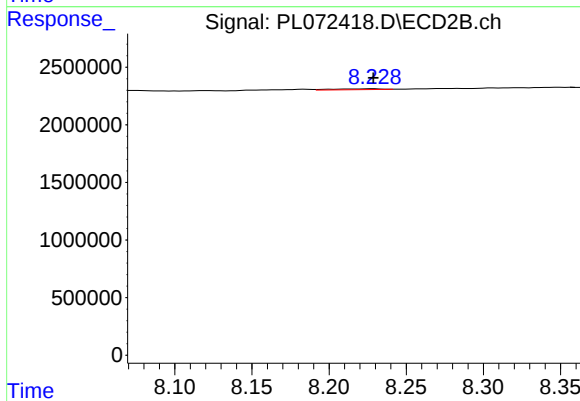

#10 gamma-Chlordane


R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 172416
Conc: 0.09 ng/ml

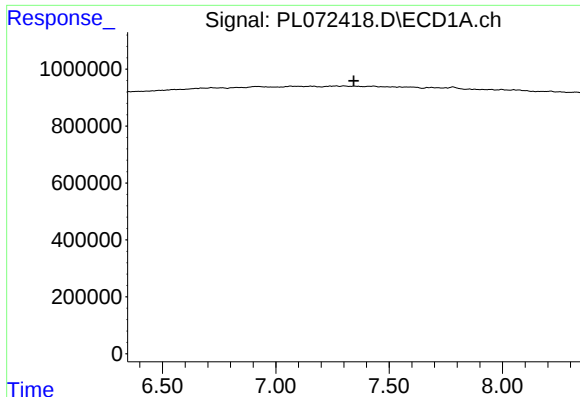

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.345 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

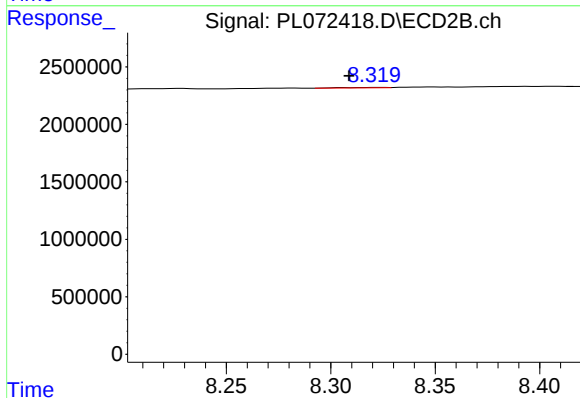


#11 alpha-Chlordane

R.T.: 8.322 min
Delta R.T.: 0.013 min
Response: 54298
Conc: 0.03 ng/ml

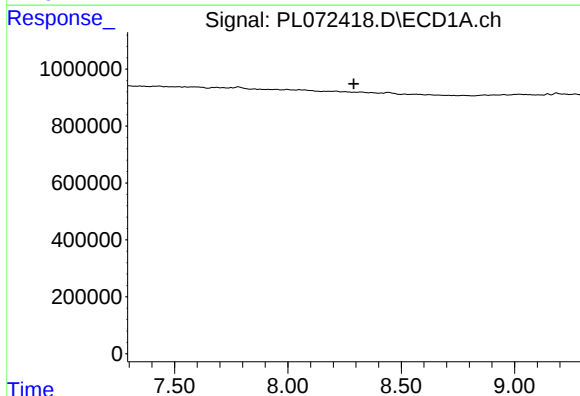


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

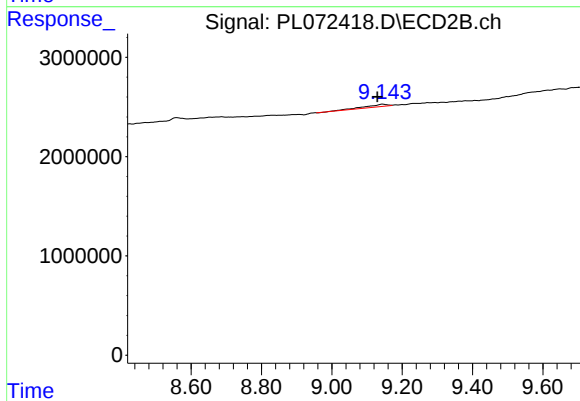

#15 Endosulfan II


R.T.: 9.145 min
Delta R.T.: 0.016 min
Response: 1075209
Conc: 0.63 ng/ml

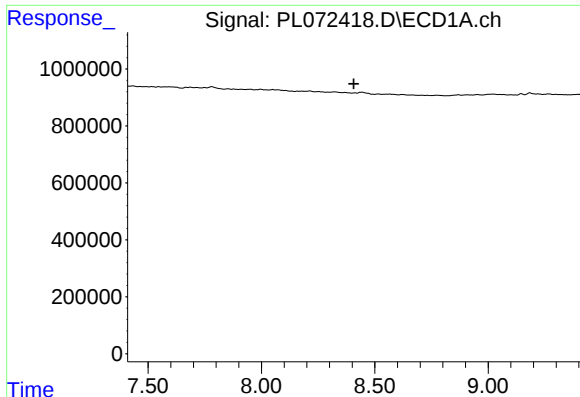

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

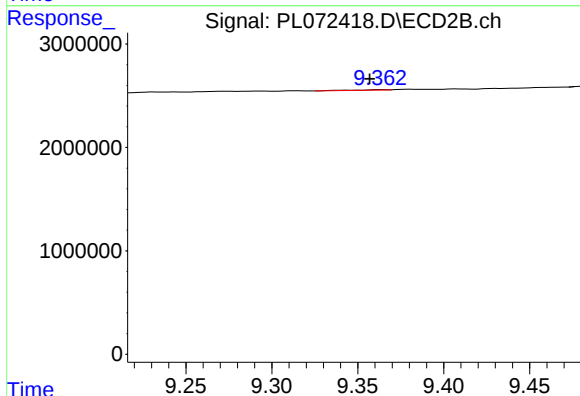


#17 4,4'-DDT

R.T.: 9.363 min
Delta R.T.: 0.006 min
Response: 72553
Conc: 0.05 ng/ml

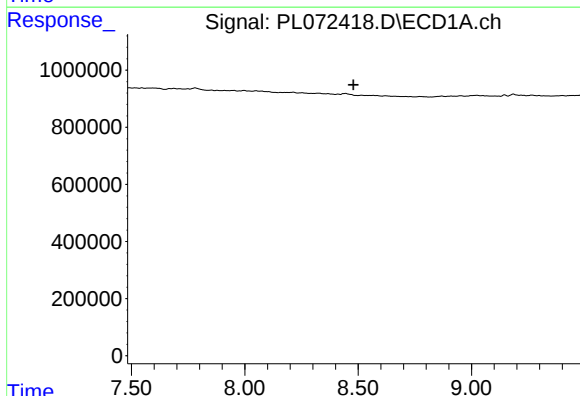


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 8.480 min
Response: 0
Conc: N.D.

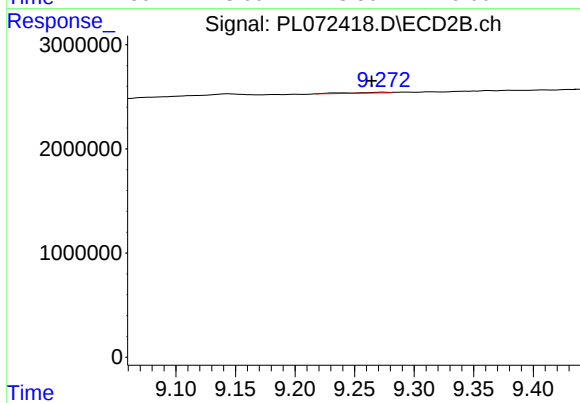

#18 Endrin aldehyde


R.T.: 9.274 min
Delta R.T.: 0.009 min
Response: 176127
Conc: 0.14 ng/ml

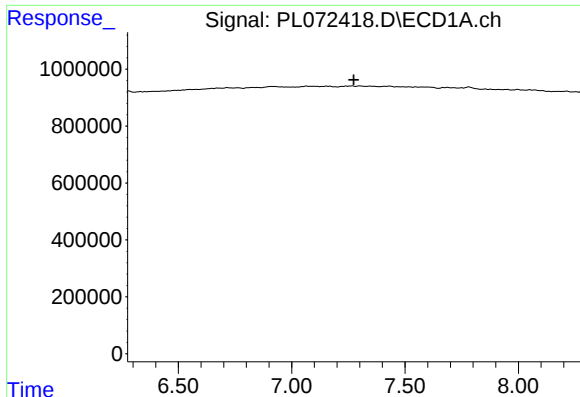

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

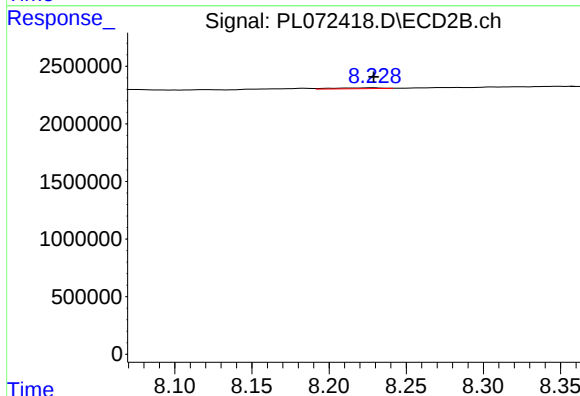


#25 Chlordane-3

R.T.: 8.229 min
Delta R.T.: 0.000 min
Response: 172416
Conc: 0.62 ng/ml

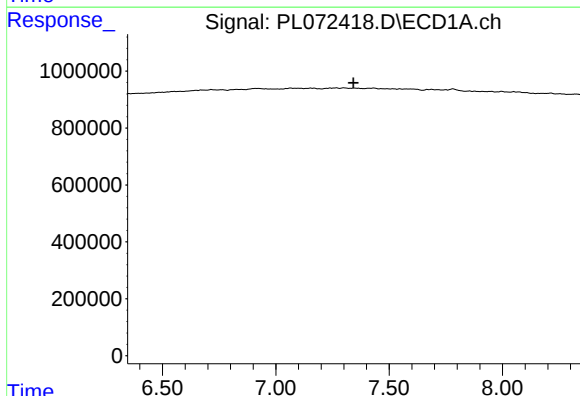


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.343 min
Response: 0
Conc: N.D.

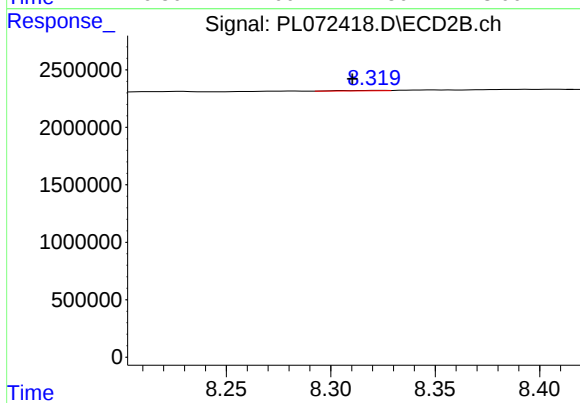

#26 Chlordane-4


R.T.: 8.322 min
Delta R.T.: 0.012 min
Response: 54298
Conc: 0.16 ng/ml

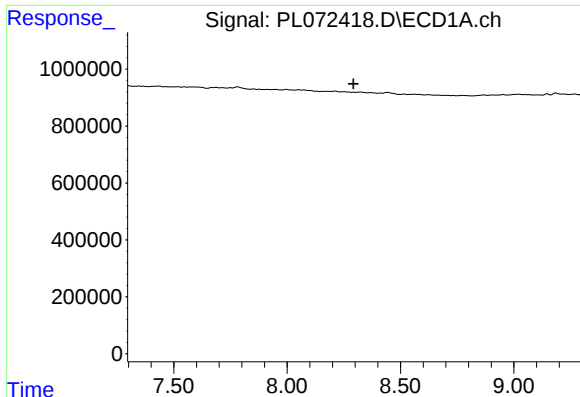

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 8.293 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

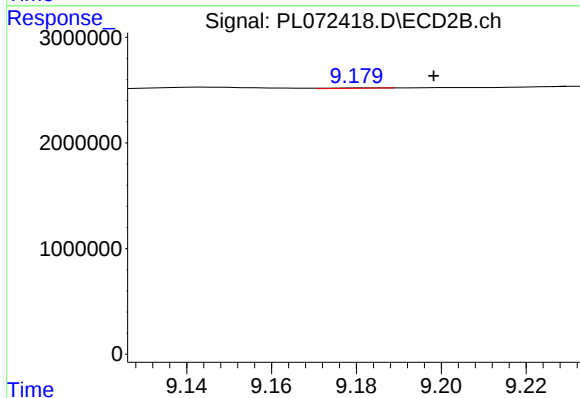


#27 Chlordane-5

R.T.: 9.182 min
Delta R.T.: -0.016 min
Response: 31587
Conc: 0.52 ng/ml

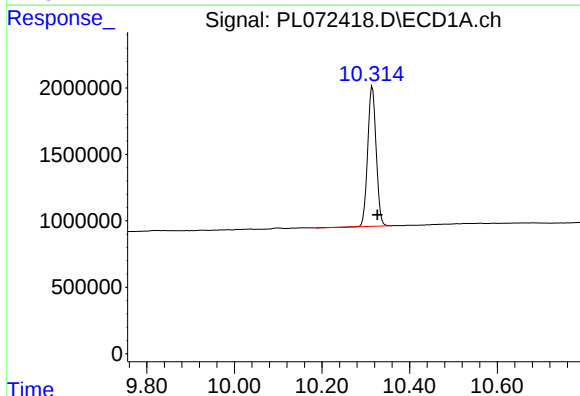

#28 Decachlorobiphenyl

R.T.: 10.315 min
Delta R.T.: -0.012 min
Response: 14133712
Conc: 15.91 ng/ml

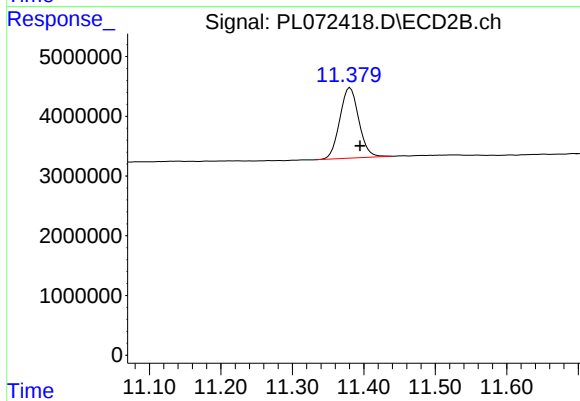

#28 Decachlorobiphenyl

R.T.: 11.381 min
Delta R.T.: -0.014 min
Response: 21783944
Conc: 13.50 ng/ml