

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020222\
 Data File : PL072426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Feb 2022 19:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 00:38:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 18 10:53:59 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.554	5.490	10265509	33560087	18.490	20.664
28)	SA Decachlor...	10.314	11.380	14865422	27071389	16.732	16.778
Target Compounds							
7)	B delta-BHC	0.000	7.014f	0	782250	N.D.	0.318 #
8)	B Heptachlo...	0.000	7.959	0	1839852	N.D.	0.919 #
10)	B gamma-Chl...	0.000	8.233	0	709179	N.D.	0.351 #
13)	MA Dieldrin	7.681	8.665	287285	198780	0.379	0.101 #
14)	MA Endrin	7.996f	0.000	443302	0	0.633	N.D. #
15)	B Endosulfa...	0.000	9.143	0	497976	N.D.	0.290 #
16)	A 4,4'-DDD	0.000	9.067f	0	291531	N.D.	0.204 #
17)	MA 4,4'-DDT	0.000	9.347	0	14751	N.D.	0.009 #
25)	Chlordane-3	0.000	8.233	0	709179	N.D.	2.553 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020222\
Data File : PL072426.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Feb 2022 19:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 00:38:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011722.M
Quant Title : GC Extractables
QLast Update : Tue Jan 18 10:53:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

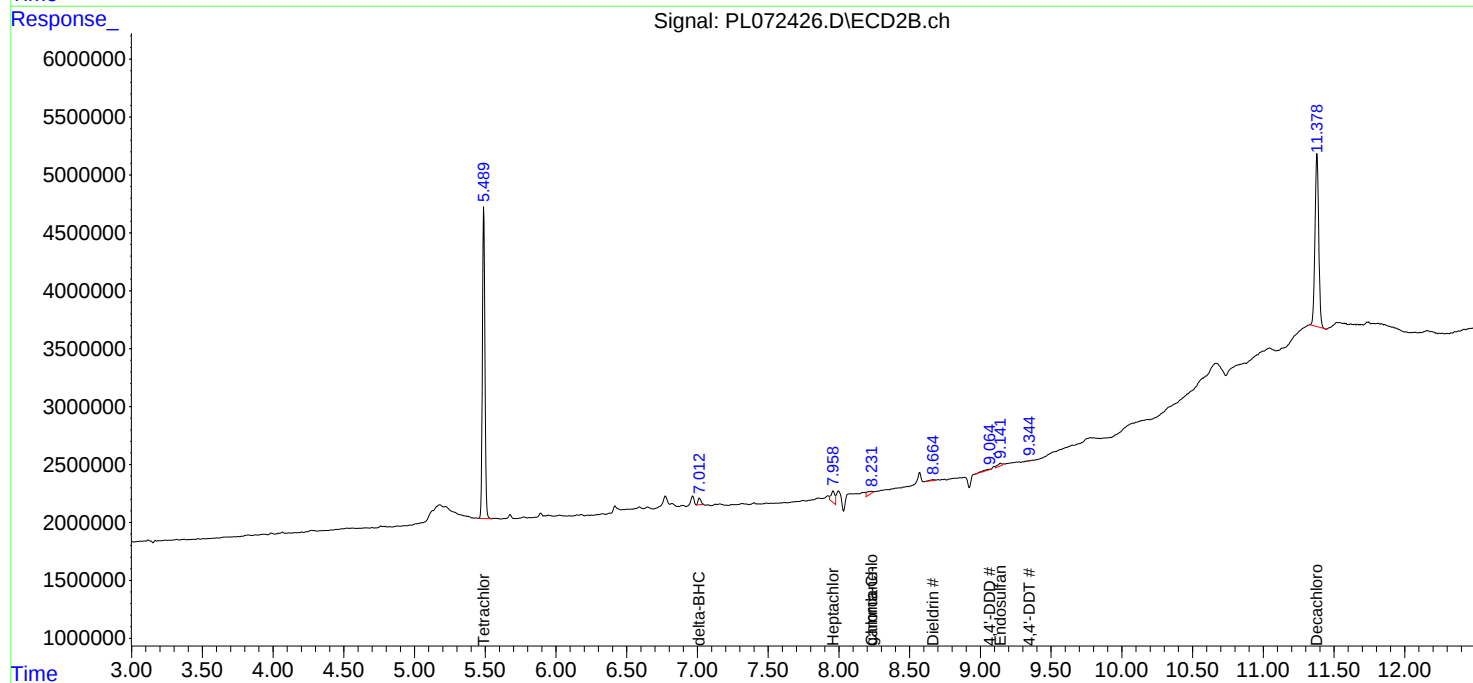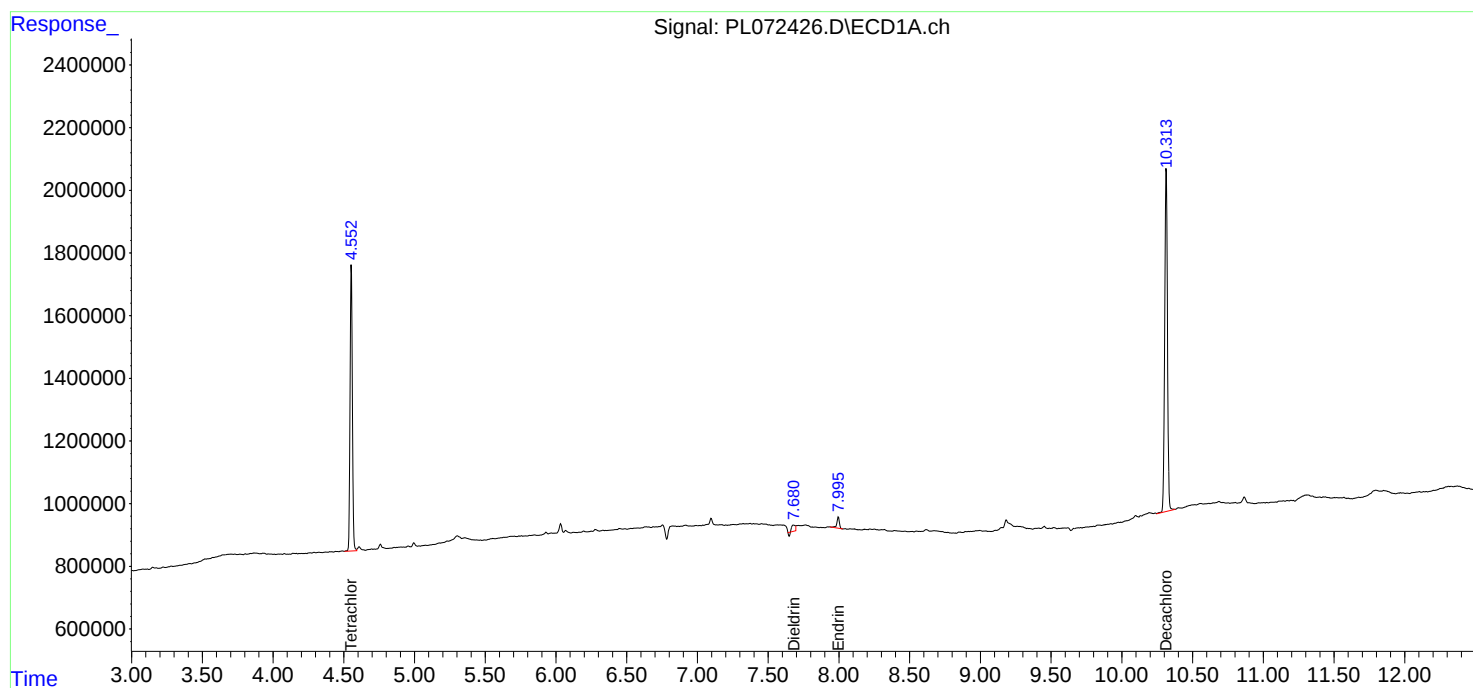


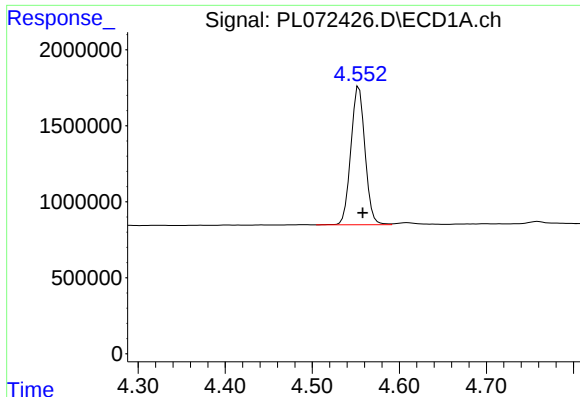

#1 Tetrachloro-m-xylene


R.T.: 4.554 min
Delta R.T.: -0.004 min
Response: 10265509
Conc: 18.49 ng/ml

Instrument :
ECD_L
ClientSampleId :

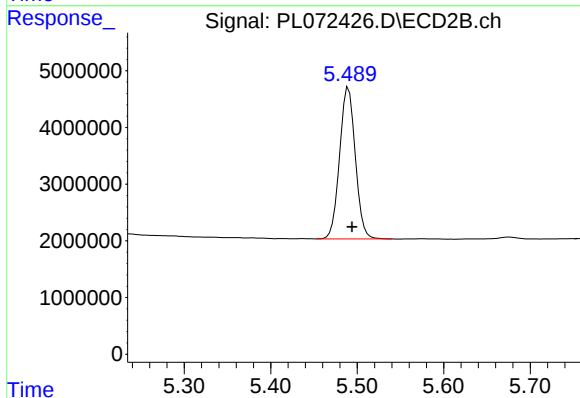


#1 Tetrachloro-m-xylene

R.T.: 5.490 min
Delta R.T.: -0.004 min
Response: 33560087
Conc: 20.66 ng/ml

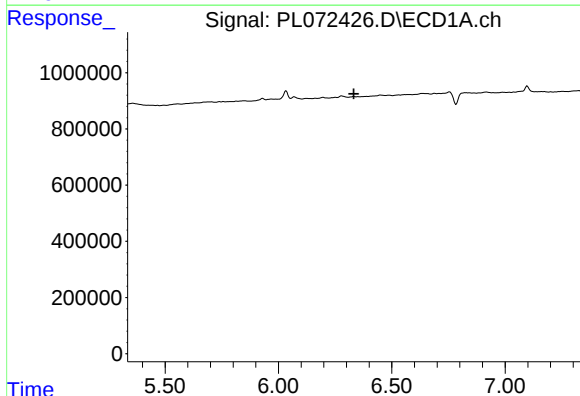


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.332 min
Response: 0
Conc: N.D.

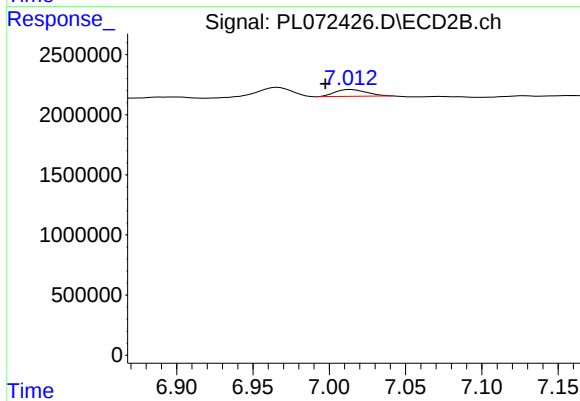

#7 delta-BHC


R.T.: 7.014 min
Delta R.T.: 0.016 min
Response: 782250
Conc: 0.32 ng/ml

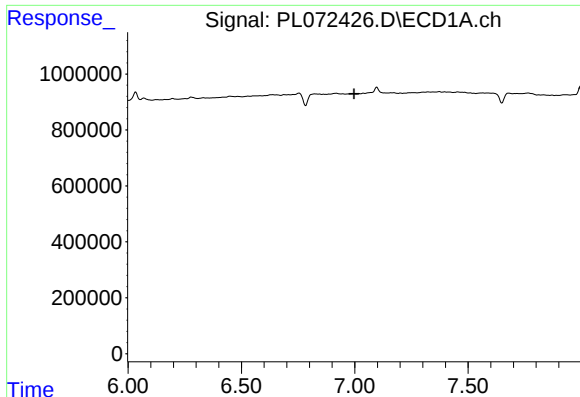

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 6.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

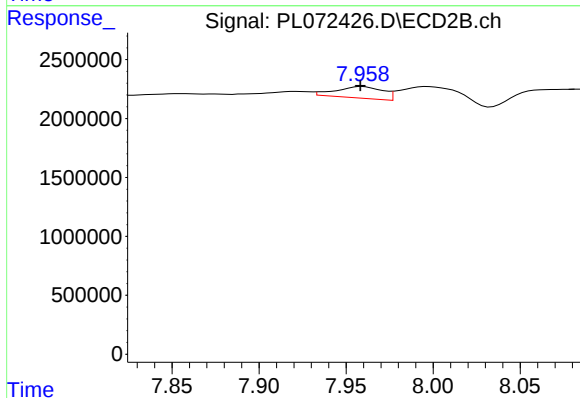


#8 Heptachlor epoxide

R.T.: 7.959 min
Delta R.T.: 0.001 min
Response: 1839852
Conc: 0.92 ng/ml

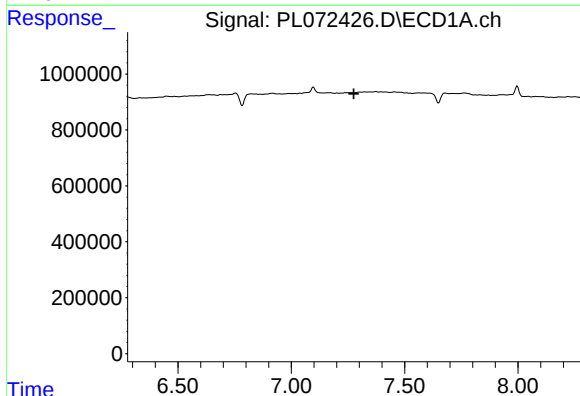


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.275 min
Response: 0
Conc: N.D.

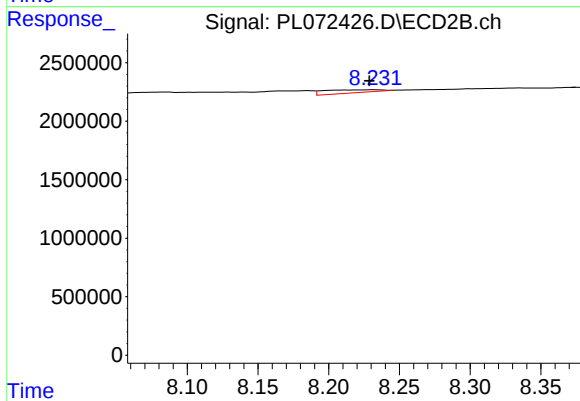

#10 gamma-Chlordane


R.T.: 8.233 min
Delta R.T.: 0.004 min
Response: 709179
Conc: 0.35 ng/ml

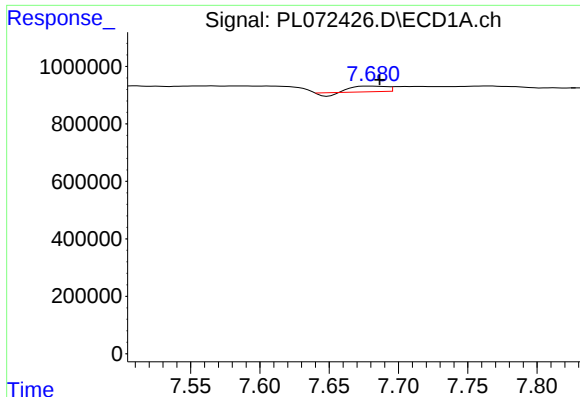

#13 Dieldrin


R.T.: 7.681 min
Delta R.T.: -0.006 min
Response: 287285
Conc: 0.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

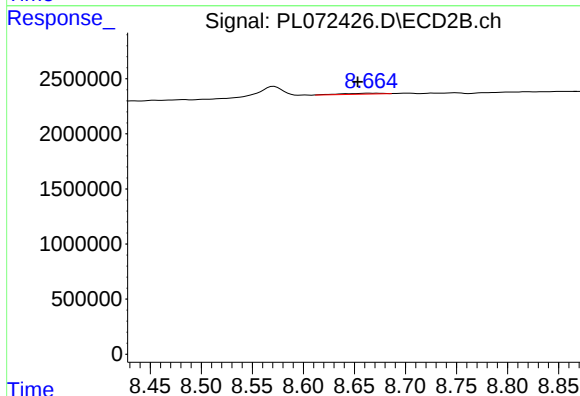


#13 Dieldrin

R.T.: 8.665 min
Delta R.T.: 0.012 min
Response: 198780
Conc: 0.10 ng/ml

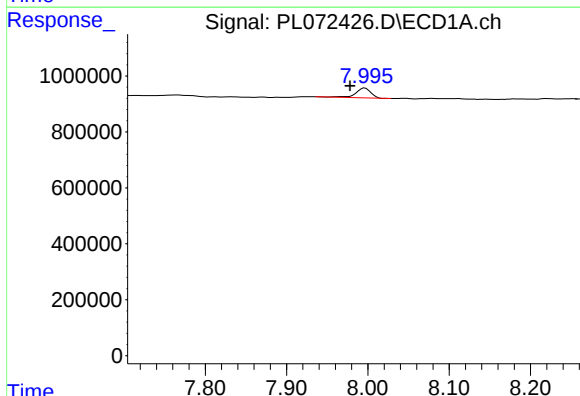


#14 Endrin

R.T.: 7.996 min
Delta R.T.: 0.018 min
Response: 443302
Conc: 0.63 ng/ml

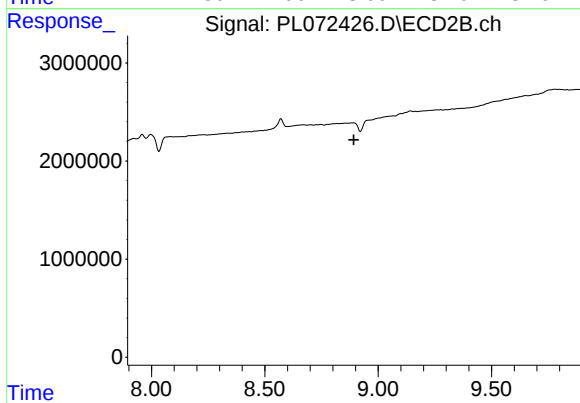

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 8.893 min
Response: 0
Conc: N.D.

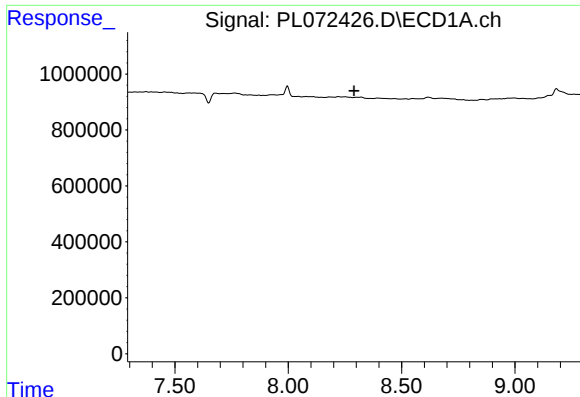

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.291 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

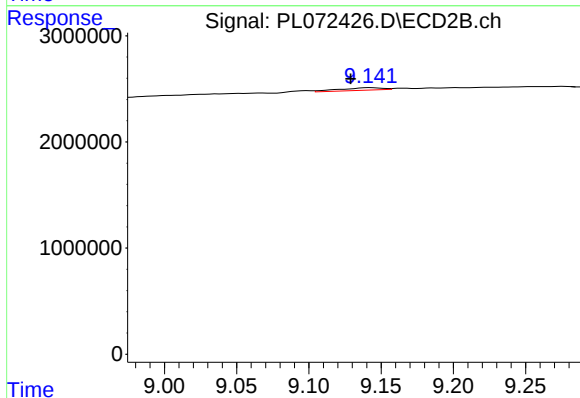


#15 Endosulfan II

R.T.: 9.143 min
Delta R.T.: 0.014 min
Response: 497976
Conc: 0.29 ng/ml

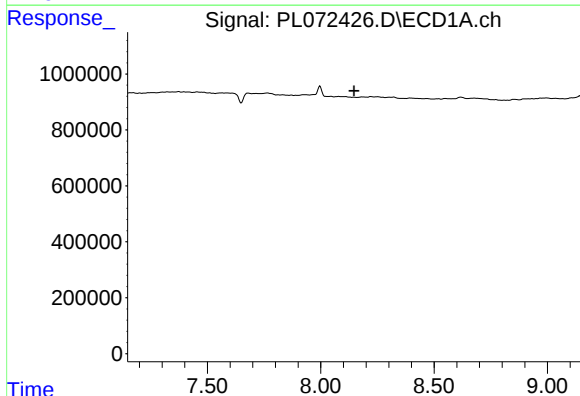


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.147 min
Response: 0
Conc: N.D.

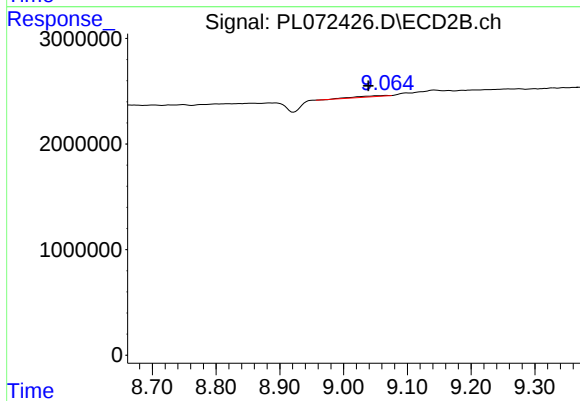

#16 4,4'-DDD


R.T.: 9.067 min
Delta R.T.: 0.029 min
Response: 291531
Conc: 0.20 ng/ml

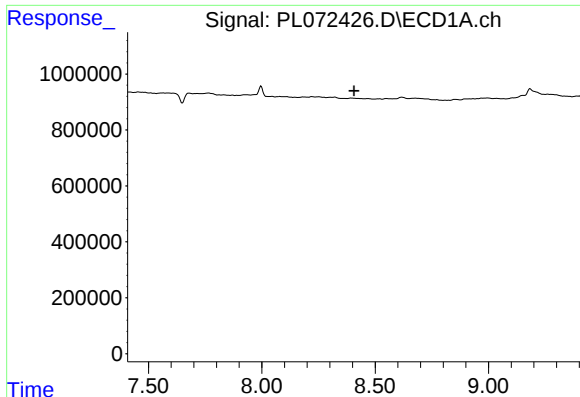

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.407 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

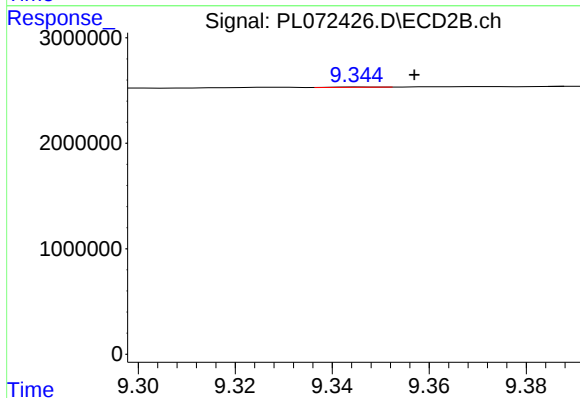


#17 4,4'-DDT

R.T.: 9.347 min
Delta R.T.: -0.010 min
Response: 14751
Conc: 0.01 ng/ml

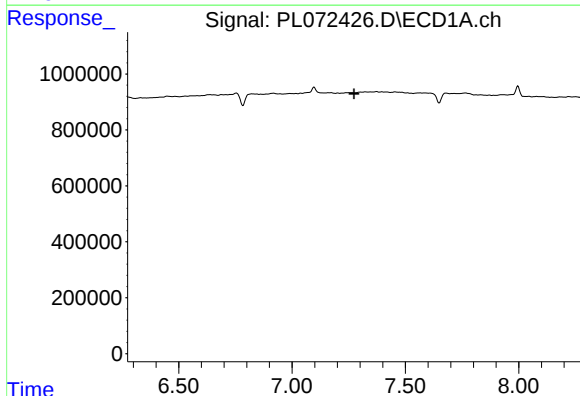


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.274 min
Response: 0
Conc: N.D.

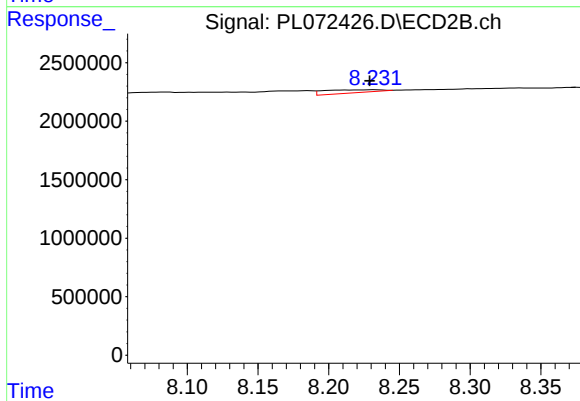

#25 Chlordane-3


R.T.: 8.233 min
Delta R.T.: 0.004 min
Response: 709179
Conc: 2.55 ng/ml

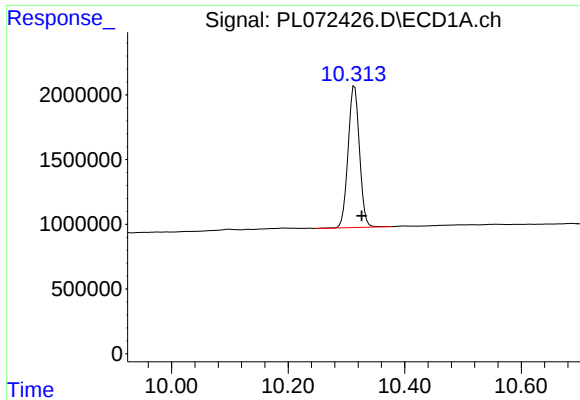

#28 Decachlorobiphenyl

R.T.: 10.314 min
Delta R.T.: -0.013 min
Response: 14865422
Conc: 16.73 ng/ml

Instrument :
ECD_L
ClientSampleId :

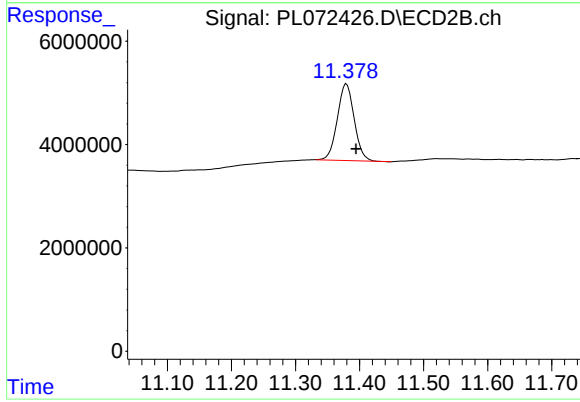

#28 Decachlorobiphenyl

R.T.: 11.380 min
Delta R.T.: -0.015 min
Response: 27071389
Conc: 16.78 ng/ml