

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
 Data File : PL056287.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2020 13:36
 Operator : AJ\MA
 Sample : L1343-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NW-SP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:28:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.016	241.4E6	66250719	23.050	22.657
28)	SA Decachlor...	8.253	9.093	198.5E6	45751775	18.853	20.227
Target Compounds							
3)	MA gamma-BHC...	4.229	4.676	7549263	7962829	0.461	1.942 #
9)	A Endosulfan I	5.577f	0.000	105.1E6	0	7.243	N.D. #
13)	MA Dieldrin	5.804	0.000	39997713	0	2.601	N.D. #
16)	A 4,4'-DDD	6.177	0.000	26775292	0	2.491	N.D. #
17)	MA 4,4'-DDT	6.421	0.000	8140037	0	0.745	N.D. #
19)	B Endosulfa...	6.727f	0.000	17547882	0	1.443	N.D. #
23)	Chlordane-1	4.375	0.000	4016307	0	10.610	N.D. #
27)	Chlordane-5	6.363f	0.000	35816018	0	86.339	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
Data File : PL056287.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2020 13:36
Operator : AJ\MA
Sample : L1343-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NW-SP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:28:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

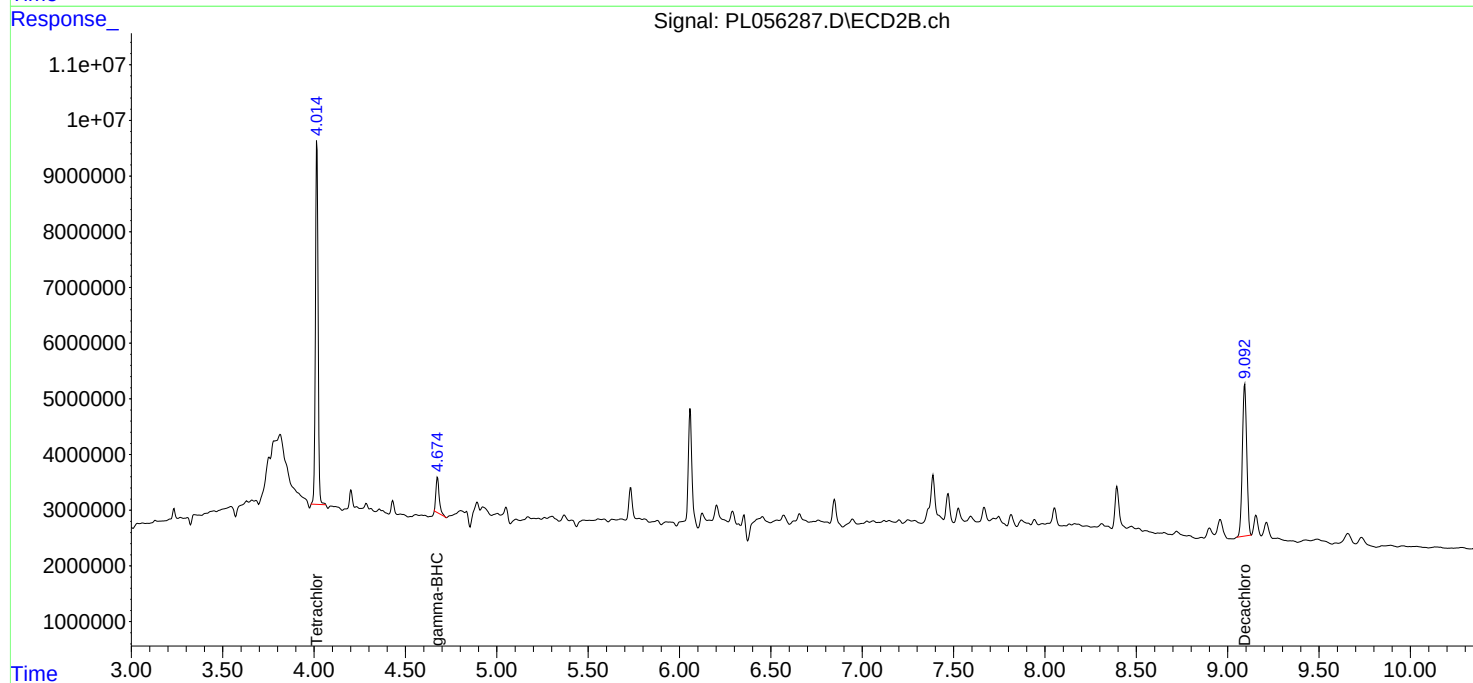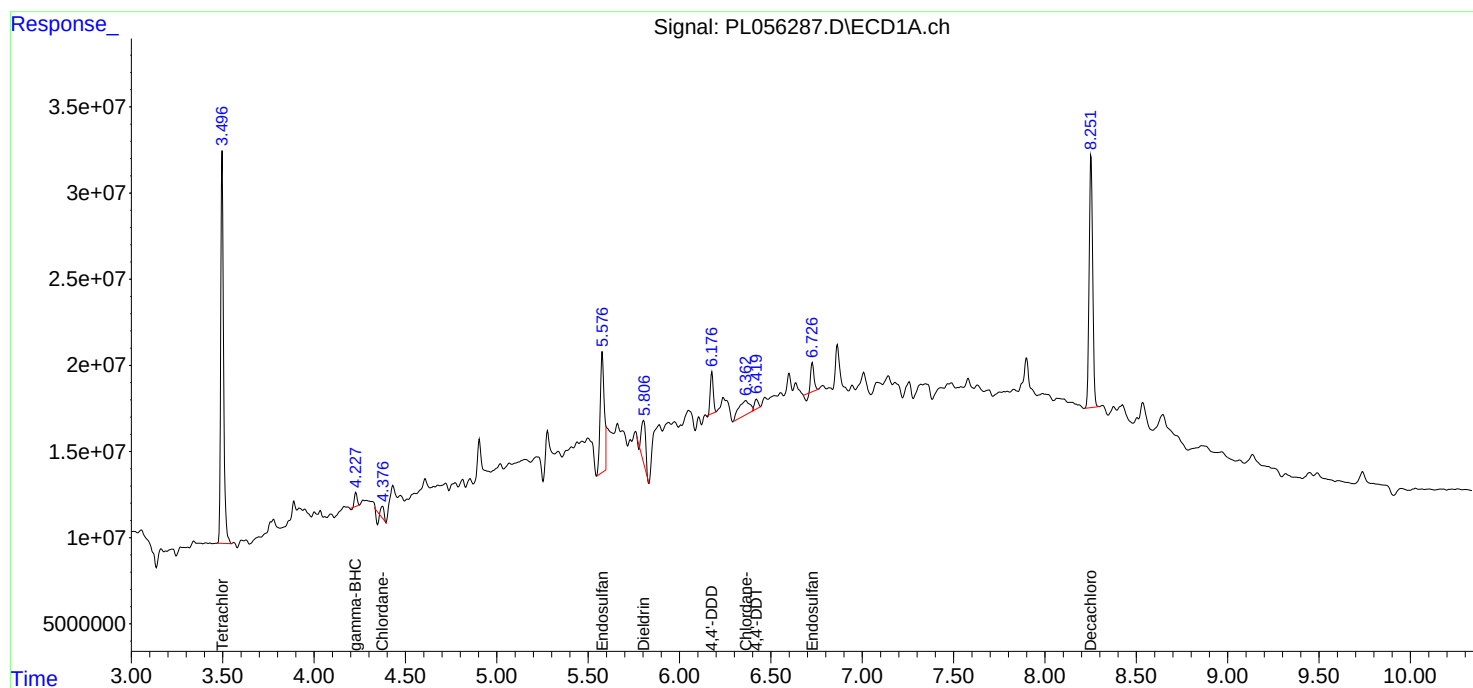


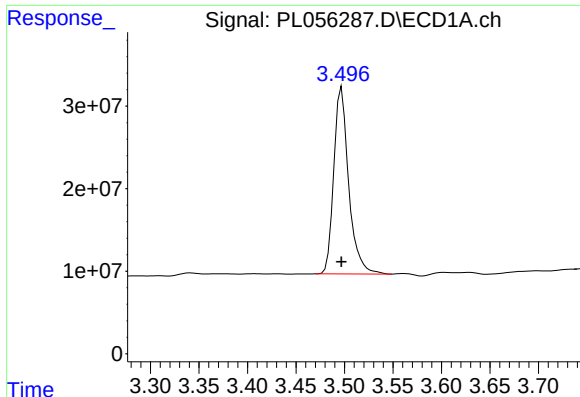

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 241398808
Conc: 23.05 ng/ml

Instrument :
ECD_L
ClientSampleId :
NW-SP

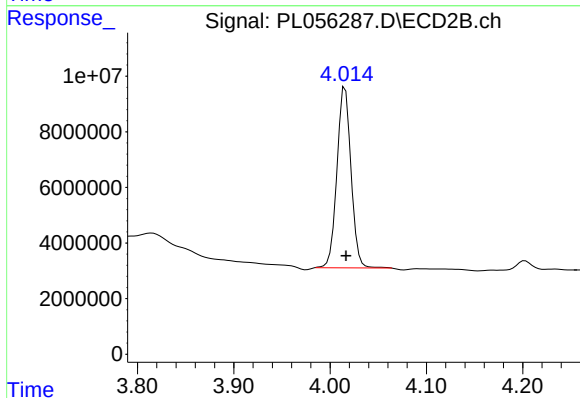


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 66250719
Conc: 22.66 ng/ml

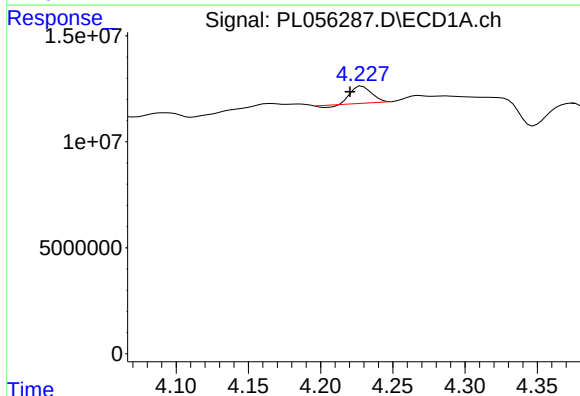


#3 gamma-BHC (Lindane)

R.T.: 4.229 min
Delta R.T.: 0.008 min
Response: 7549263
Conc: 0.46 ng/ml

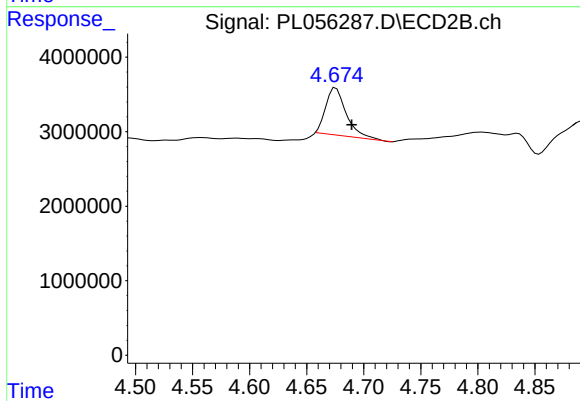

#3 gamma-BHC (Lindane)


R.T.: 4.676 min
Delta R.T.: -0.014 min
Response: 7962829
Conc: 1.94 ng/ml

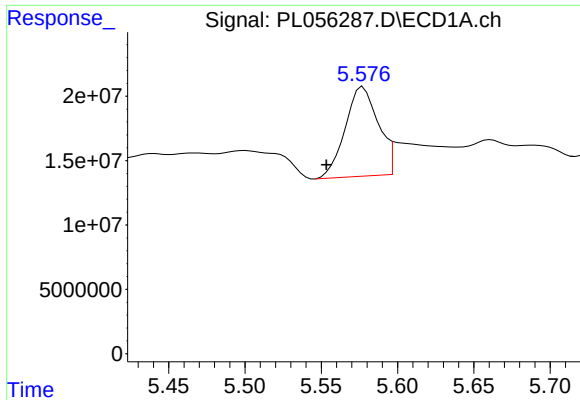

#9 Endosulfan I


R.T.: 5.577 min
Delta R.T.: 0.024 min
Response: 105111108
Conc: 7.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
NW-SP

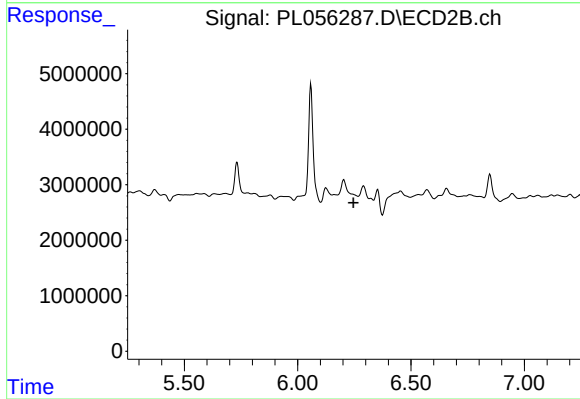


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.246 min
Response: 0
Conc: N.D.

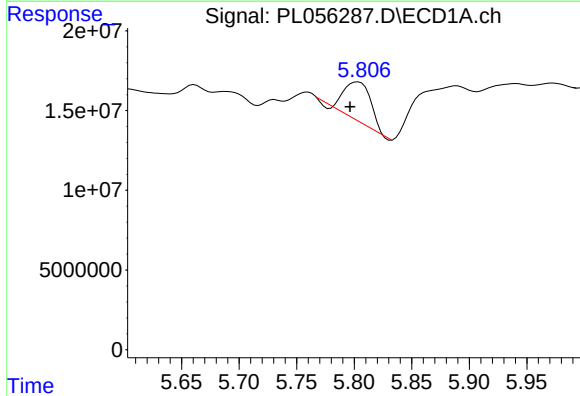


#13 Dieldrin

R.T.: 5.804 min
Delta R.T.: 0.007 min
Response: 39997713
Conc: 2.60 ng/ml

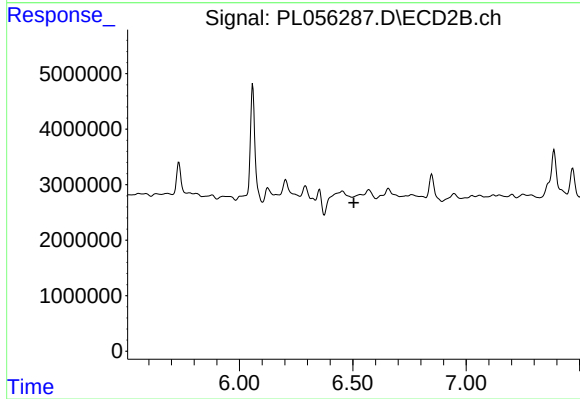

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.504 min
Response: 0
Conc: N.D.

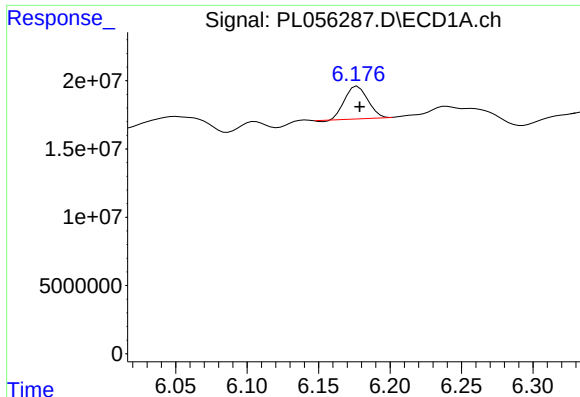

#16 4,4'-DDD


R.T.: 6.177 min
Delta R.T.: -0.001 min
Response: 26775292
Conc: 2.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
NW-SP

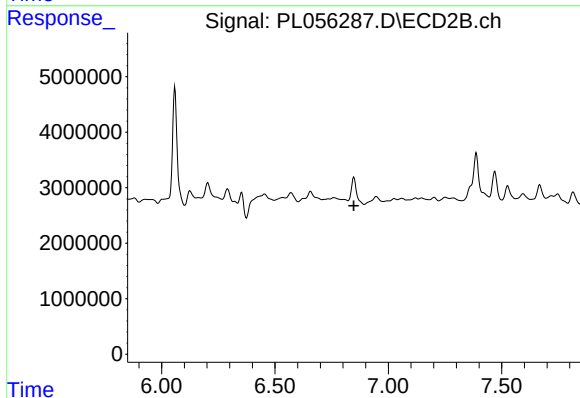


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.847 min
Response: 0
Conc: N.D.

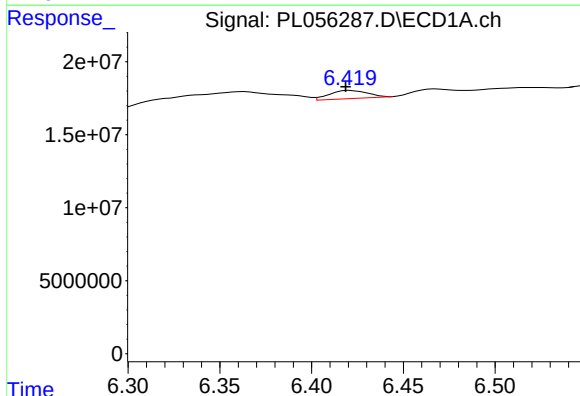


#17 4,4'-DDT

R.T.: 6.421 min
Delta R.T.: 0.002 min
Response: 8140037
Conc: 0.74 ng/ml

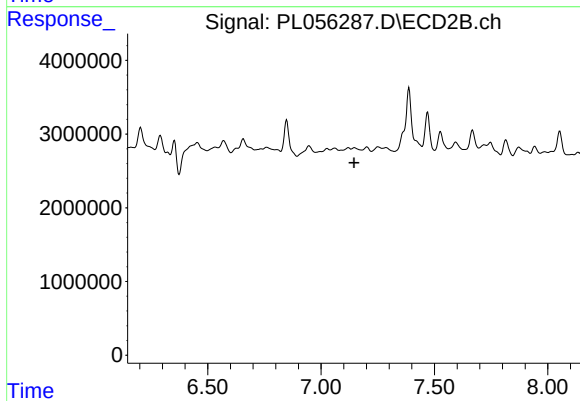

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

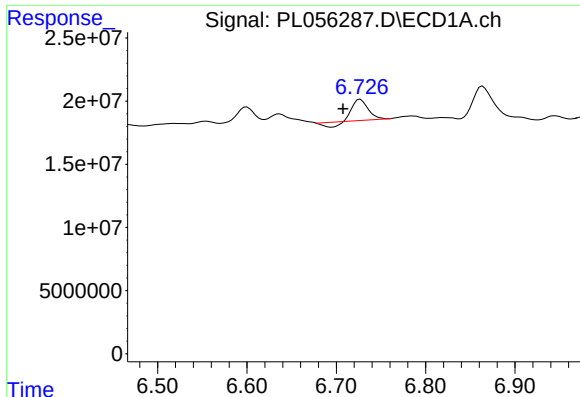

#19 Endosulfan Sulfate


R.T.: 6.727 min
Delta R.T.: 0.019 min
Response: 17547882
Conc: 1.44 ng/ml

Instrument :
ECD_L
ClientSampleId :
NW-SP

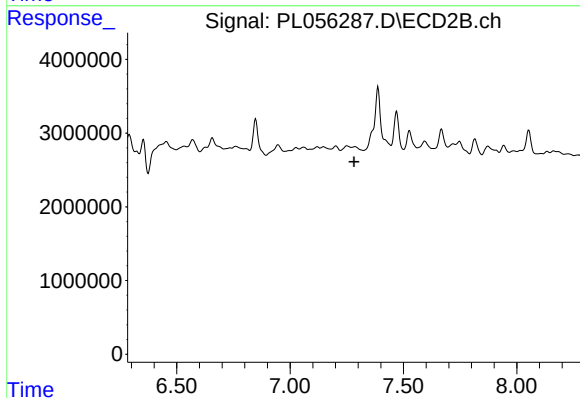


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.282 min
Response: 0
Conc: N.D.

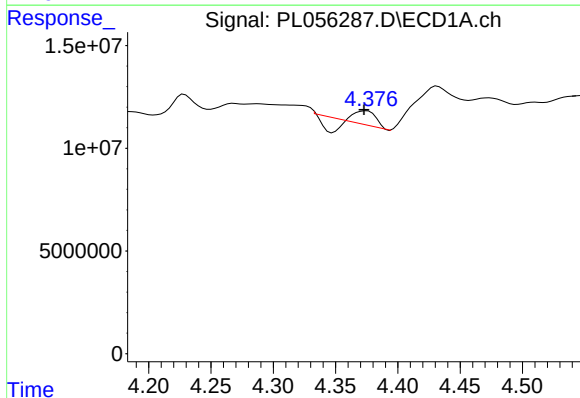


#23 Chlordane-1

R.T.: 4.375 min
Delta R.T.: 0.002 min
Response: 4016307
Conc: 10.61 ng/ml

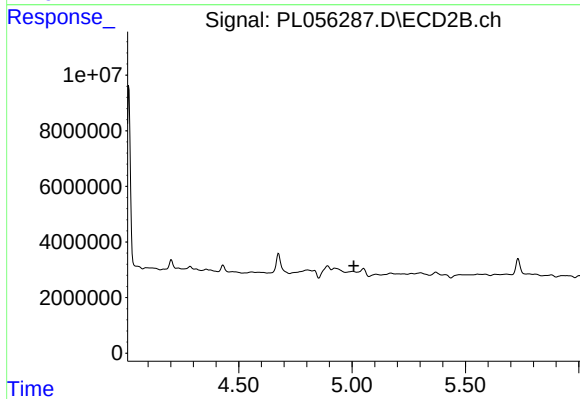

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

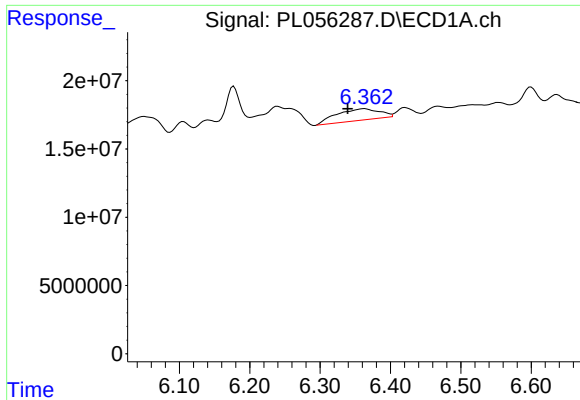

#27 Chlordane-5


R.T.: 6.363 min
Delta R.T.: 0.024 min
Response: 35816018
Conc: 86.34 ng/ml

Instrument :
ECD_L
ClientSampleId :
NW-SP

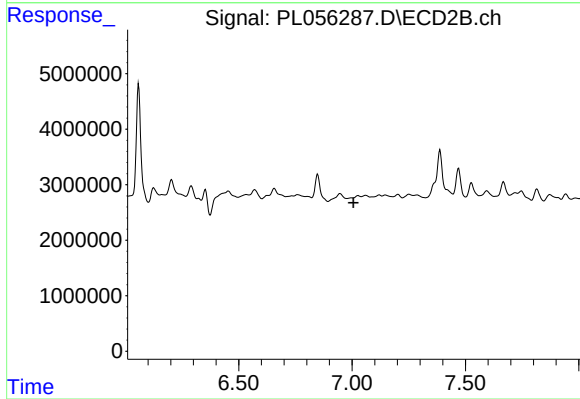


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.007 min
Response: 0
Conc: N.D.

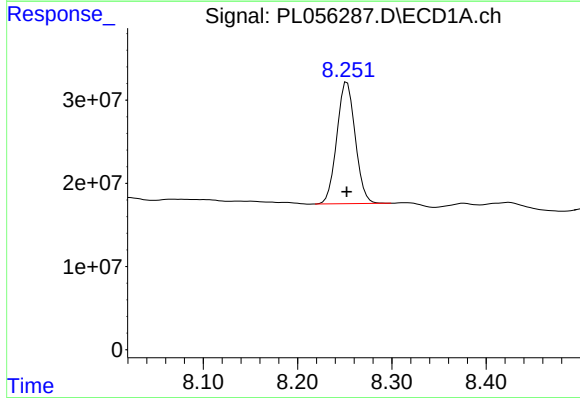

#28 Decachlorobiphenyl

R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 198481314
Conc: 18.85 ng/ml

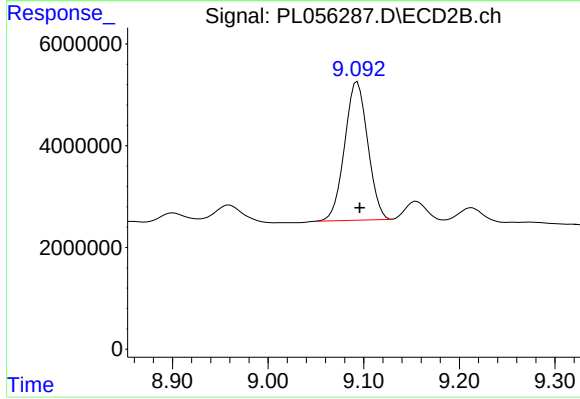

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.003 min
Response: 45751775
Conc: 20.23 ng/ml