

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
 Data File : PL056294.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2020 15:14
 Operator : AJ\MA
 Sample : L1351-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TAL-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:30:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.498	4.016	122.7E6	34870501	11.711	11.925
28)	SA Decachlor...	8.252	9.094	130.3E6	30750068	12.379	13.594
Target Compounds							
2)	A alpha-BHC	0.000	4.431f	0	13288185	N.D.	3.036 #
10)	B gamma-Chl...	5.461f	0.000	7041741	0	0.449	N.D. #
11)	B alpha-Chl...	0.000	6.200	0	7400773	N.D.	2.335 #
12)	B 4,4'-DDE	5.661	6.356	14420113	6802214	0.995	2.271 #
13)	MA Dieldrin	5.789	0.000	15860216	0	1.031	N.D. #
17)	MA 4,4'-DDT	6.416	0.000	24296555	0	2.223	N.D. #
25)	Chlordane-3	5.461f	0.000	7041741	0	5.577	N.D. #
26)	Chlordane-4	0.000	6.200	0	7400773	N.D.	16.845 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
Data File : PL056294.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2020 15:14
Operator : AJ\MA
Sample : L1351-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TAL-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:30:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

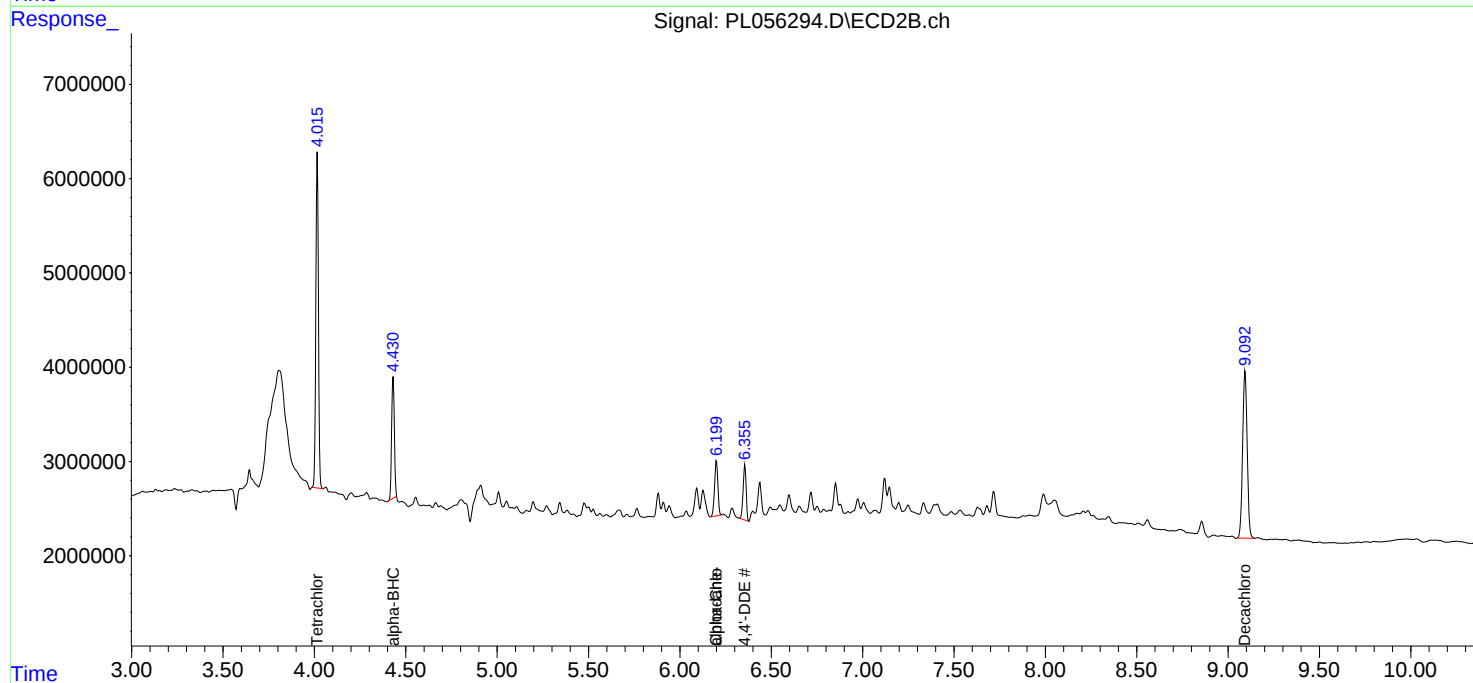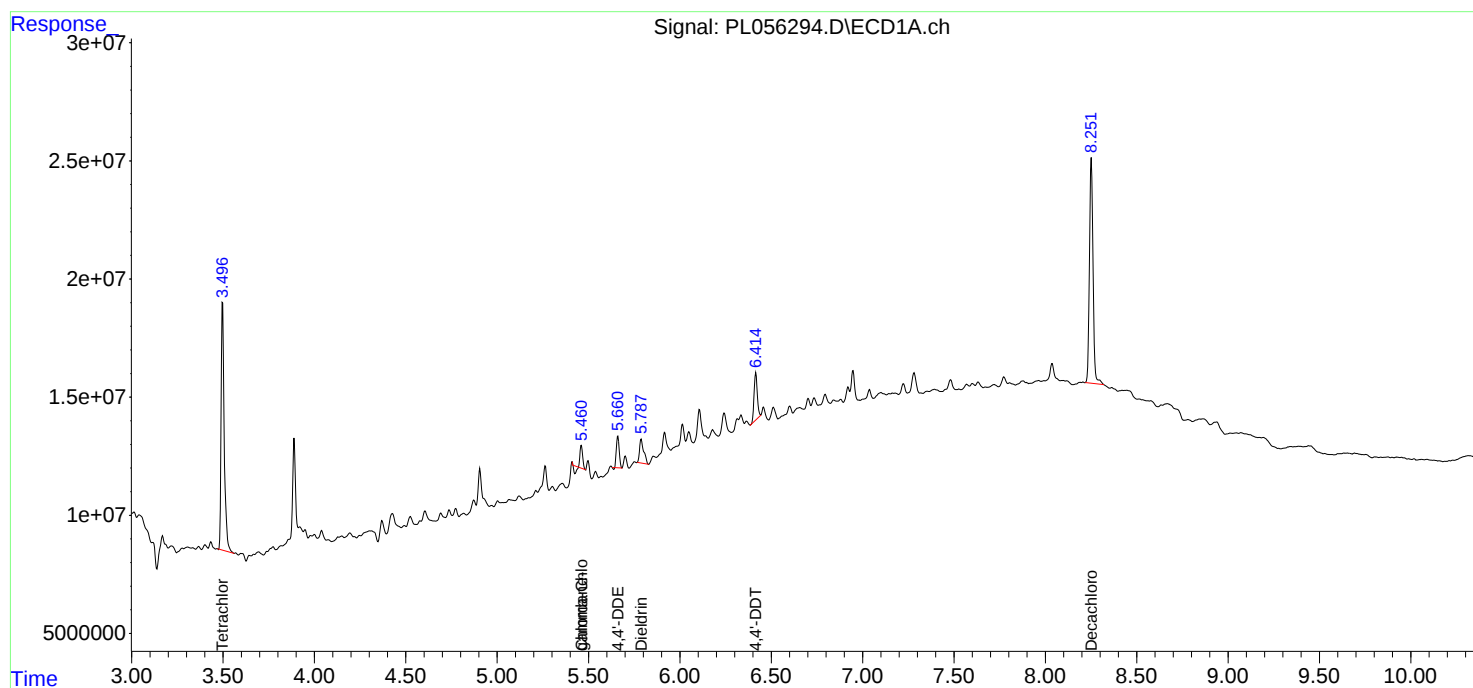


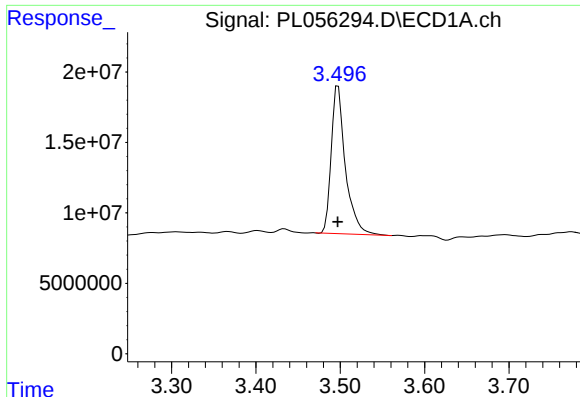

#1 Tetrachloro-m-xylene


R.T.: 3.498 min
Delta R.T.: 0.000 min
Response: 122651315
Conc: 11.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-1

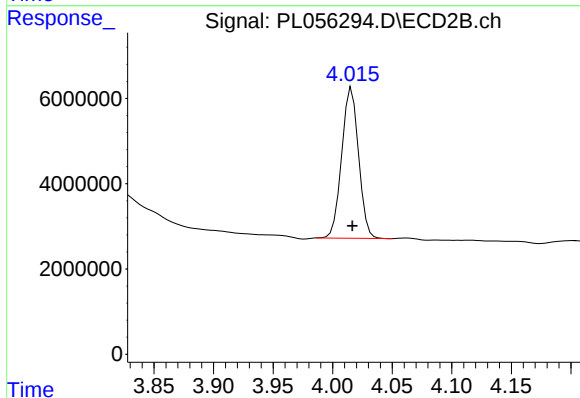


#1 Tetrachloro-m-xylene

R.T.: 4.016 min
Delta R.T.: 0.000 min
Response: 34870501
Conc: 11.93 ng/ml

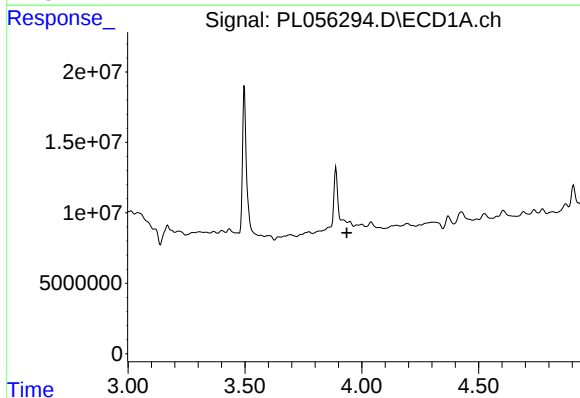


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

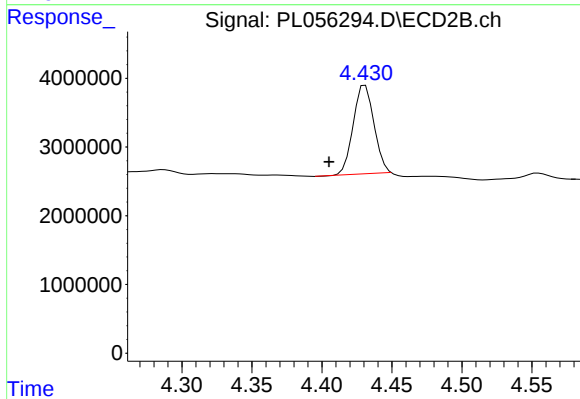

#2 alpha-BHC


R.T.: 4.431 min
Delta R.T.: 0.026 min
Response: 13288185
Conc: 3.04 ng/ml

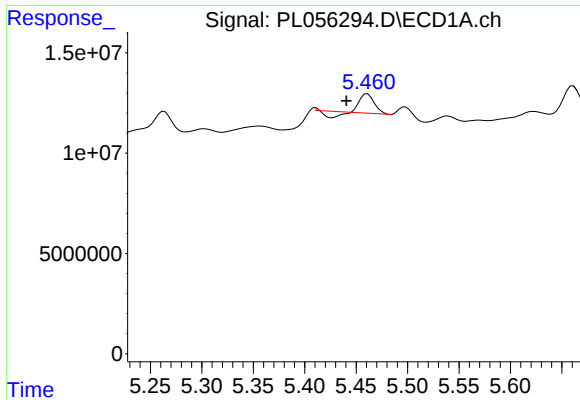

#10 gamma-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.020 min
Response: 7041741
Conc: 0.45 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-1

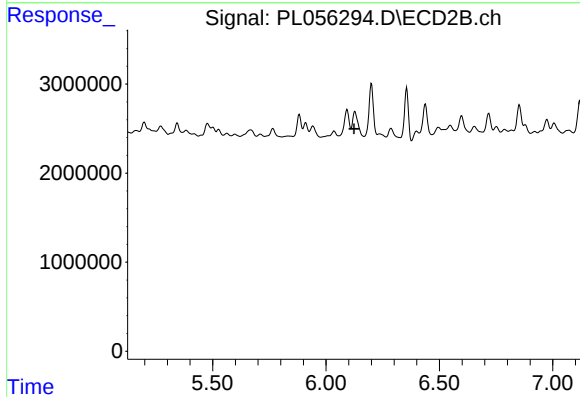


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.124 min
Response: 0
Conc: N.D.

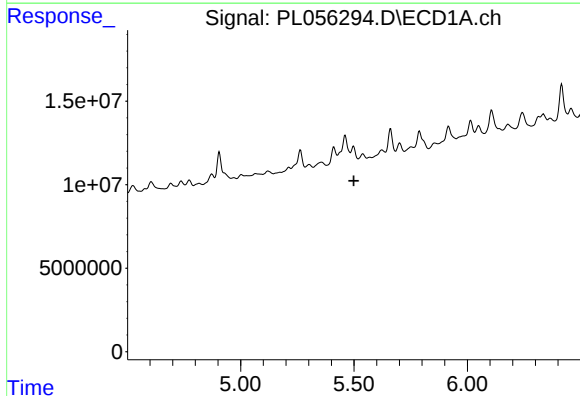


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

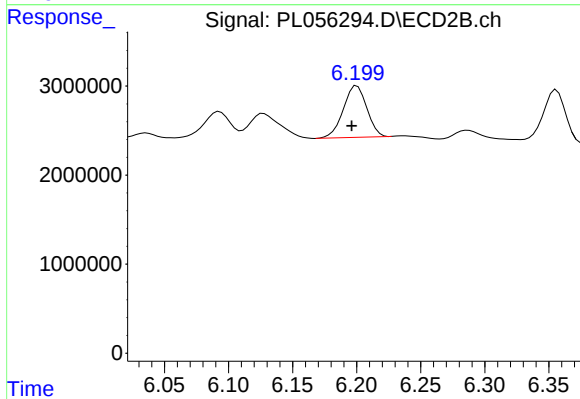

#11 alpha-Chlordane


R.T.: 6.200 min
Delta R.T.: 0.004 min
Response: 7400773
Conc: 2.33 ng/ml

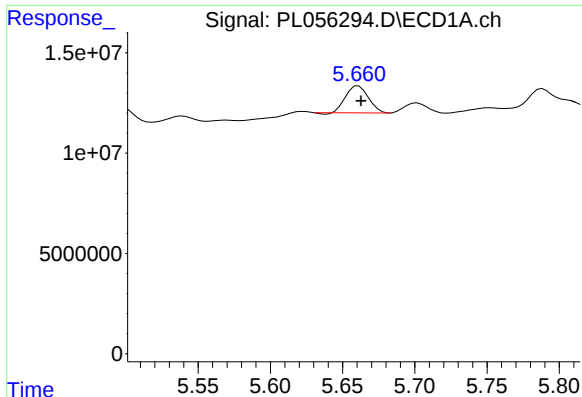

#12 4,4'-DDE


R.T.: 5.661 min
Delta R.T.: -0.002 min
Response: 14420113
Conc: 0.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-1

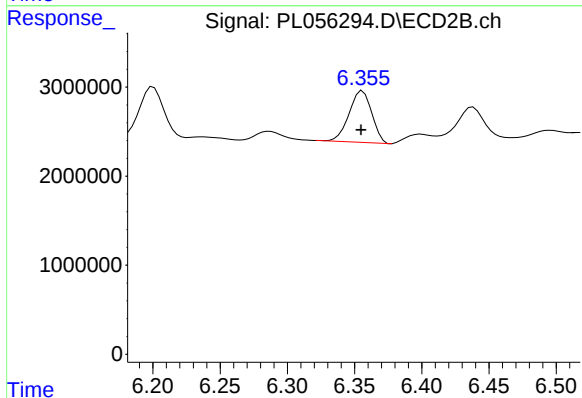


#12 4,4'-DDE

R.T.: 6.356 min
Delta R.T.: 0.001 min
Response: 6802214
Conc: 2.27 ng/ml

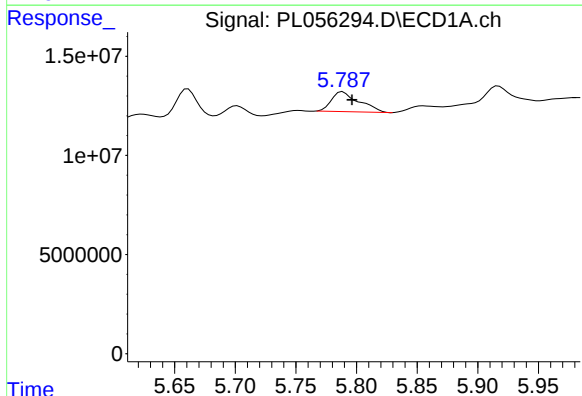


#13 Dieldrin

R.T.: 5.789 min
Delta R.T.: -0.008 min
Response: 15860216
Conc: 1.03 ng/ml

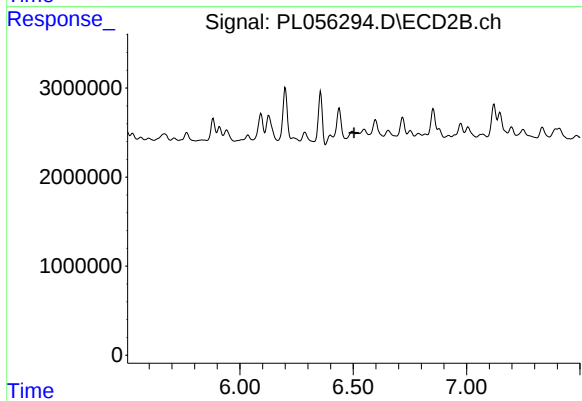

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.504 min
Response: 0
Conc: N.D.

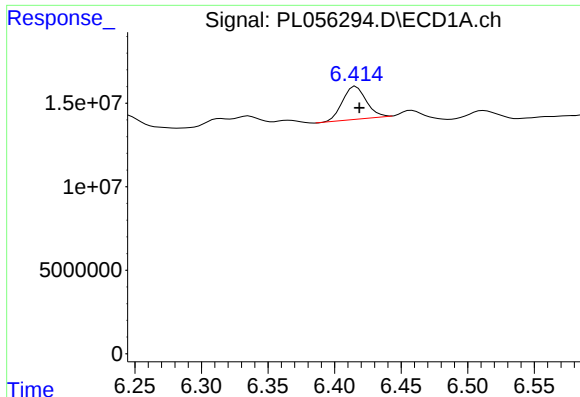

#17 4,4'-DDT


R.T.: 6.416 min
Delta R.T.: -0.003 min
Response: 24296555
Conc: 2.22 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-1

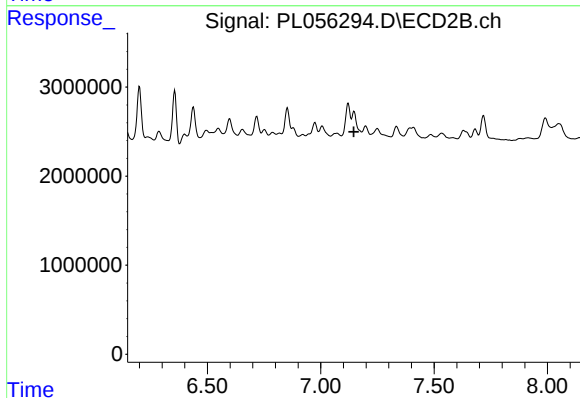


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

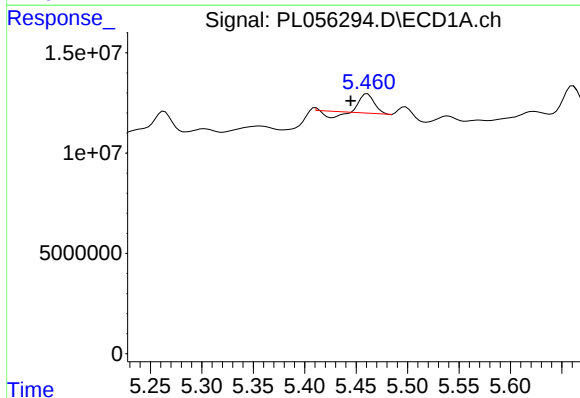


#25 Chlordane-3

R.T.: 5.461 min
Delta R.T.: 0.016 min
Response: 7041741
Conc: 5.58 ng/ml

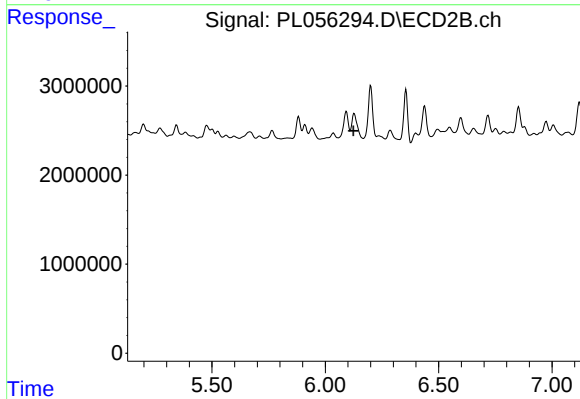

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

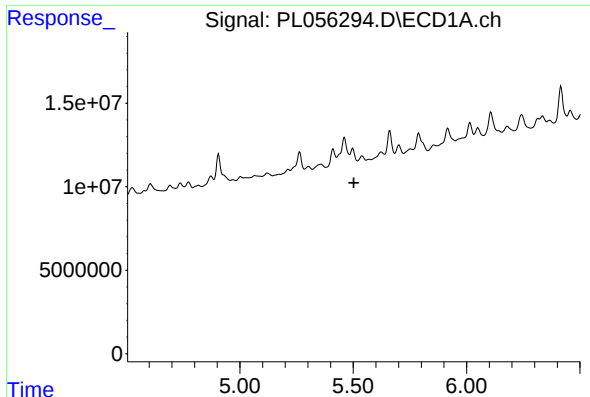

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 5.502 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
TAL-1

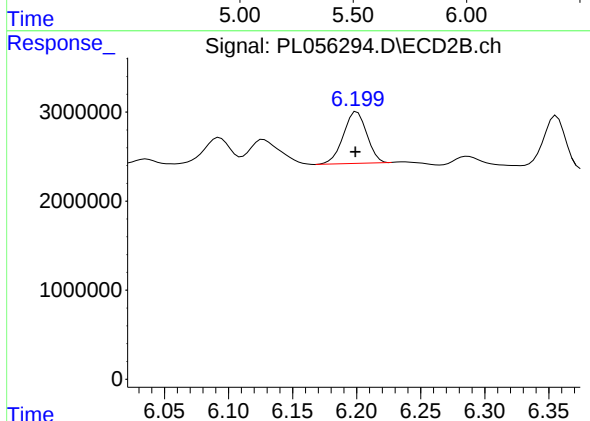


#26 Chlordane-4

R.T.: 6.200 min
Delta R.T.: 0.001 min
Response: 7400773
Conc: 16.84 ng/ml

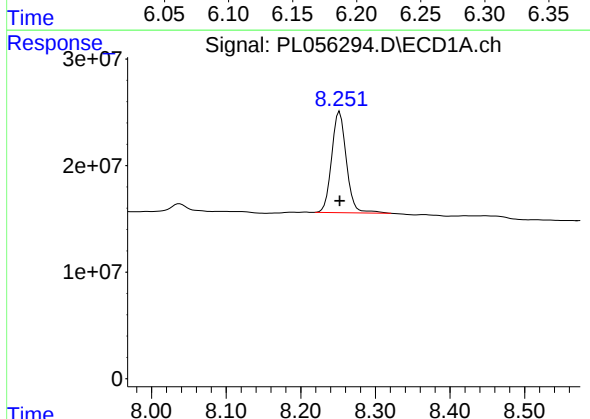

#28 Decachlorobiphenyl

R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 130325091
Conc: 12.38 ng/ml

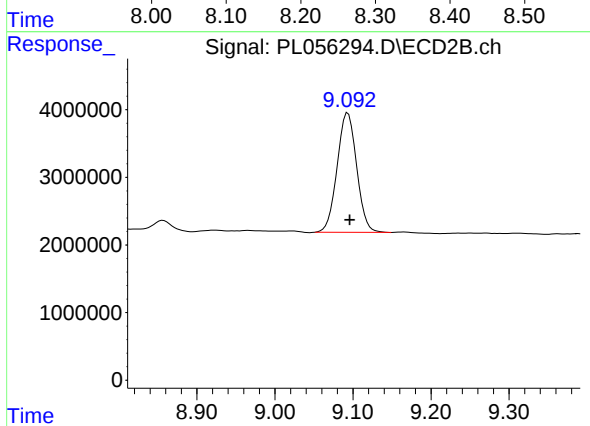

#28 Decachlorobiphenyl

R.T.: 9.094 min
Delta R.T.: -0.002 min
Response: 30750068
Conc: 13.59 ng/ml