

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
 Data File : PL056296.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2020 15:42
 Operator : AJ\MA
 Sample : L1351-03
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 TAL-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 00:30:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
 Quant Title : GC Extractables
 QLast Update : Tue Jan 28 13:10:37 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.497	4.015	121.9E6	33679882	11.644	11.518
28)	SA Decachlor...	8.251	9.093	128.5E6	29523044	12.209	13.052
Target Compounds							
2)	A alpha-BHC	0.000	4.430f	0	12479364	N.D.	2.851 #
10)	B gamma-Chl...	5.461f	0.000	11117678	0	0.709	N.D. #
11)	B alpha-Chl...	0.000	6.199	0	10547366	N.D.	3.328 #
12)	B 4,4'-DDE	5.661	6.355	21917740	9289022	1.512	3.101 #
13)	MA Dieldrin	5.789	0.000	24588438	0	1.599	N.D. #
17)	MA 4,4'-DDT	6.415	0.000	27002611	0	2.471	N.D. #
23)	Chlordane-1	4.370	0.000	12108039	0	31.986	N.D. #
25)	Chlordane-3	5.461f	0.000	11117678	0	8.806	N.D. #
26)	Chlordane-4	0.000	6.199	0	10547366	N.D.	24.006 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020320\
Data File : PL056296.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2020 15:42
Operator : AJ\MA
Sample : L1351-03
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
TAL-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 00:30:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012820.M
Quant Title : GC Extractables
QLast Update : Tue Jan 28 13:10:37 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

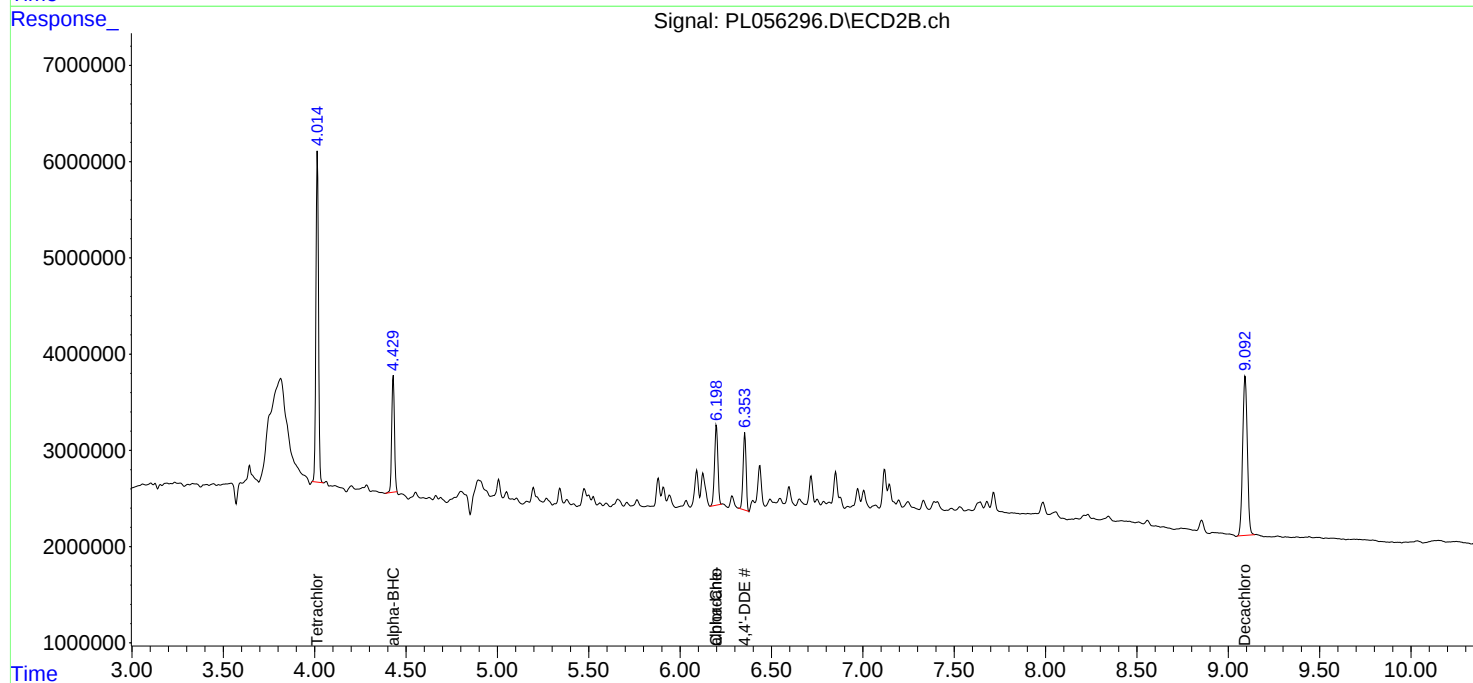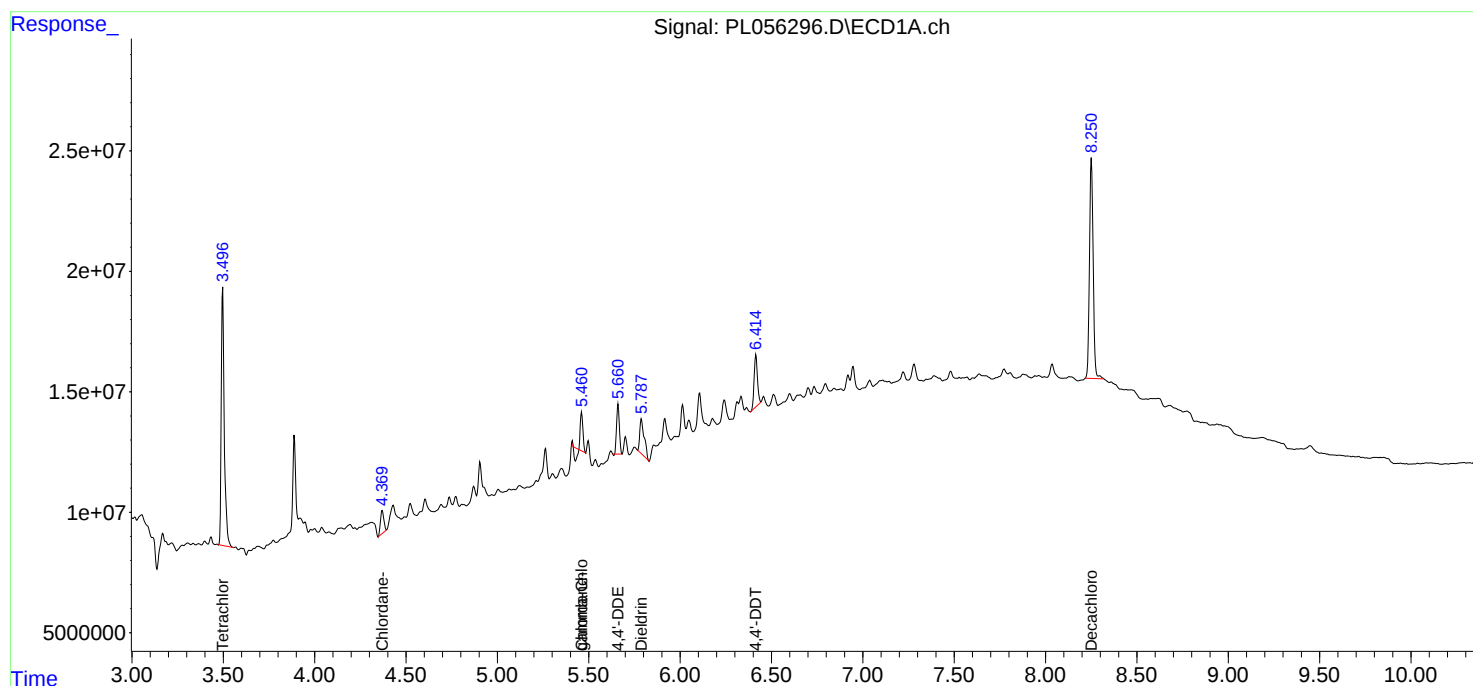


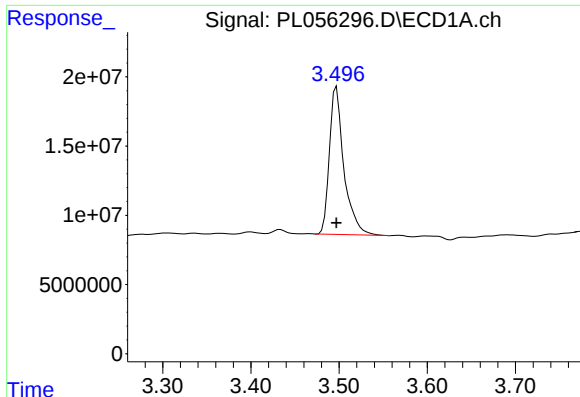

#1 Tetrachloro-m-xylene


R.T.: 3.497 min
Delta R.T.: 0.000 min
Response: 121945188
Conc: 11.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

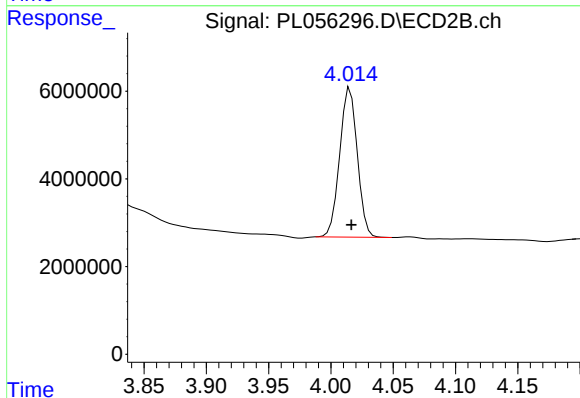


#1 Tetrachloro-m-xylene

R.T.: 4.015 min
Delta R.T.: -0.001 min
Response: 33679882
Conc: 11.52 ng/ml

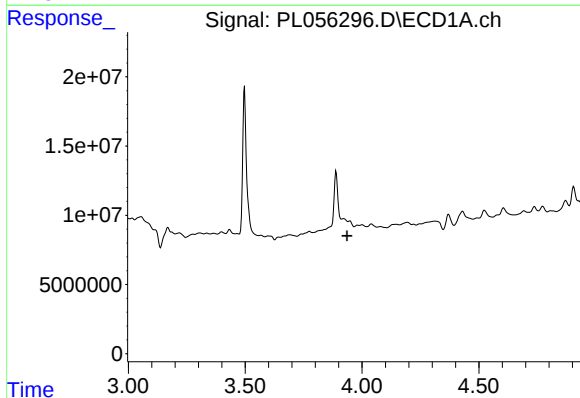


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.936 min
Response: 0
Conc: N.D.

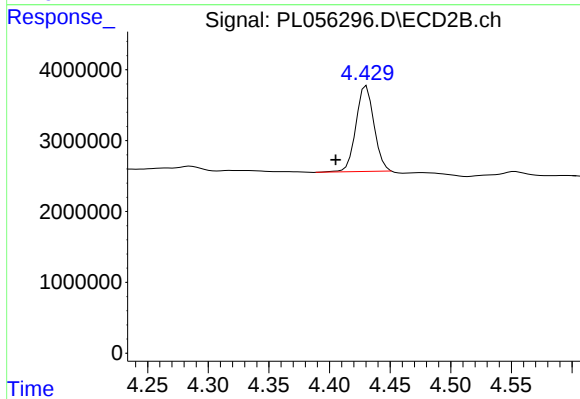

#2 alpha-BHC


R.T.: 4.430 min
Delta R.T.: 0.025 min
Response: 12479364
Conc: 2.85 ng/ml

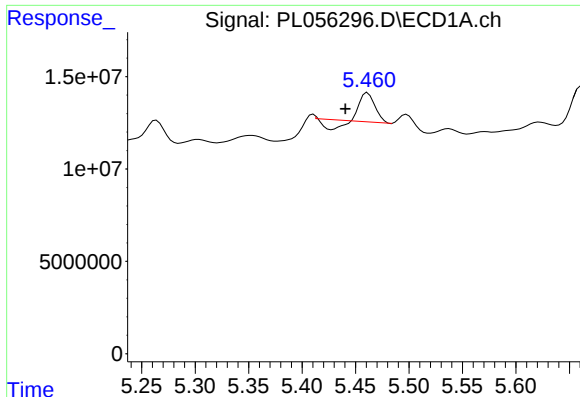

#10 gamma-Chlordane


R.T.: 5.461 min
Delta R.T.: 0.021 min
Response: 11117678
Conc: 0.71 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

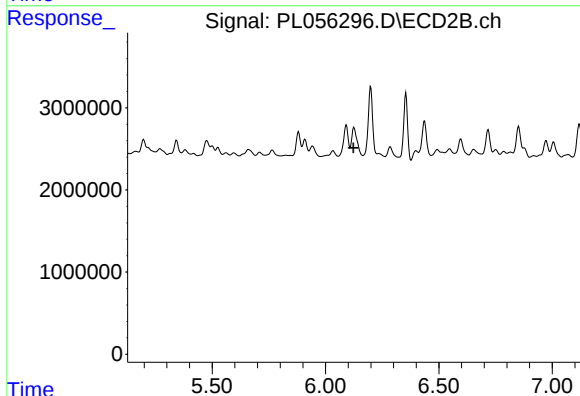


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.124 min
Response: 0
Conc: N.D.

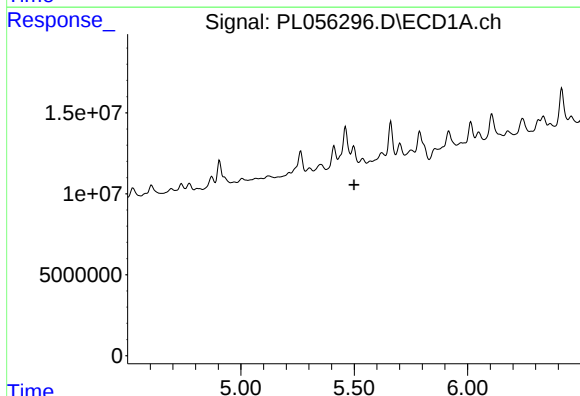


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.499 min
Response: 0
Conc: N.D.

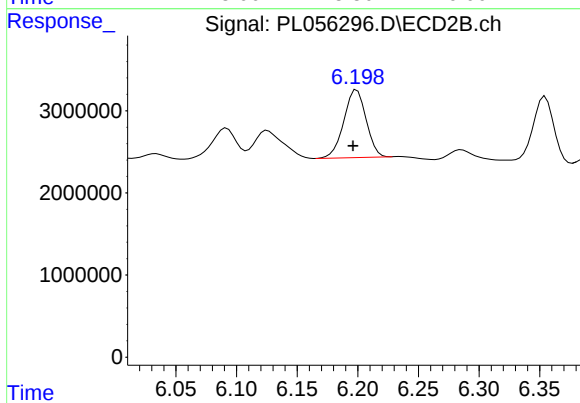

#11 alpha-Chlordane


R.T.: 6.199 min
Delta R.T.: 0.003 min
Response: 10547366
Conc: 3.33 ng/ml

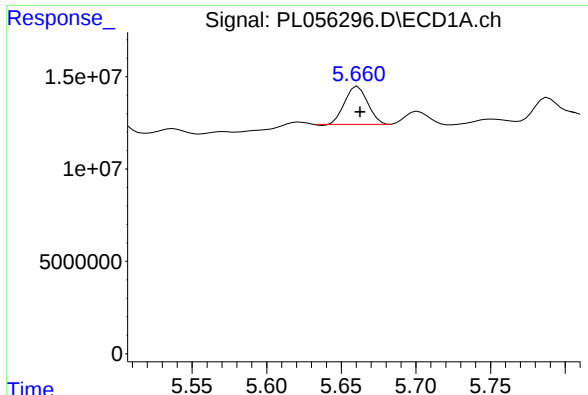

#12 4,4'-DDE


R.T.: 5.661 min
Delta R.T.: -0.002 min
Response: 21917740
Conc: 1.51 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

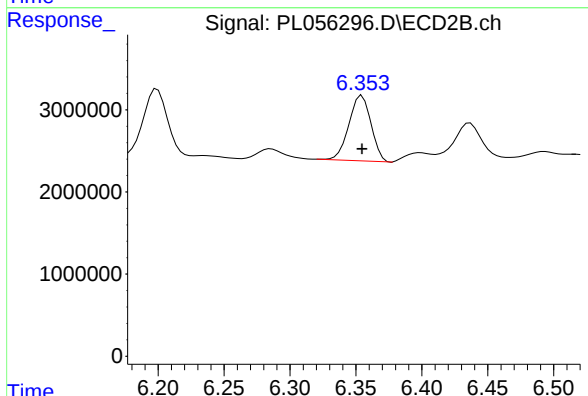


#12 4,4'-DDE

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 9289022
Conc: 3.10 ng/ml

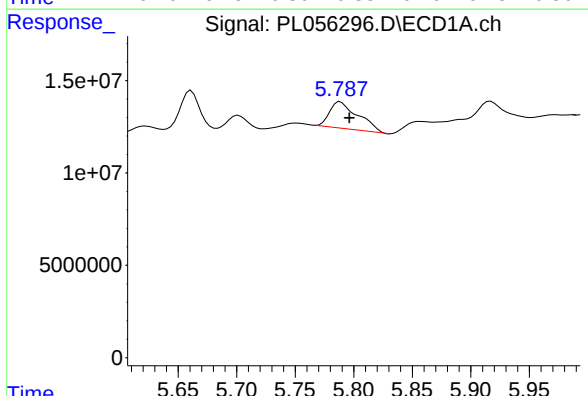


#13 Dieldrin

R.T.: 5.789 min
Delta R.T.: -0.008 min
Response: 24588438
Conc: 1.60 ng/ml

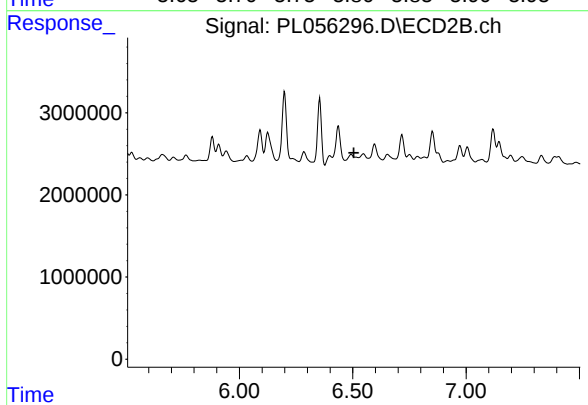

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.504 min
Response: 0
Conc: N.D.

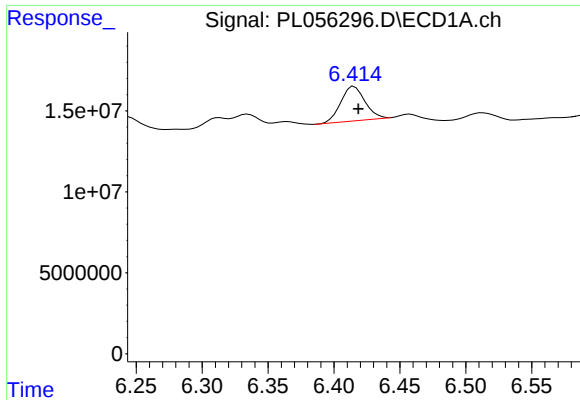

#17 4,4'-DDT


R.T.: 6.415 min
Delta R.T.: -0.003 min
Response: 27002611
Conc: 2.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

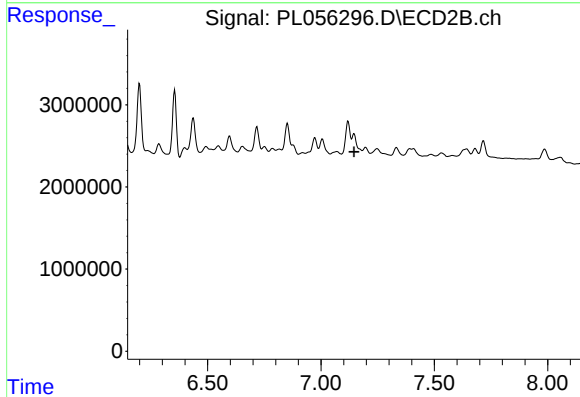


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.146 min
Response: 0
Conc: N.D.

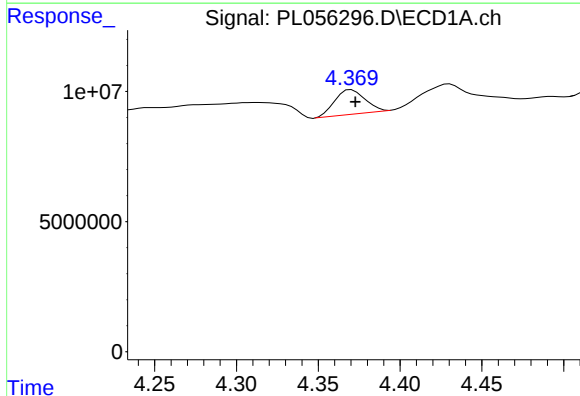


#23 Chlordane-1

R.T.: 4.370 min
Delta R.T.: -0.002 min
Response: 12108039
Conc: 31.99 ng/ml

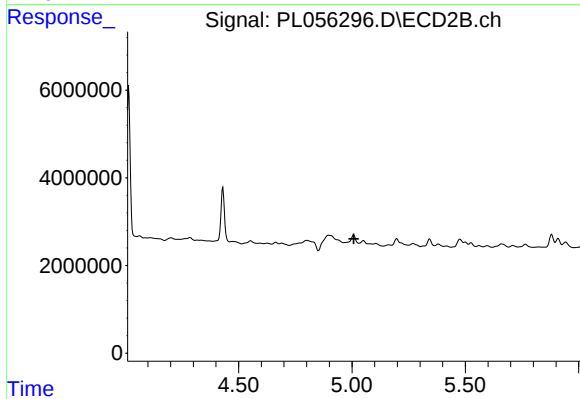

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.008 min
Response: 0
Conc: N.D.

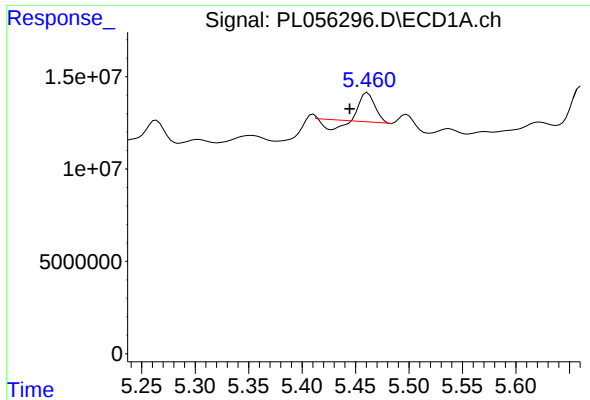

#25 Chlordane-3


R.T.: 5.461 min
Delta R.T.: 0.017 min
Response: 11117678
Conc: 8.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

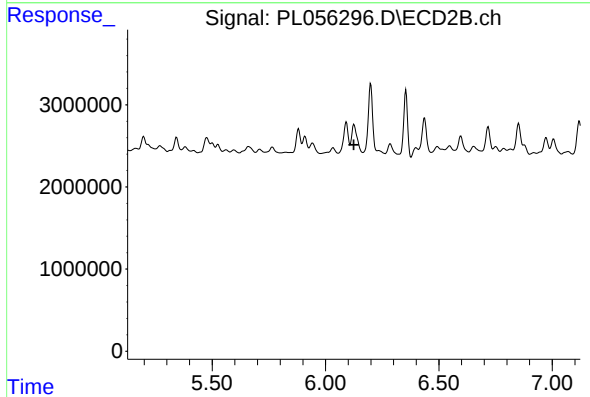


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.125 min
Response: 0
Conc: N.D.

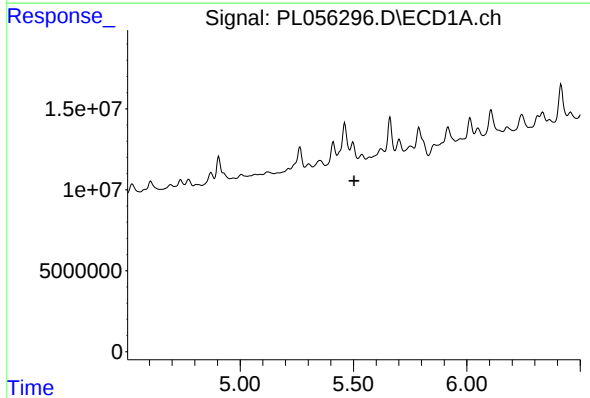


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 5.502 min
Response: 0
Conc: N.D.

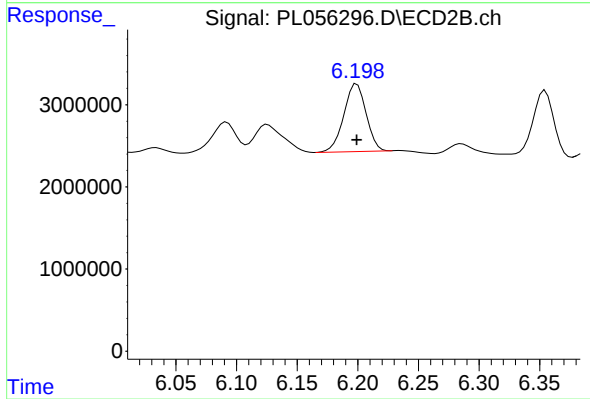

#26 Chlordane-4


R.T.: 6.199 min
Delta R.T.: 0.000 min
Response: 10547366
Conc: 24.01 ng/ml

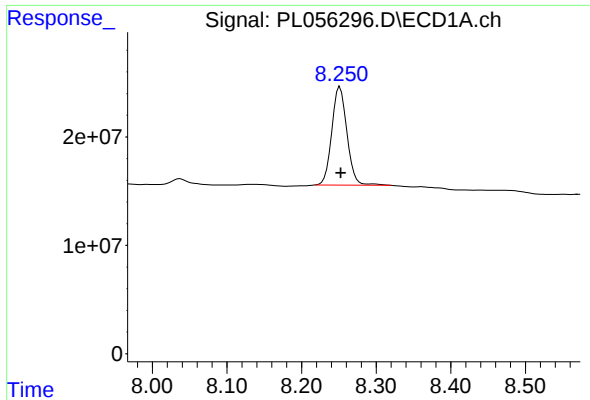

#28 Decachlorobiphenyl

R.T.: 8.251 min
Delta R.T.: 0.000 min
Response: 128535597
Conc: 12.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
TAL-3

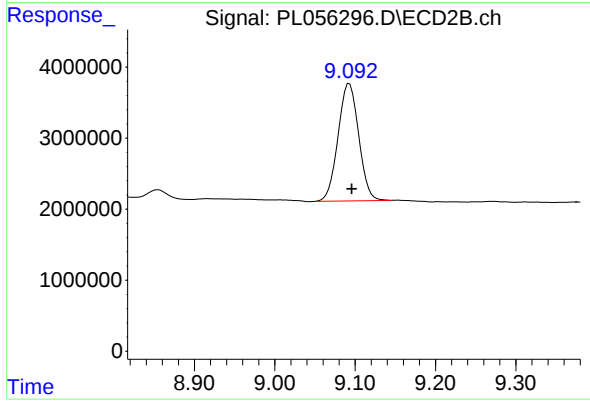

#28 Decachlorobiphenyl

R.T.: 9.093 min
Delta R.T.: -0.003 min
Response: 29523044
Conc: 13.05 ng/ml