

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064550.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 11:01
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 15:46:14 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA Heptachlor	0.000	5.309	0	1149181	N.D.	0.330 #
6) B beta-BHC	0.000	4.987	0	5599021	N.D.	3.309 #
8) B Heptachlo...	0.000	6.014	0	11292274	N.D.	4.408 #
14) MA Endrin	5.970	0.000	3467351	0	0.948	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064550.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 11:01
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 15:46:14 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

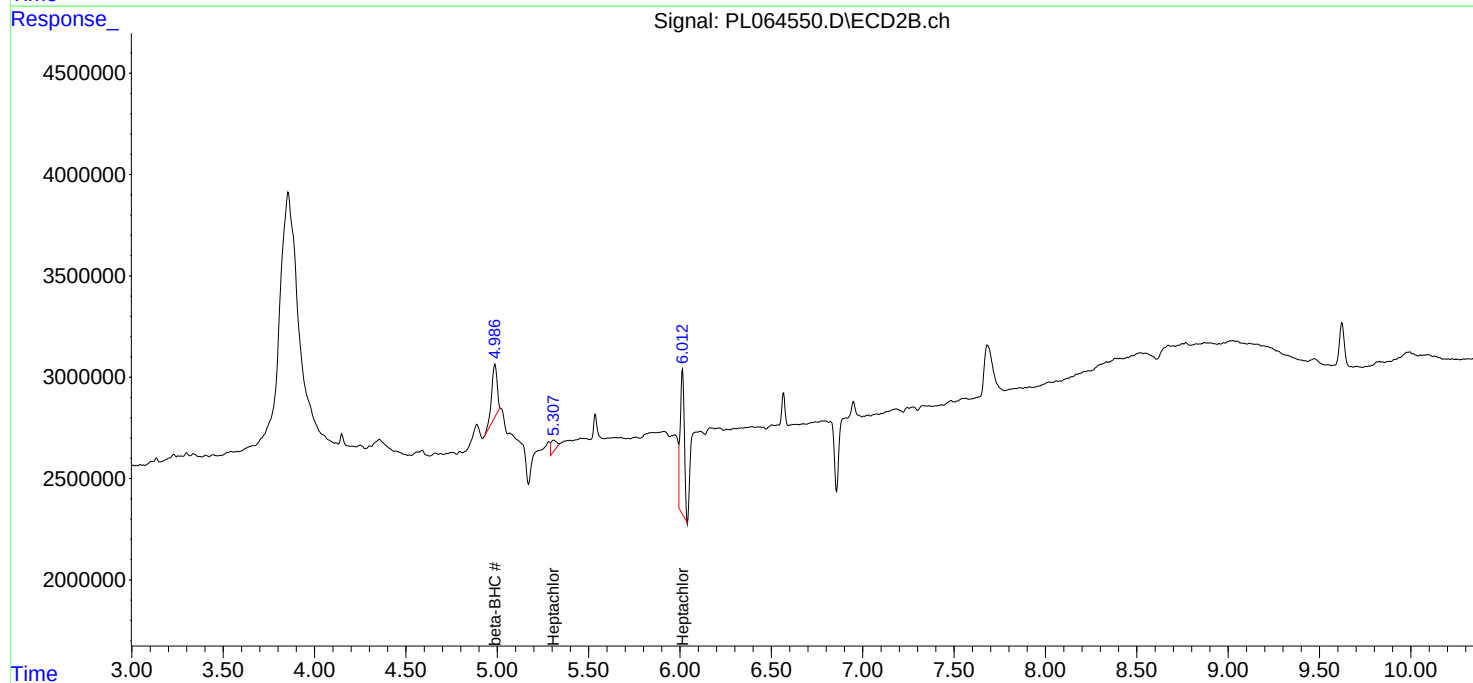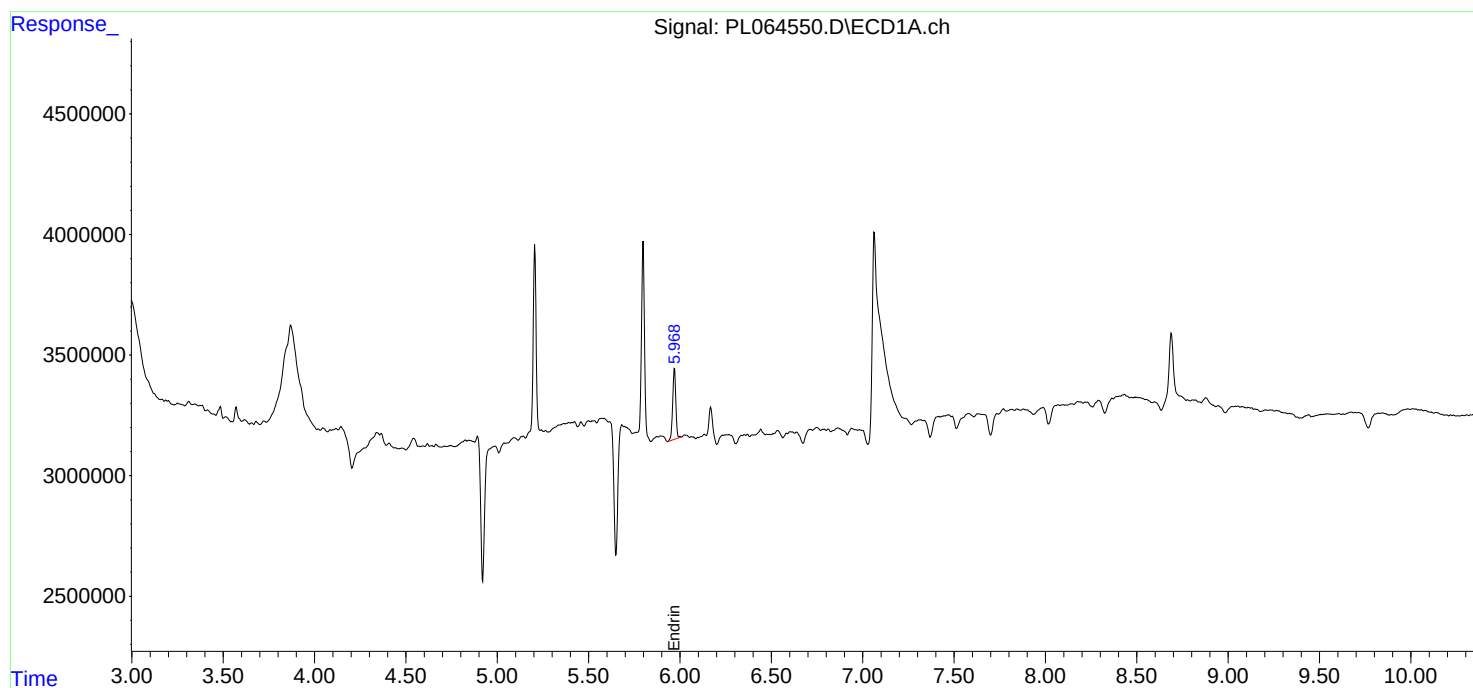


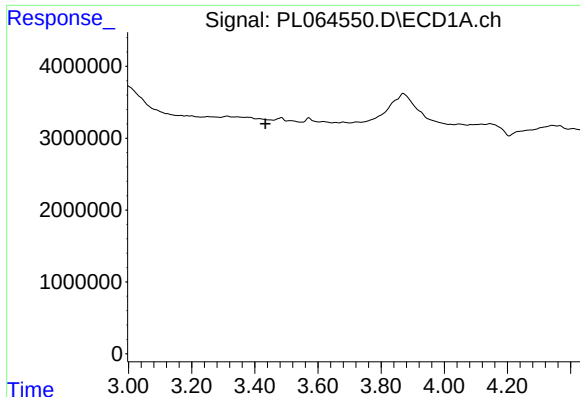

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.433 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

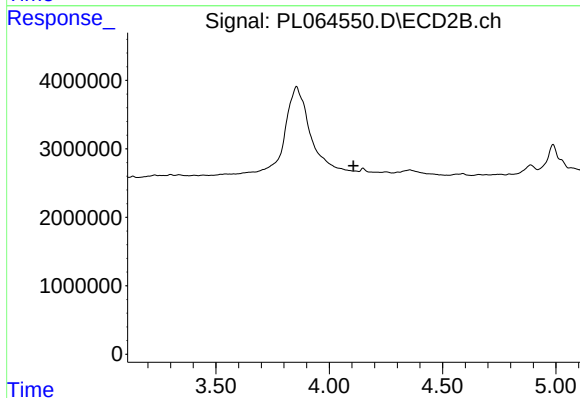


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

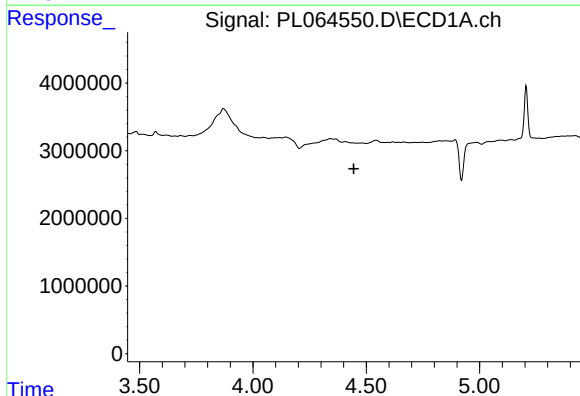


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

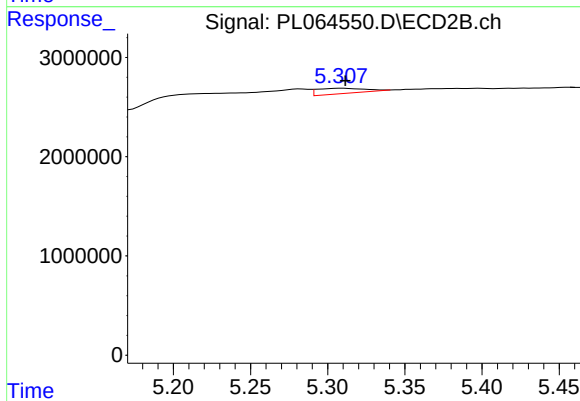

#4 Heptachlor


R.T.: 5.309 min
Delta R.T.: -0.003 min
Response: 1149181
Conc: 0.33 ng/ml

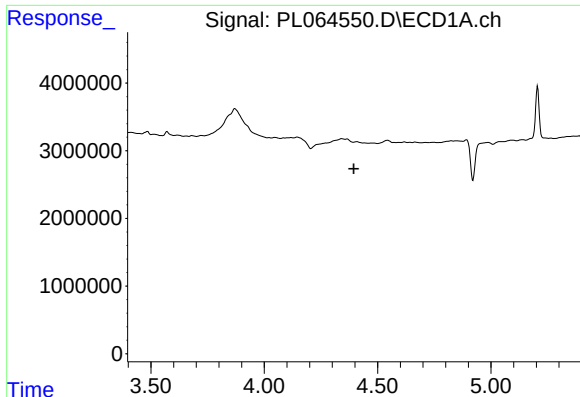

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

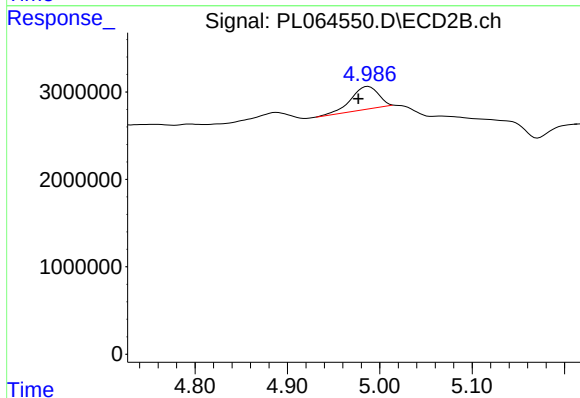


#6 beta-BHC

R.T.: 4.987 min
Delta R.T.: 0.010 min
Response: 5599021
Conc: 3.31 ng/ml

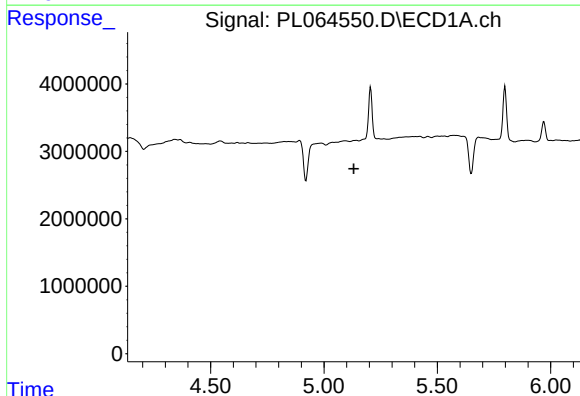


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.131 min
Response: 0
Conc: N.D.

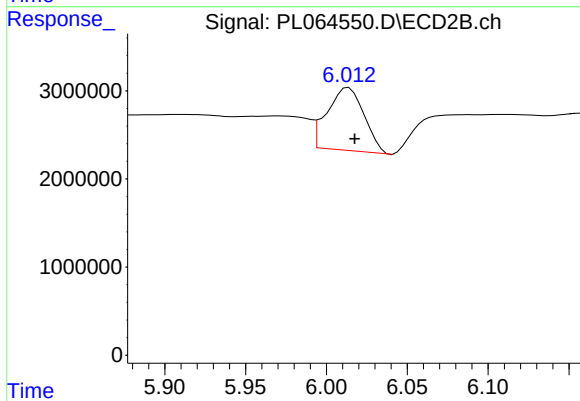

#8 Heptachlor epoxide


R.T.: 6.014 min
Delta R.T.: -0.004 min
Response: 11292274
Conc: 4.41 ng/ml

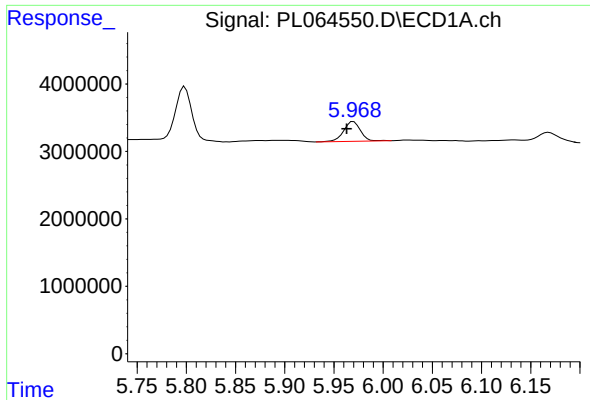

#14 Endrin


R.T.: 5.970 min
Delta R.T.: 0.007 min
Response: 3467351
Conc: 0.95 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

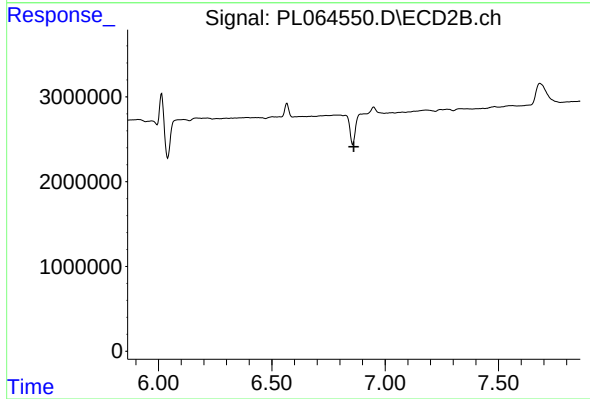


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.862 min
Response: 0
Conc: N.D.

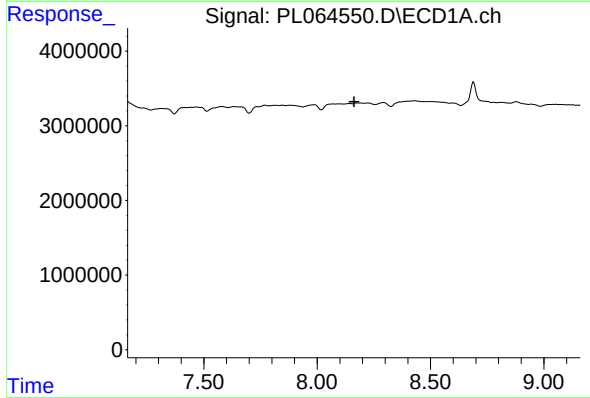

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.163 min
Response: 0
Conc: N.D.

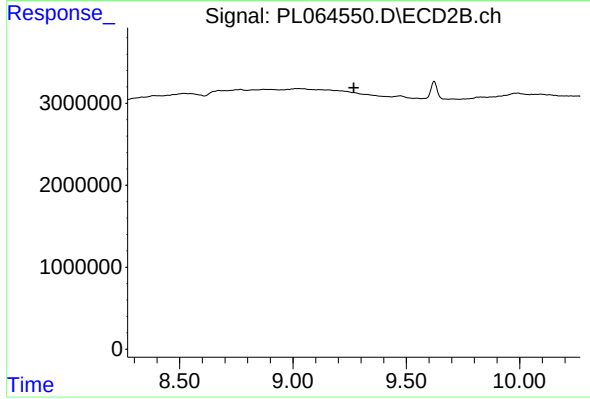

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.268 min
Response: 0
Conc: N.D.