

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064557.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 13:01
 Operator : AR\AJ
 Sample : M1286-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 JJ BH 02 0-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 15:47:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	41562113	34600580	13.653	14.526
28)	SA Decachlor...	8.165	9.273	35491421	27483341	11.262	13.424
Target Compounds							
2)	A alpha-BHC	0.000	4.532f	0	1942461	N.D.	0.562 #
6)	B beta-BHC	0.000	4.990	0	3979425	N.D.	2.352 #
7)	B delta-BHC	0.000	5.198	0	875378	N.D.	0.284 #
10)	B gamma-Chl...	5.359	6.255	1041508	3160159	0.252	1.087 #
11)	B alpha-Chl...	5.416	6.327	1756612	4943805	0.428	1.680 #
12)	B 4,4'-DDE	5.582	6.485	2018947	2738174	0.536	1.057 #
17)	MA 4,4'-DDT	6.331	0.000	1985572	0	0.647	N.D. #
23)	Chlordane-1	4.294	0.000	2127479	0	19.354	N.D. #
25)	Chlordane-3	5.359	6.255	1041508	3160159	2.887	8.815 #
26)	Chlordane-4	5.416	6.327	1756612	4943805	5.906	11.242 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064557.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 13:01
Operator : AR\AJ
Sample : M1286-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 15:47:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

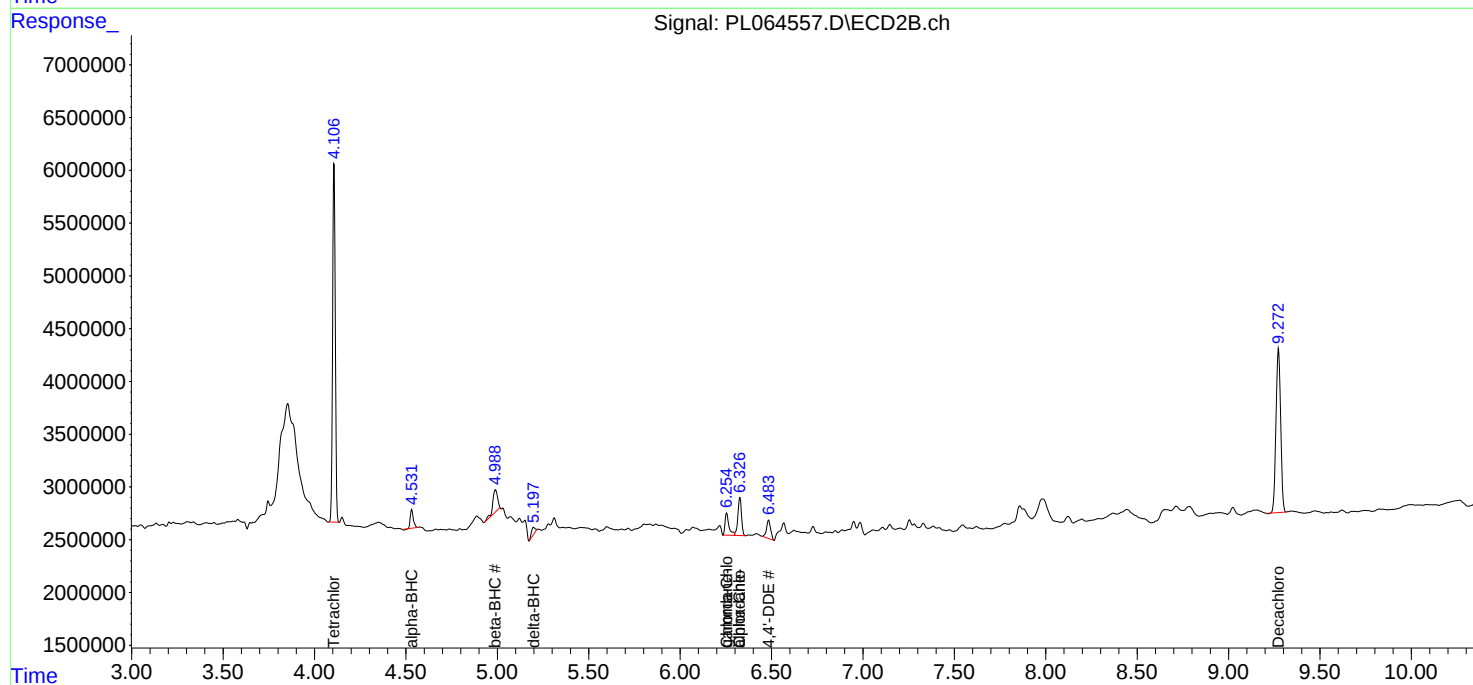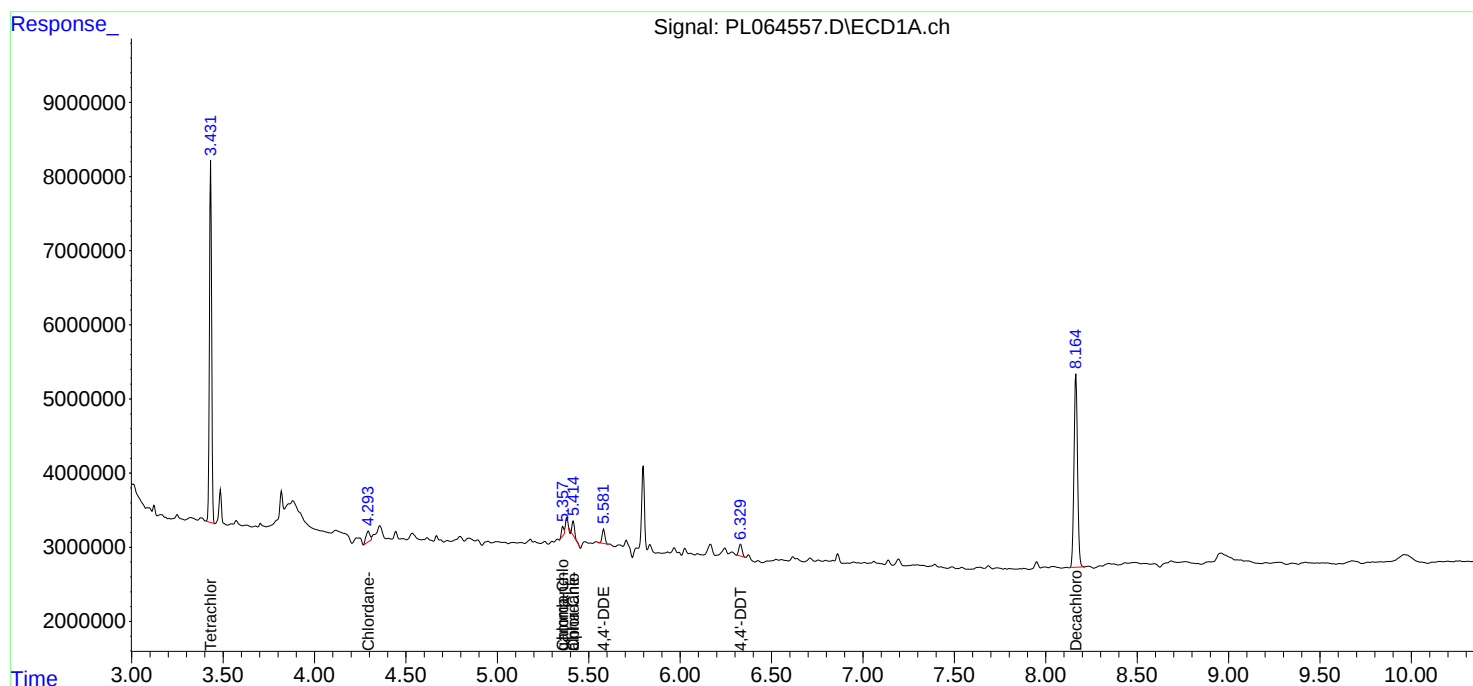


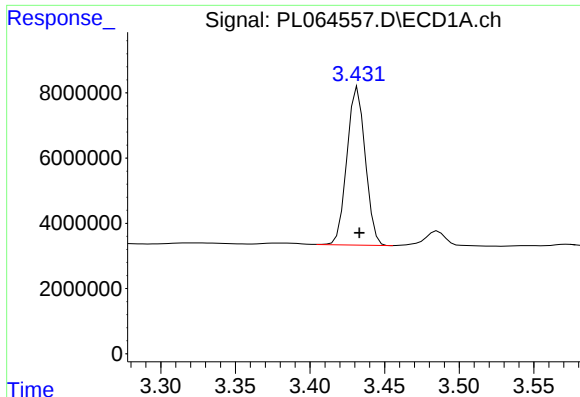

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 41562113
Conc: 13.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

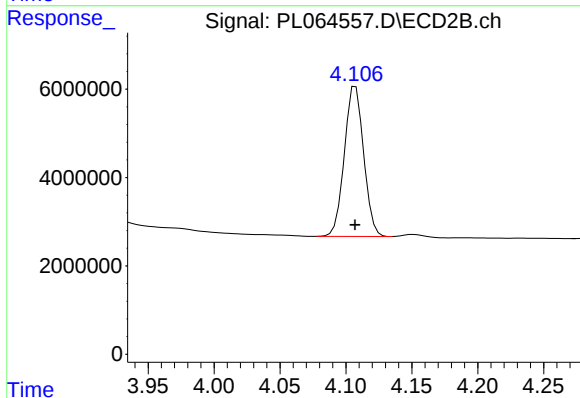


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 34600580
Conc: 14.53 ng/ml

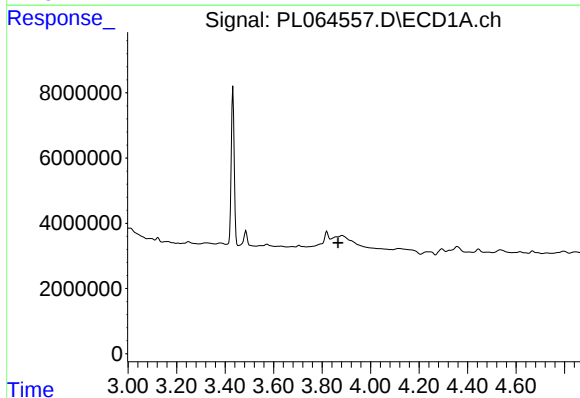


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.866 min
Response: 0
Conc: N.D.

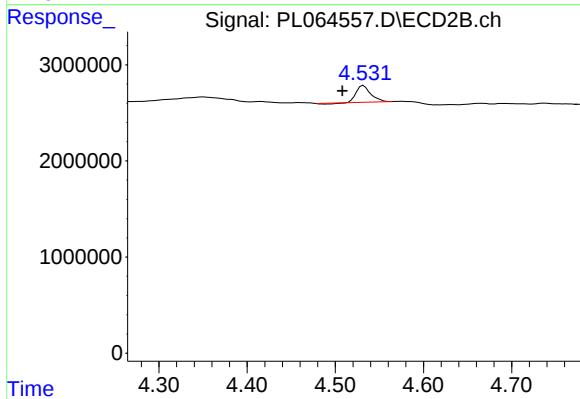

#2 alpha-BHC


R.T.: 4.532 min
Delta R.T.: 0.024 min
Response: 1942461
Conc: 0.56 ng/ml

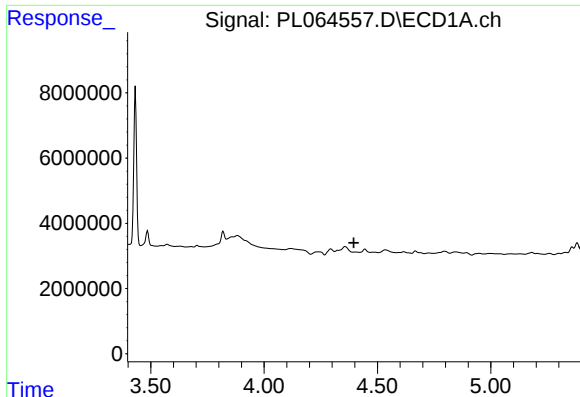

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

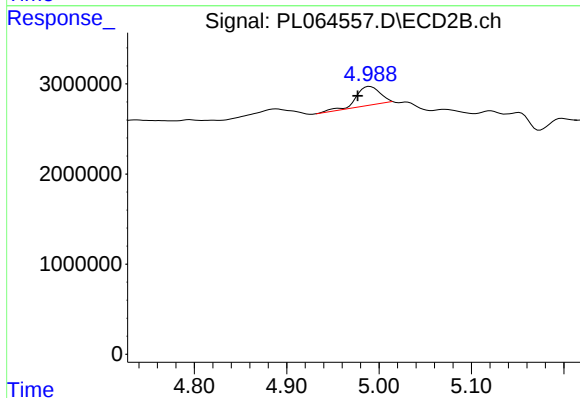


#6 beta-BHC

R.T.: 4.990 min
Delta R.T.: 0.013 min
Response: 3979425
Conc: 2.35 ng/ml

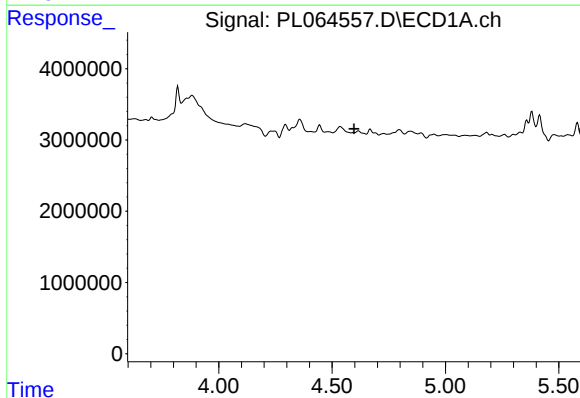


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

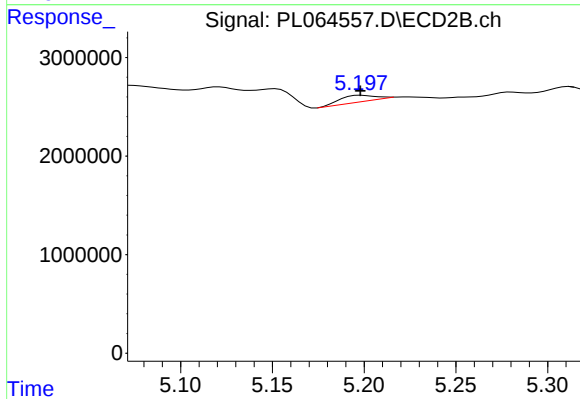

#7 delta-BHC


R.T.: 5.198 min
Delta R.T.: 0.000 min
Response: 875378
Conc: 0.28 ng/ml

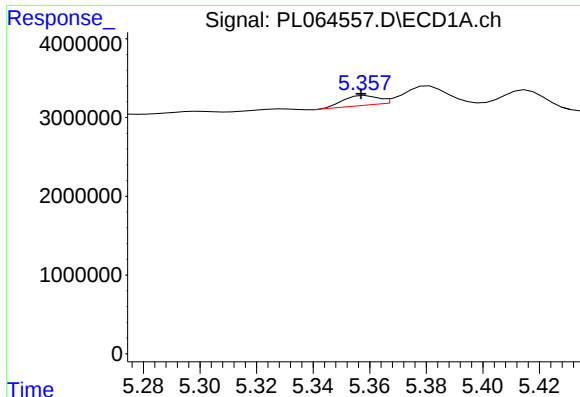

#10 gamma-Chlordane


R.T.: 5.359 min
Delta R.T.: 0.002 min
Response: 1041508
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

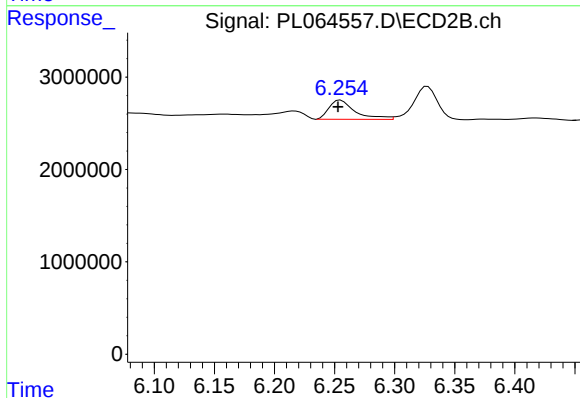


#10 gamma-Chlordane

R.T.: 6.255 min
Delta R.T.: 0.002 min
Response: 3160159
Conc: 1.09 ng/ml

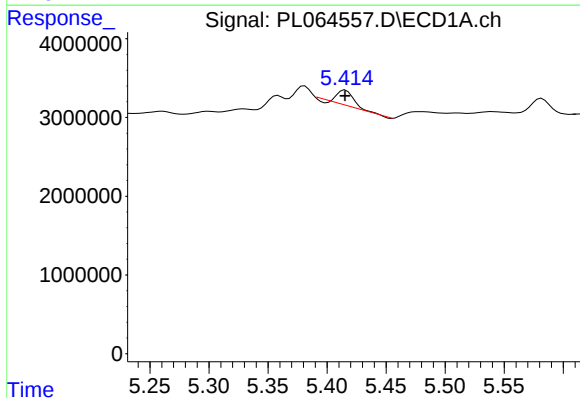


#11 alpha-Chlordane

R.T.: 5.416 min
Delta R.T.: 0.000 min
Response: 1756612
Conc: 0.43 ng/ml

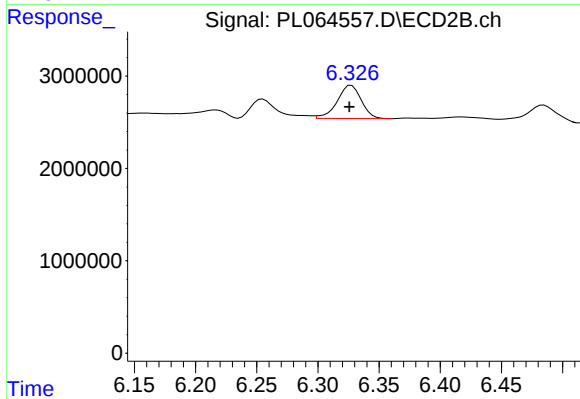

#11 alpha-Chlordane


R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 4943805
Conc: 1.68 ng/ml

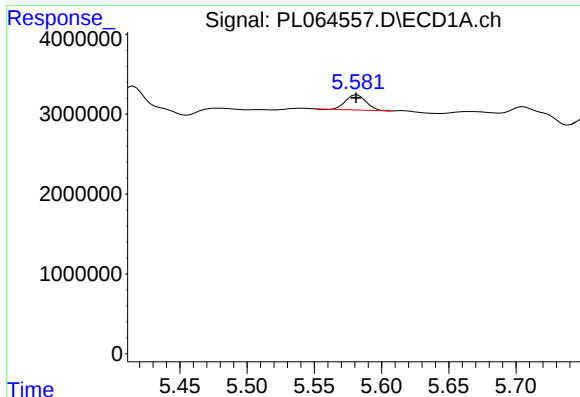

#12 4,4'-DDE


R.T.: 5.582 min
Delta R.T.: 0.000 min
Response: 2018947
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :
JJ_BH_02_0-1

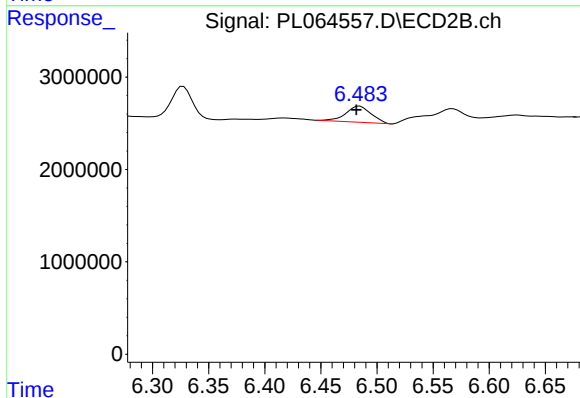


#12 4,4'-DDE

R.T.: 6.485 min
Delta R.T.: 0.003 min
Response: 2738174
Conc: 1.06 ng/ml

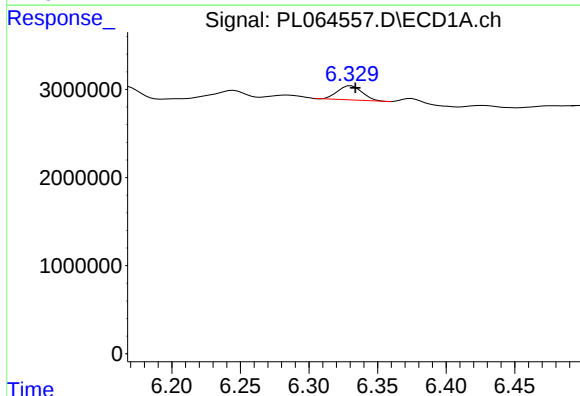


#17 4,4'-DDT

R.T.: 6.331 min
Delta R.T.: -0.003 min
Response: 1985572
Conc: 0.65 ng/ml

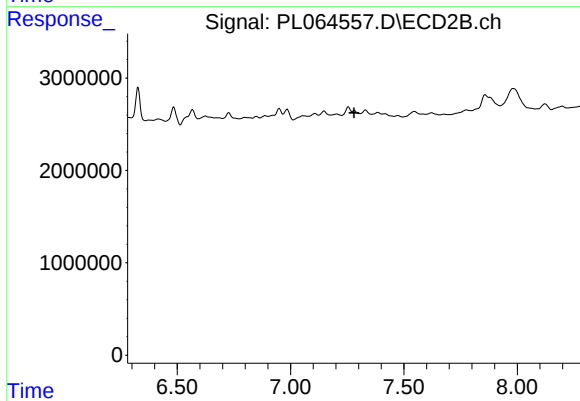

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 7.280 min
Response: 0
Conc: N.D.

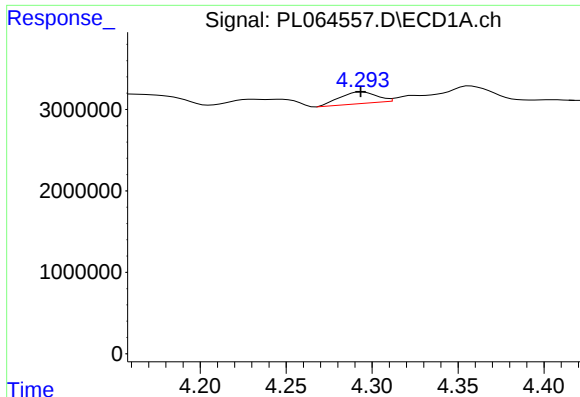

#23 Chlordane-1


R.T.: 4.294 min
Delta R.T.: 0.000 min
Response: 2127479
Conc: 19.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

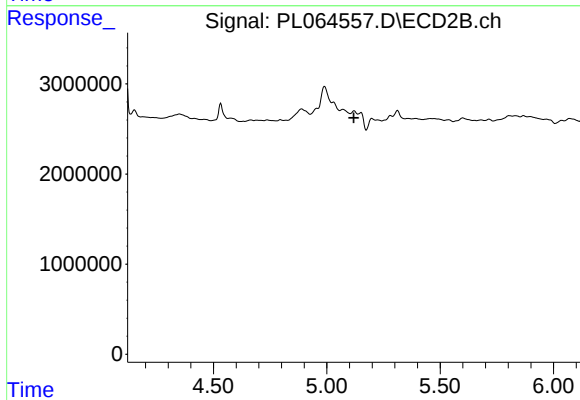


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

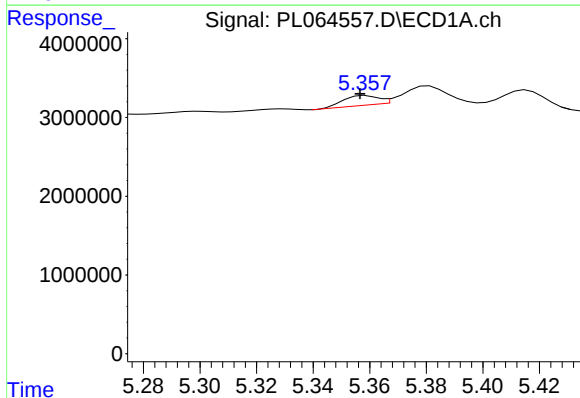


#25 Chlordane-3

R.T.: 5.359 min
Delta R.T.: 0.002 min
Response: 1041508
Conc: 2.89 ng/ml

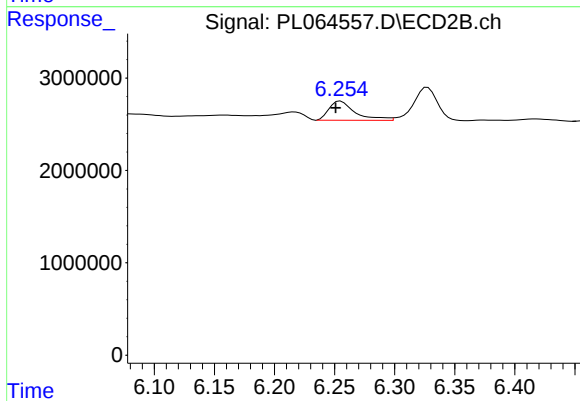

#25 Chlordane-3


R.T.: 6.255 min
Delta R.T.: 0.004 min
Response: 3160159
Conc: 8.82 ng/ml

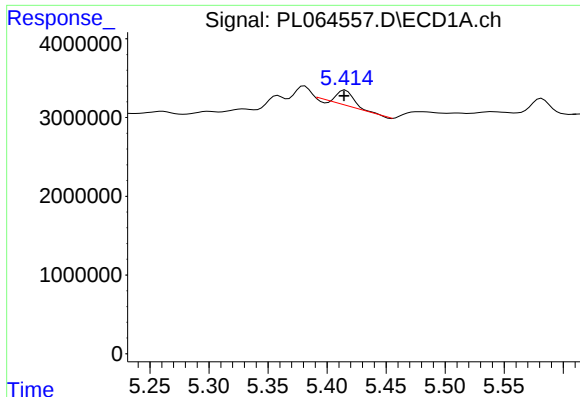

#26 Chlordane-4


R.T.: 5.416 min
Delta R.T.: 0.001 min
Response: 1756612
Conc: 5.91 ng/ml

Instrument :
ECD_L
ClientSampleId :
JJ BH 02 0-1

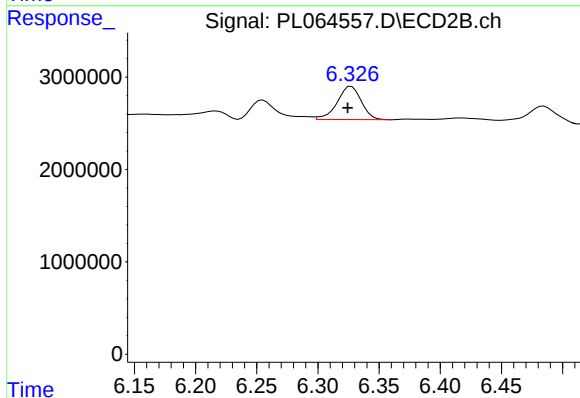


#26 Chlordane-4

R.T.: 6.327 min
Delta R.T.: 0.003 min
Response: 4943805
Conc: 11.24 ng/ml

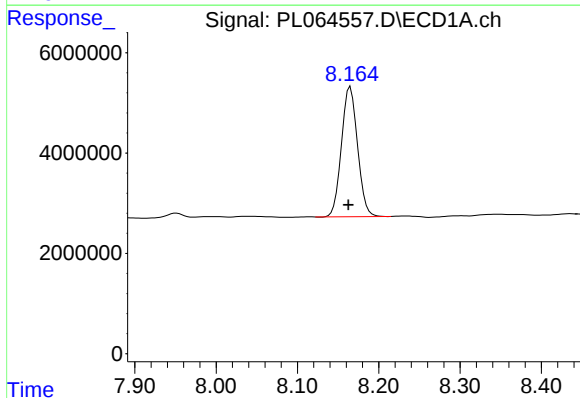

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.003 min
Response: 35491421
Conc: 11.26 ng/ml

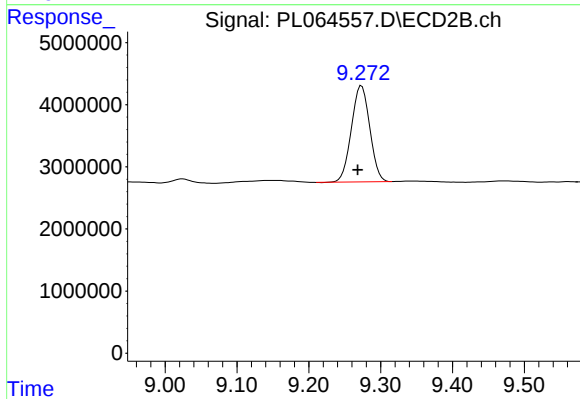

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.005 min
Response: 27483341
Conc: 13.42 ng/ml