

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064562.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 14:13
 Operator : AR\AJ
 Sample : M1292-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-003-0205

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 15:47:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	63413893	51048714	20.831	21.431
28)	SA Decachlor...	8.165	9.273	54634982	40375477	17.337	19.720
Target Compounds							
4)	MA Heptachlor	0.000	5.305	0	2271170	N.D.	0.652 #
6)	B beta-BHC	0.000	4.988	0	3023189	N.D.	1.787 #
7)	B delta-BHC	0.000	5.222f	0	4379387	N.D.	1.422 #
15)	B Endosulfa...	0.000	7.080	0	2342436	N.D.	0.949 #
18)	B Endrin al...	6.375f	0.000	3119400	0	1.017	N.D. #
19)	B Endosulfa...	6.618	0.000	2723069	0	0.749	N.D. #
20)	A Methoxychlor	6.863f	0.000	3845020	0	2.129	N.D. #
22)	Mirex	0.000	8.370	0	2022770	N.D.	1.053 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064562.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 14:13
Operator : AR\AJ
Sample : M1292-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 15:47:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

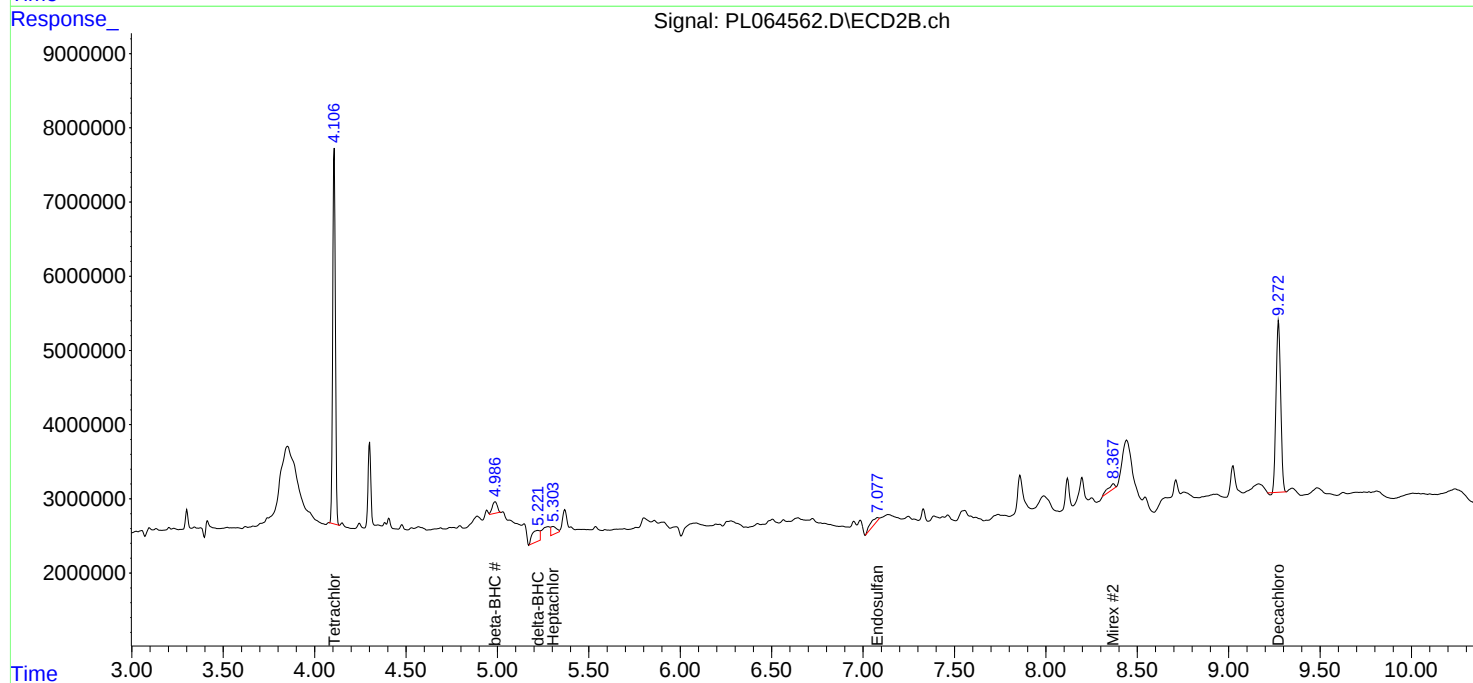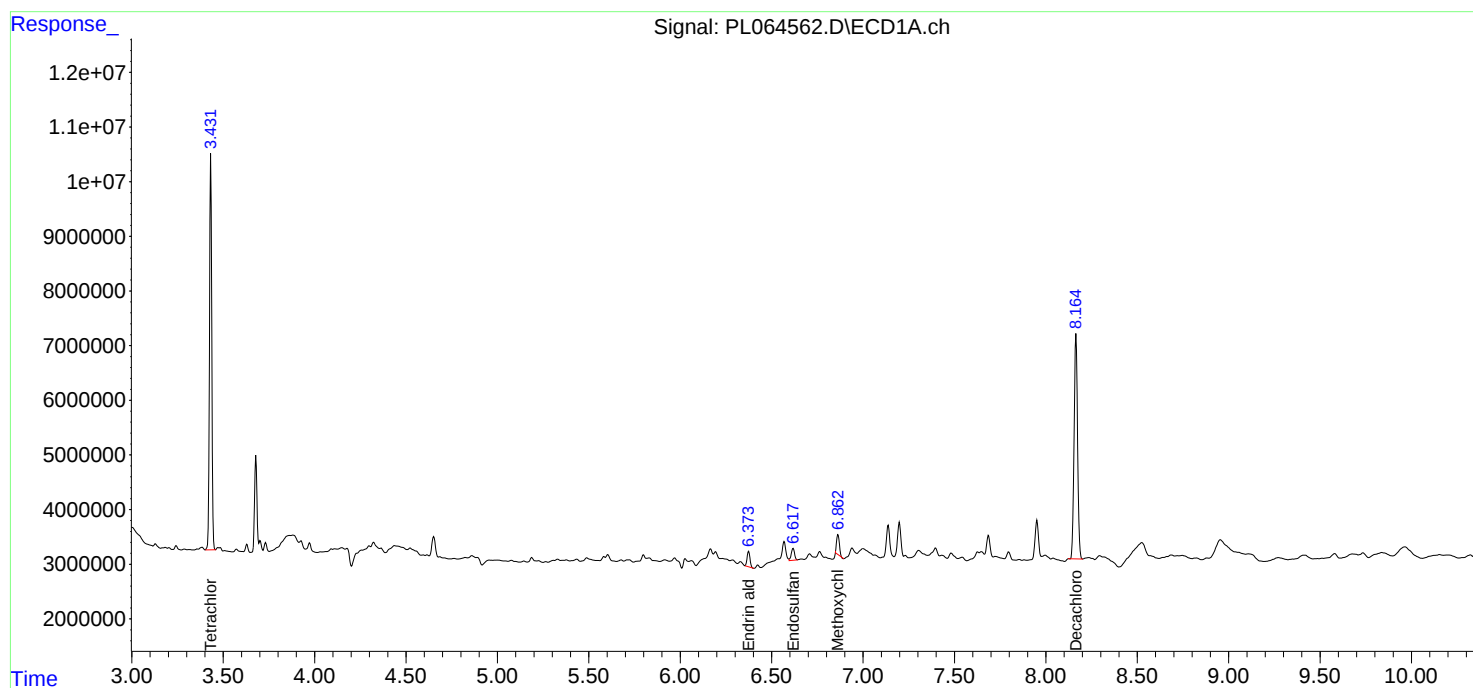


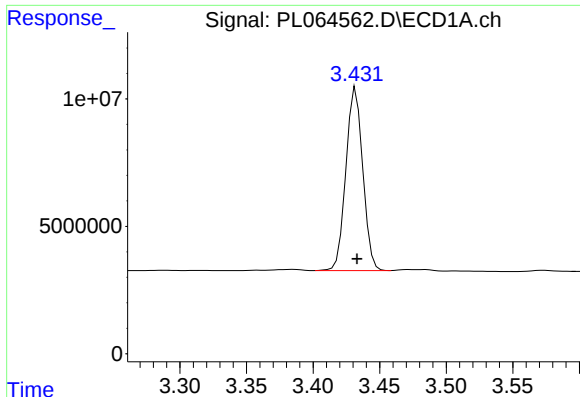

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 63413893
Conc: 20.83 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

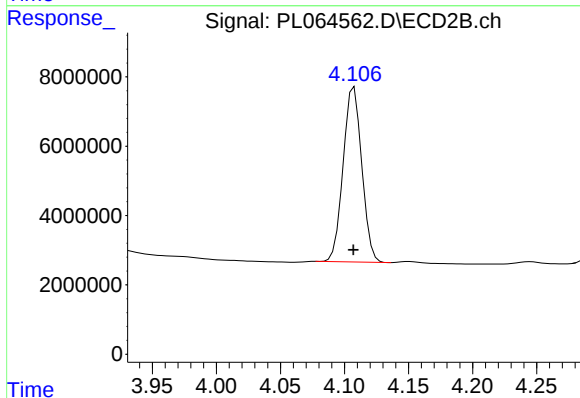


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 51048714
Conc: 21.43 ng/ml

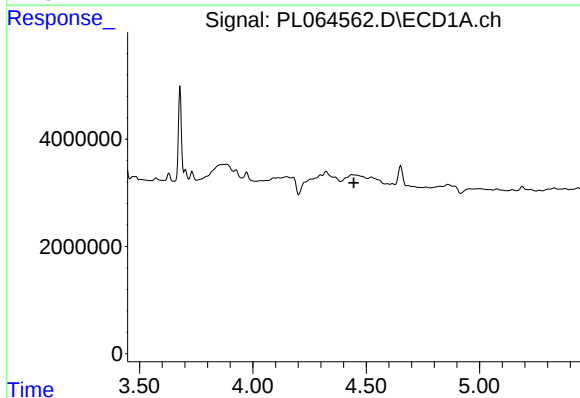


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

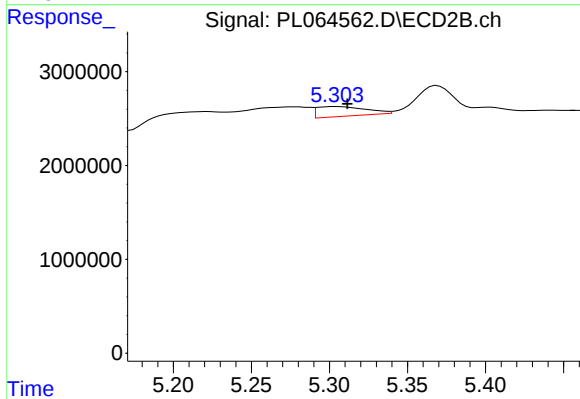

#4 Heptachlor


R.T.: 5.305 min
Delta R.T.: -0.007 min
Response: 2271170
Conc: 0.65 ng/ml

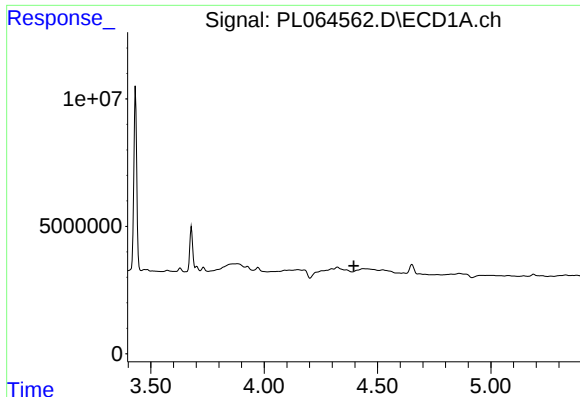

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

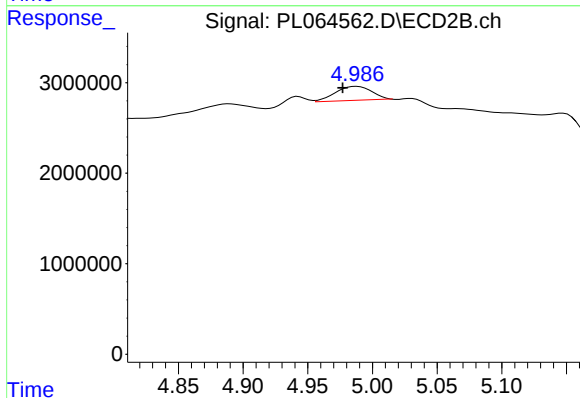


#6 beta-BHC

R.T.: 4.988 min
Delta R.T.: 0.011 min
Response: 3023189
Conc: 1.79 ng/ml

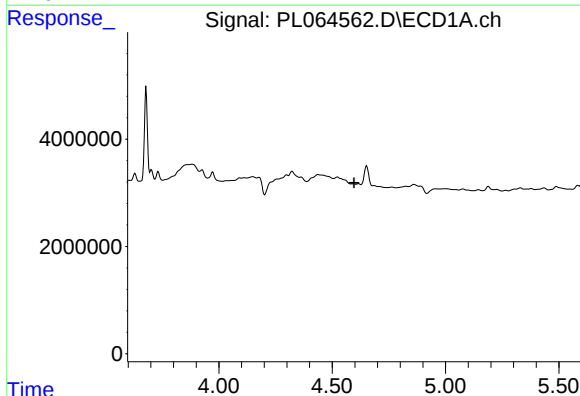


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

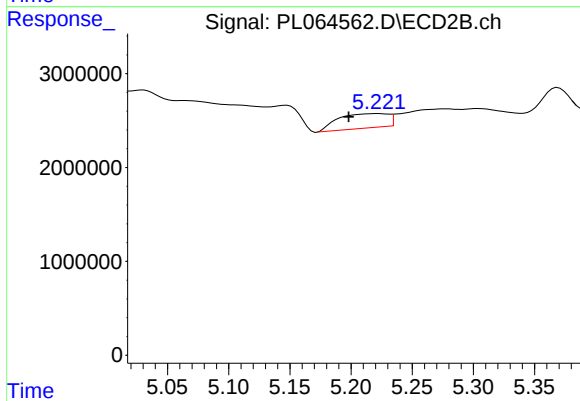

#7 delta-BHC


R.T.: 5.222 min
Delta R.T.: 0.024 min
Response: 4379387
Conc: 1.42 ng/ml

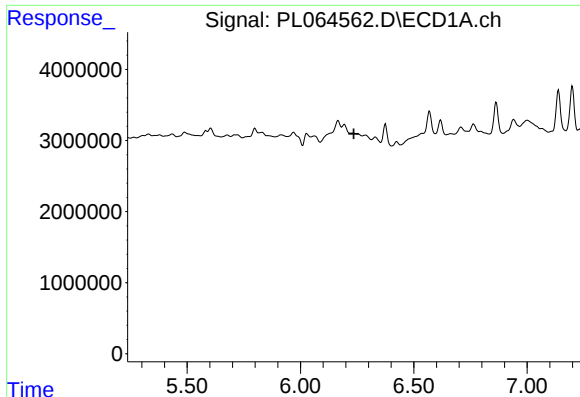

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

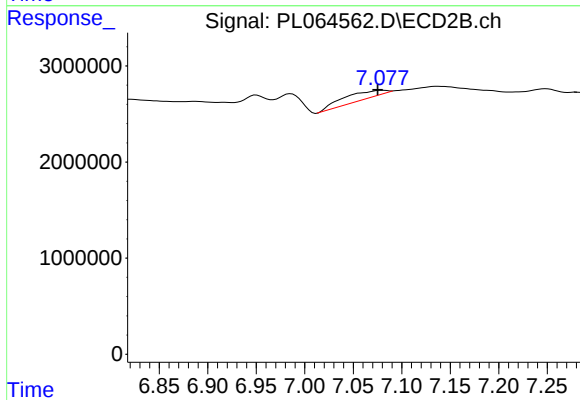


#15 Endosulfan II

R.T.: 7.080 min
Delta R.T.: 0.004 min
Response: 2342436
Conc: 0.95 ng/ml

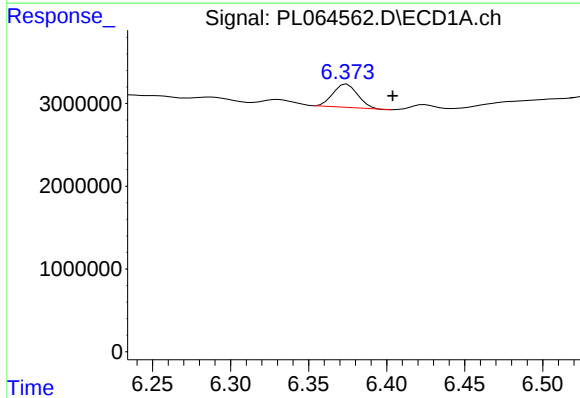


#18 Endrin aldehyde

R.T.: 6.375 min
Delta R.T.: -0.029 min
Response: 3119400
Conc: 1.02 ng/ml

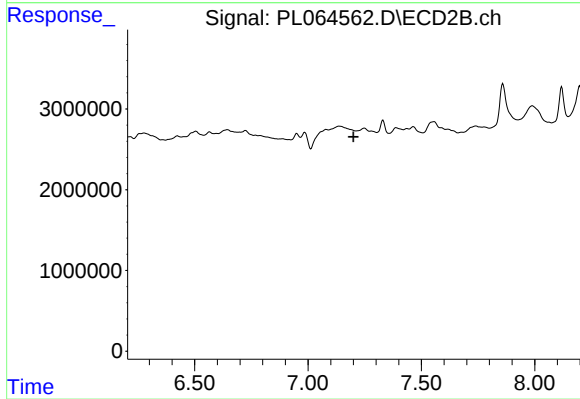

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.201 min
Response: 0
Conc: N.D.

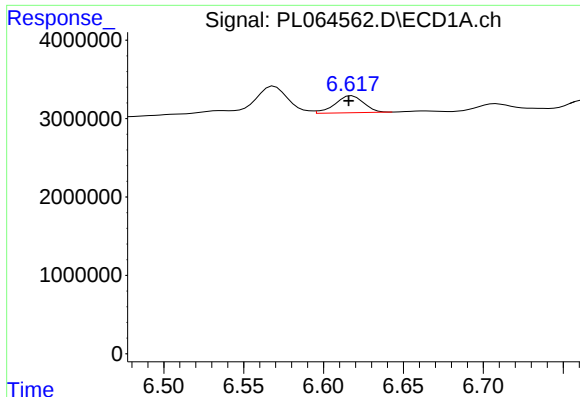

#19 Endosulfan Sulfate


R.T.: 6.618 min
Delta R.T.: 0.002 min
Response: 2723069
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

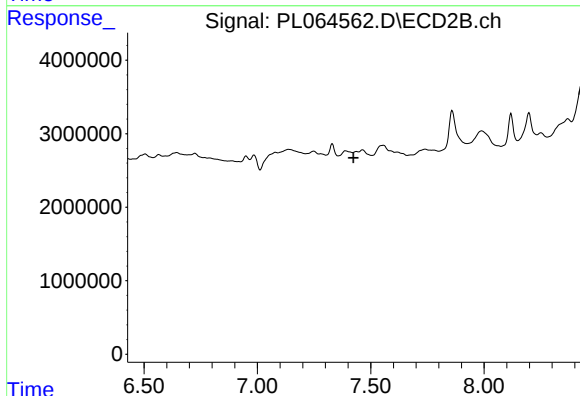


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

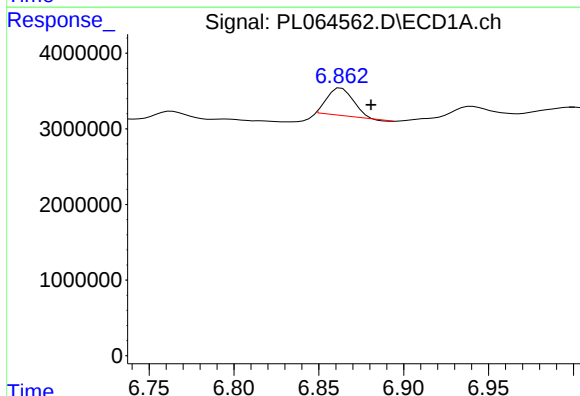


#20 Methoxychlor

R.T.: 6.863 min
Delta R.T.: -0.017 min
Response: 3845020
Conc: 2.13 ng/ml

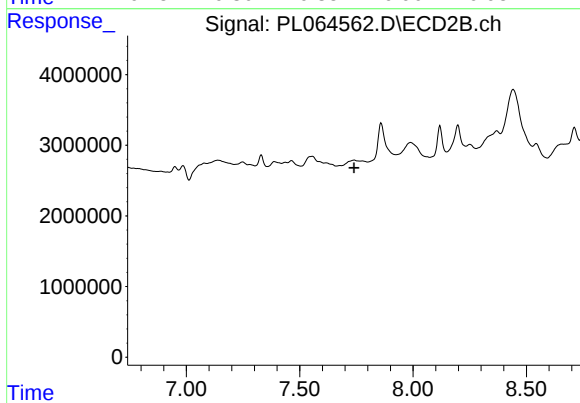

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

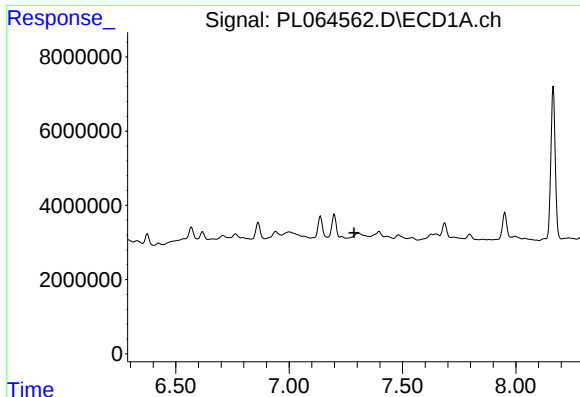

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-003-0205

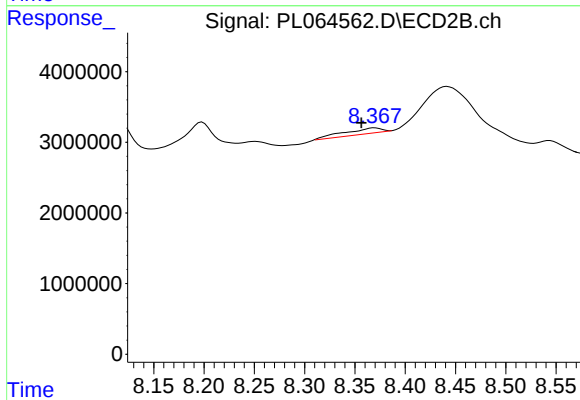


#22 Mirex

R.T.: 8.370 min
Delta R.T.: 0.013 min
Response: 2022770
Conc: 1.05 ng/ml

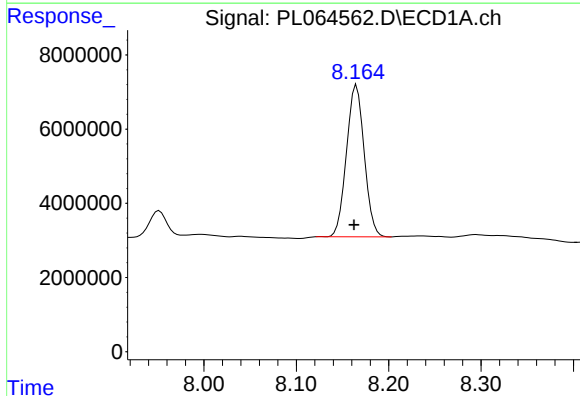

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.003 min
Response: 54634982
Conc: 17.34 ng/ml

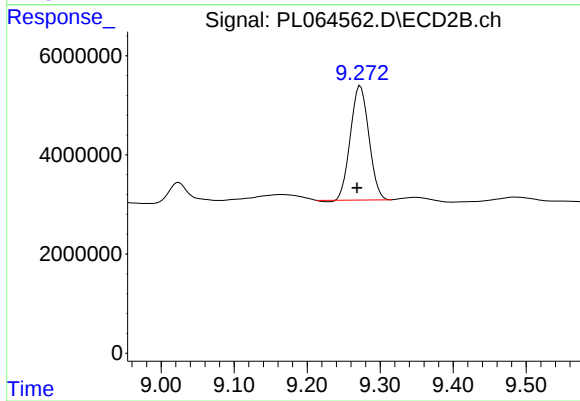

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 40375477
Conc: 19.72 ng/ml