

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064568.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 15:39
 Operator : AR\AJ
 Sample : M1292-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-009-0205

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:34:47 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.108	62590963	52511401	20.561	22.045
28)	SA Decachlor...	8.165	9.272	56817316	39403266	18.029	19.246
Target Compounds							
4)	MA Heptachlor	0.000	5.306	0	24686598	N.D.	7.083 #
6)	B beta-BHC	0.000	4.987	0	5911411	N.D.	3.493 #
9)	A Endosulfan I	0.000	6.361f	0	705881	N.D.	0.265 #
10)	B gamma-Chl...	0.000	6.259	0	5361145	N.D.	1.844 #
15)	B Endosulfa...	0.000	7.051f	0	2527630	N.D.	1.024 #
25)	Chlordane-3	0.000	6.259	0	5361145	N.D.	14.955 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064568.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 15:39
Operator : AR\AJ
Sample : M1292-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
OU421-009-0205

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:34:47 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

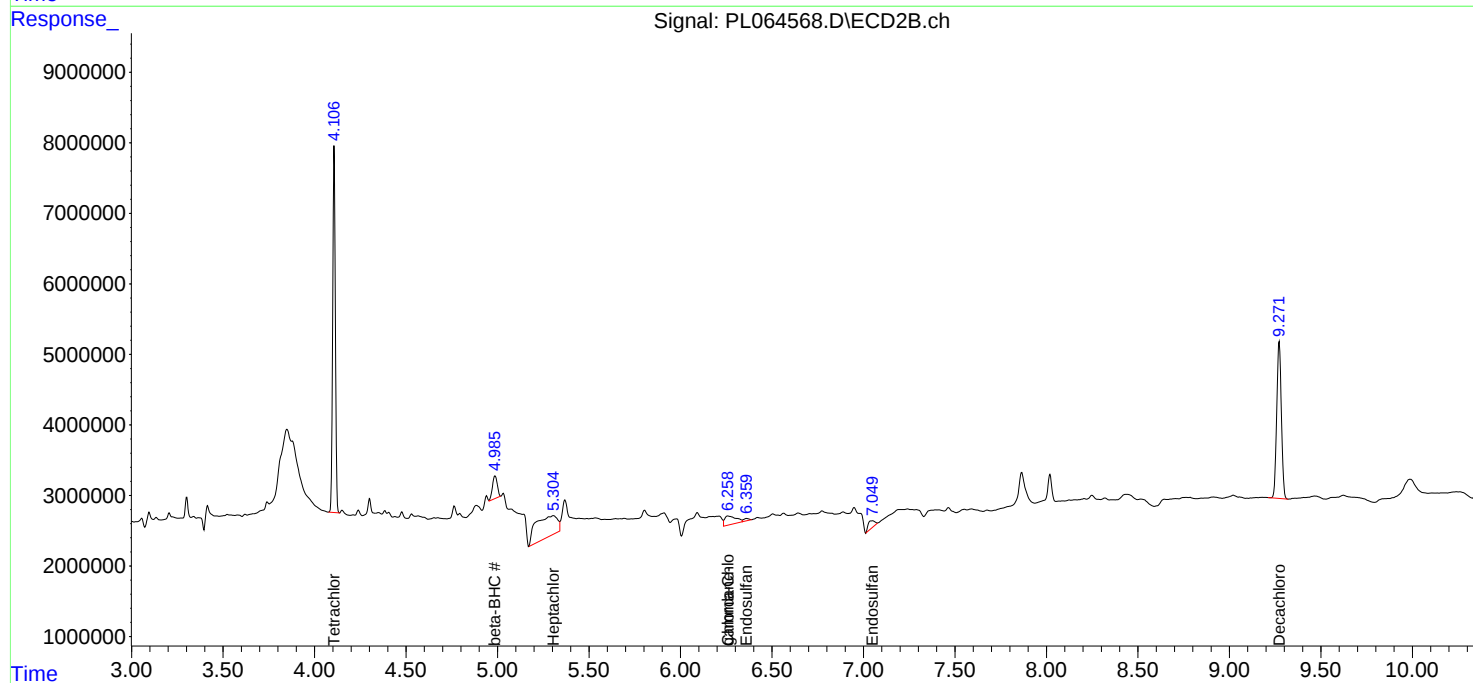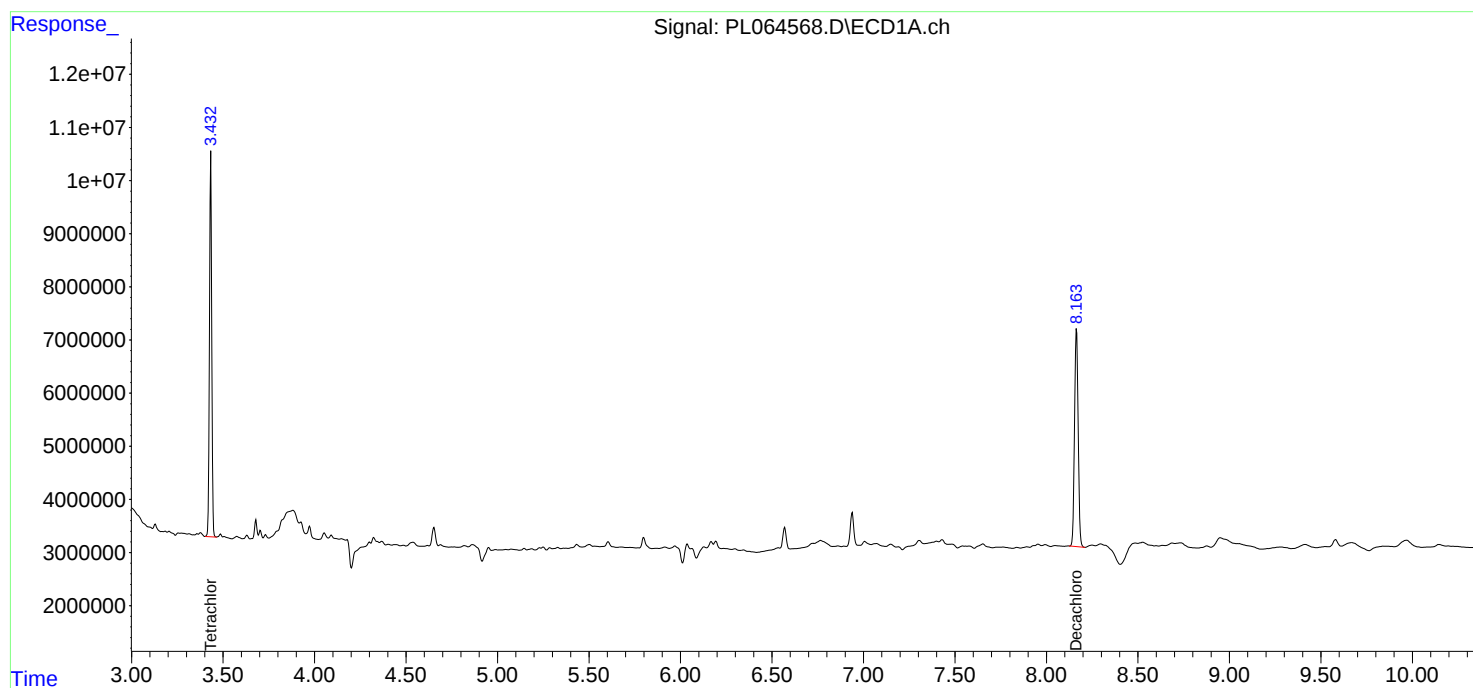


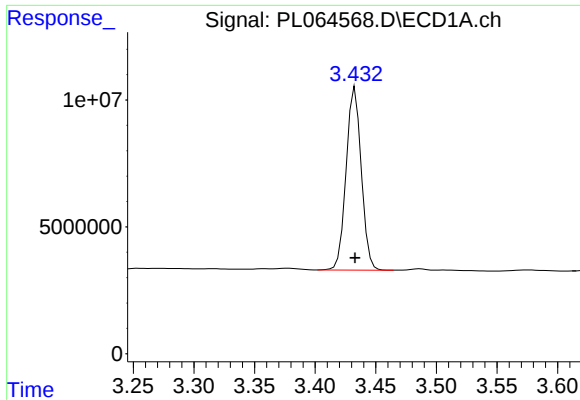

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 62590963
Conc: 20.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-009-0205

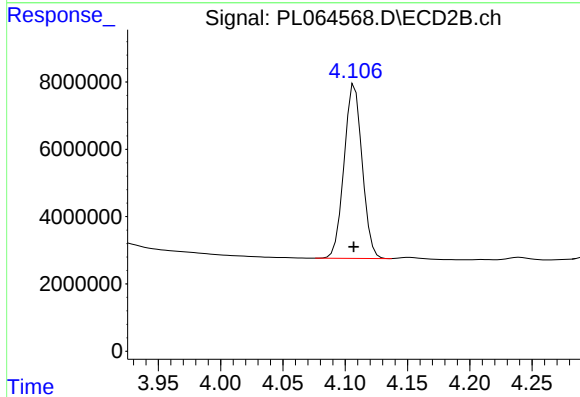


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 52511401
Conc: 22.04 ng/ml

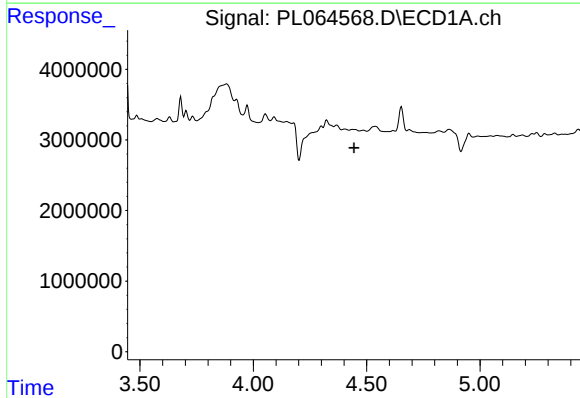


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

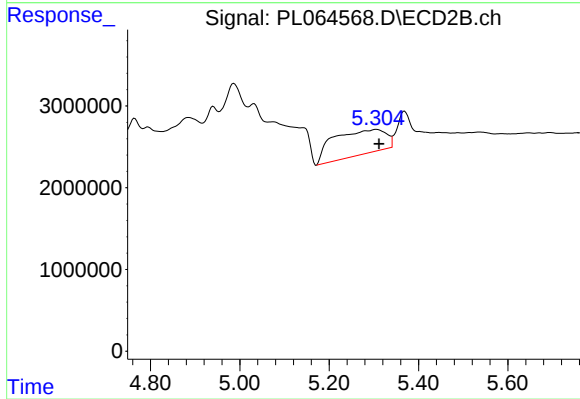

#4 Heptachlor


R.T.: 5.306 min
Delta R.T.: -0.006 min
Response: 24686598
Conc: 7.08 ng/ml

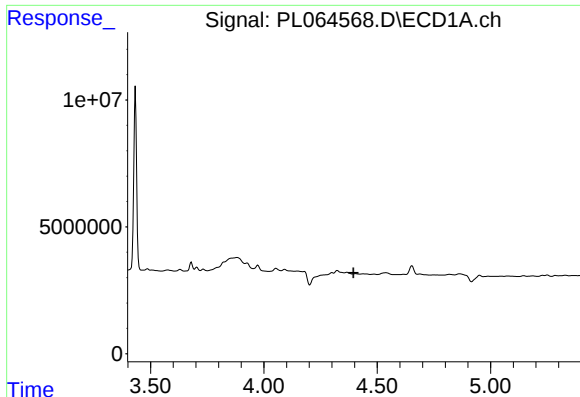

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-009-0205

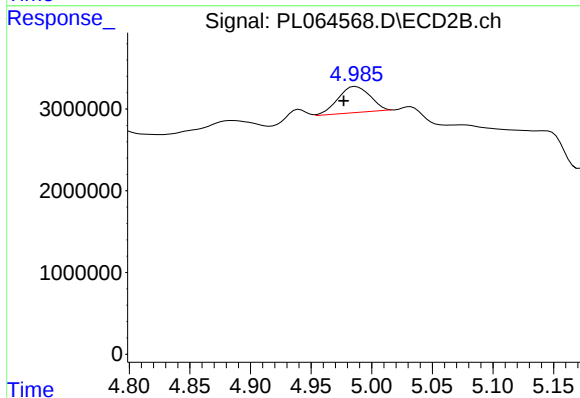


#6 beta-BHC

R.T.: 4.987 min
Delta R.T.: 0.010 min
Response: 5911411
Conc: 3.49 ng/ml

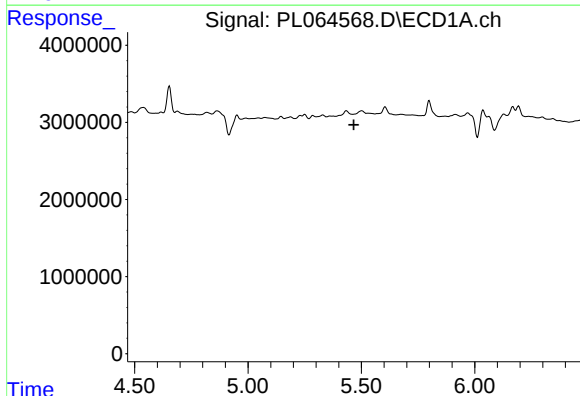


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.467 min
Response: 0
Conc: N.D.

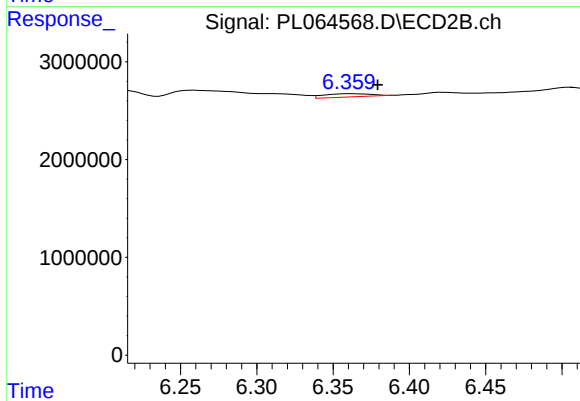

#9 Endosulfan I


R.T.: 6.361 min
Delta R.T.: -0.018 min
Response: 705881
Conc: 0.27 ng/ml

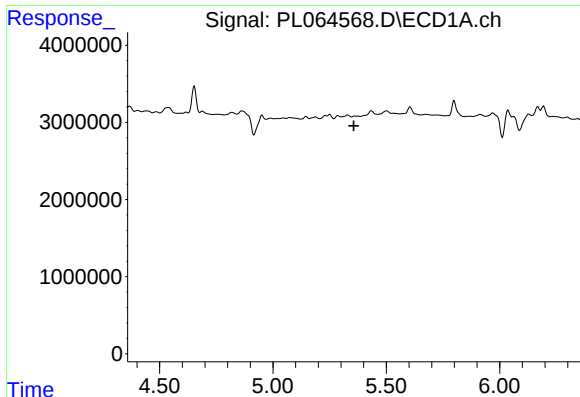

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-009-0205

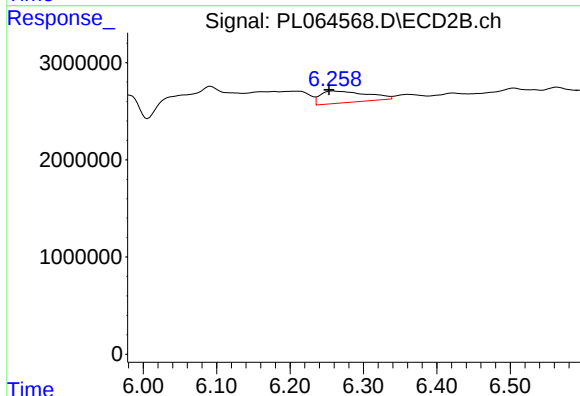


#10 gamma-Chlordane

R.T.: 6.259 min
Delta R.T.: 0.006 min
Response: 5361145
Conc: 1.84 ng/ml

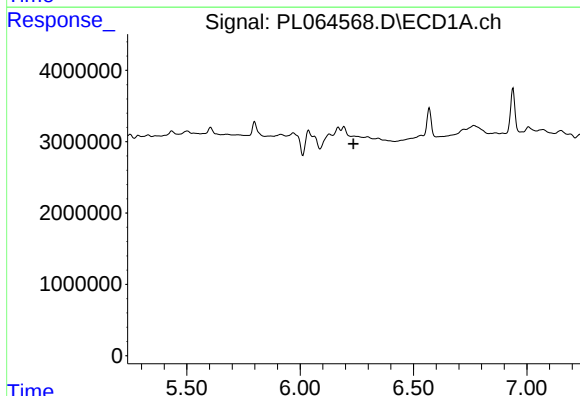


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

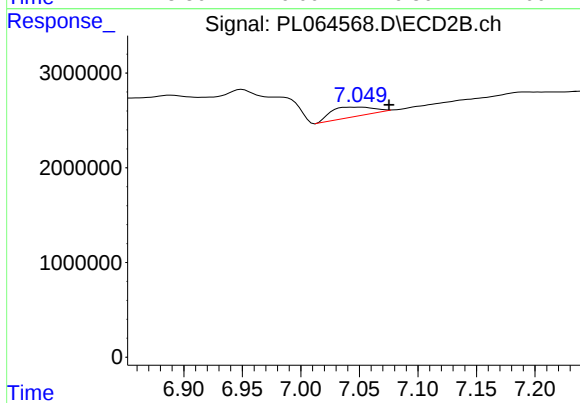

#15 Endosulfan II


R.T.: 7.051 min
Delta R.T.: -0.024 min
Response: 2527630
Conc: 1.02 ng/ml

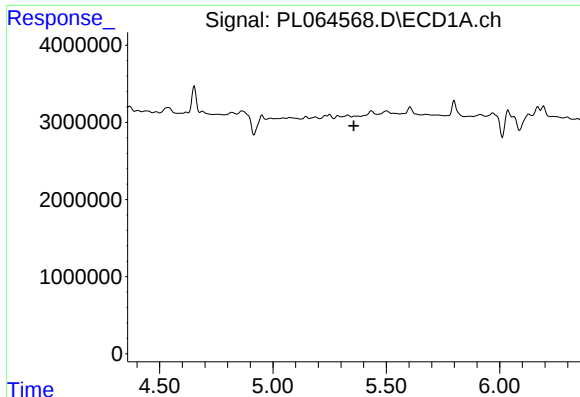

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-009-0205

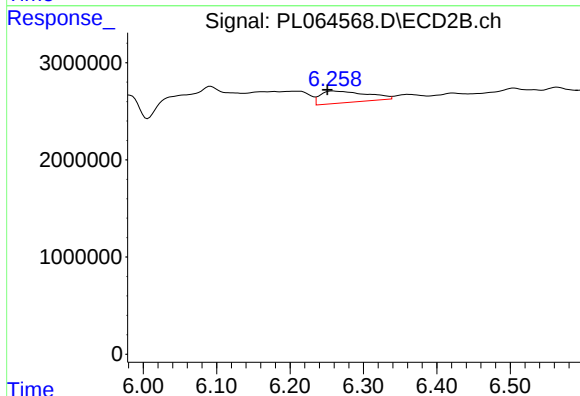


#25 Chlordane-3

R.T.: 6.259 min
Delta R.T.: 0.008 min
Response: 5361145
Conc: 14.95 ng/ml

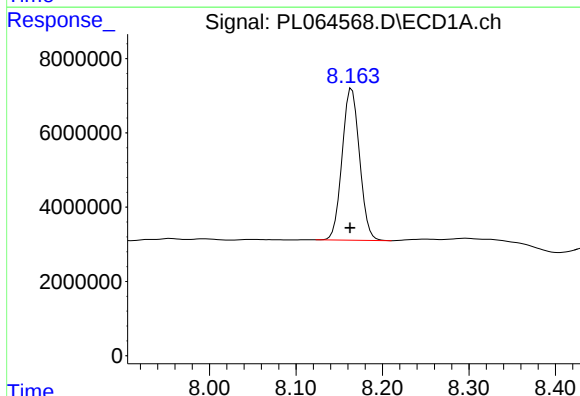

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 56817316
Conc: 18.03 ng/ml

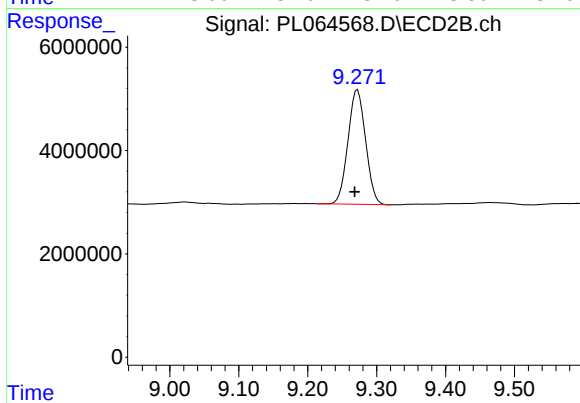

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.004 min
Response: 39403266
Conc: 19.25 ng/ml