

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064576.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 17:33
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:36:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.108	59420919	49307282	19.520	20.700
28)	SA Decachlor...	8.165	9.273	61252071	42973028	19.437	20.989
Target Compounds							
6)	B beta-BHC	0.000	4.985	0	4758824	N.D.	2.812 #
7)	B delta-BHC	0.000	5.222f	0	5062991	N.D.	1.644 #
16)	A 4,4'-DDD	0.000	6.950f	0	1872402	N.D.	0.813 #
23)	Chlordane-1	4.320f	0.000	2358705	0	21.458	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064576.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 17:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:36:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

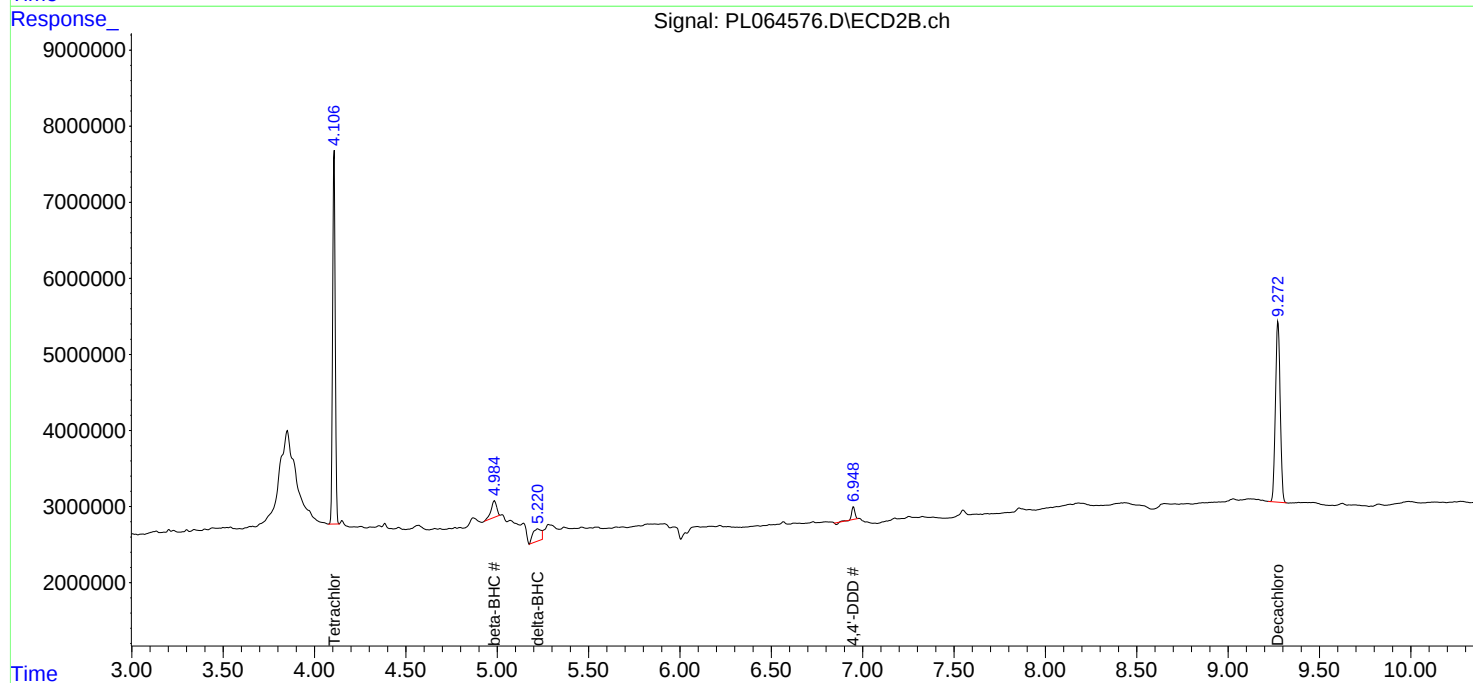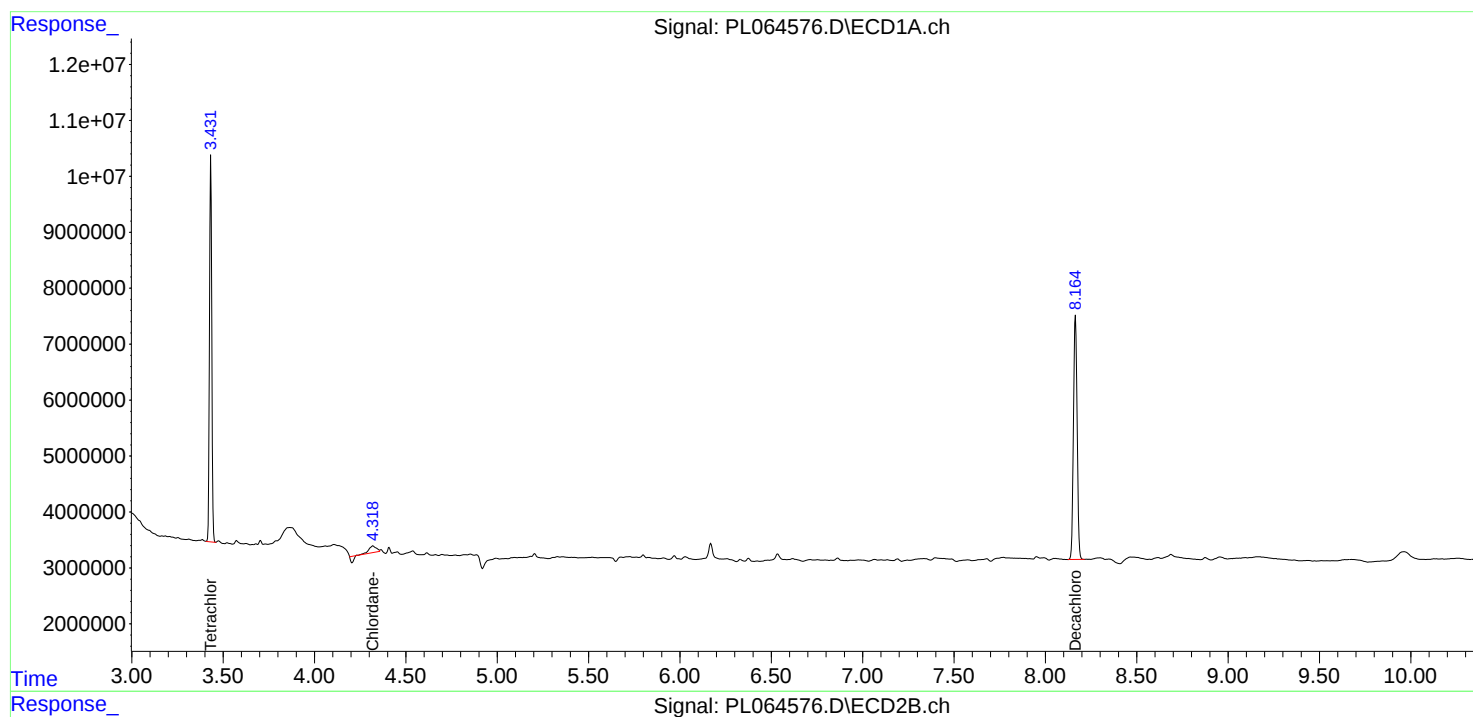


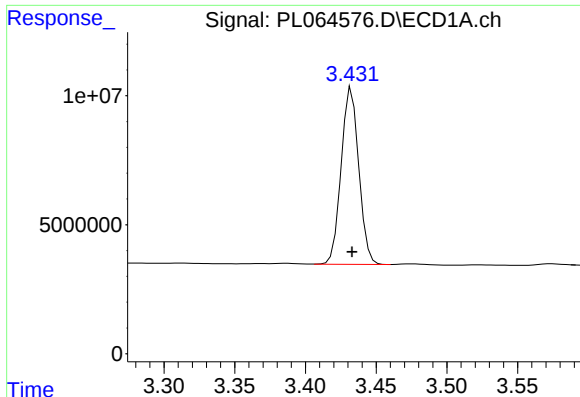

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 59420919
Conc: 19.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

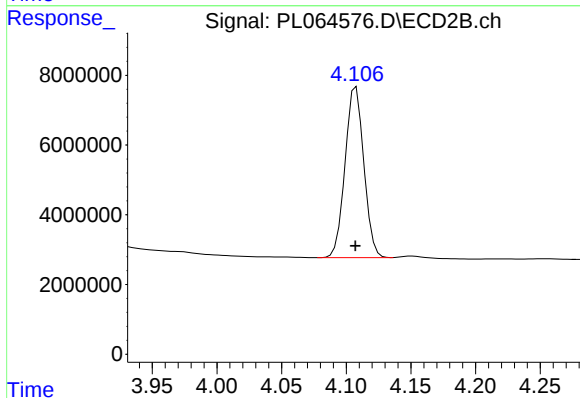


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 49307282
Conc: 20.70 ng/ml

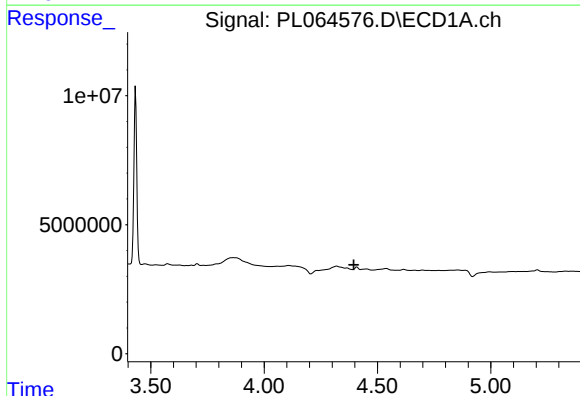


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.395 min
Response: 0
Conc: N.D.

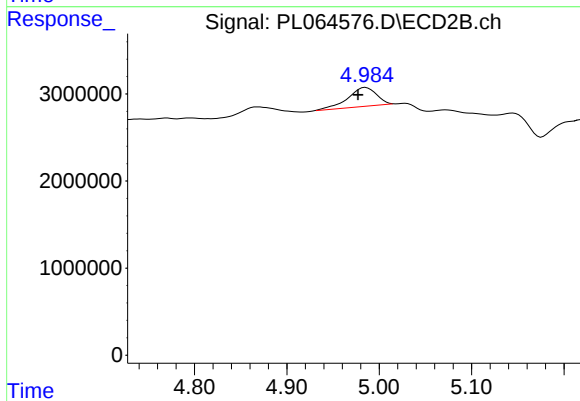

#6 beta-BHC


R.T.: 4.985 min
Delta R.T.: 0.008 min
Response: 4758824
Conc: 2.81 ng/ml

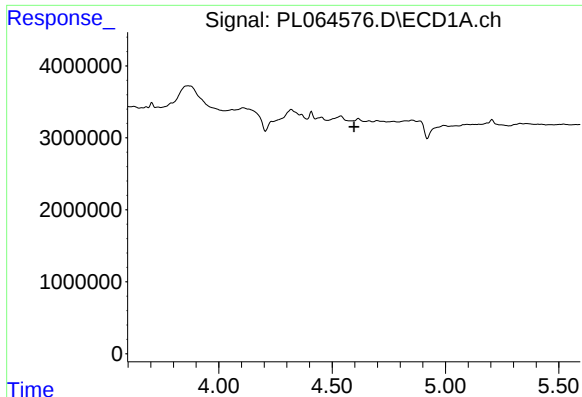

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

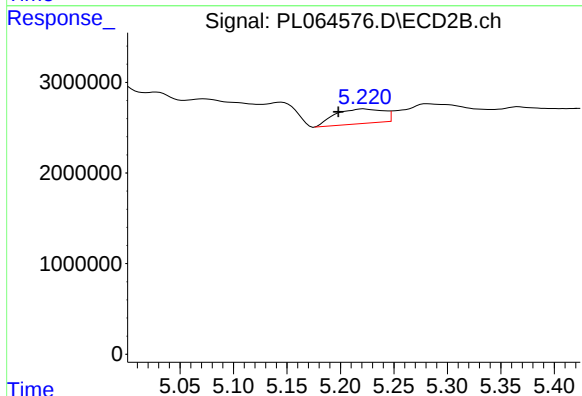


#7 delta-BHC

R.T.: 5.222 min
Delta R.T.: 0.024 min
Response: 5062991
Conc: 1.64 ng/ml

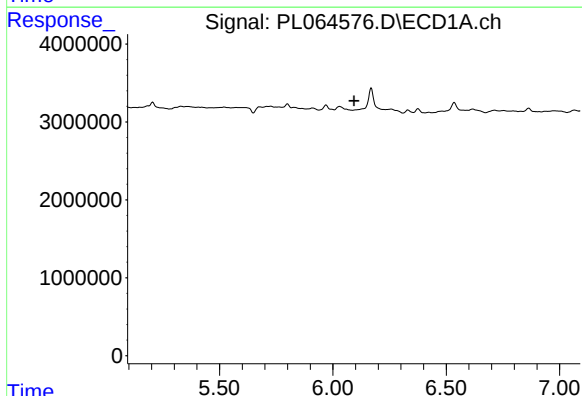


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

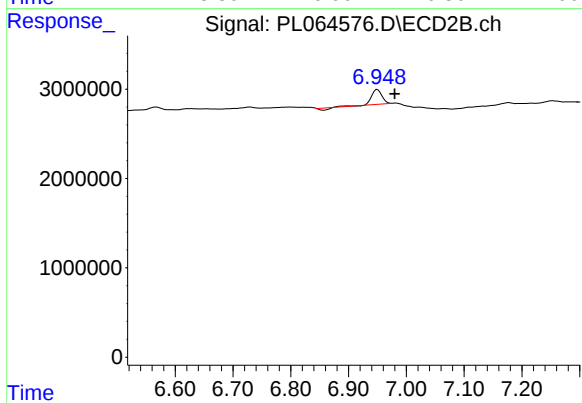

#16 4,4'-DDD


R.T.: 6.950 min
Delta R.T.: -0.030 min
Response: 1872402
Conc: 0.81 ng/ml

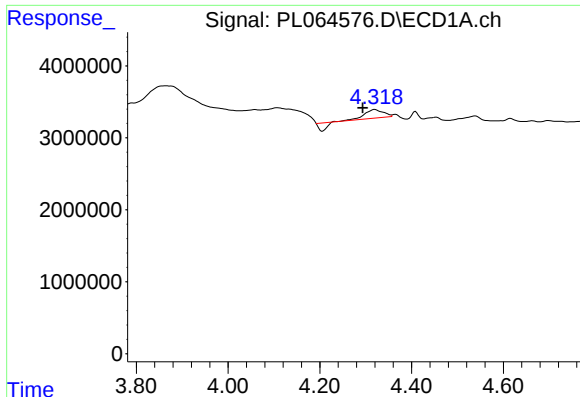

#23 Chlordane-1


R.T.: 4.320 min
Delta R.T.: 0.027 min
Response: 2358705
Conc: 21.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

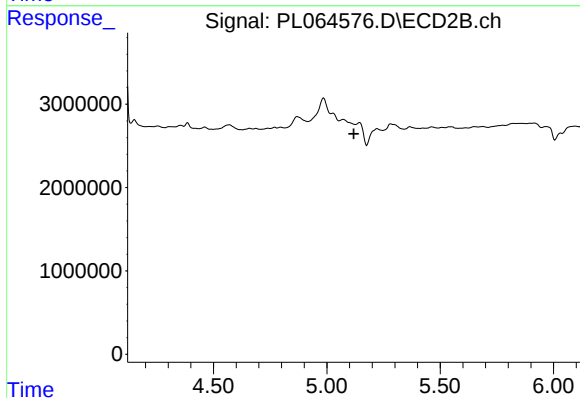


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

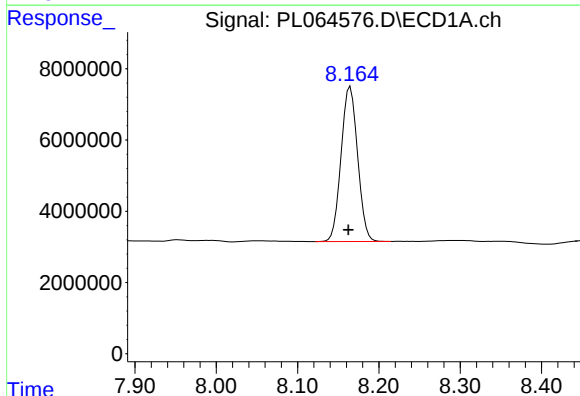

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 61252071
Conc: 19.44 ng/ml

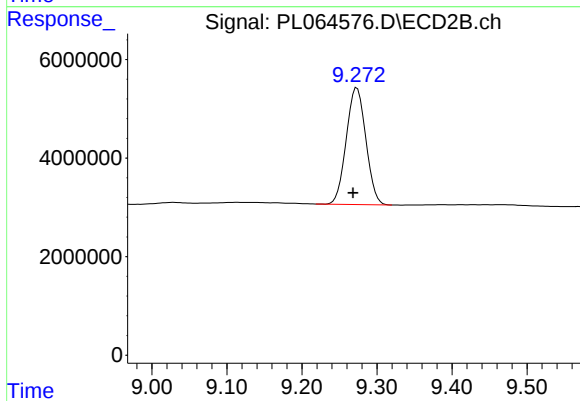

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.005 min
Response: 42973028
Conc: 20.99 ng/ml