

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064585.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 19:42
 Operator : AR\AJ
 Sample : M1291-07
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-006-0510

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:37:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.108	37959888	31393420	12.470	13.179
28)	SA Decachlor...	8.164	9.274	44619323	29853192	14.159	14.581
Target Compounds							
4)	MA Heptachlor	0.000	5.301	0	11019800	N.D.	3.162 #
6)	B beta-BHC	0.000	4.986	0	3977491	N.D.	2.350 #
13)	MA Dieldrin	5.706	0.000	1888635	0	0.472	N.D. #
15)	B Endosulfa...	0.000	7.054f	0	1587174	N.D.	0.643 #
16)	A 4,4'-DDD	0.000	6.950f	0	5232651	N.D.	2.273 #
17)	MA 4,4'-DDT	6.331	7.255f	2019065	1007369	0.658	0.490 #
18)	B Endrin al...	6.375f	0.000	5650984	0	1.842	N.D. #
19)	B Endosulfa...	6.618	0.000	4164365	0	1.146	N.D. #
20)	A Methoxychlor	6.862f	0.000	4134007	0	2.289	N.D. #
22)	Mirex	0.000	8.372f	0	1915973	N.D.	0.998 #
23)	Chlordane-1	4.311f	0.000	424522	0	3.862	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064585.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 19:42
Operator : AR\AJ
Sample : M1291-07
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
OU421-006-0510

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:37:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

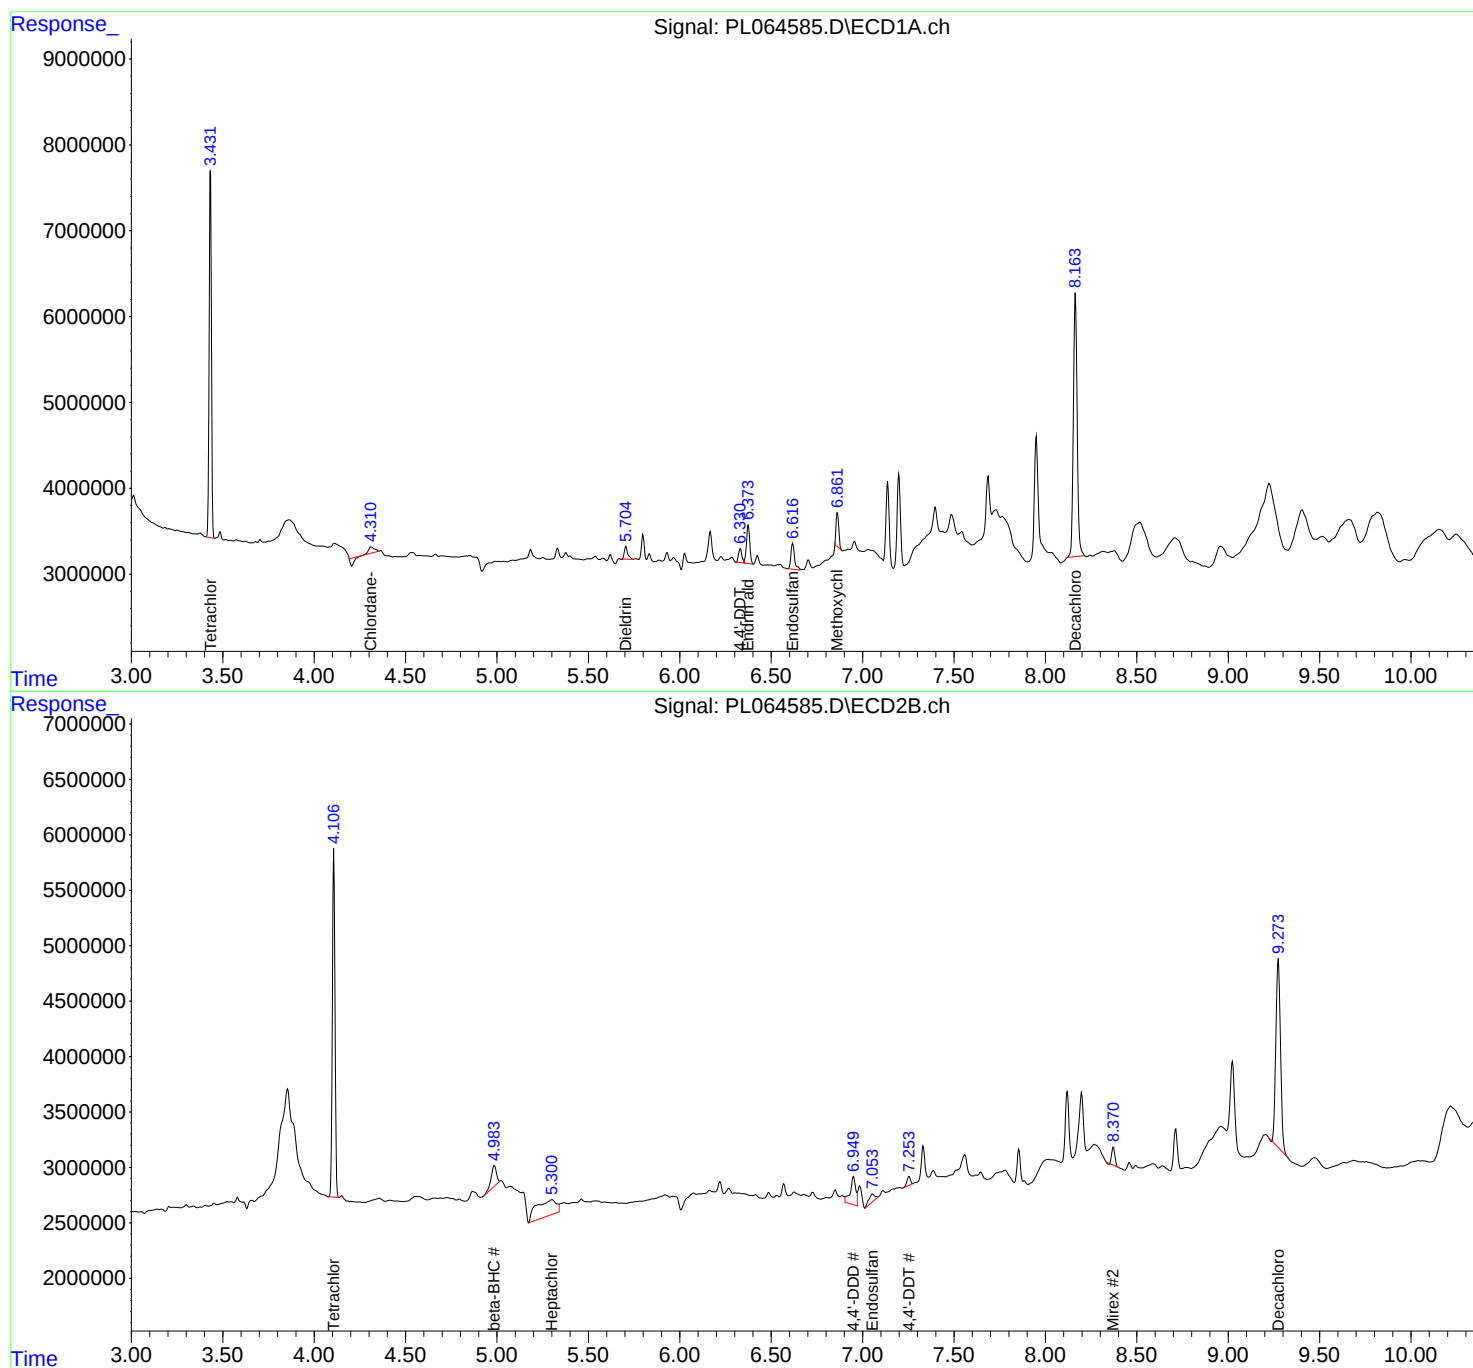


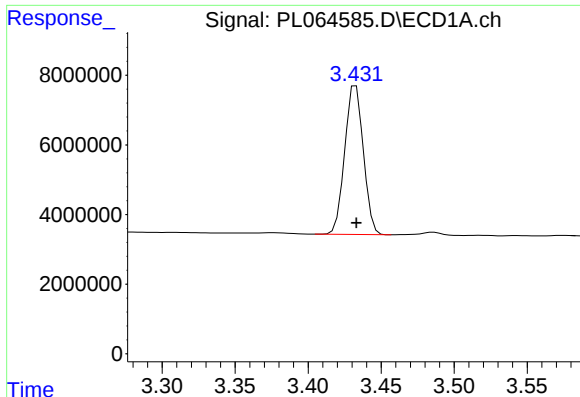

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 37959888
Conc: 12.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

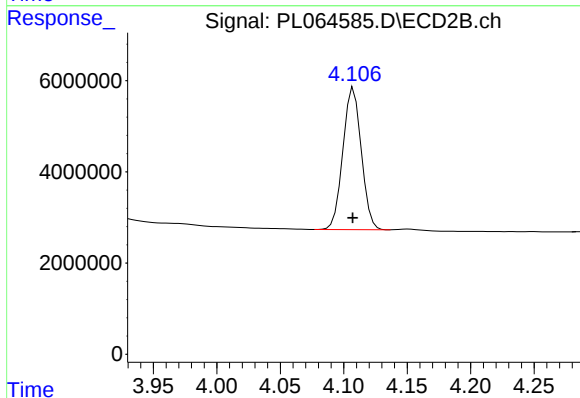


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 31393420
Conc: 13.18 ng/ml

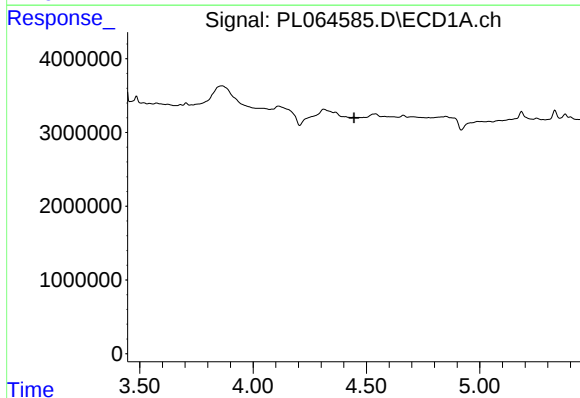


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

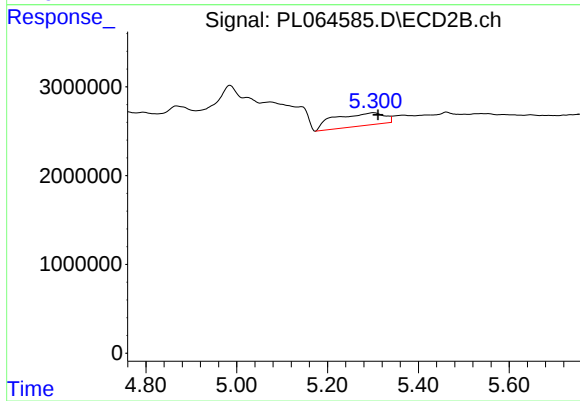

#4 Heptachlor


R.T.: 5.301 min
Delta R.T.: -0.010 min
Response: 11019800
Conc: 3.16 ng/ml

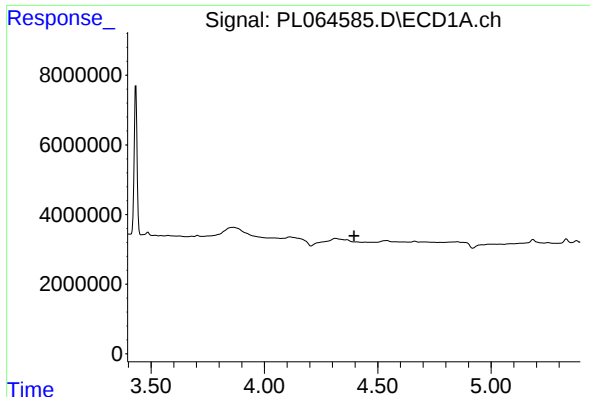

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

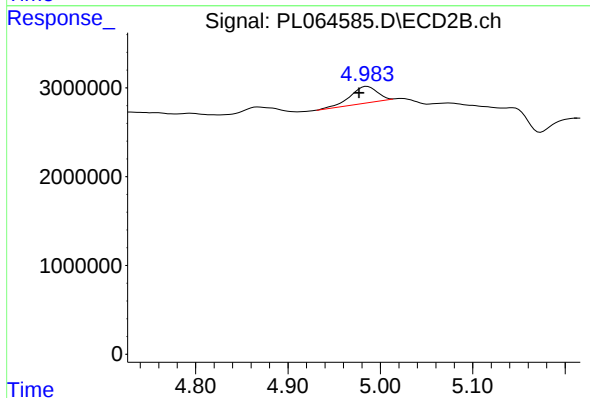


#6 beta-BHC

R.T.: 4.986 min
Delta R.T.: 0.008 min
Response: 3977491
Conc: 2.35 ng/ml

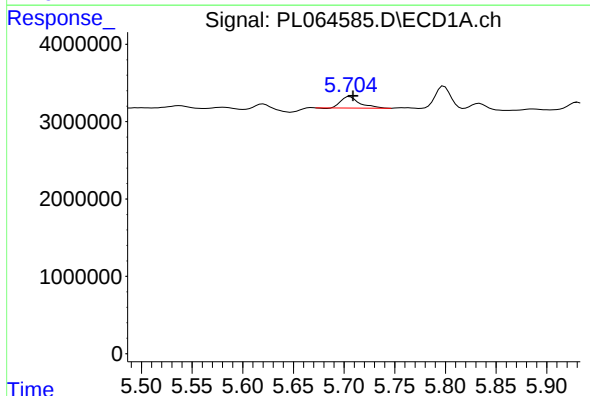


#13 Dieldrin

R.T.: 5.706 min
Delta R.T.: -0.003 min
Response: 1888635
Conc: 0.47 ng/ml

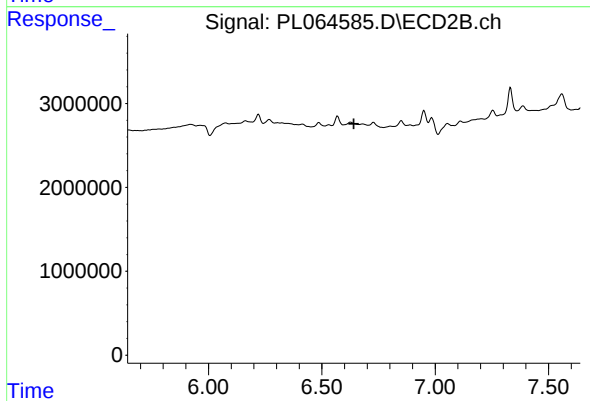

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.640 min
Response: 0
Conc: N.D.

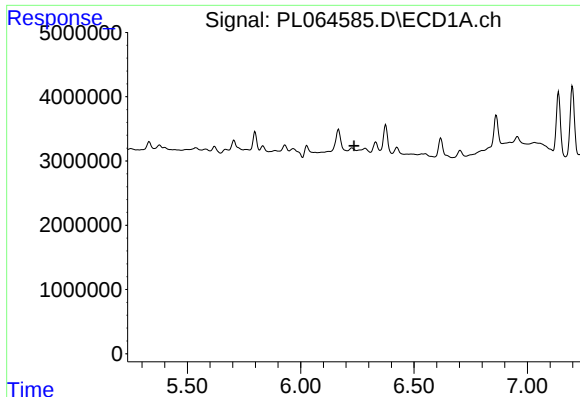

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.236 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

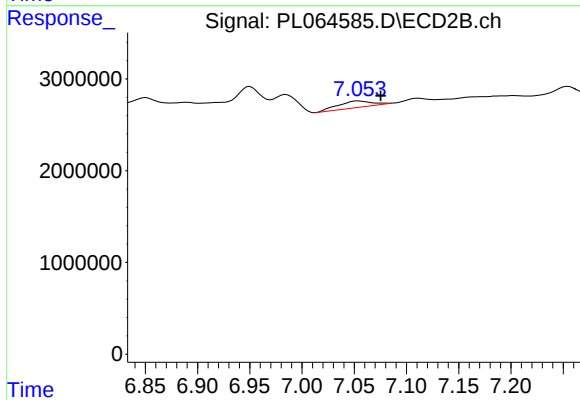


#15 Endosulfan II

R.T.: 7.054 min
Delta R.T.: -0.021 min
Response: 1587174
Conc: 0.64 ng/ml

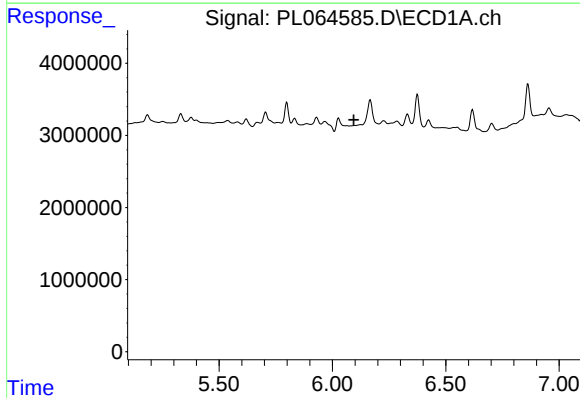


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

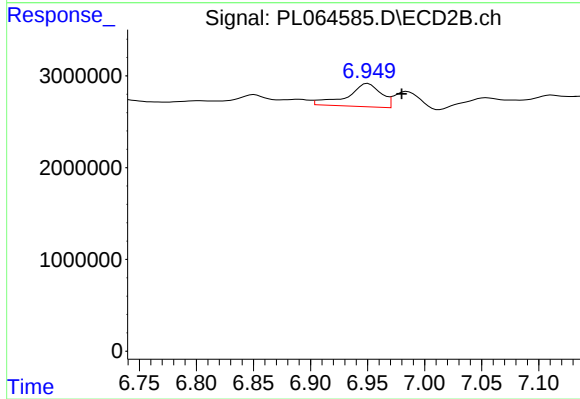

#16 4,4'-DDD


R.T.: 6.950 min
Delta R.T.: -0.030 min
Response: 5232651
Conc: 2.27 ng/ml

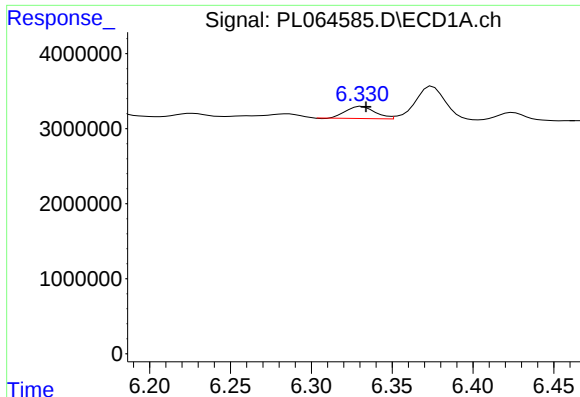

#17 4,4'-DDT


R.T.: 6.331 min
Delta R.T.: -0.003 min
Response: 2019065
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

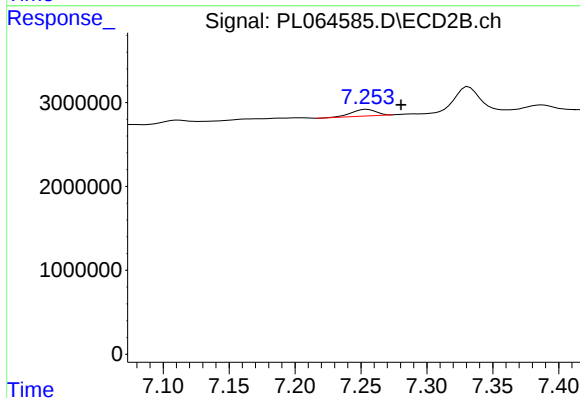


#17 4,4'-DDT

R.T.: 7.255 min
Delta R.T.: -0.026 min
Response: 1007369
Conc: 0.49 ng/ml

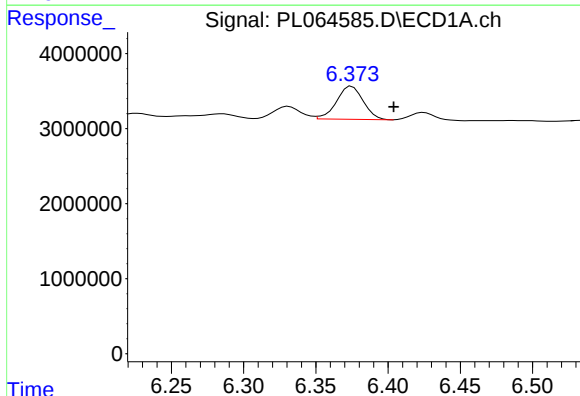


#18 Endrin aldehyde

R.T.: 6.375 min
Delta R.T.: -0.029 min
Response: 5650984
Conc: 1.84 ng/ml

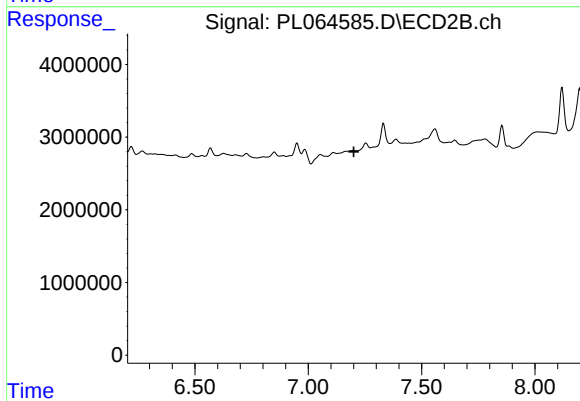

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.201 min
Response: 0
Conc: N.D.

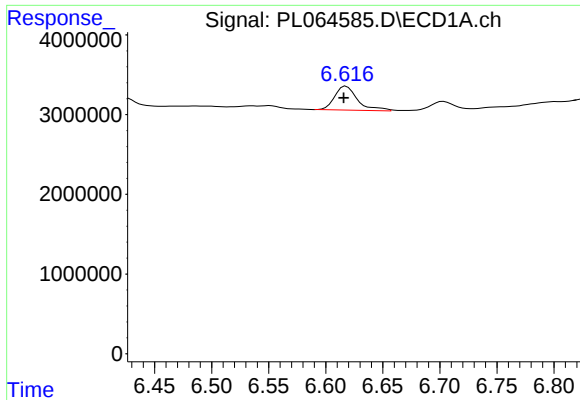

#19 Endosulfan Sulfate


R.T.: 6.618 min
Delta R.T.: 0.002 min
Response: 4164365
Conc: 1.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

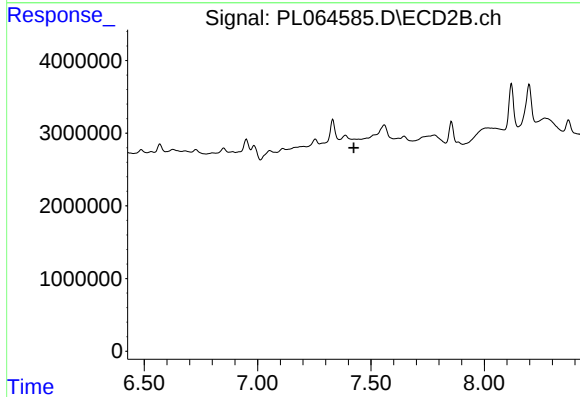


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.425 min
Response: 0
Conc: N.D.

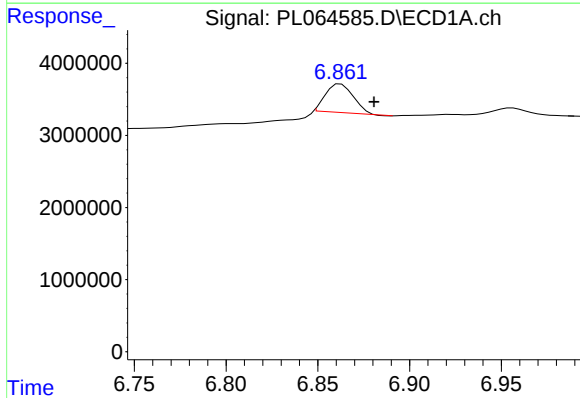


#20 Methoxychlor

R.T.: 6.862 min
Delta R.T.: -0.018 min
Response: 4134007
Conc: 2.29 ng/ml

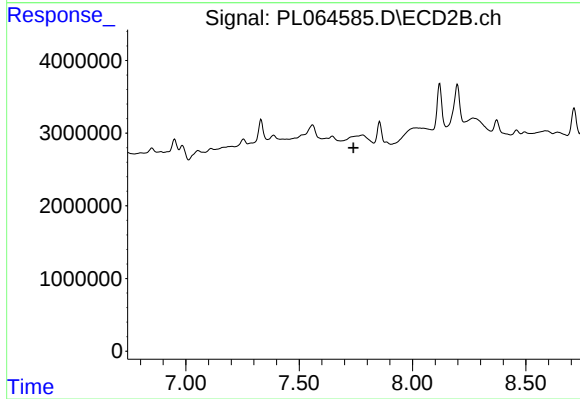

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.740 min
Response: 0
Conc: N.D.

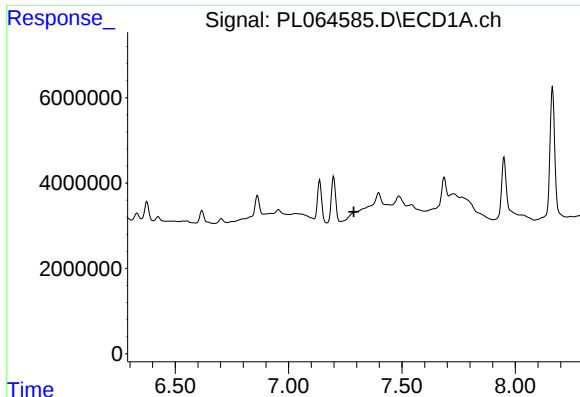

#22 Mirex


R.T.: 0.000 min
Exp R.T.: 7.287 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

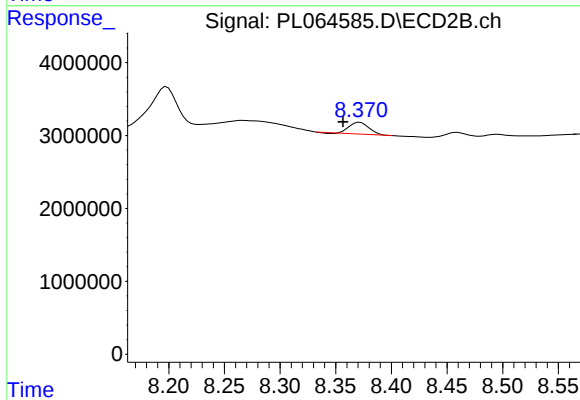


#22 Mirex

R.T.: 8.372 min
Delta R.T.: 0.015 min
Response: 1915973
Conc: 1.00 ng/ml

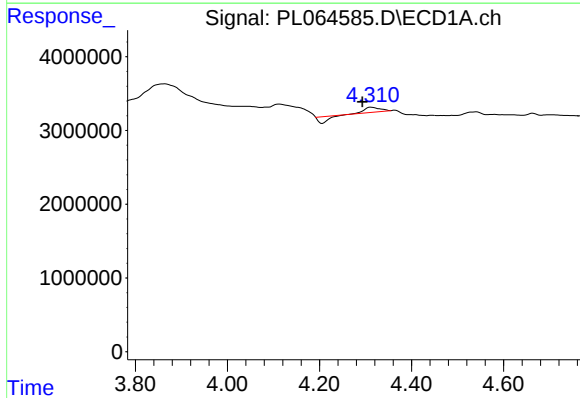


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.018 min
Response: 424522
Conc: 3.86 ng/ml

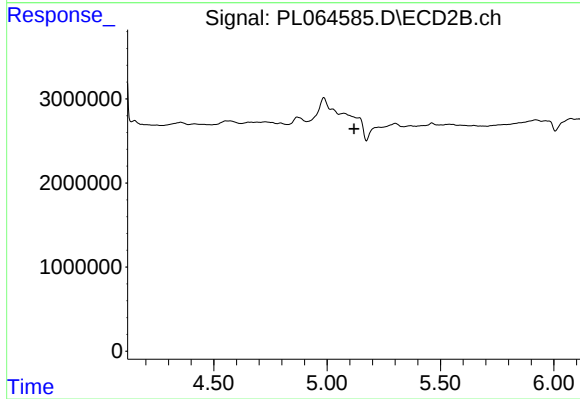

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

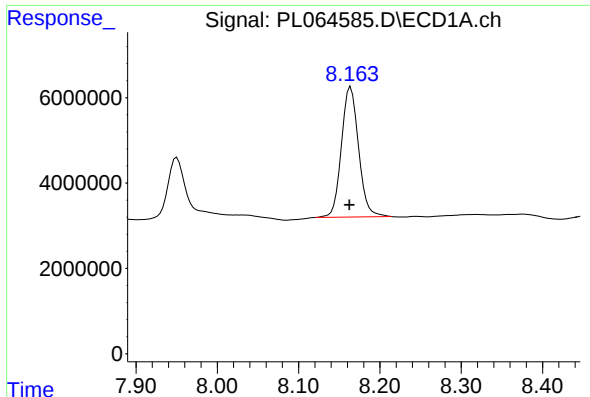

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 44619323
Conc: 14.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-006-0510

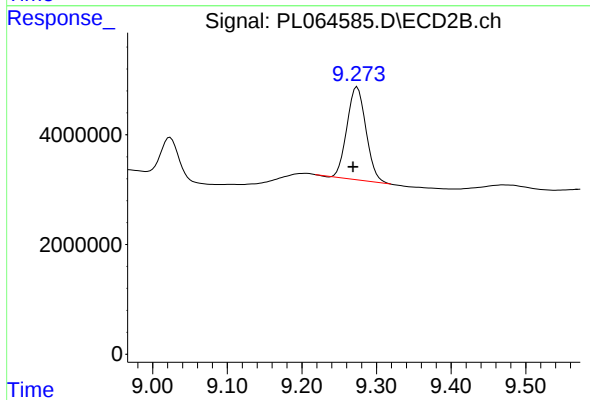

#28 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: 0.006 min
Response: 29853192
Conc: 14.58 ng/ml