

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064588.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 20:25
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:38:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.108	62132737	50903219	20.410	21.370
28)	SA Decachlor...	8.164	9.272	61372352	44394103	19.475	21.683
Target Compounds							
4)	MA Heptachlor	0.000	5.301	0	1130915	N.D.	0.324 #
6)	B beta-BHC	0.000	4.986	0	4475789	N.D.	2.645 #
7)	B delta-BHC	0.000	5.222f	0	3700861	N.D.	1.201 #
16)	A 4,4'-DDD	0.000	6.950f	0	1759710	N.D.	0.764 #
23)	Chlordane-1	4.321f	0.000	703989	0	6.404	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064588.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 20:25
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:38:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

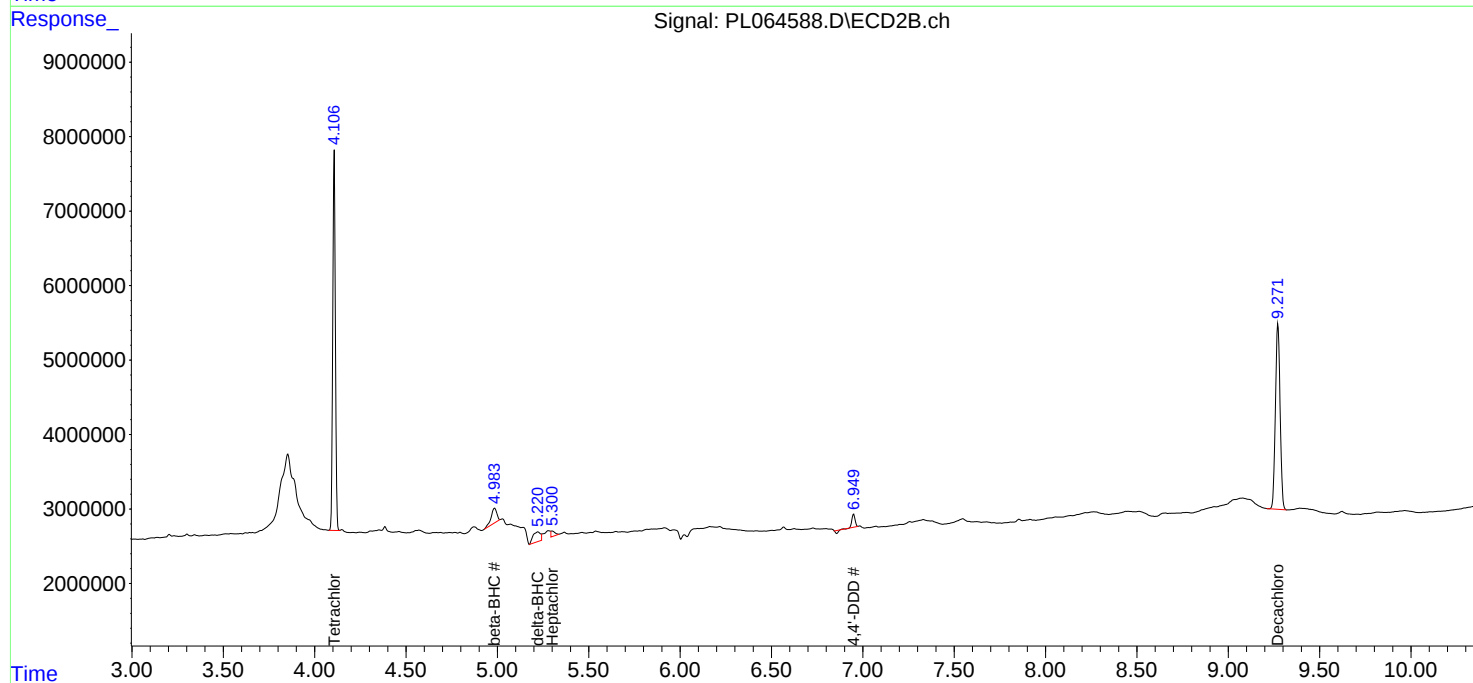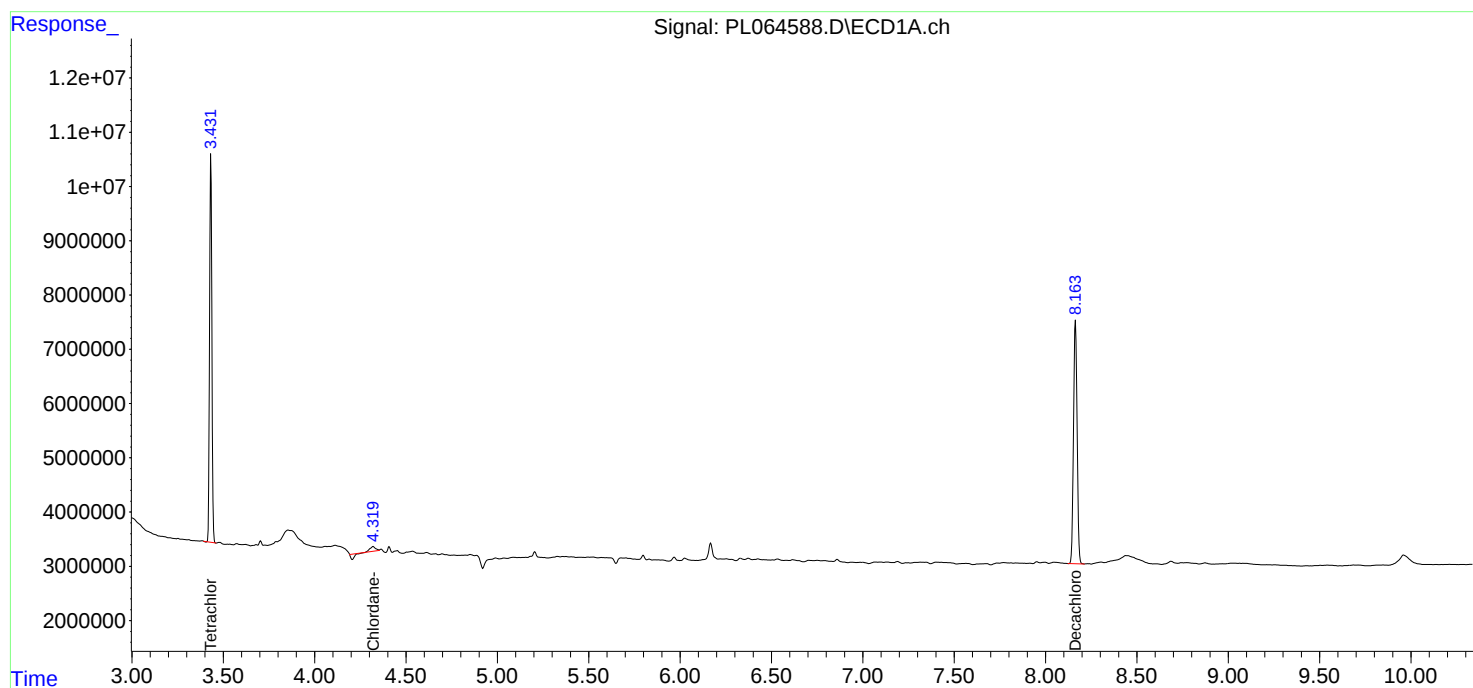


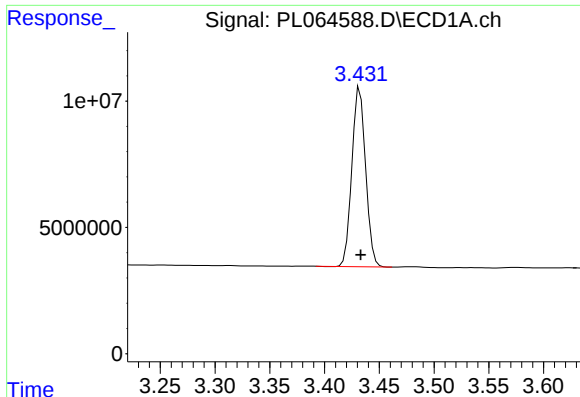

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 62132737
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

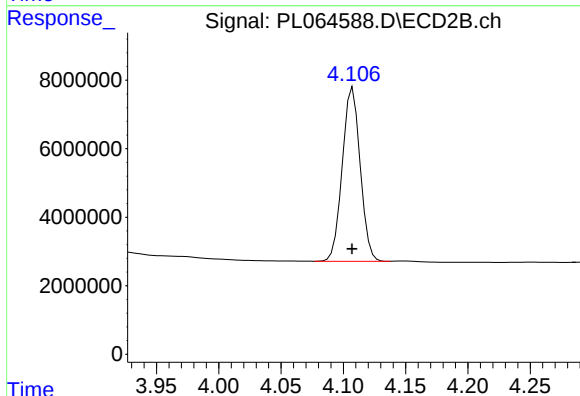


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 50903219
Conc: 21.37 ng/ml

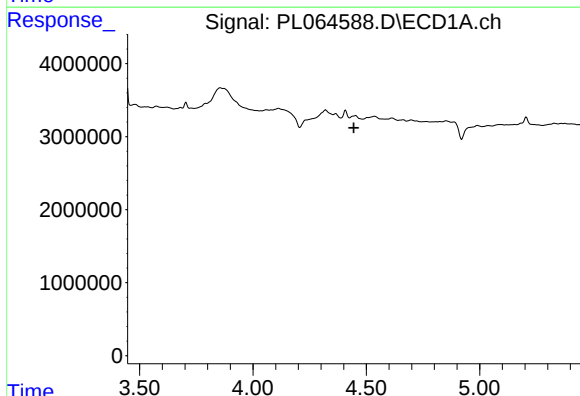


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

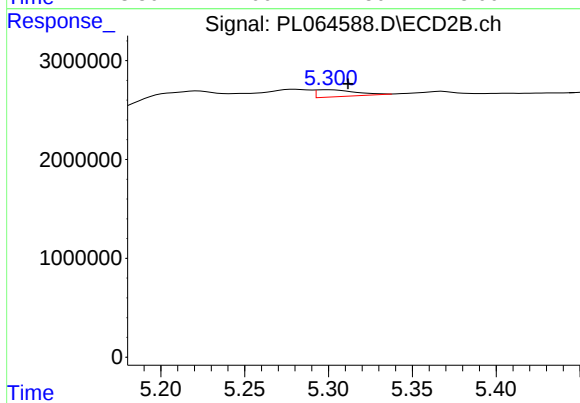

#4 Heptachlor


R.T.: 5.301 min
Delta R.T.: -0.011 min
Response: 1130915
Conc: 0.32 ng/ml

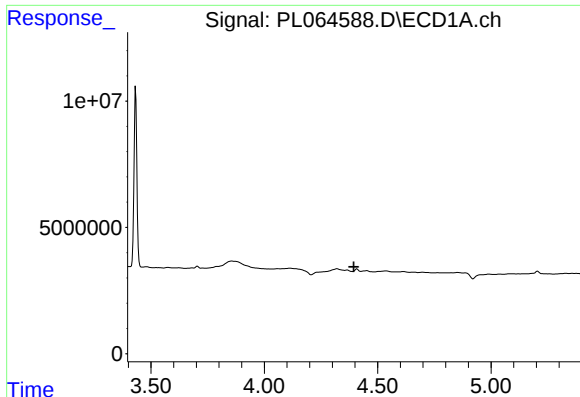

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

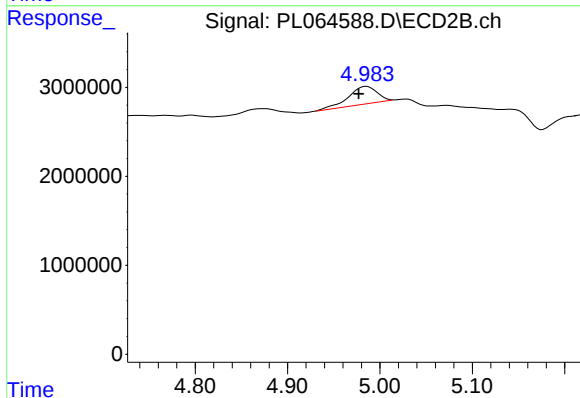


#6 beta-BHC

R.T.: 4.986 min
Delta R.T.: 0.009 min
Response: 4475789
Conc: 2.64 ng/ml

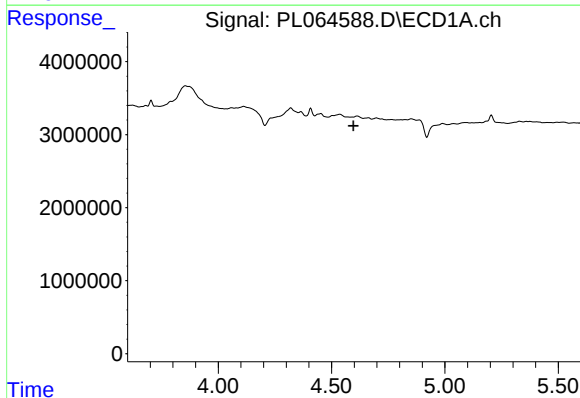


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

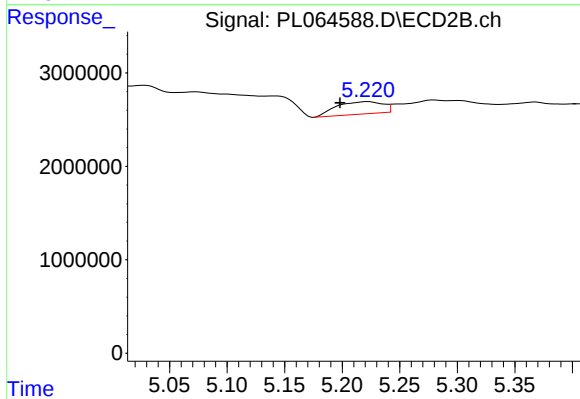

#7 delta-BHC


R.T.: 5.222 min
Delta R.T.: 0.024 min
Response: 3700861
Conc: 1.20 ng/ml

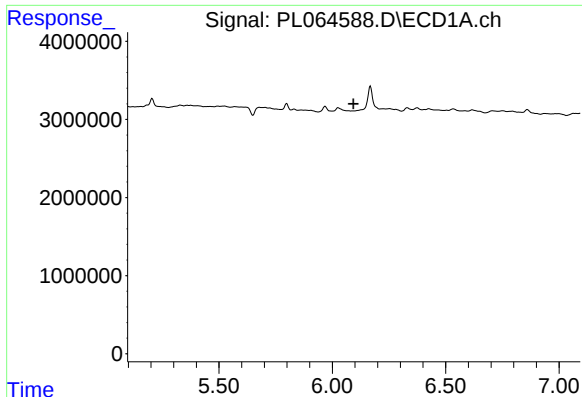

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.094 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

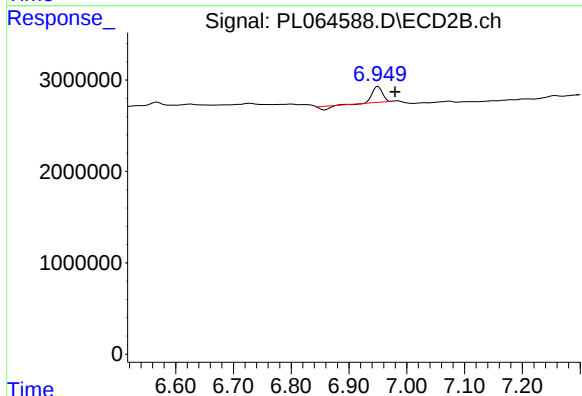


#16 4,4'-DDD

R.T.: 6.950 min
Delta R.T.: -0.030 min
Response: 1759710
Conc: 0.76 ng/ml

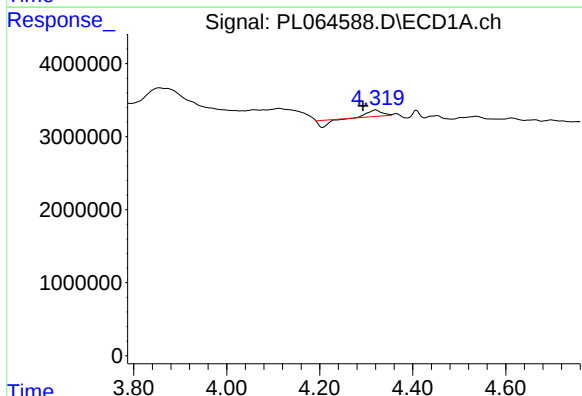


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.027 min
Response: 703989
Conc: 6.40 ng/ml

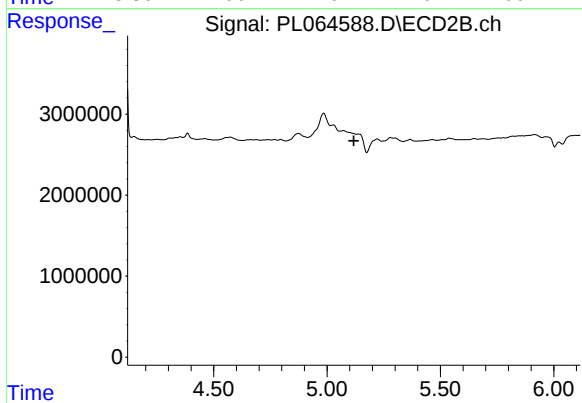

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

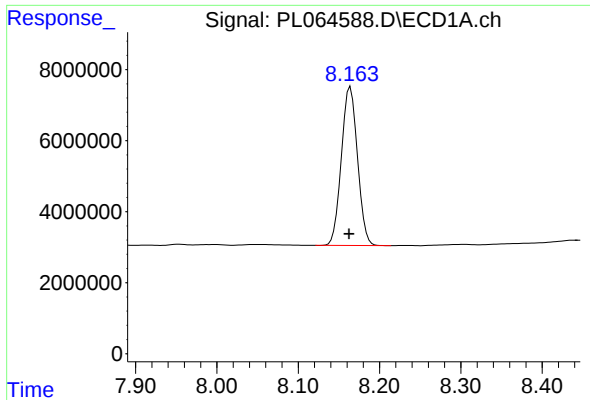

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 61372352
Conc: 19.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

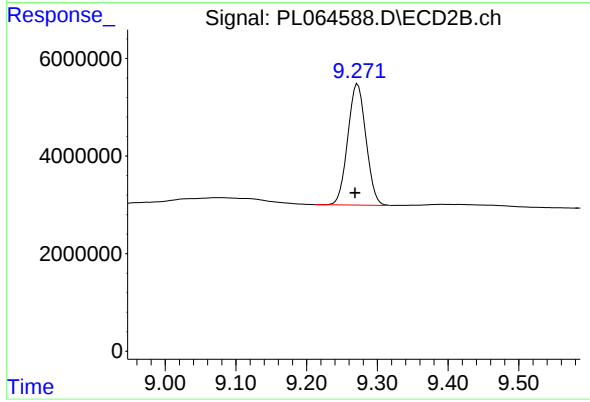

#28 Decachlorobiphenyl

R.T.: 9.272 min
Delta R.T.: 0.004 min
Response: 44394103
Conc: 21.68 ng/ml