

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 13:59
 Operator : AR\AJ
 Sample : M1292-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-003-0002

Manual Integrations
 APPROVED

Ankita
 2/4/2021 12:51:35 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 06:13:09 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	60338067	49101990	19.821	20.613
28)	SA Decachlor...	8.165	9.273	48248988	52100293	15.310	25.447 #
Target Compounds							
12)	B 4,4'-DDE	5.582	6.483	43358958	34655342	11.502	13.384m
17)	MA 4,4'-DDT	6.334	7.281	58232948	36567122	18.975m	17.803m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 13:59
Operator : AR\AJ
Sample : M1292-05
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU421-003-0002


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:35 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 06:13:09 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

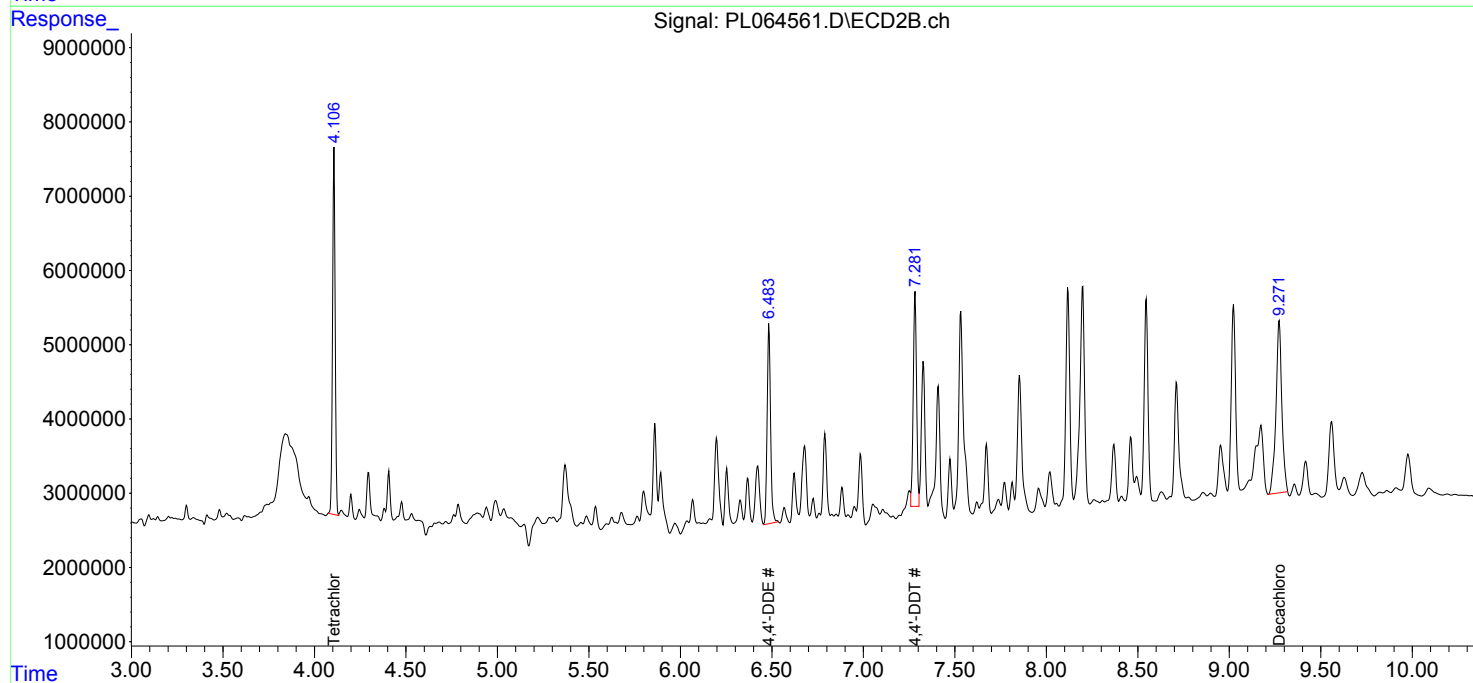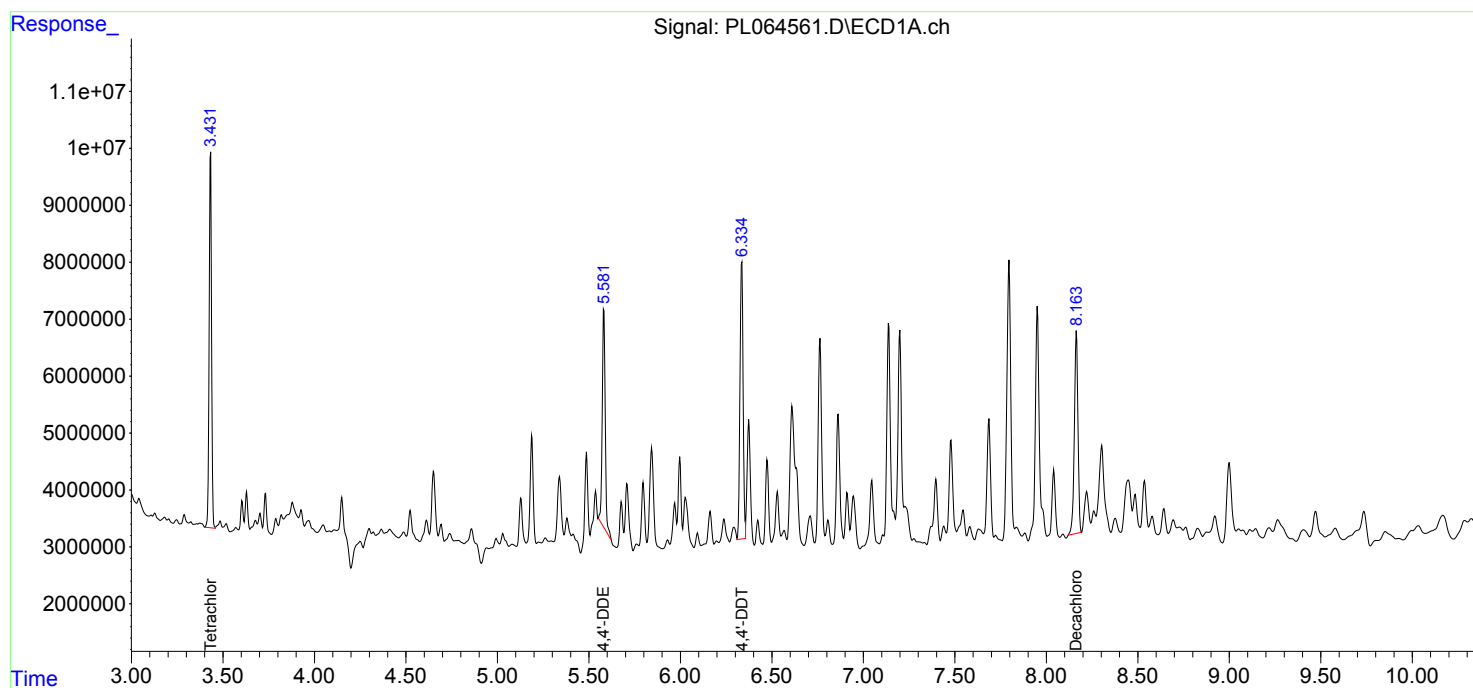

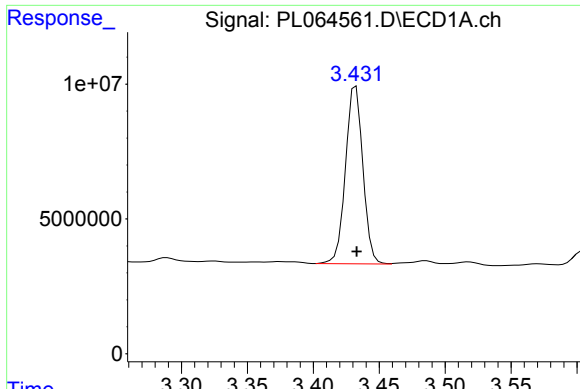


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 60338067
Conc: 19.82 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-0002


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:35 PM

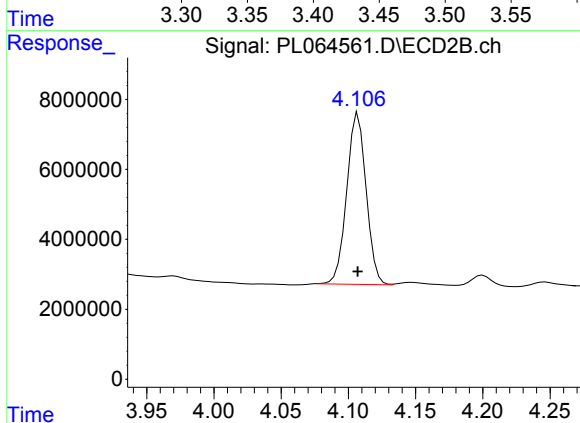


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 49101990
Conc: 20.61 ng/ml

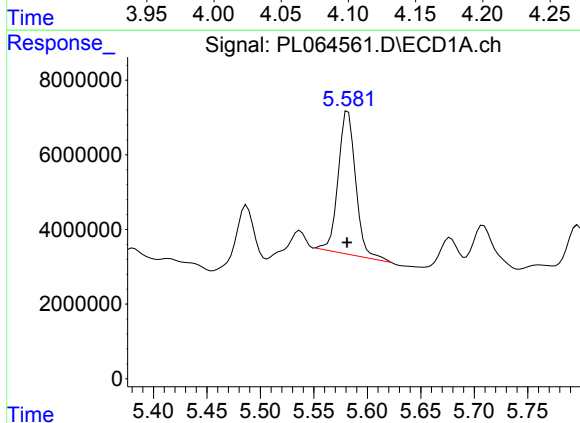


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 43358958
Conc: 11.50 ng/ml

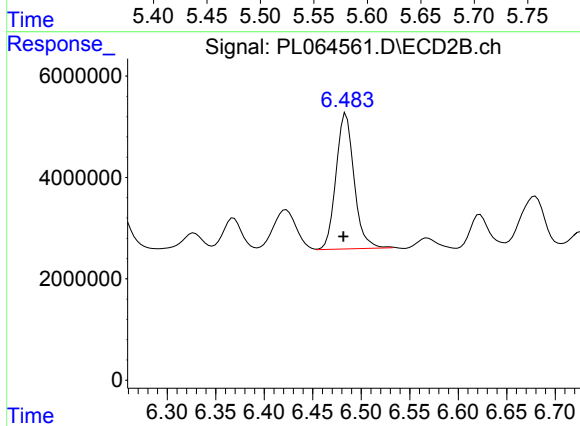

#12 4,4'-DDE

R.T.: 6.483 min
Delta R.T.: 0.001 min
Response: 34655342
Conc: 13.38 ng/ml m

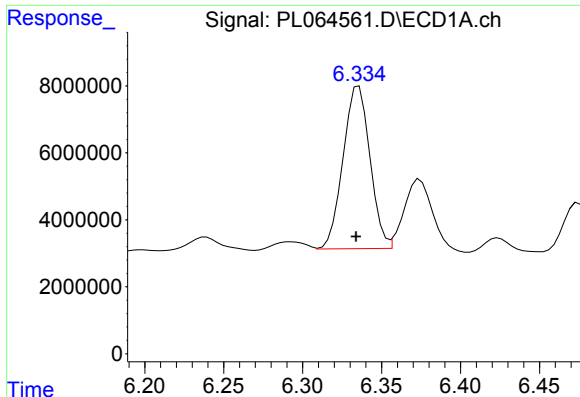


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 58232948
Conc: 18.97 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OU421-003-0002


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:35 PM

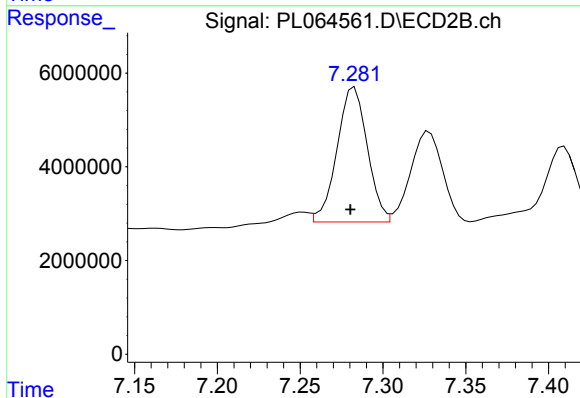


#17 4,4'-DDT

R.T.: 7.281 min
Delta R.T.: 0.001 min
Response: 36567122
Conc: 17.80 ng/ml m

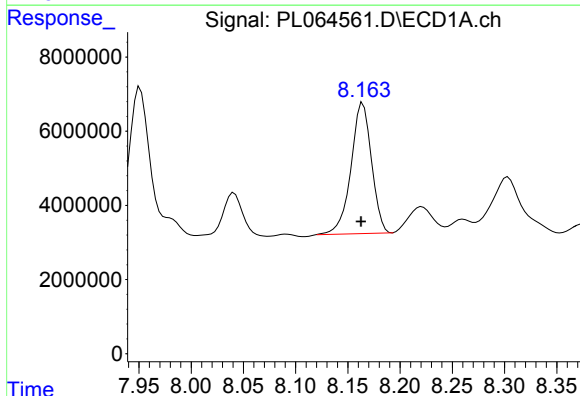

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: 0.002 min
Response: 48248988
Conc: 15.31 ng/ml

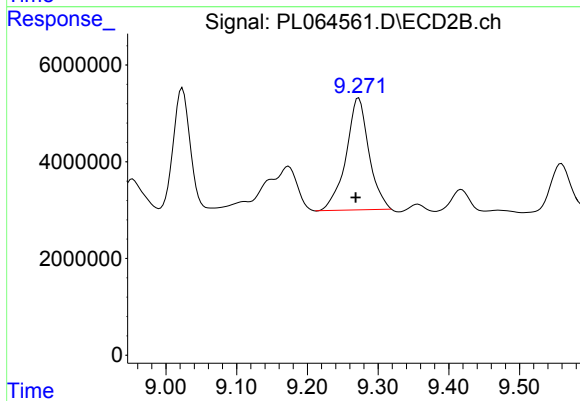

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.004 min
Response: 52100293
Conc: 25.45 ng/ml