

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064566.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2021 15:10
 Operator : AR\AJ
 Sample : M1292-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-003-1015

Manual Integrations
 APPROVED

Ankita
 2/4/2021 12:51:39 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:34:05 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.433	4.108	70475761	58512443	23.151	24.564
28) SA Decachlor...	8.164	9.273	87932122	65113831	27.903	31.803
Target Compounds						
12) B 4,4'-DDE	5.581	6.485	5360899	3781263	1.422m	1.460
17) MA 4,4'-DDT	6.335	7.283	6540900	3509586	2.131	1.709m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064566.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2021 15:10
Operator : AR\AJ
Sample : M1292-08
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:39 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:34:05 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

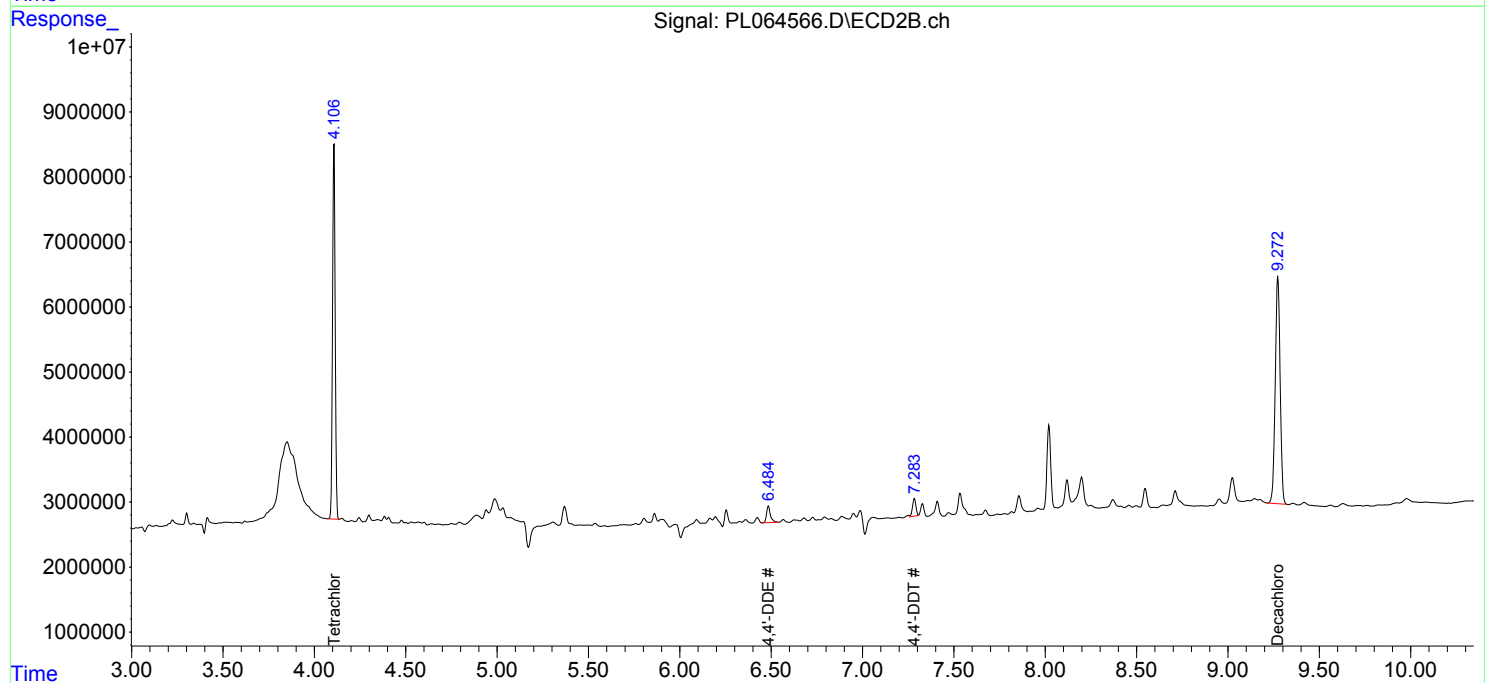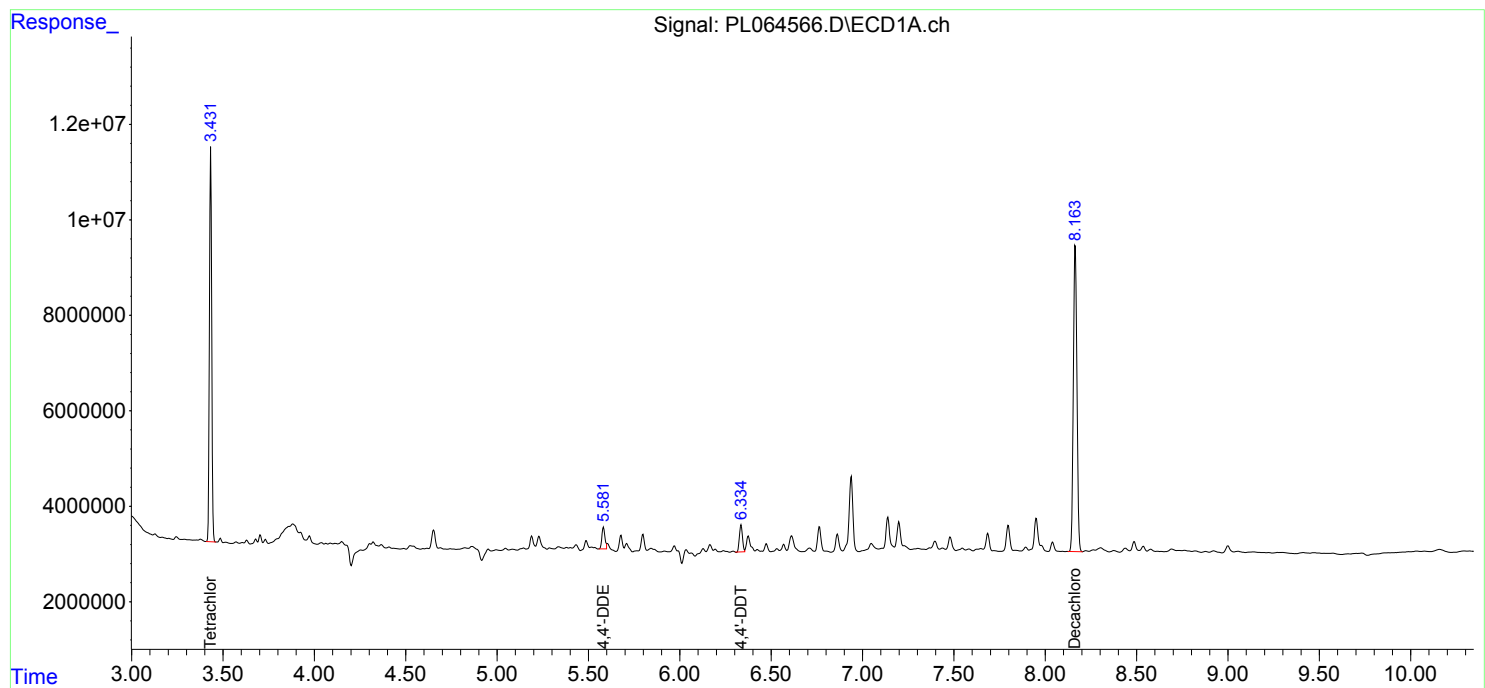

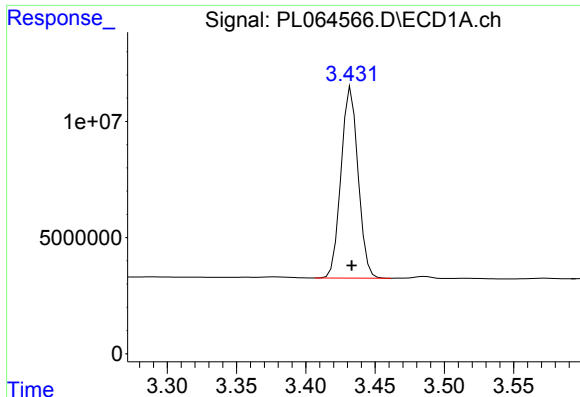


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 70475761
Conc: 23.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:39 PM

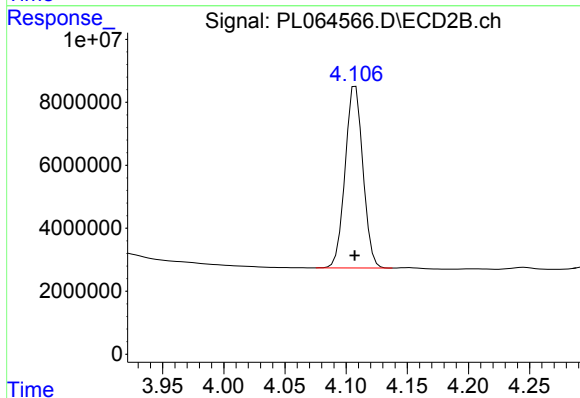


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 58512443
Conc: 24.56 ng/ml

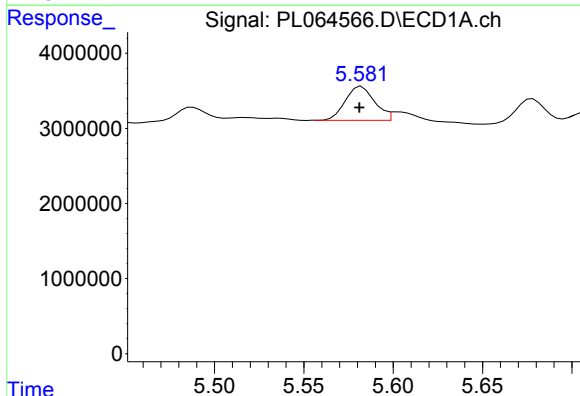


#12 4,4'-DDE

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 5360899
Conc: 1.42 ng/ml m

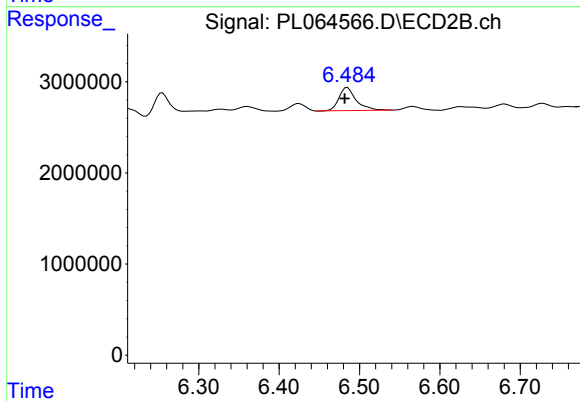

#12 4,4'-DDE

R.T.: 6.485 min
Delta R.T.: 0.003 min
Response: 3781263
Conc: 1.46 ng/ml

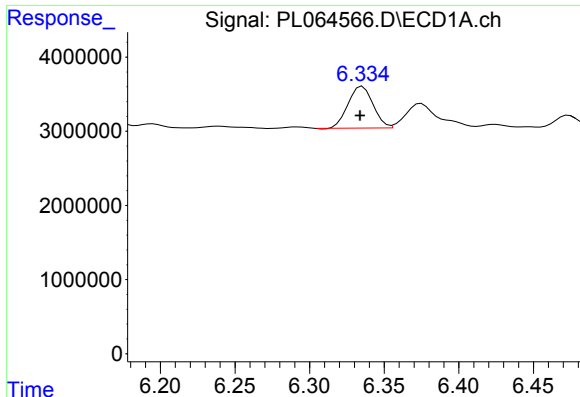


#17 4,4'-DDT

R.T.: 6.335 min
Delta R.T.: 0.002 min
Response: 6540900
Conc: 2.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-1015


Manual Integrations
APPROVED

Ankita
2/4/2021 12:51:39 PM

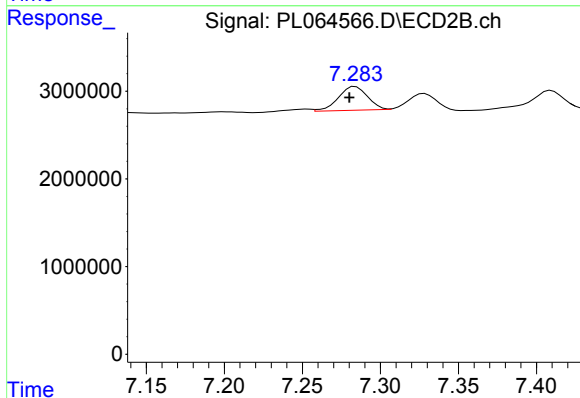


#17 4,4'-DDT

R.T.: 7.283 min
Delta R.T.: 0.002 min
Response: 3509586
Conc: 1.71 ng/ml m

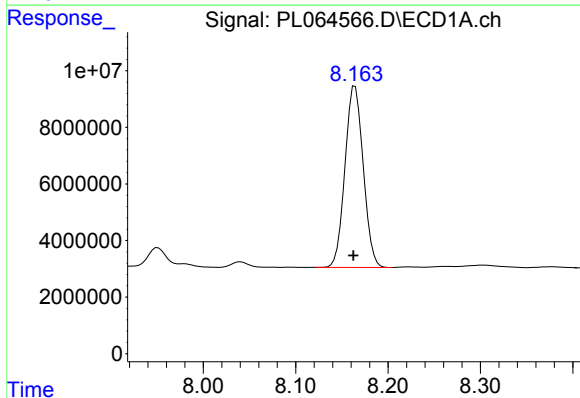

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 87932122
Conc: 27.90 ng/ml

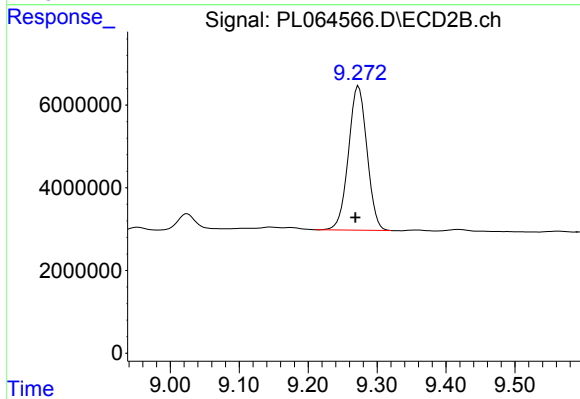

#28 Decachlorobiphenyl

R.T.: 9.273 min
Delta R.T.: 0.005 min
Response: 65113831
Conc: 31.80 ng/ml