

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
 Data File : PL064608.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 01:40
 Operator : AR\AJ
 Sample : M1292-18
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 2021-01-28-EB

Manual Integrations
 APPROVED

Ankita
 2/4/2021 12:52:19 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 04 03:52:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.108	79474122	45971984	26.107	19.299 #
28)	SA Decachlor...	8.164	9.271	50340431	34044349	15.974	16.628m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020321\
Data File : PL064608.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 01:40
Operator : AR\AJ
Sample : M1292-18
Misc :
ALS Vial : 50 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
2021-01-28-EB


Manual Integrations
APPROVED

Ankita
2/4/2021 12:52:19 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 04 03:52:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

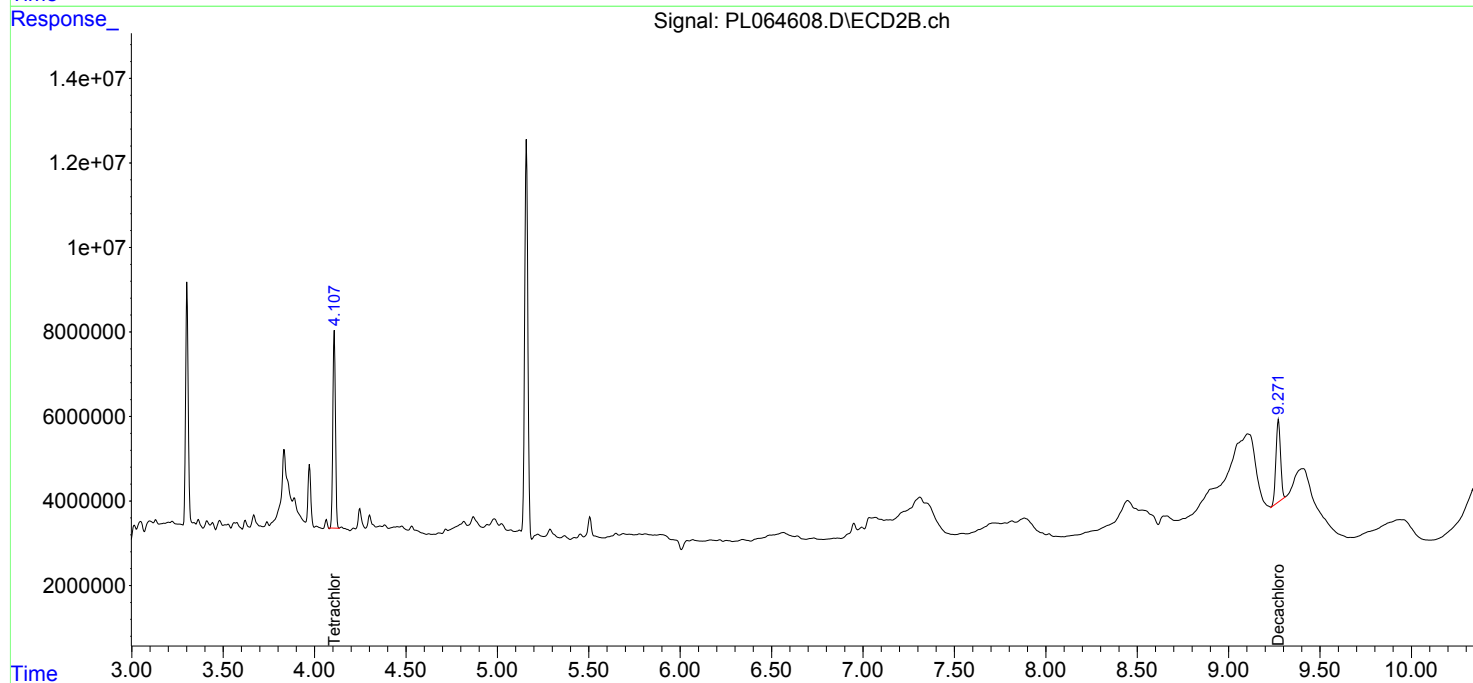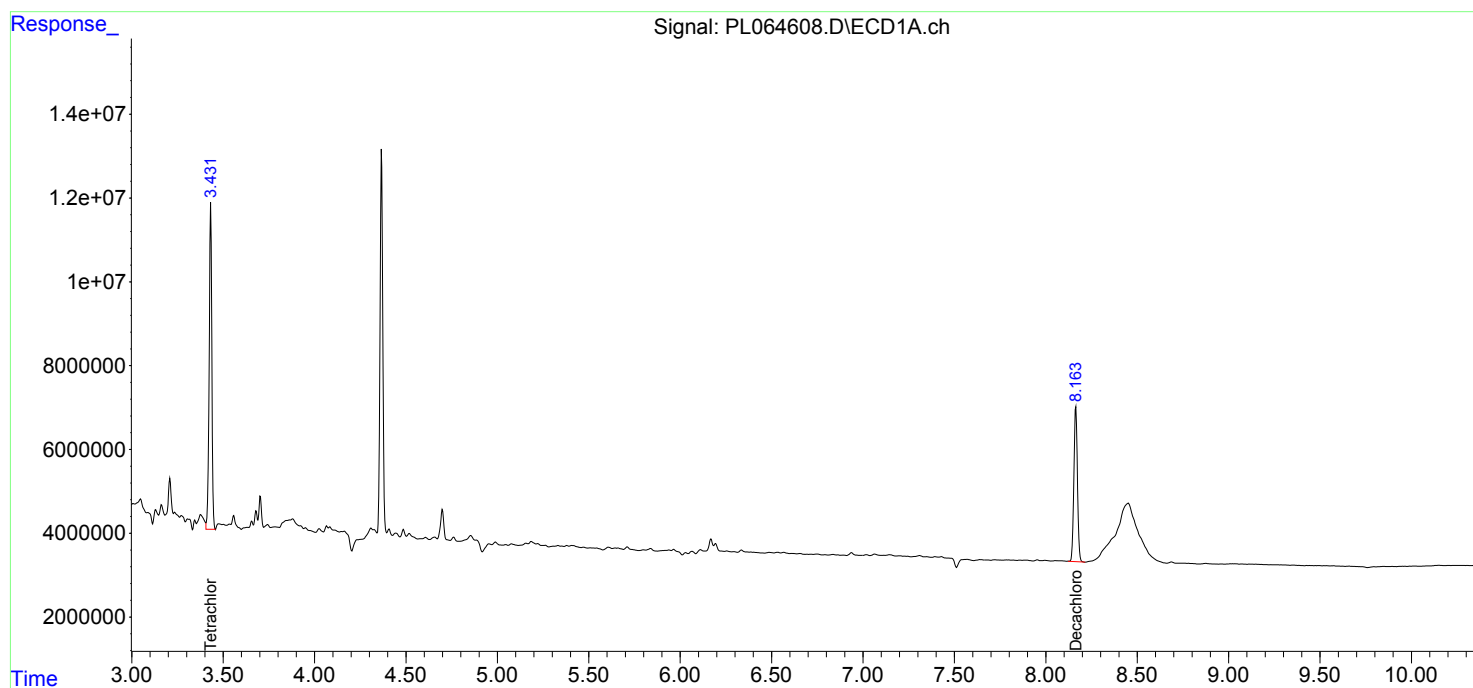

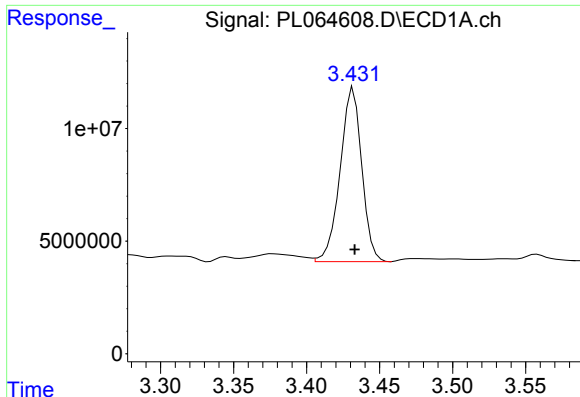


#1 Tetrachloro-m-xylene

R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 79474122
Conc: 26.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
2021-01-28-EB


Manual Integrations
APPROVED

Ankita
2/4/2021 12:52:19 PM

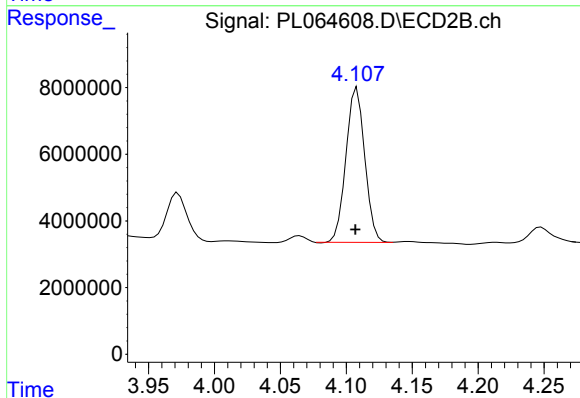


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 45971984
Conc: 19.30 ng/ml

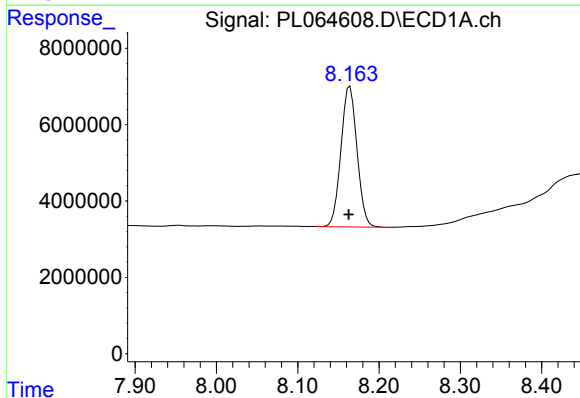

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.002 min
Response: 50340431
Conc: 15.97 ng/ml

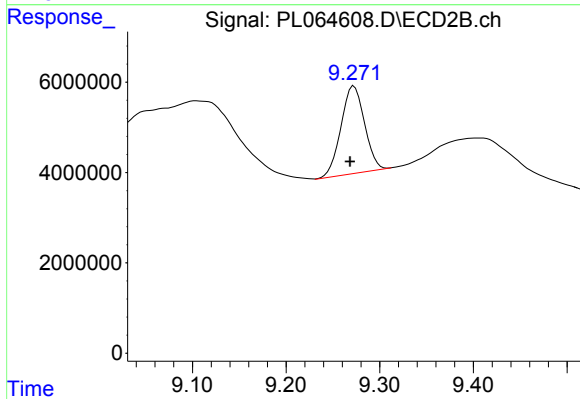

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.002 min
Response: 34044349
Conc: 16.63 ng/ml m