

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020323\
 Data File : PL080724.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Feb 2023 12:05
 Operator : AR\AJ
 Sample : 01397-01RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BI-WEEKLY-INFLUENTRE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 02/06/2023
 Supervised By :Ankita Jodhani 02/06/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 03 23:40:44 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
 Quant Title : GC Extractables
 QLast Update : Sun Jan 22 23:56:48 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.351	2.689	19944797	13389777	9.299	6.096 #
28) SA Decachlor...	8.787	7.834	54883228	8874475	31.348	3.725m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020323\
Data File : PL080724.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Feb 2023 12:05
Operator : AR\AJ
Sample : 01397-01RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 02/06/2023
Supervised By : Ankita Jodhani 02/06/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 03 23:40:44 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012023.M
Quant Title : GC Extractables
QLast Update : Sun Jan 22 23:56:48 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

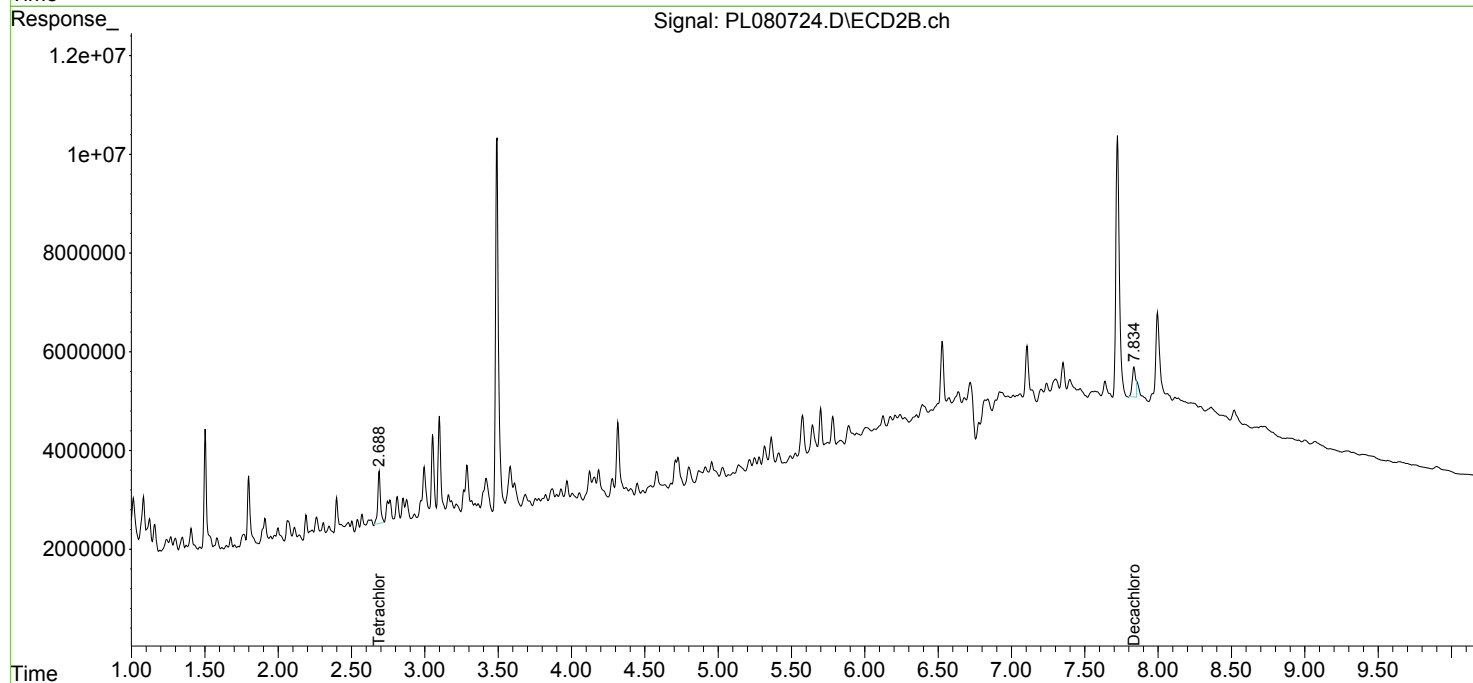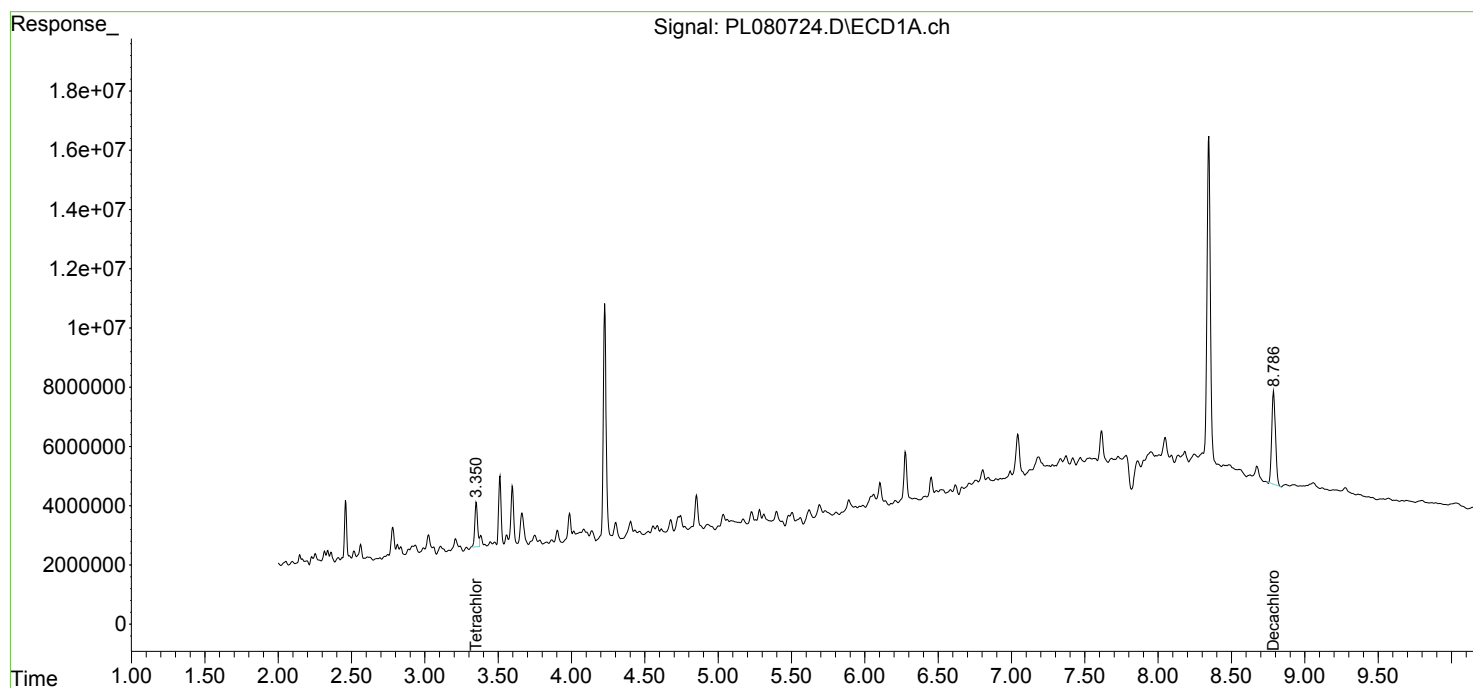

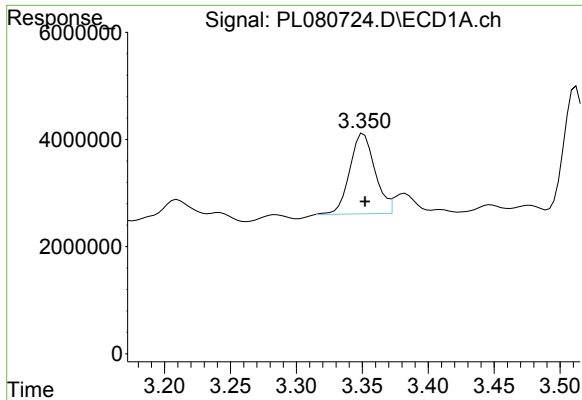


#1 Tetrachloro-m-xylene

R.T.: 3.351 min
Delta R.T.: 0.000 min
Response: 19944797
Conc: 9.30 ng/ml

Instrument :
ECD_L
ClientSampleId :
BI-WEEKLY-INFLUENTRE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 02/06/2023
Supervised By :Ankita Jodhani 02/06/2023

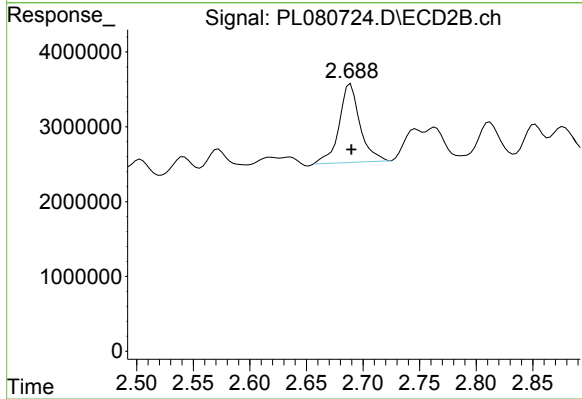


#1 Tetrachloro-m-xylene

R.T.: 2.689 min
Delta R.T.: 0.000 min
Response: 13389777
Conc: 6.10 ng/ml

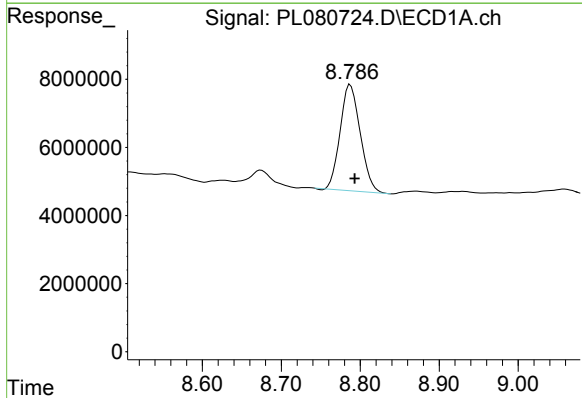

#28 Decachlorobiphenyl

R.T.: 8.787 min
Delta R.T.: -0.006 min
Response: 54883228
Conc: 31.35 ng/ml

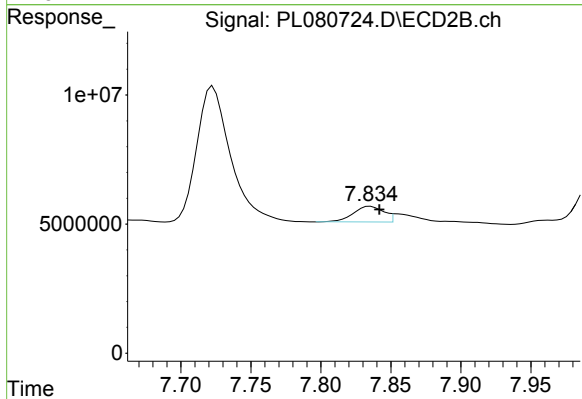

#28 Decachlorobiphenyl

R.T.: 7.834 min
Delta R.T.: -0.008 min
Response: 8874475
Conc: 3.72 ng/ml m